

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
 Data File : PL067949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2021 18:55
 Operator : AR\AJ
 Sample : M2904-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:18:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.527	11541057	21012510	20.992	22.289
28)	SA Decachlor...	10.219	11.425	13990444	20455854	19.741	20.537
Target Compounds							
3)	MA gamma-BHC...	5.584f	0.000	307488	0	0.410	N.D. #
6)	B beta-BHC	0.000	6.740f	0	203178	N.D.	0.374 #
8)	B Heptachlo...	6.936f	0.000	354523	0	0.507	N.D. #
9)	A Endosulfan I	7.320	0.000	611112	0	0.909	N.D. #
13)	MA Dieldrin	7.593	0.000	33726	0	0.048	N.D. #
15)	B Endosulfa...	8.183	9.176f	622454	917971	1.011	1.151
16)	A 4,4'-DDD	8.027f	0.000	859714	0	1.479	N.D. #
17)	MA 4,4'-DDT	0.000	9.385	0	440612	N.D.	0.601 #
19)	B Endosulfa...	8.586f	0.000	1485970	0	2.341	N.D. #
20)	A Methoxychlor	8.909	0.000	354728	0	0.998	N.D. #
21)	B Endrin ke...	0.000	10.049f	0	49557	N.D.	0.055 #
27)	Chlordane-5	8.183	0.000	622454	0	28.450	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
Data File : PL067949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2021 18:55
Operator : AR\AJ
Sample : M2904-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:18:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

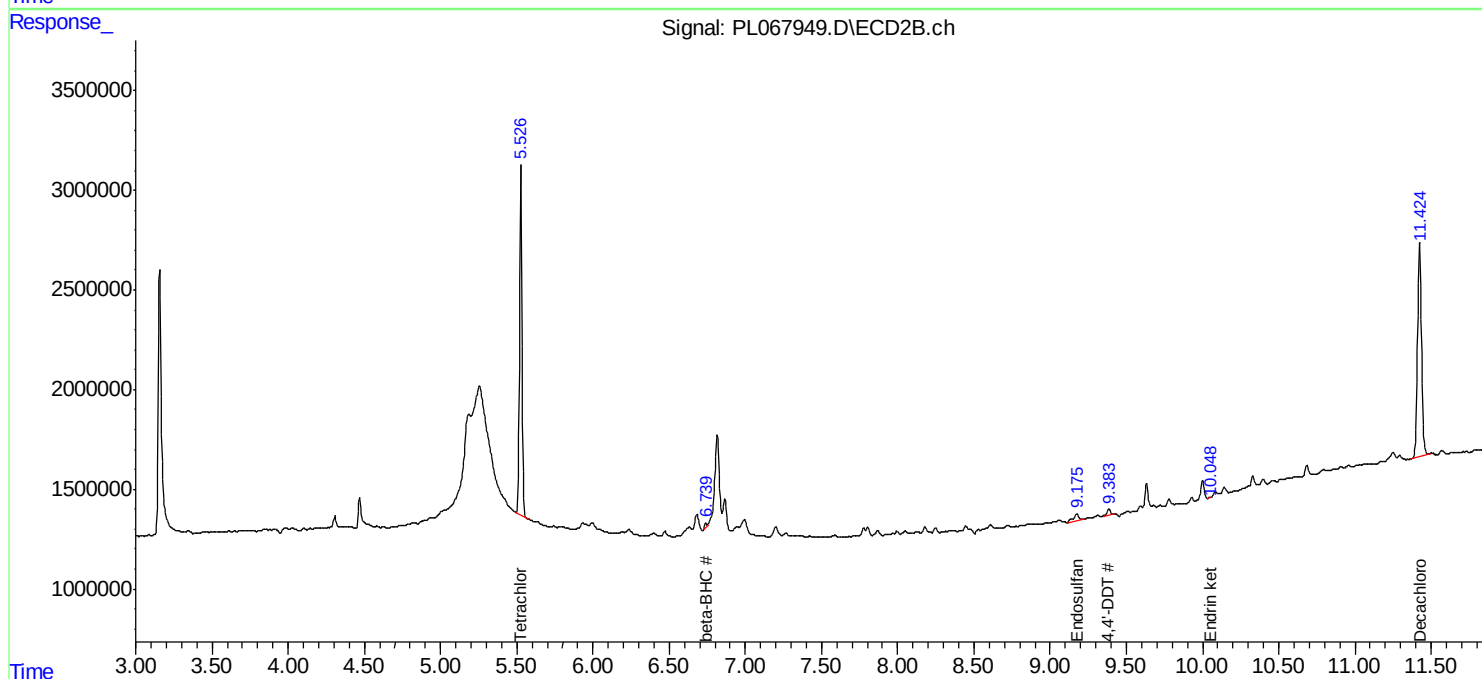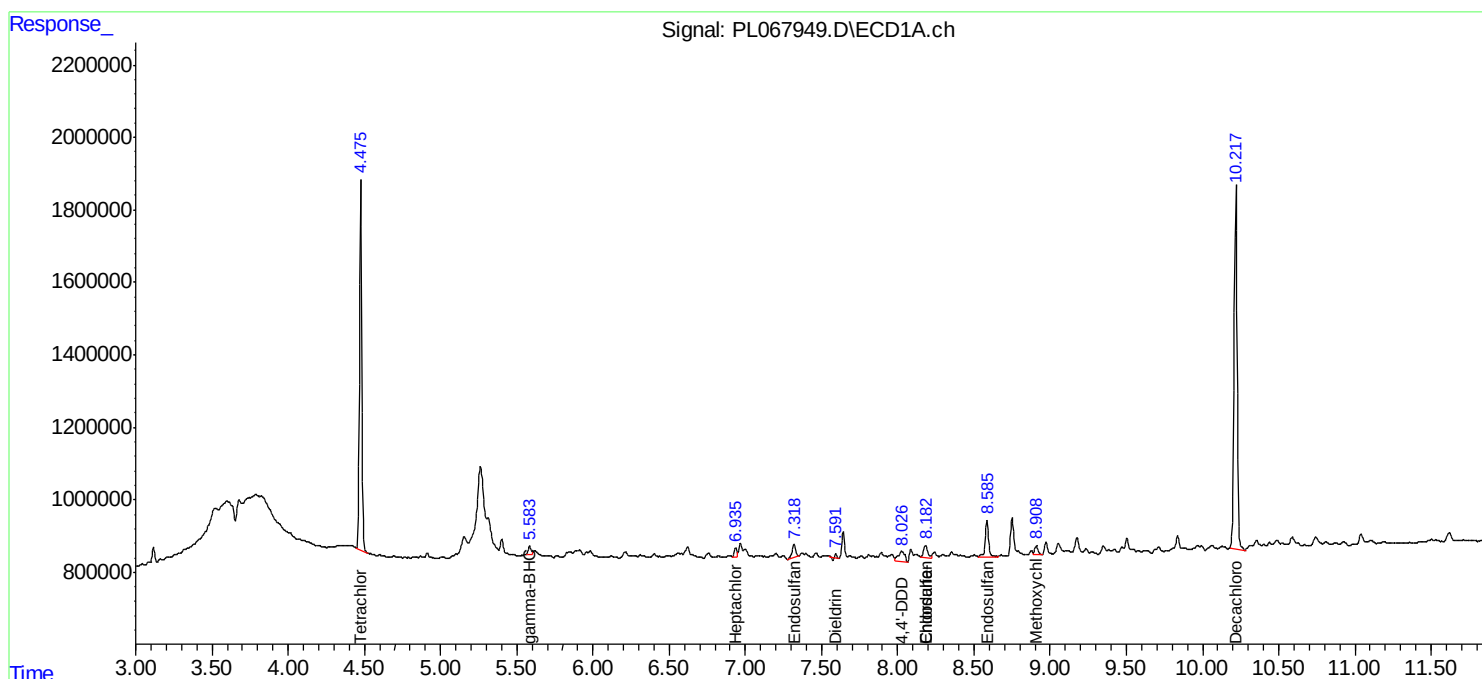


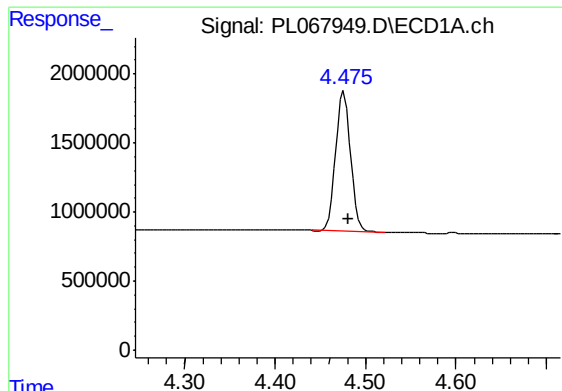

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 11541057
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

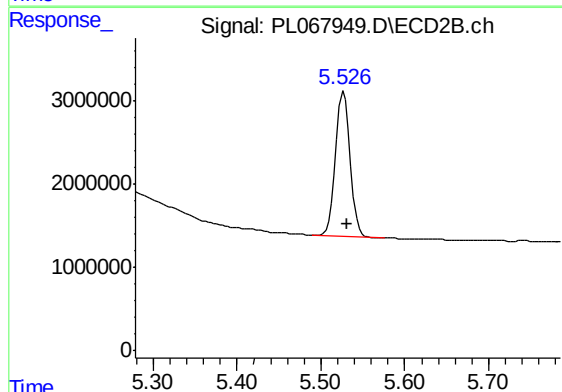


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 21012510
Conc: 22.29 ng/ml

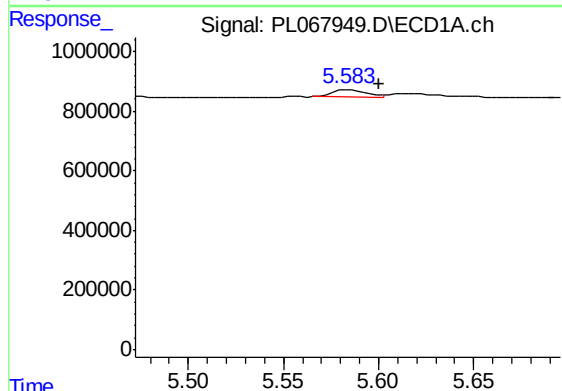


#3 gamma-BHC (Lindane)

R.T.: 5.584 min
Delta R.T.: -0.016 min
Response: 307488
Conc: 0.41 ng/ml

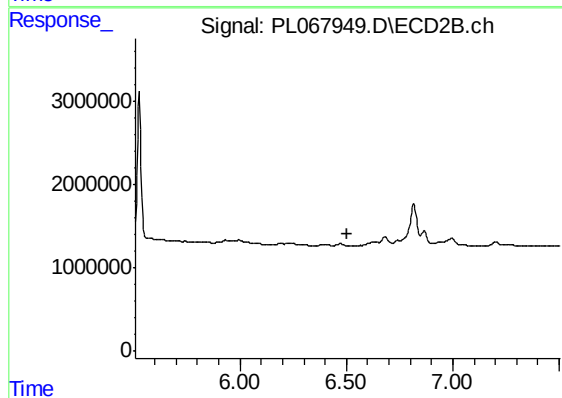

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

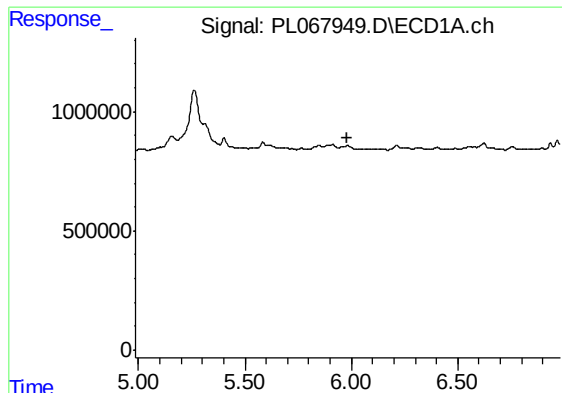

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

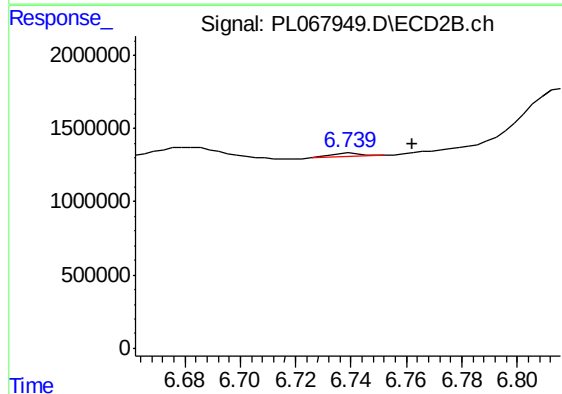


#6 beta-BHC

R.T.: 6.740 min
Delta R.T.: -0.022 min
Response: 203178
Conc: 0.37 ng/ml

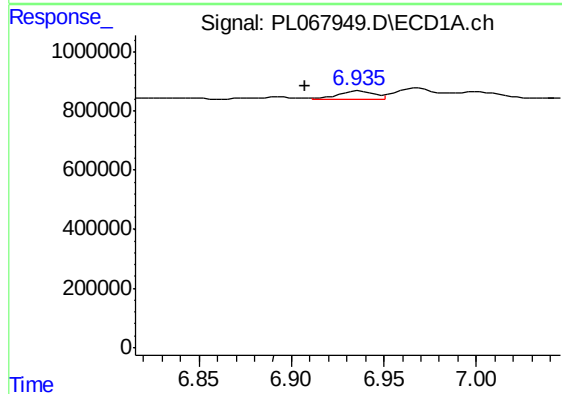


#8 Heptachlor epoxide

R.T.: 6.936 min
Delta R.T.: 0.029 min
Response: 354523
Conc: 0.51 ng/ml

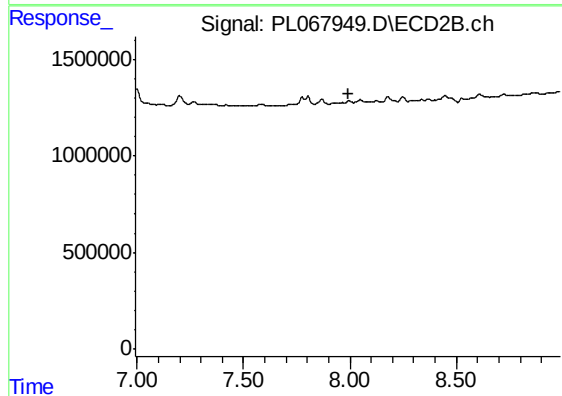

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.991 min
Response: 0
Conc: N.D.

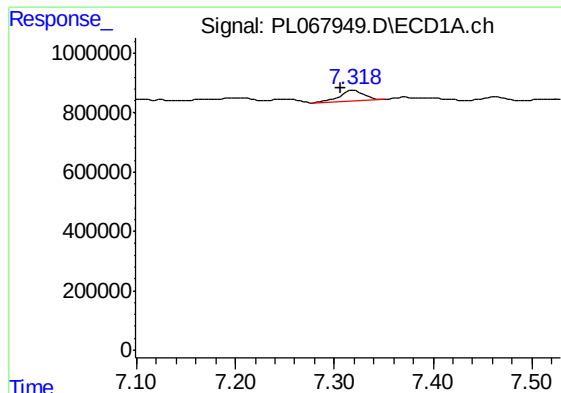

#9 Endosulfan I


R.T.: 7.320 min
Delta R.T.: 0.013 min
Response: 611112
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

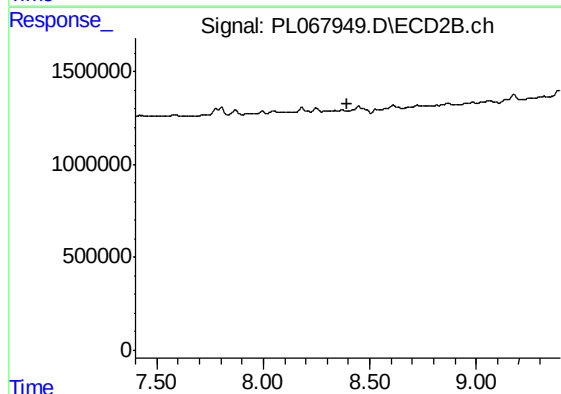


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.397 min
Response: 0
Conc: N.D.

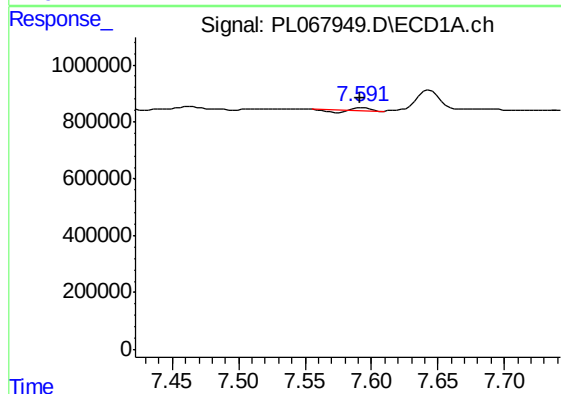


#13 Dieldrin

R.T.: 7.593 min
Delta R.T.: 0.000 min
Response: 33726
Conc: 0.05 ng/ml

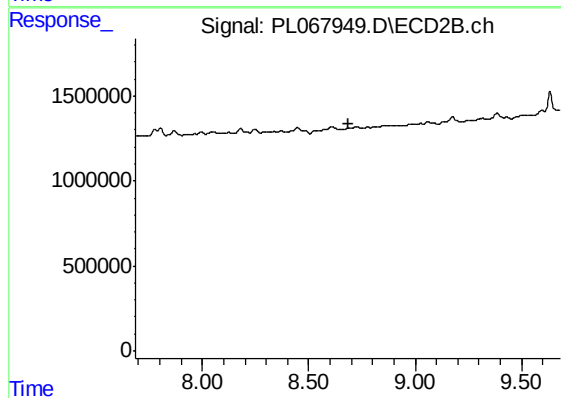

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.685 min
Response: 0
Conc: N.D.

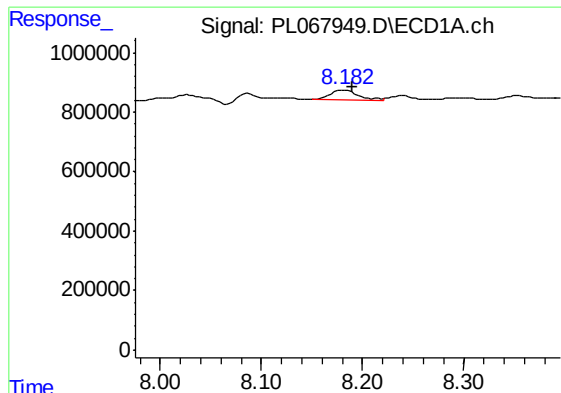

#15 Endosulfan II


R.T.: 8.183 min
Delta R.T.: -0.007 min
Response: 622454
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

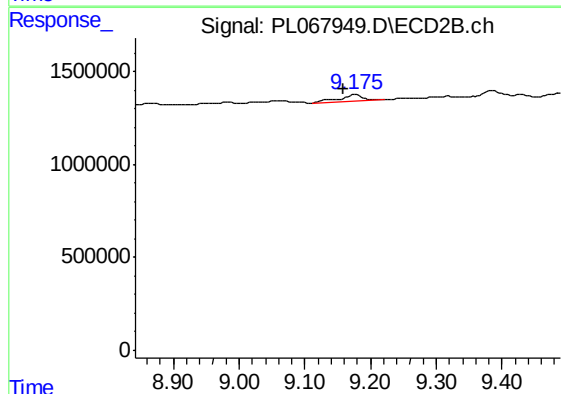


#15 Endosulfan II

R.T.: 9.176 min
Delta R.T.: 0.018 min
Response: 917971
Conc: 1.15 ng/ml

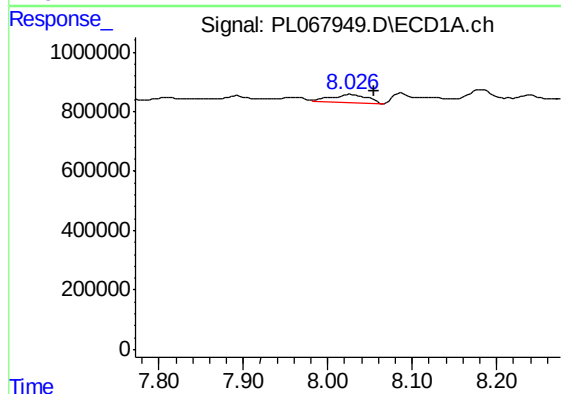


#16 4,4'-DDD

R.T.: 8.027 min
Delta R.T.: -0.028 min
Response: 859714
Conc: 1.48 ng/ml

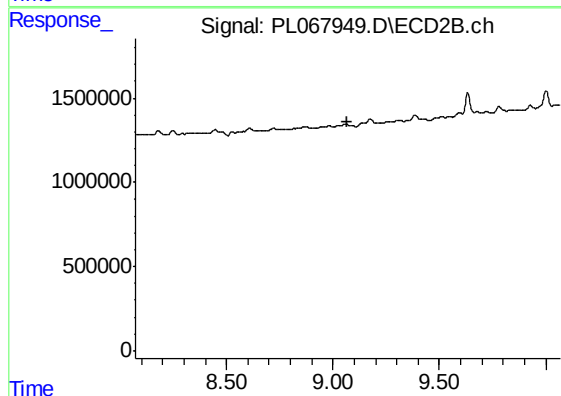

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

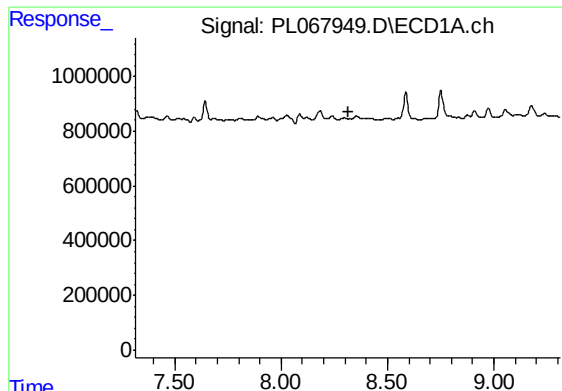

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-3

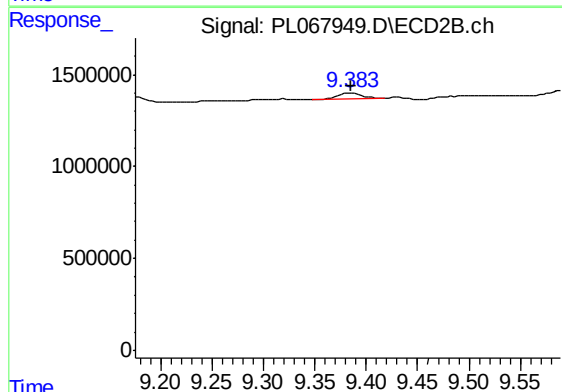


#17 4,4'-DDT

R.T.: 9.385 min
Delta R.T.: 0.000 min
Response: 440612
Conc: 0.60 ng/ml

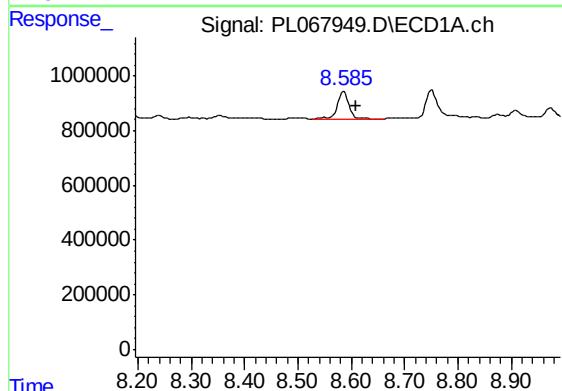


#19 Endosulfan Sulfate

R.T.: 8.586 min
Delta R.T.: -0.022 min
Response: 1485970
Conc: 2.34 ng/ml

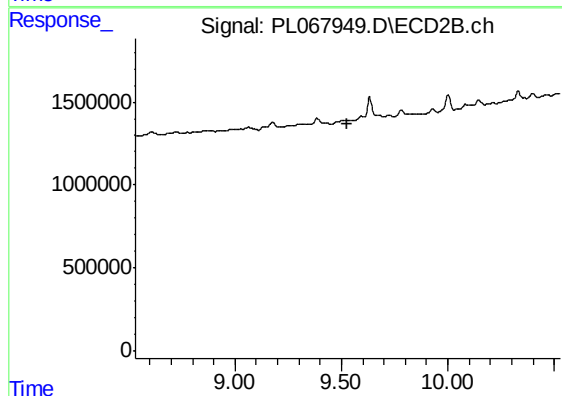

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

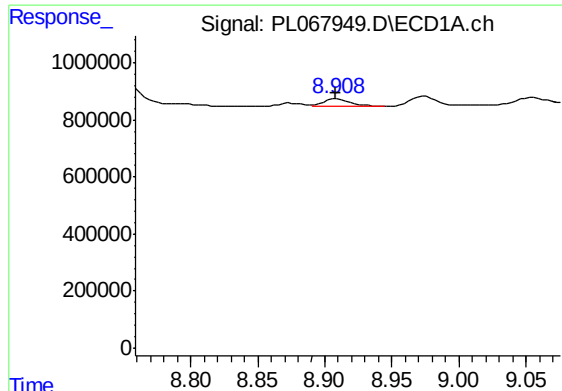

#20 Methoxychlor


R.T.: 8.909 min
Delta R.T.: 0.002 min
Response: 354728
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

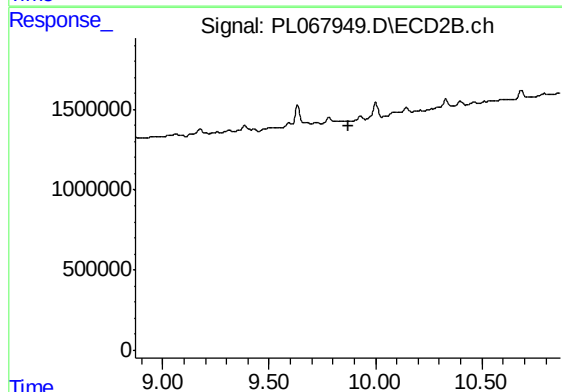


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.872 min
Response: 0
Conc: N.D.

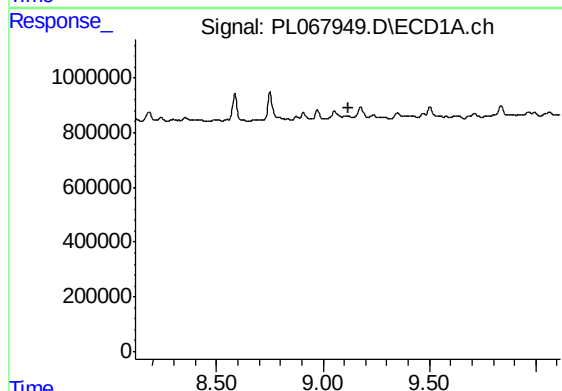


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

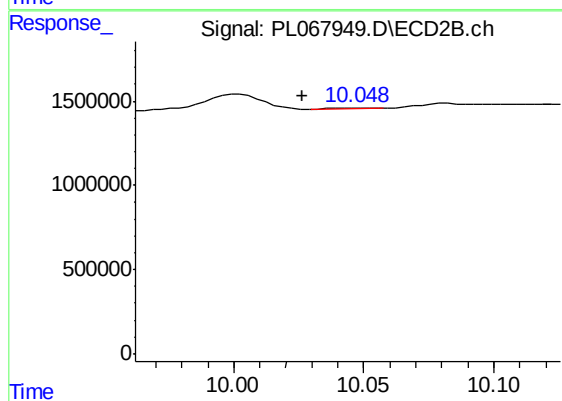

#21 Endrin ketone


R.T.: 10.049 min
Delta R.T.: 0.022 min
Response: 49557
Conc: 0.05 ng/ml

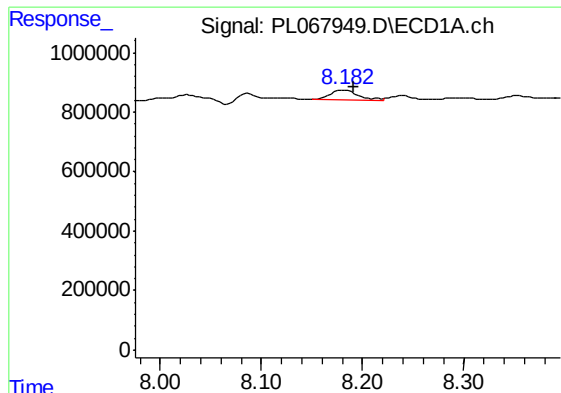

#27 Chlordane-5


R.T.: 8.183 min
Delta R.T.: -0.008 min
Response: 622454
Conc: 28.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

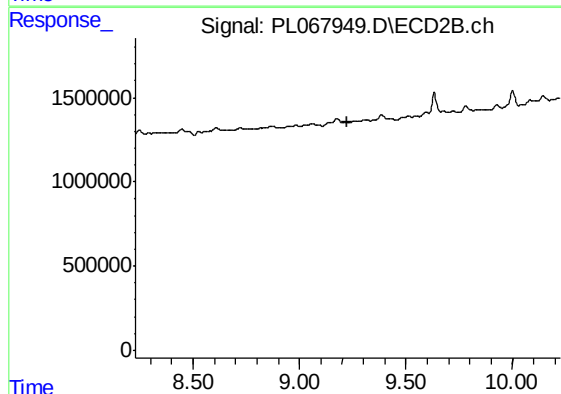


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

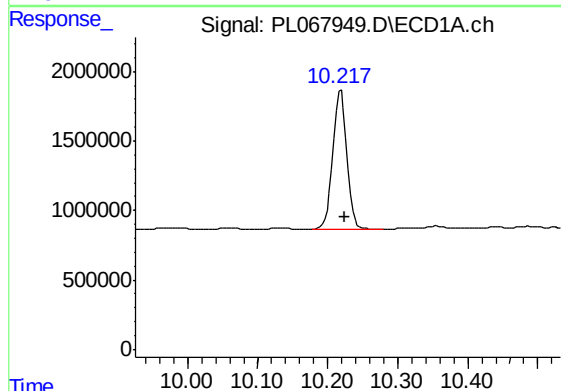

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 13990444
Conc: 19.74 ng/ml

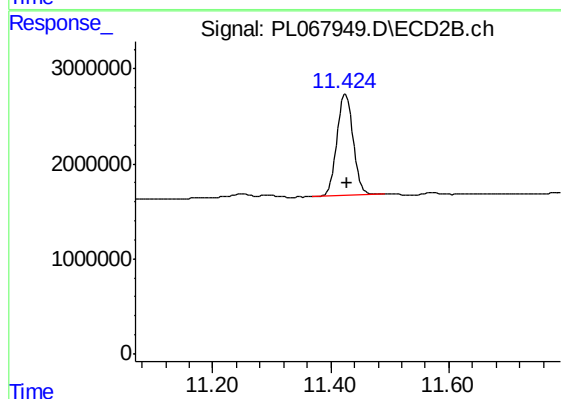

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 20455854
Conc: 20.54 ng/ml