

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
 Data File : PL037667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 18:25
 Operator : UA\AJ
 Sample : J3818-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:11:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	66614513	24260138	8.421	8.769
28)	SA Decachlor...	8.011	8.945	58239611	17372443	9.652	8.757
Target Compounds							
10)	B gamma-Chl...	5.246	0.000	7972176	0	0.851	N.D. #
11)	B alpha-Chl...	5.246f	0.000	7972176	0	0.878	N.D. #
12)	B 4,4'-DDE	5.451	6.247	12388202	14978108	1.403	5.886 #
14)	MA Endrin	5.890f	0.000	7292614	0	0.926	N.D. #
15)	B Endosulfa...	0.000	6.855f	0	165.6E6	N.D.	66.756 #
17)	MA 4,4'-DDT	6.196	0.000	24880401	0	3.854	N.D. #
20)	A Methoxychlor	0.000	7.424f	0	21169808	N.D.	18.913 #
21)	B Endrin ke...	0.000	7.575f	0	5992075	N.D.	2.952 #
25)	Chlordane-3	5.246	0.000	7972176	0	7.500	N.D. #
26)	Chlordane-4	5.246	0.000	7972176	0	8.274	N.D. #
27)	Chlordane-5	5.890	6.855	7292614	165.6E6	55.725	1839.889 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
Data File : PL037667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 18:25
Operator : UA\AJ
Sample : J3818-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:11:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

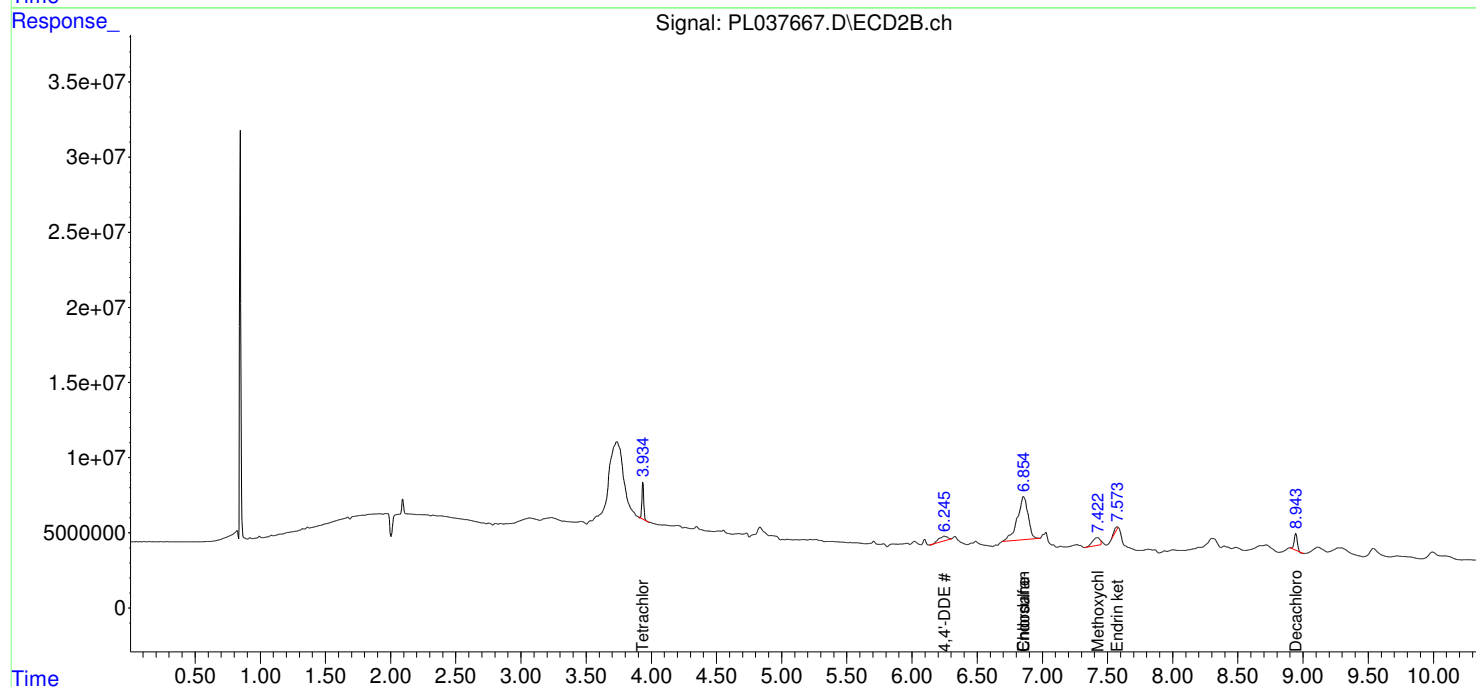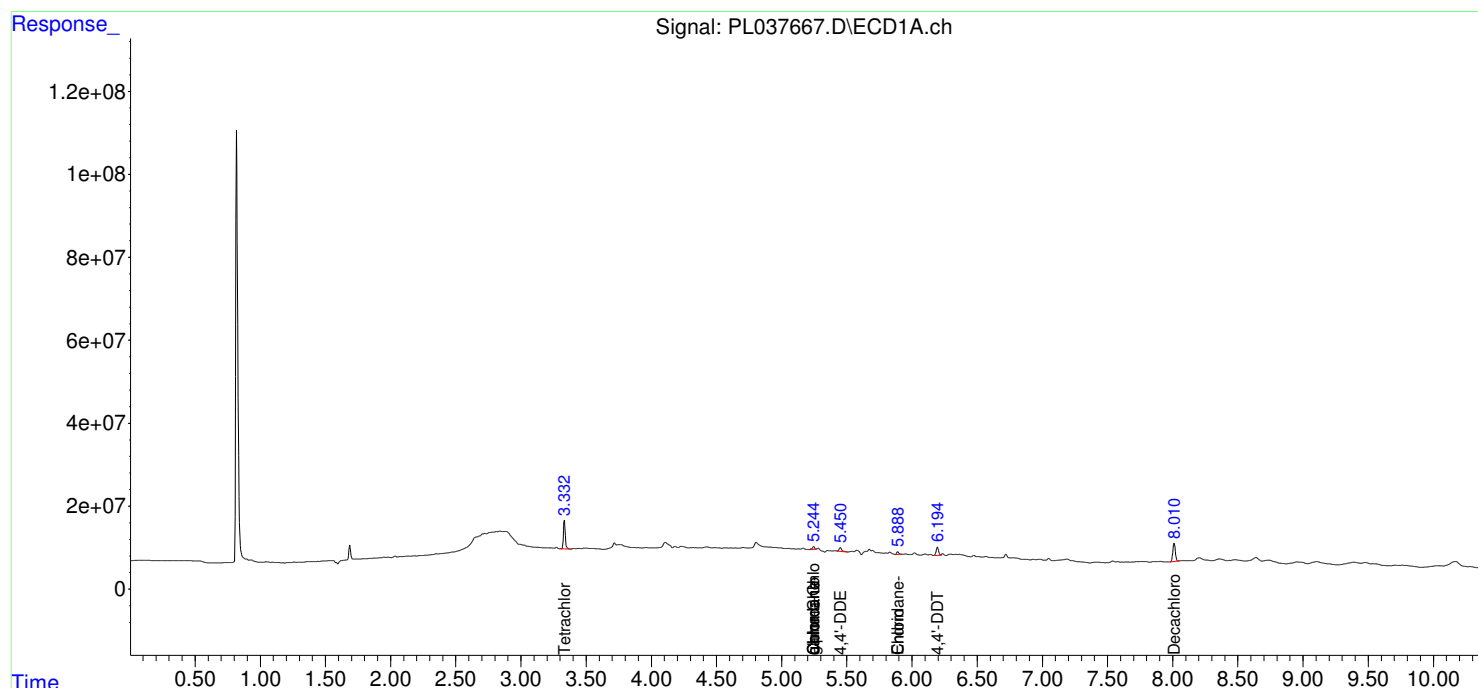


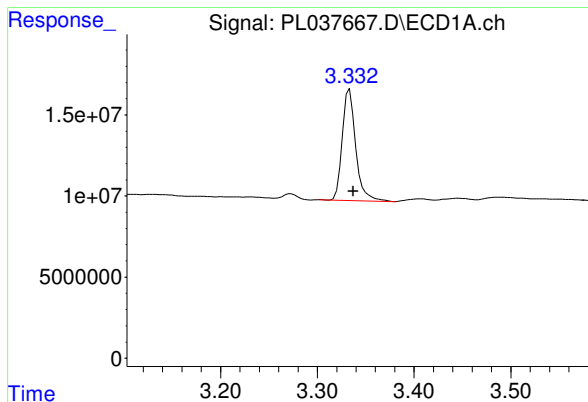

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 66614513
Conc: 8.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

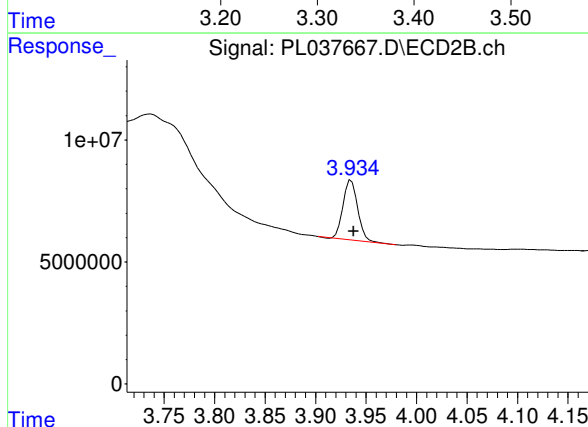


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 24260138
Conc: 8.77 ng/ml

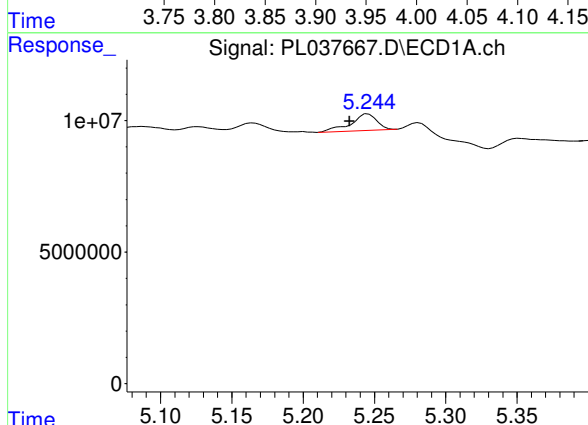


#10 gamma-Chlordane

R.T.: 5.246 min
Delta R.T.: 0.013 min
Response: 7972176
Conc: 0.85 ng/ml

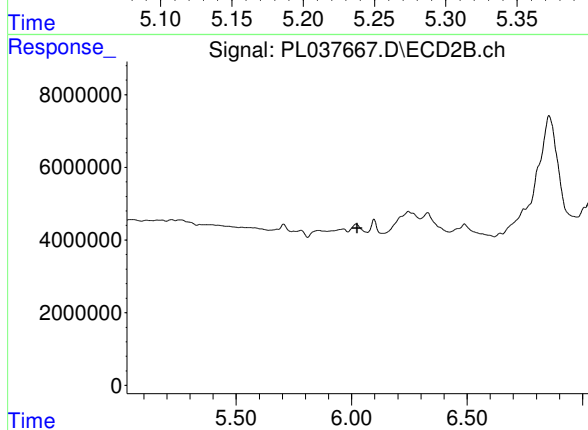

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

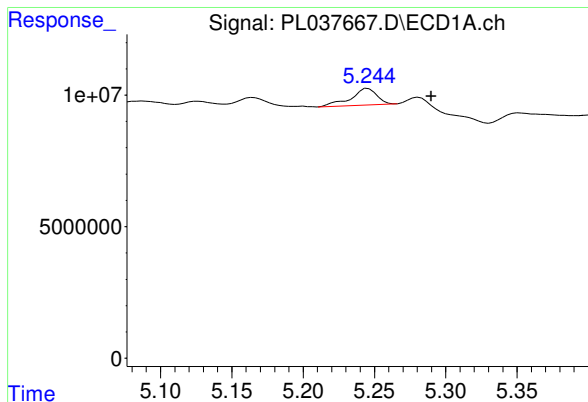

#11 alpha-Chlordane


R.T.: 5.246 min
Delta R.T.: -0.044 min
Response: 7972176
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

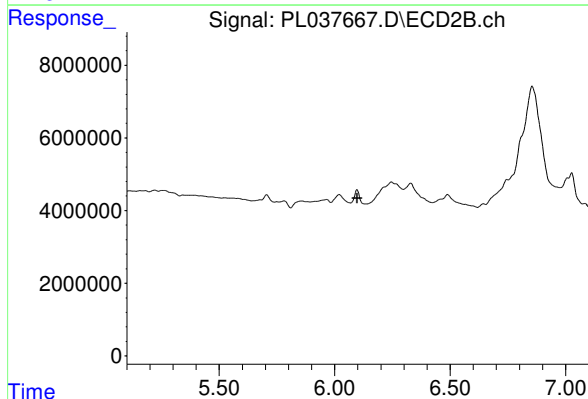


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

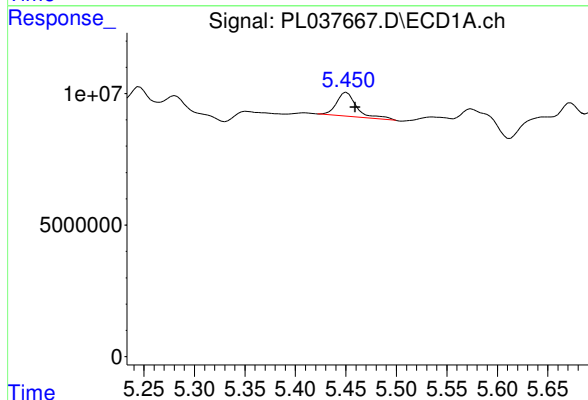


#12 4,4'-DDE

R.T.: 5.451 min
Delta R.T.: -0.008 min
Response: 12388202
Conc: 1.40 ng/ml

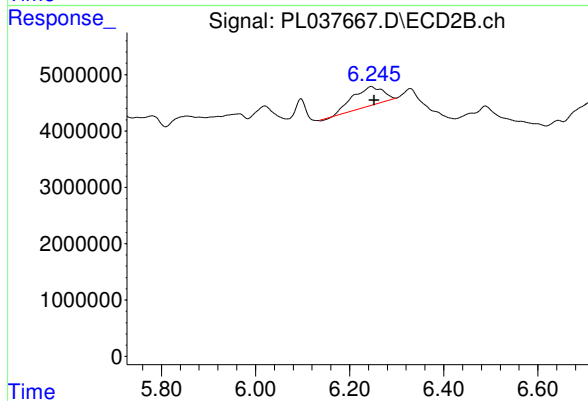

#12 4,4'-DDE


R.T.: 6.247 min
Delta R.T.: -0.006 min
Response: 14978108
Conc: 5.89 ng/ml

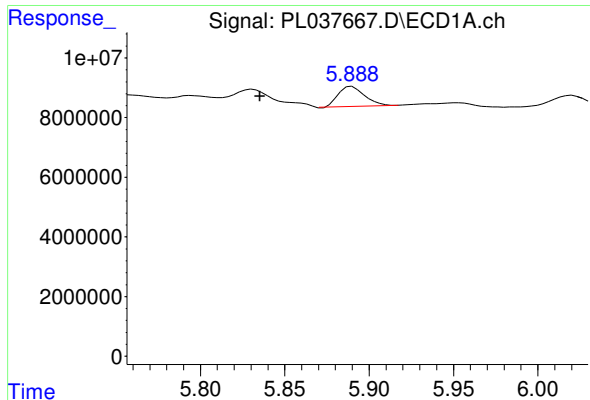

#14 Endrin


R.T.: 5.890 min
Delta R.T.: 0.055 min
Response: 7292614
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

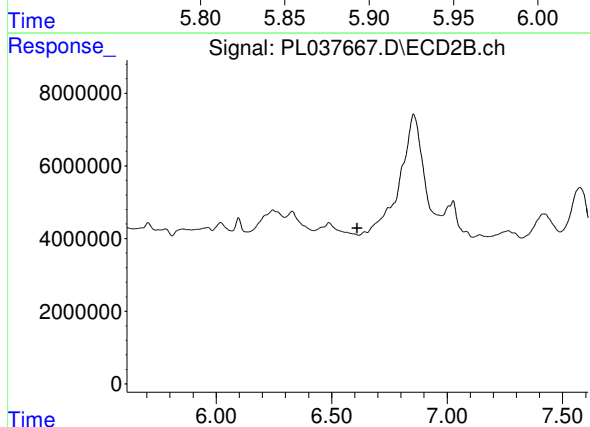


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

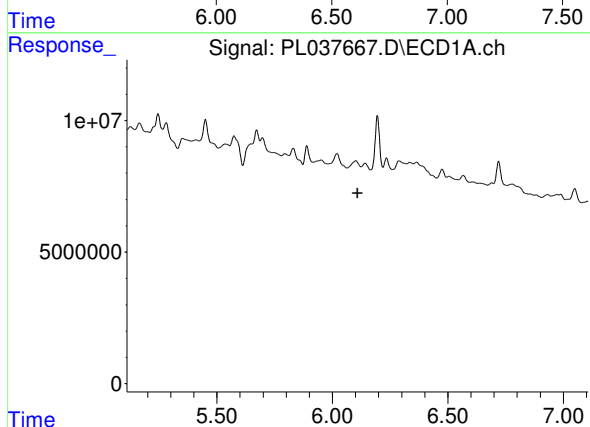


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.110 min
Response: 0
Conc: N.D.

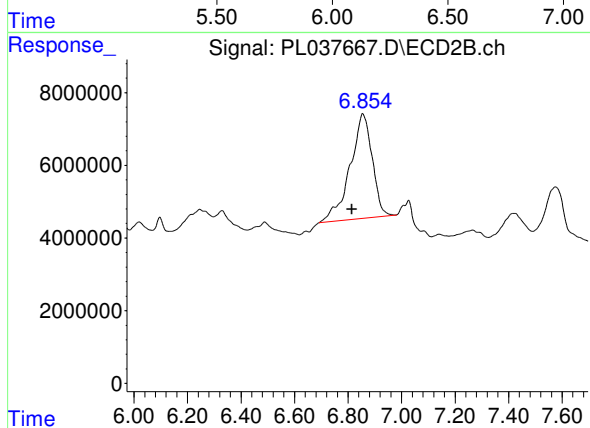

#15 Endosulfan II


R.T.: 6.855 min
Delta R.T.: 0.041 min
Response: 16555888
Conc: 66.76 ng/ml

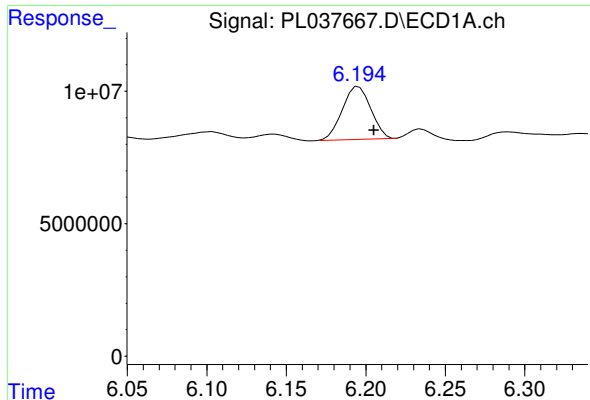

#17 4,4'-DDT


R.T.: 6.196 min
Delta R.T.: -0.010 min
Response: 24880401
Conc: 3.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

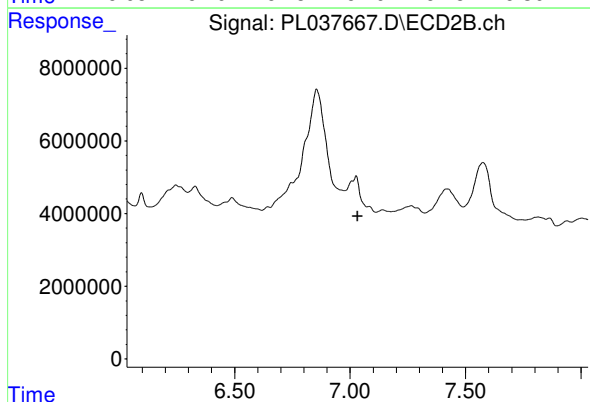


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.033 min
Response: 0
Conc: N.D.

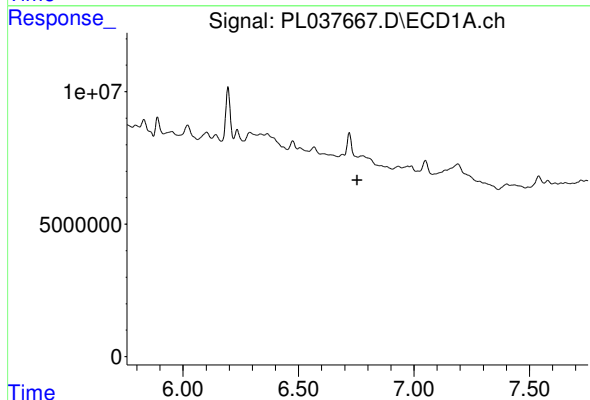


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.755 min
Response: 0
Conc: N.D.

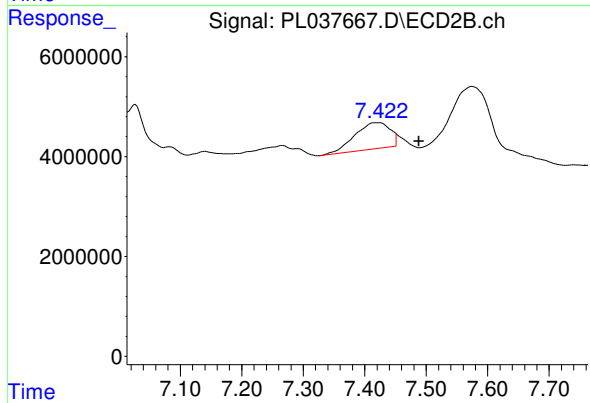

#20 Methoxychlor


R.T.: 7.424 min
Delta R.T.: -0.064 min
Response: 21169808
Conc: 18.91 ng/ml

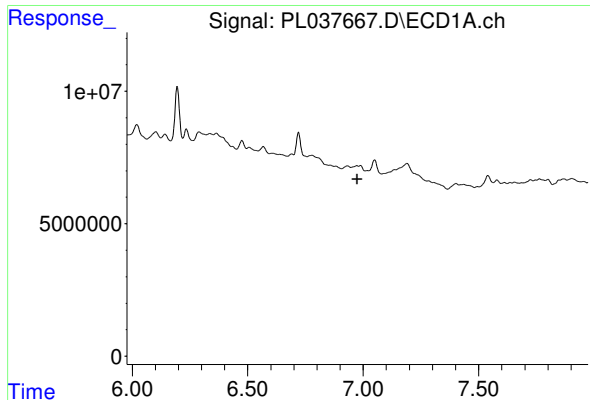

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.974 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

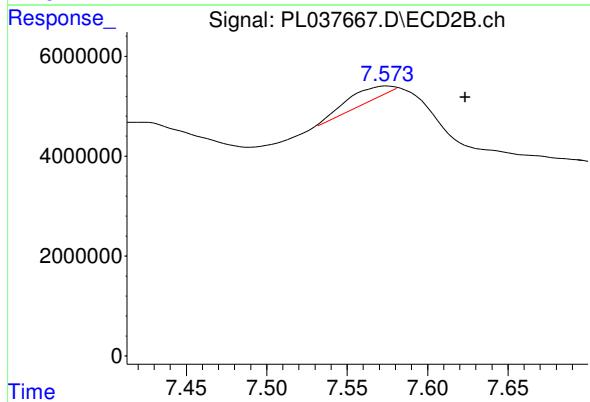


#21 Endrin ketone

R.T.: 7.575 min
Delta R.T.: -0.048 min
Response: 5992075
Conc: 2.95 ng/ml

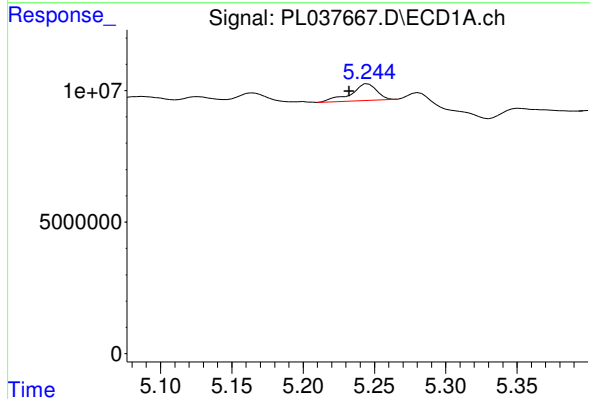


#25 Chlordane-3

R.T.: 5.246 min
Delta R.T.: 0.013 min
Response: 7972176
Conc: 7.50 ng/ml

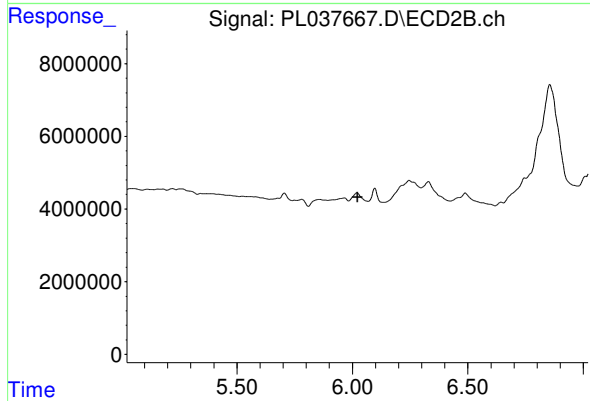

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

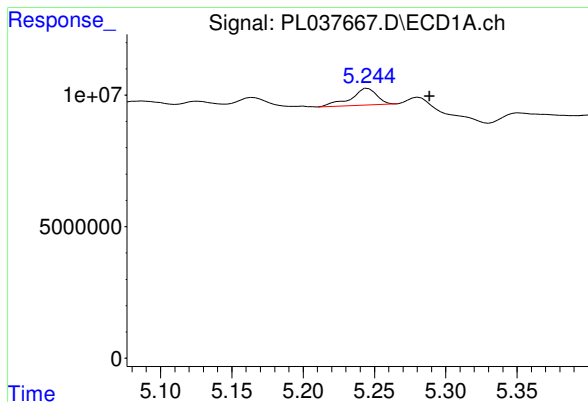

#26 Chlordane-4


R.T.: 5.246 min
Delta R.T.: -0.043 min
Response: 7972176
Conc: 8.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

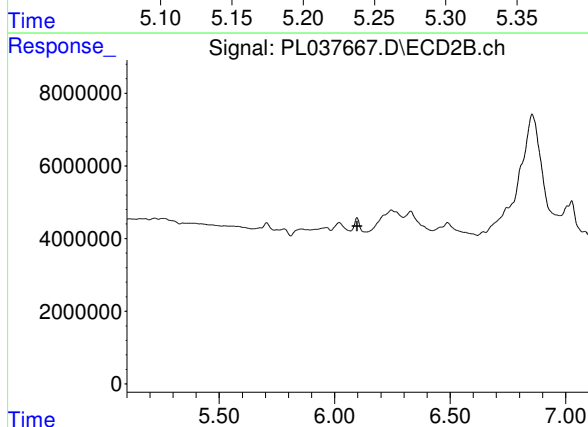


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

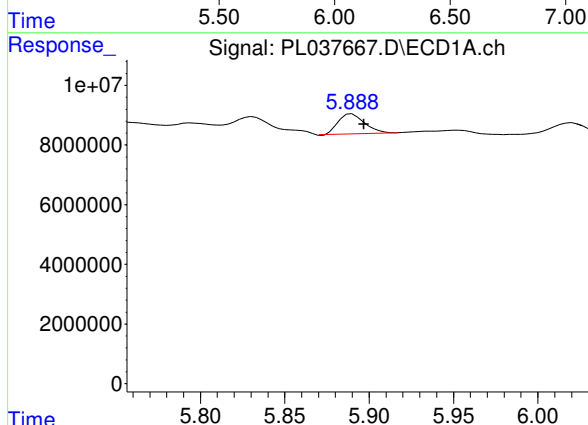


#27 Chlordane-5

R.T.: 5.890 min
Delta R.T.: -0.007 min
Response: 7292614
Conc: 55.72 ng/ml

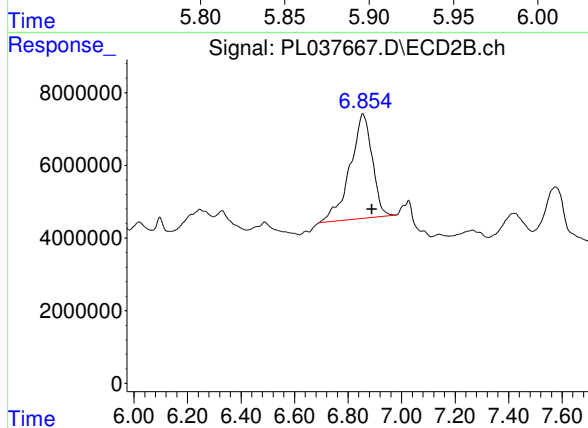

#27 Chlordane-5


R.T.: 6.855 min
Delta R.T.: -0.034 min
Response: 16555888
Conc: 1839.89 ng/ml

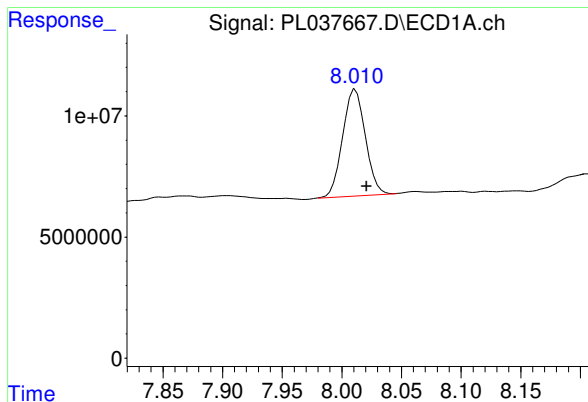

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.009 min
Response: 58239611
Conc: 9.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

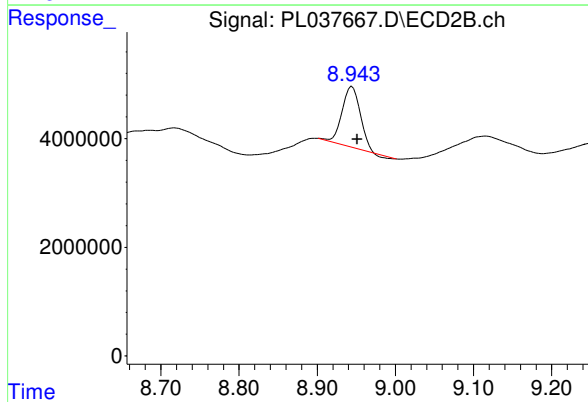

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 17372443
Conc: 8.76 ng/ml