

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
 Data File : PL037671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 19:21
 Operator : UA\AJ
 Sample : J3840-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:11:56 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.936	129.0E6	49589241	16.312	17.923
28)	SA Decachlor...	8.010	8.946	72023826	25245052	11.936	12.725
Target Compounds							
6)	B beta-BHC	4.259f	0.000	11066144	0	2.426	N.D. #
8)	B Heptachlo...	5.066f	0.000	26095334	0	2.786	N.D. #
10)	B gamma-Chl...	5.171f	0.000	6139367	0	0.655	N.D. #
16)	A 4,4'-DDD	5.961	0.000	8221346	0	1.252	N.D. #
25)	Chlordane-3	5.171	0.000	6139367	0	5.776	N.D. #
27)	Chlordane-5	5.961	0.000	8221346	0	62.822	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
Data File : PL037671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 19:21
Operator : UA\AJ
Sample : J3840-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:11:56 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

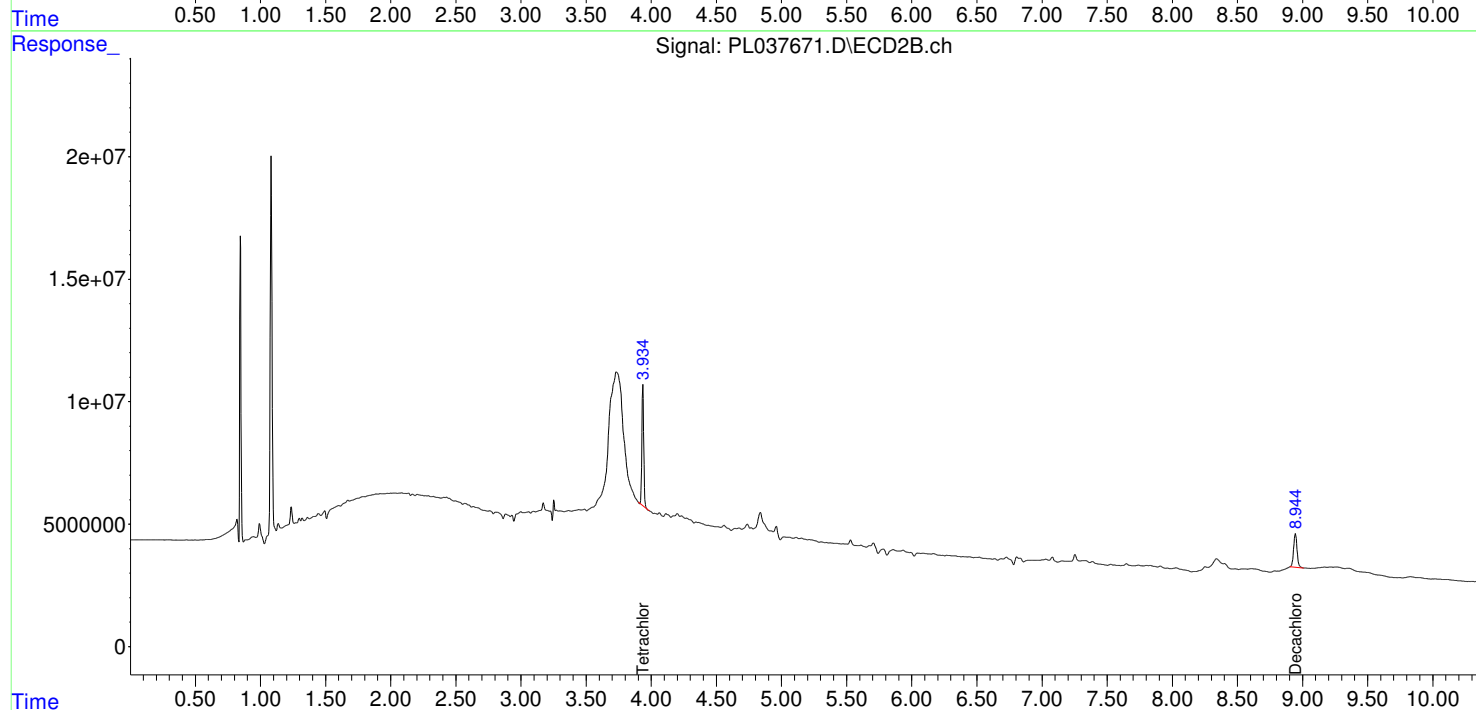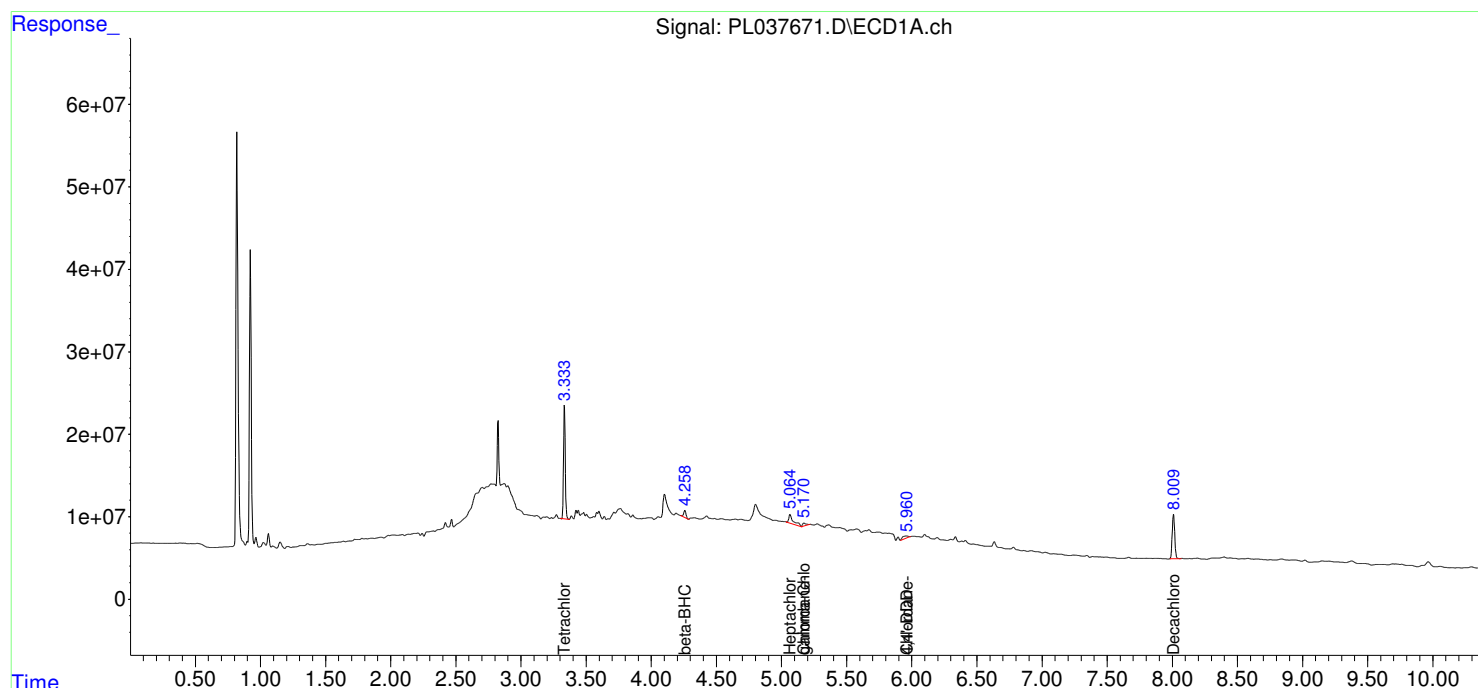


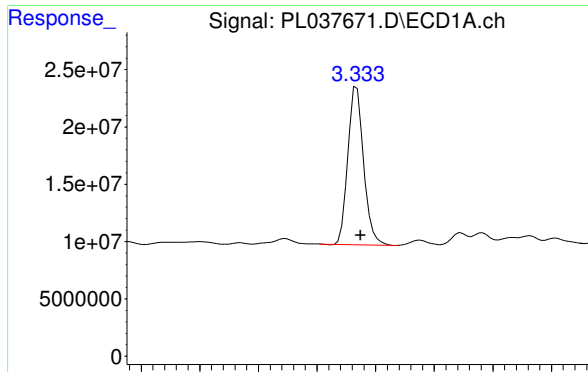

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 129031049
Conc: 16.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

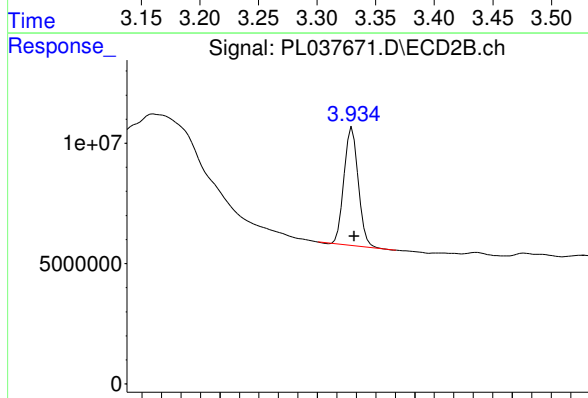


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 49589241
Conc: 17.92 ng/ml

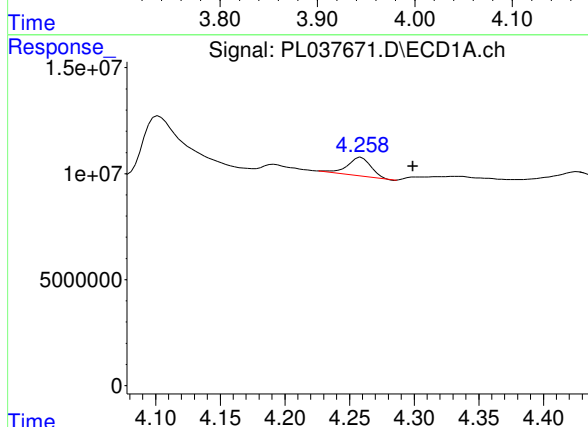


#6 beta-BHC

R.T.: 4.259 min
Delta R.T.: -0.040 min
Response: 11066144
Conc: 2.43 ng/ml

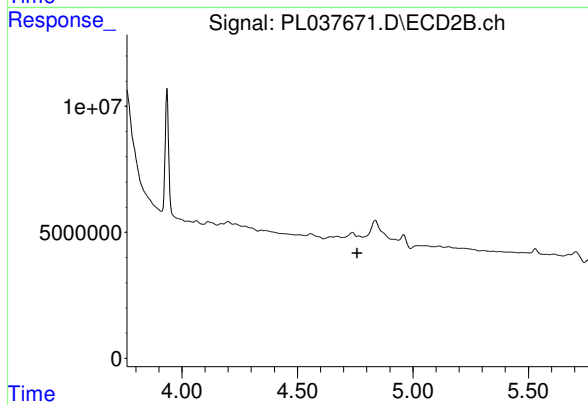

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

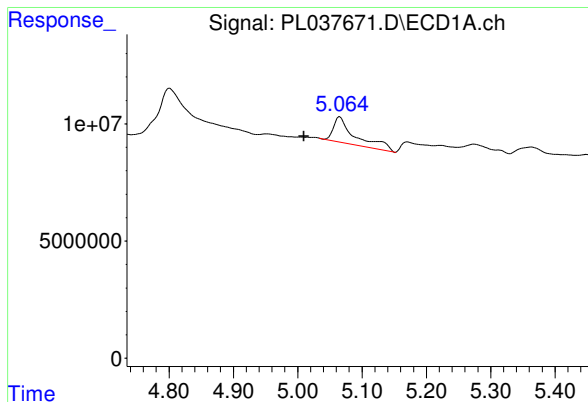

#8 Heptachlor epoxide


R.T.: 5.066 min
Delta R.T.: 0.056 min
Response: 26095334
Conc: 2.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

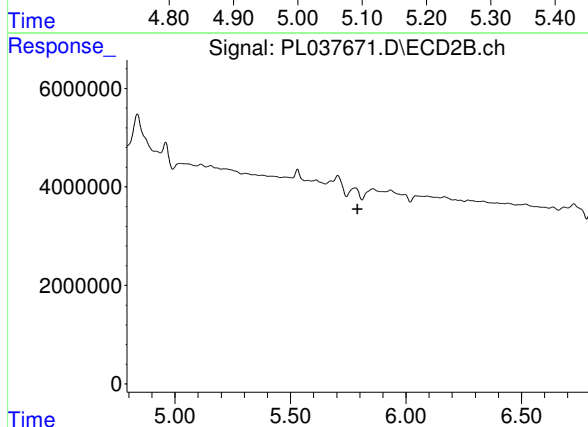


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

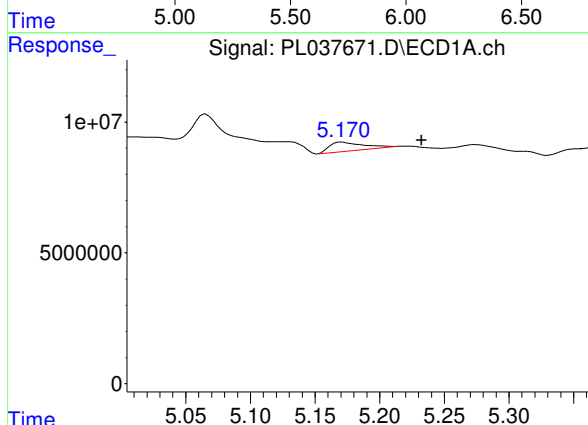


#10 gamma-Chlordane

R.T.: 5.171 min
Delta R.T.: -0.061 min
Response: 6139367
Conc: 0.66 ng/ml

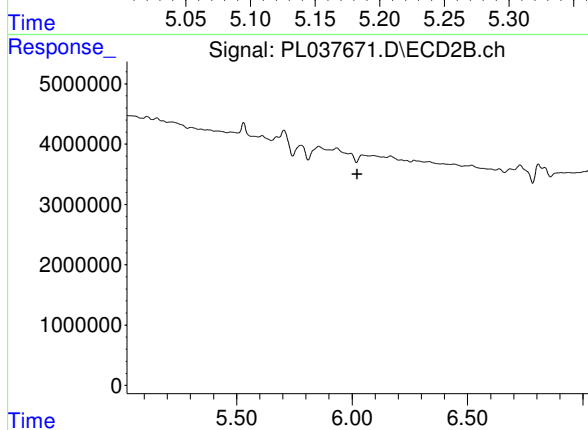

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

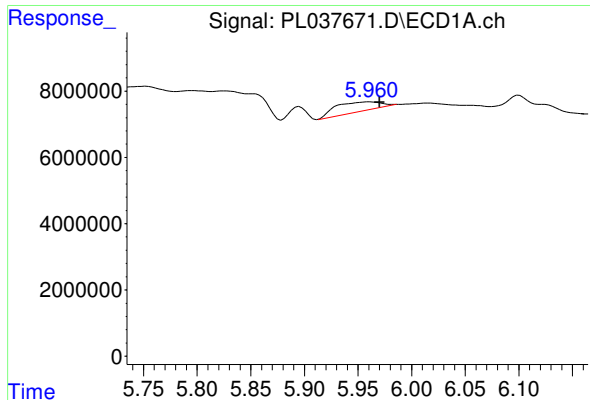

#16 4,4'-DDD


R.T.: 5.961 min
Delta R.T.: -0.009 min
Response: 8221346
Conc: 1.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

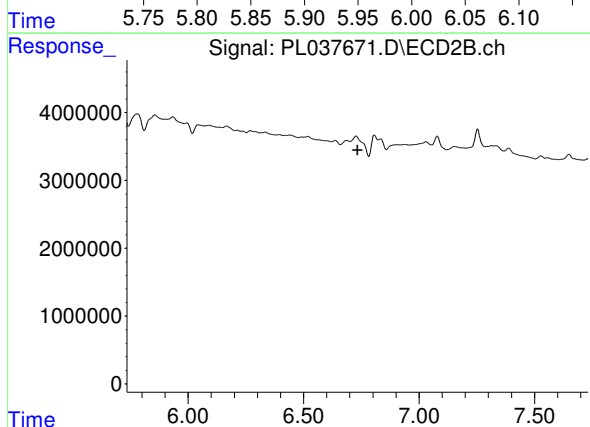


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.734 min
Response: 0
Conc: N.D.

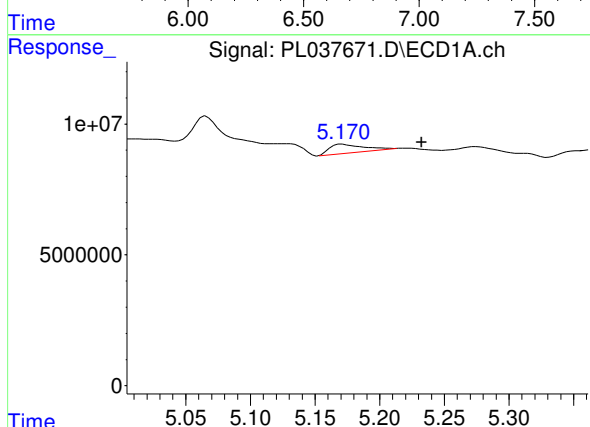


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: -0.061 min
Response: 6139367
Conc: 5.78 ng/ml

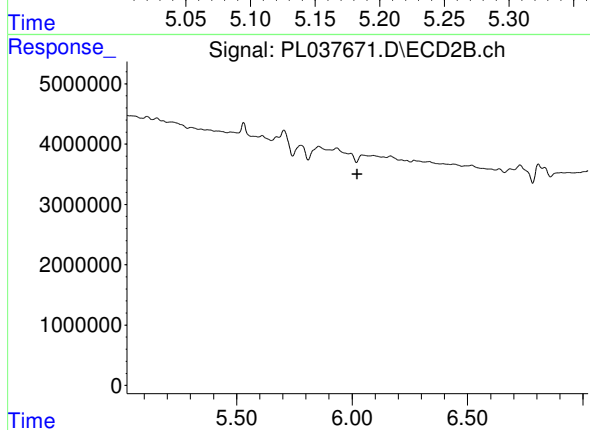

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

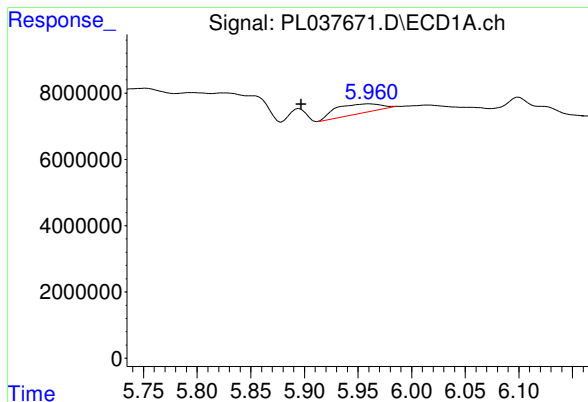

#27 Chlordane-5


R.T.: 5.961 min
Delta R.T.: 0.064 min
Response: 8221346
Conc: 62.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

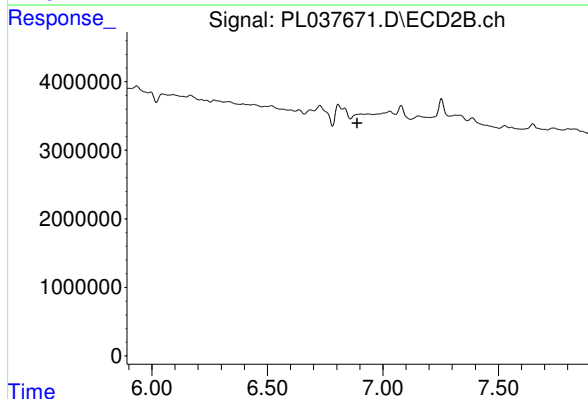


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.889 min
Response: 0
Conc: N.D.

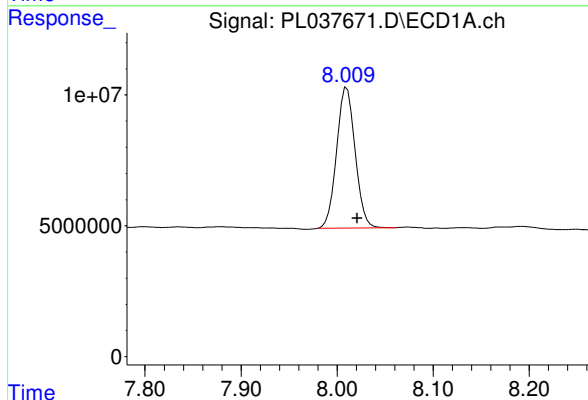

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 72023826
Conc: 11.94 ng/ml

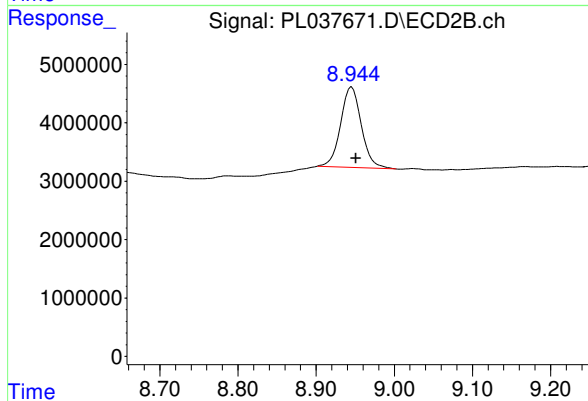

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.005 min
Response: 25245052
Conc: 12.72 ng/ml