

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
 Data File : PL037689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 23:34
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:13:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.333	3.936	129.9E6	49658723	16.421	17.949
28) SA Decachlor...	8.010	8.945	123.4E6	40254747	20.445	20.290
Target Compounds						
8) B Heptachlo...	0.000	5.779	0	7065423	N.D.	2.479 #
13) MA Dieldrin	5.534f	0.000	4602939	0	0.520	N.D. #
14) MA Endrin	5.846	0.000	7685848	0	0.976	N.D. #
21) B Endrin ke...	6.931f	0.000	15062828	0	2.118	N.D. #
24) Chlordane-2	0.000	5.317	0	8816164	N.D.	69.665 #
27) Chlordane-5	5.846	0.000	7685848	0	58.730	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070318\
Data File : PL037689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 23:34
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:13:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

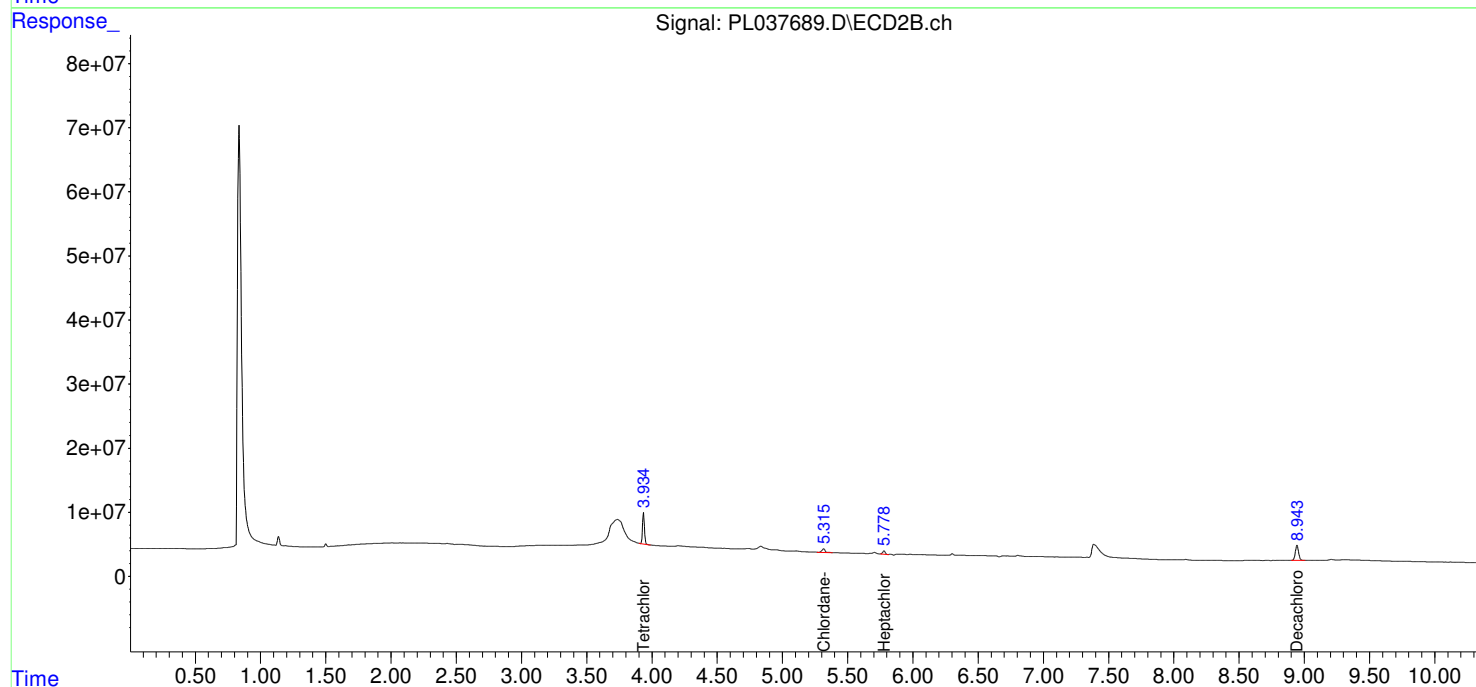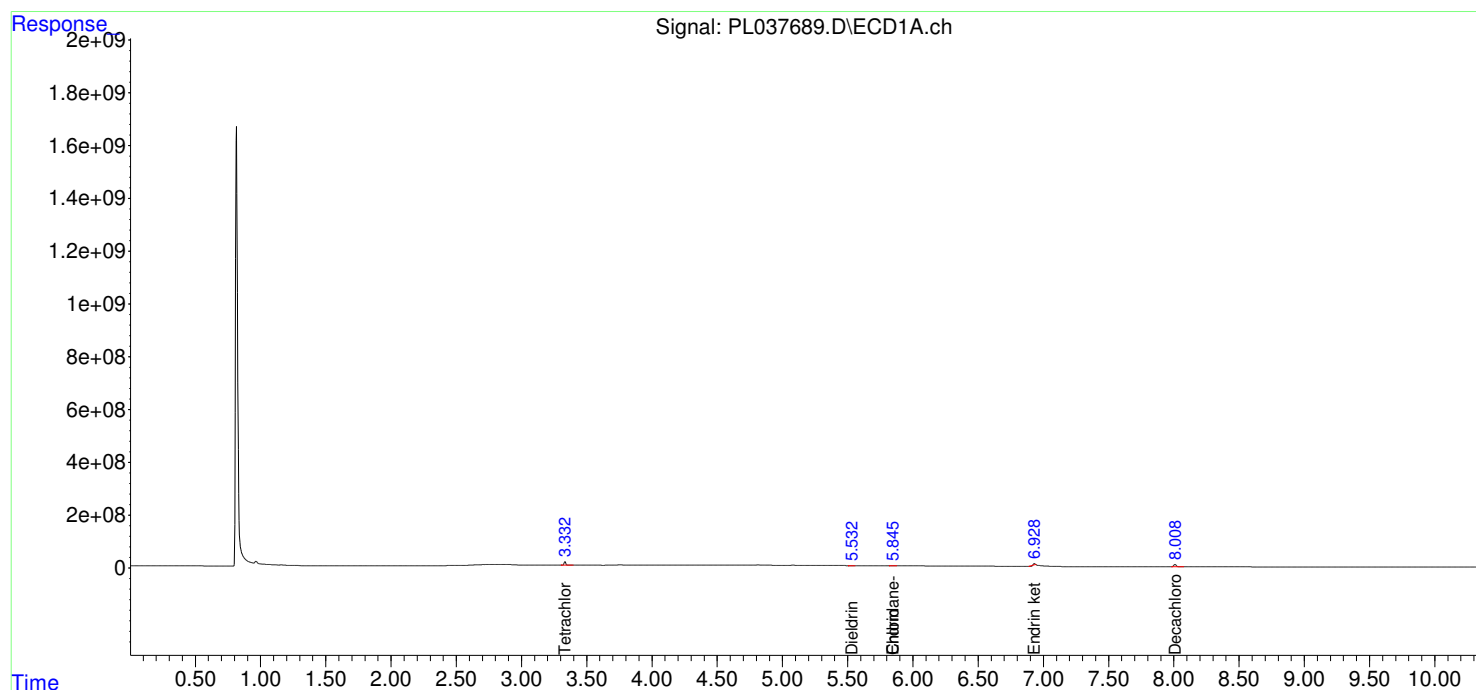


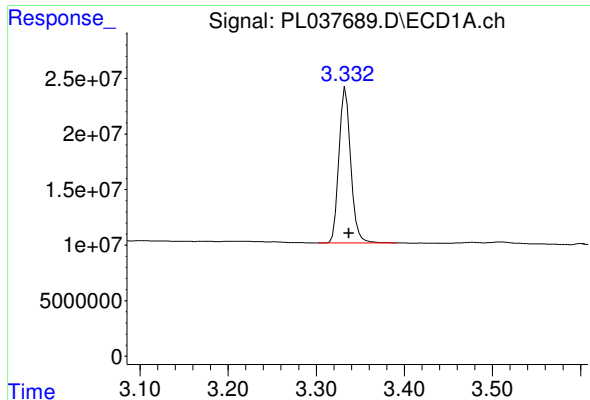

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 129893425
Conc: 16.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

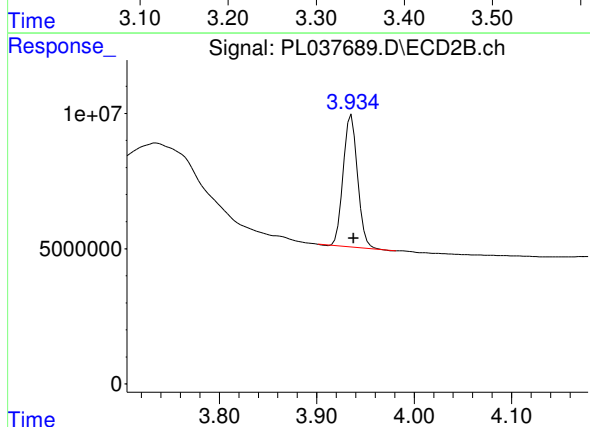


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 49658723
Conc: 17.95 ng/ml

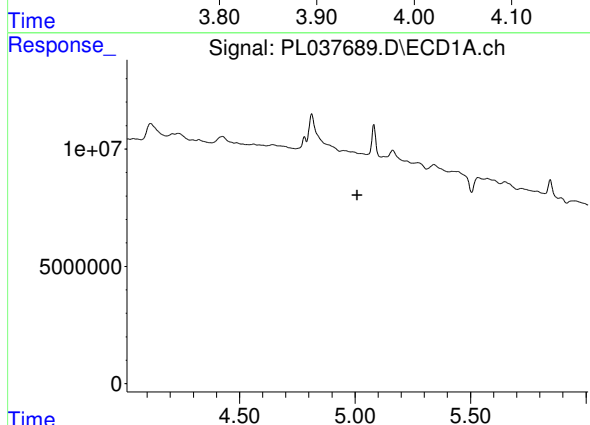


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

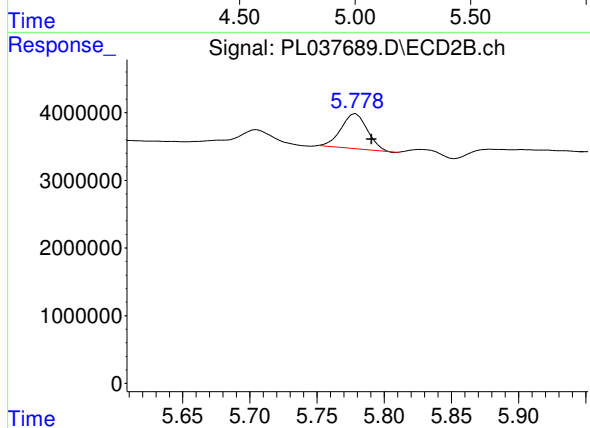

#8 Heptachlor epoxide


R.T.: 5.779 min
Delta R.T.: -0.011 min
Response: 7065423
Conc: 2.48 ng/ml

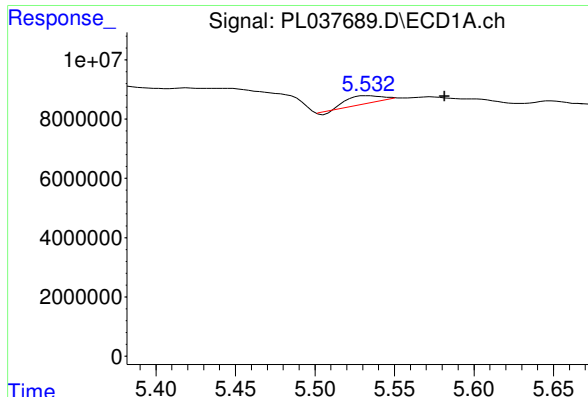

#13 Dieldrin


R.T.: 5.534 min
Delta R.T.: -0.048 min
Response: 4602939
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

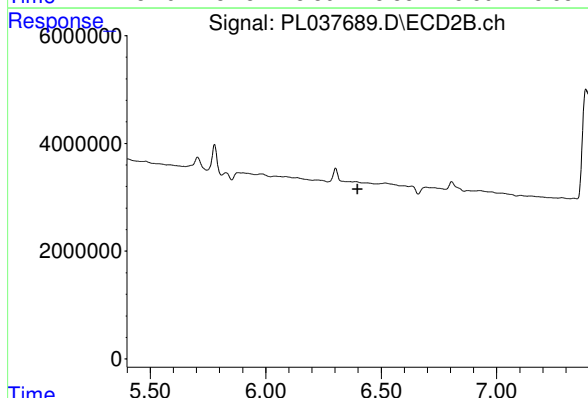


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

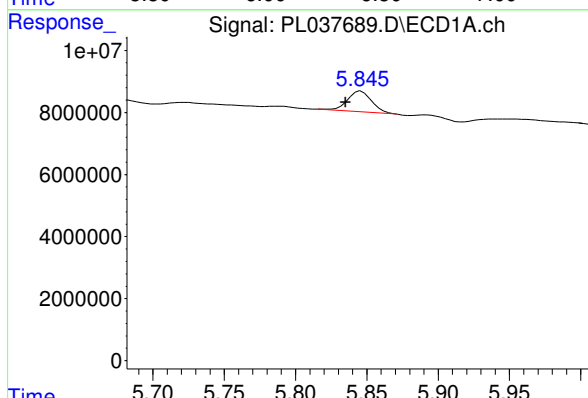


#14 Endrin

R.T.: 5.846 min
Delta R.T.: 0.011 min
Response: 7685848
Conc: 0.98 ng/ml

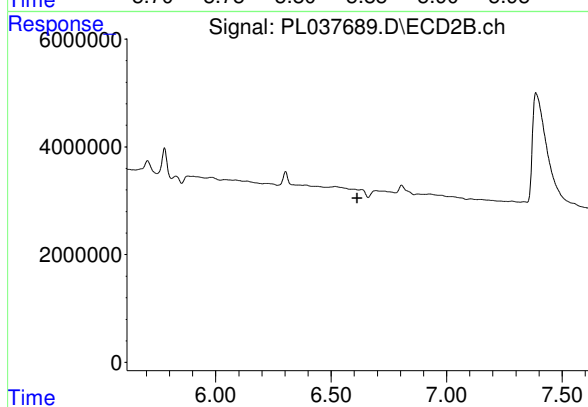

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

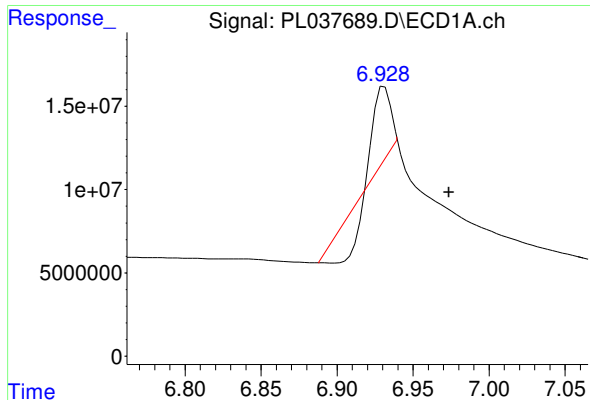

#21 Endrin ketone


R.T.: 6.931 min
Delta R.T.: -0.042 min
Response: 15062828
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

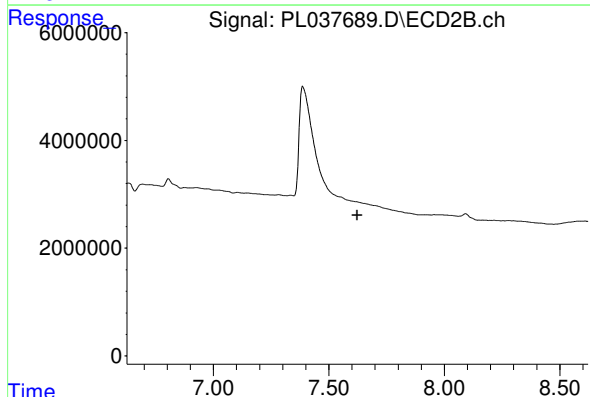


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

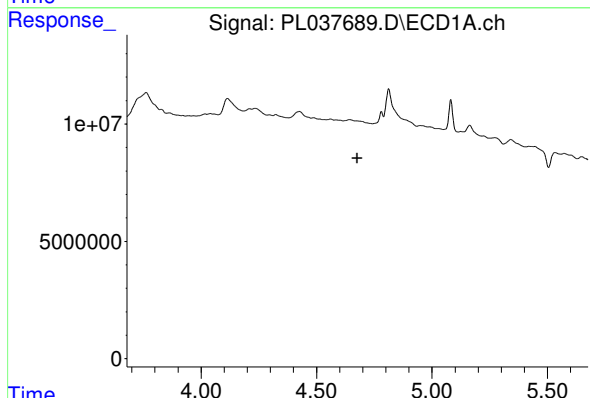


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

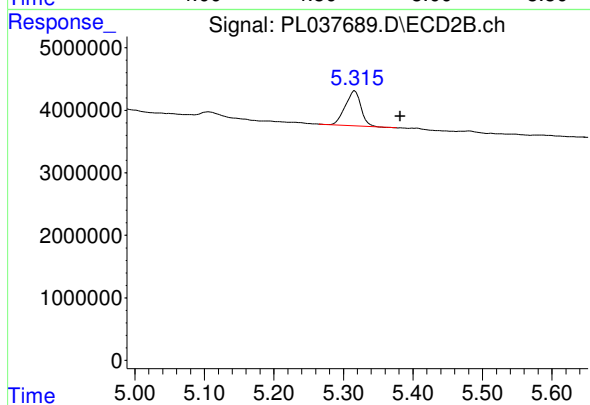

#24 Chlordane-2


R.T.: 5.317 min
Delta R.T.: -0.065 min
Response: 8816164
Conc: 69.67 ng/ml

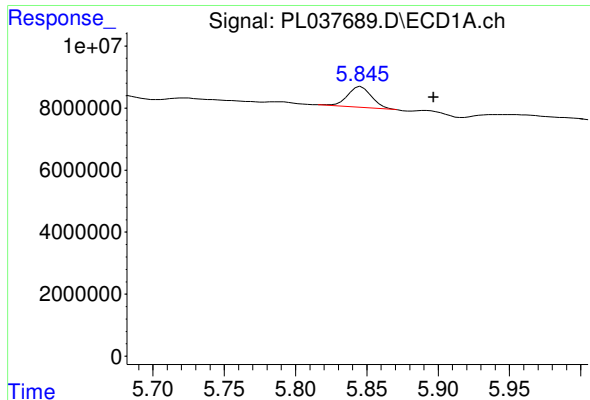

#27 Chlordane-5


R.T.: 5.846 min
Delta R.T.: -0.051 min
Response: 7685848
Conc: 58.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

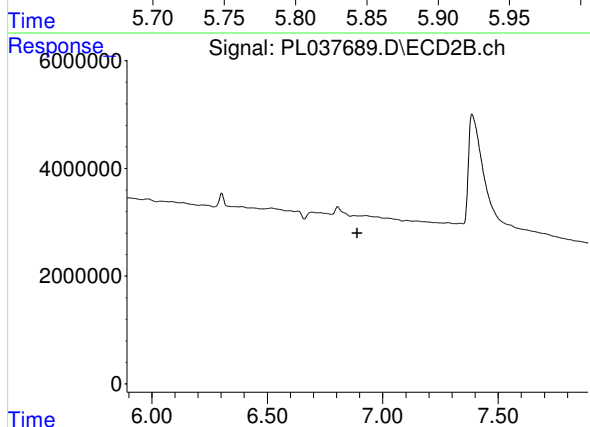


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

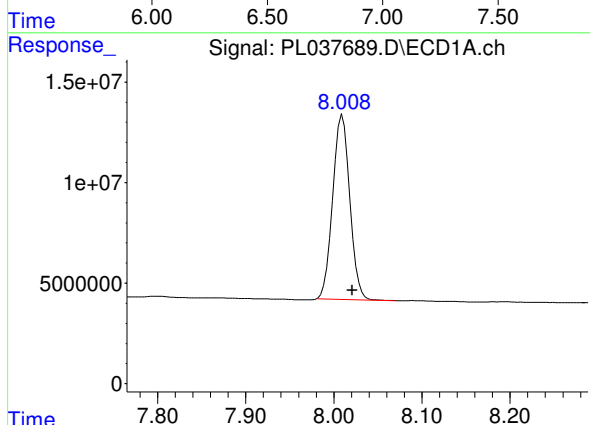

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 123368595
Conc: 20.45 ng/ml

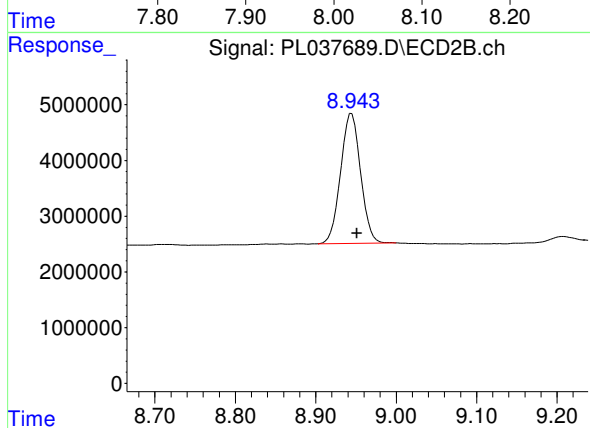

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 40254747
Conc: 20.29 ng/ml