

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL070318\  
 Data File : PL037670.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Jul 2018 19:07  
 Operator : UA\AJ  
 Sample : J3840-03  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 TP-6-S

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 04 00:11:52 2018  
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL062018.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 21 02:27:11 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml | ng/ml |
|-----------------------------|-----------------|-------|-------|----------|----------|-------|-------|
| -----                       |                 |       |       |          |          |       |       |
| System Monitoring Compounds |                 |       |       |          |          |       |       |
| 1)                          | SA Tetrachlo... | 3.333 | 3.936 | 69943507 | 26592971 | 8.842 | 9.612 |
| 28)                         | SA Decachlor... | 8.010 | 8.946 | 47534398 | 18775385 | 7.878 | 9.464 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL070318\  
Data File : PL037670.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Jul 2018 19:07  
Operator : UA\AJ  
Sample : J3840-03  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
TP-6-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 04 00:11:52 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL062018.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 21 02:27:11 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

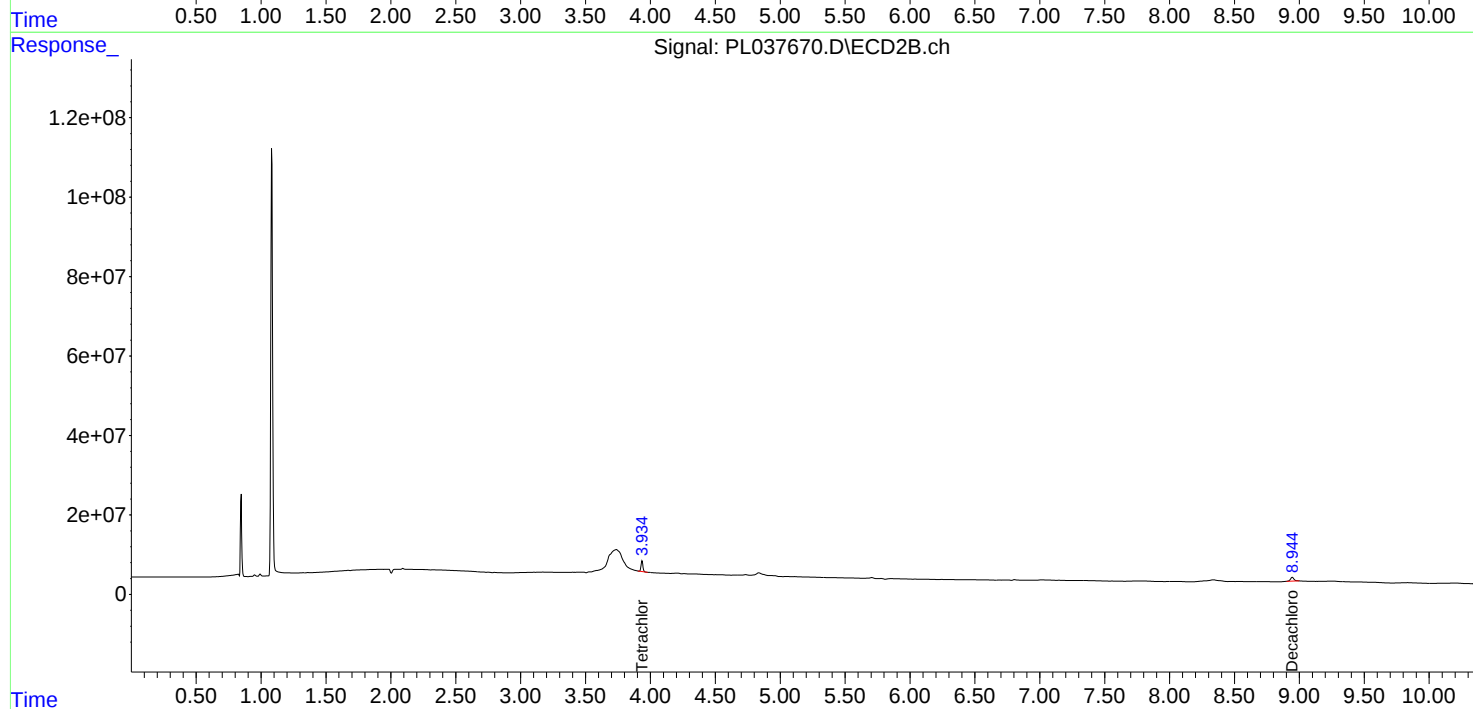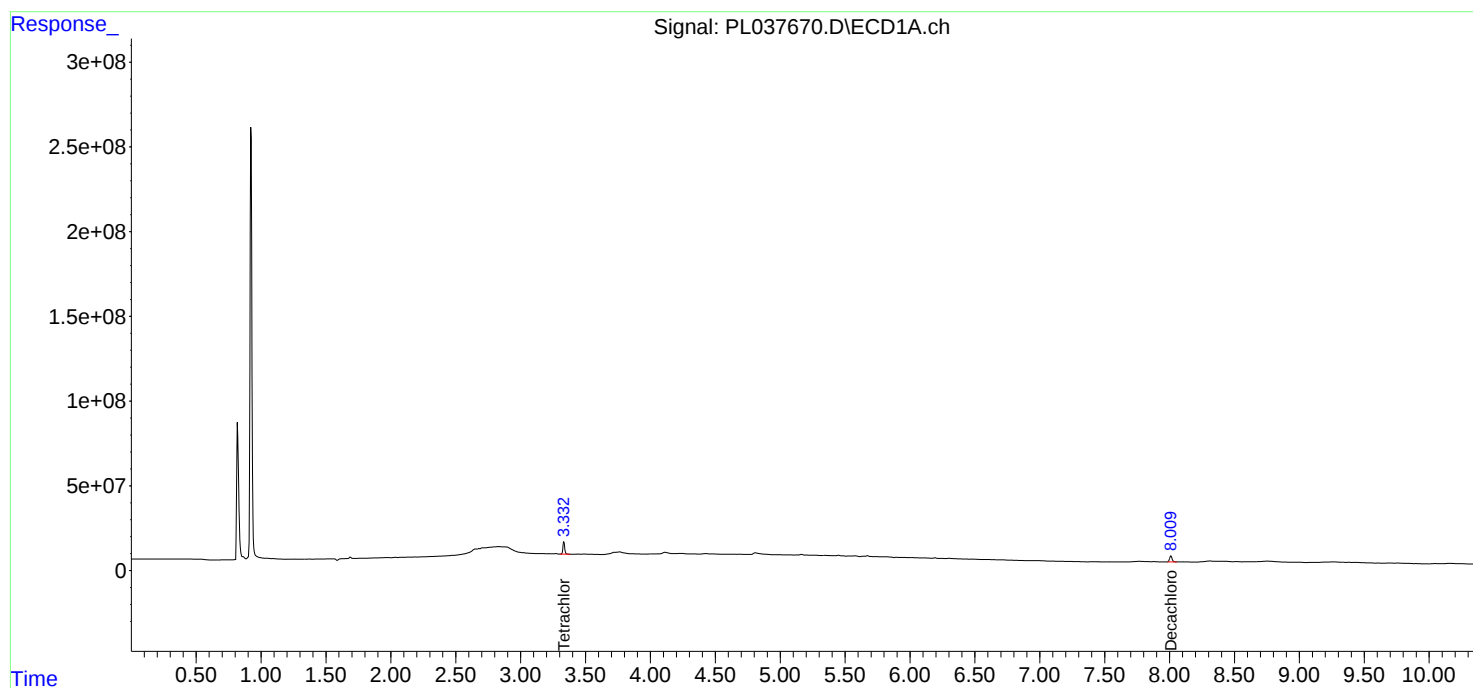


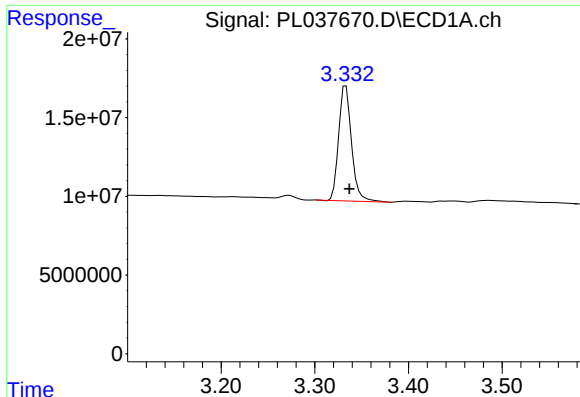

#1 Tetrachloro-m-xylene


R.T.: 3.333 min  
Delta R.T.: -0.004 min  
Response: 69943507  
Conc: 8.84 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-6-S

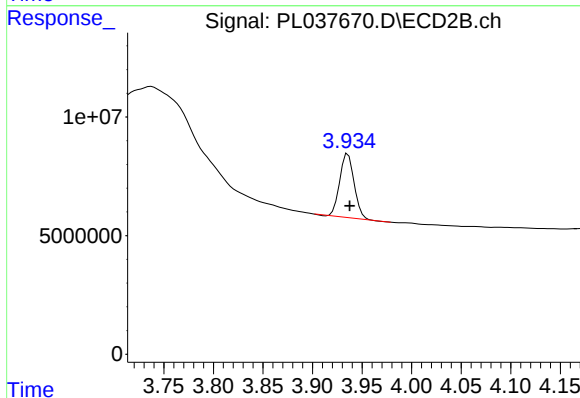


#1 Tetrachloro-m-xylene

R.T.: 3.936 min  
Delta R.T.: -0.002 min  
Response: 26592971  
Conc: 9.61 ng/ml

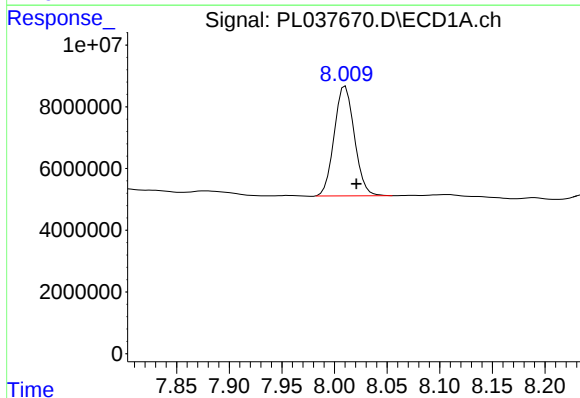

#28 Decachlorobiphenyl

R.T.: 8.010 min  
Delta R.T.: -0.011 min  
Response: 47534398  
Conc: 7.88 ng/ml

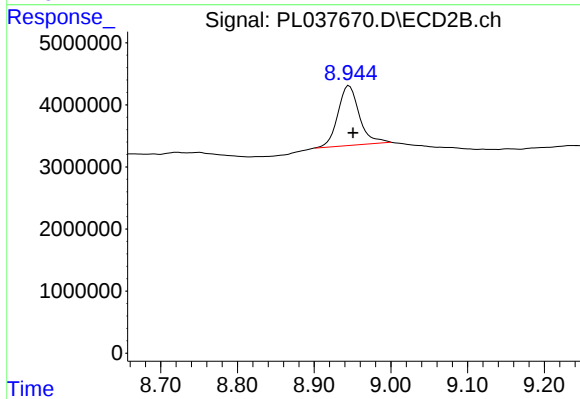

#28 Decachlorobiphenyl

R.T.: 8.946 min  
Delta R.T.: -0.005 min  
Response: 18775385  
Conc: 9.46 ng/ml