

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070319\
 Data File : PL050167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 14:57
 Operator : SM\AJ
 Sample : K3618-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-070219

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:18:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.932	326.4E6	18048775	28.938	5.895 #
28)	SA Decachlor...	7.986	8.966	112.1E6	50869757	8.821	15.153 #
Target Compounds							
2)	A alpha-BHC	3.763	4.342f	39820941	13942174	2.120	3.114 #
6)	B beta-BHC	0.000	4.795	0	9302858	N.D.	4.803 #
10)	B gamma-Chl...	5.197	0.000	30506999	0	1.785	N.D. #
11)	B alpha-Chl...	0.000	6.094	0	13672456	N.D.	3.697 #
16)	A 4,4'-DDD	5.932	0.000	40951624	0	3.244	N.D. #
24)	Chlordane-2	4.684f	0.000	150.0E6	0	256.802	N.D. #
25)	Chlordane-3	5.197	0.000	30506999	0	16.243	N.D. #
26)	Chlordane-4	0.000	6.094	0	13672456	N.D.	23.004 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070319\
Data File : PL050167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 14:57
Operator : SM\AJ
Sample : K3618-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:18:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

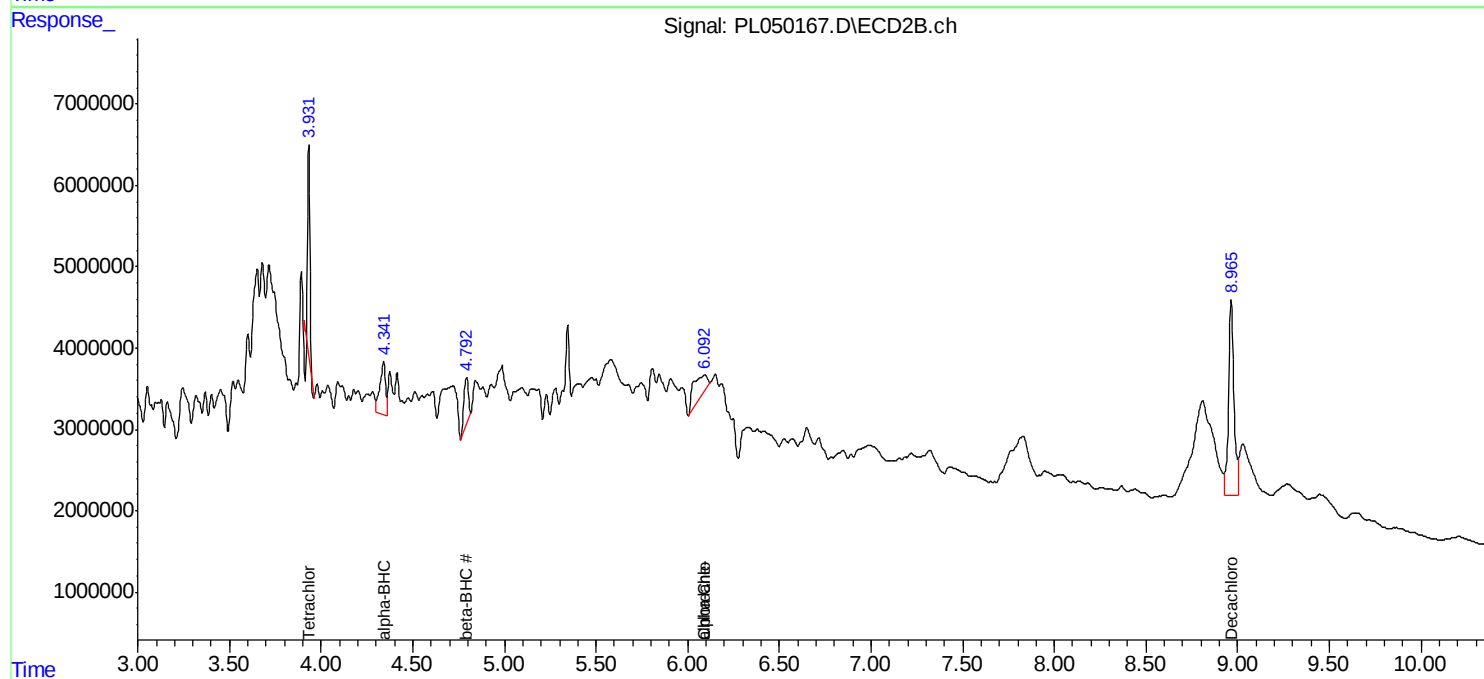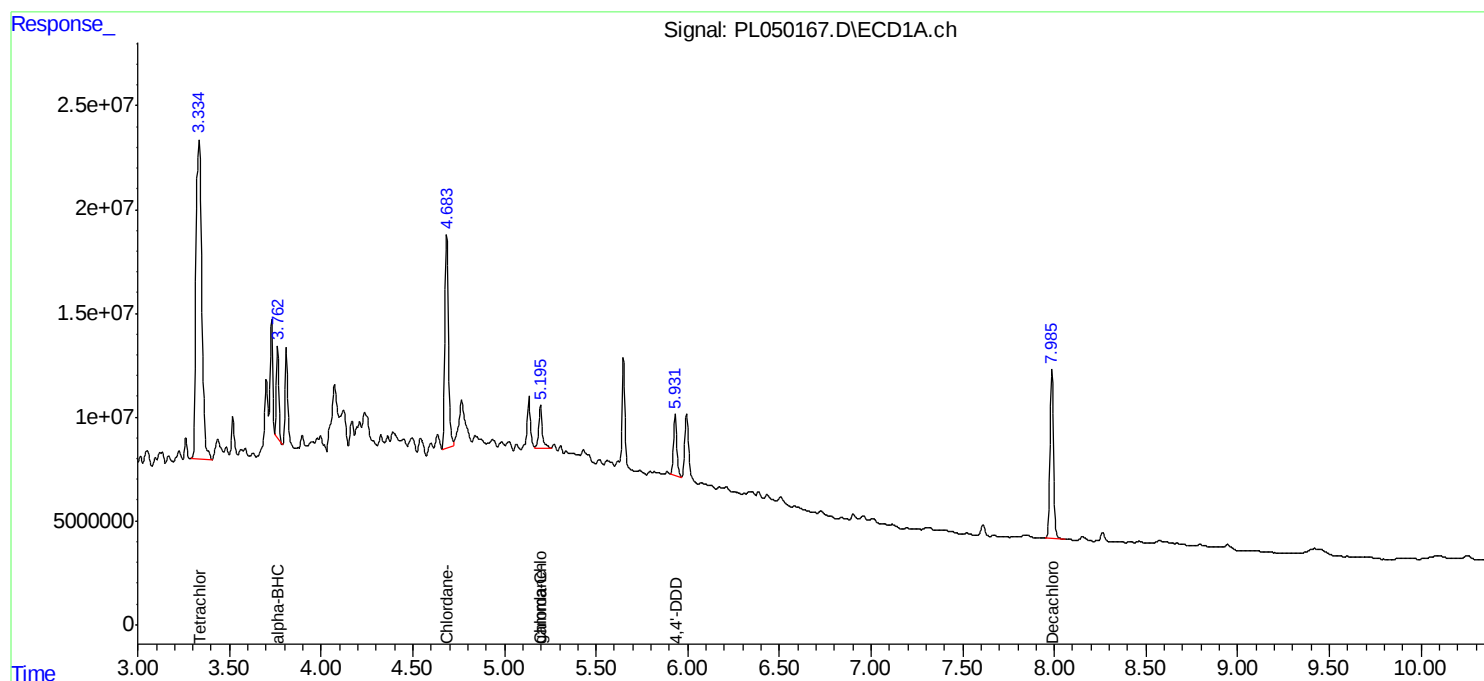


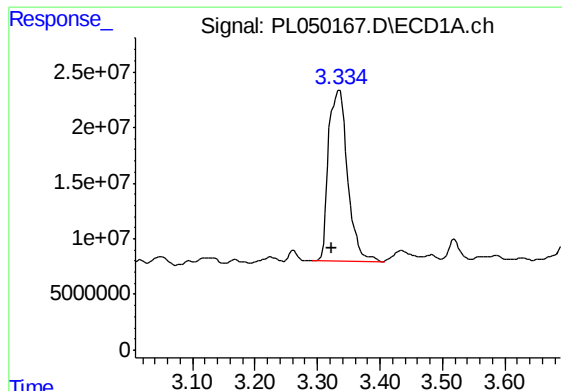

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.011 min
Response: 326356768
Conc: 28.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

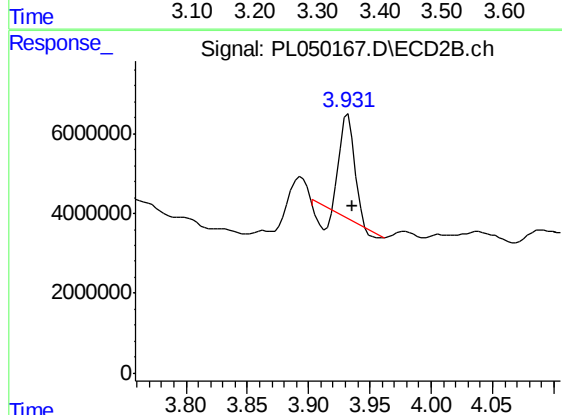


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 18048775
Conc: 5.89 ng/ml

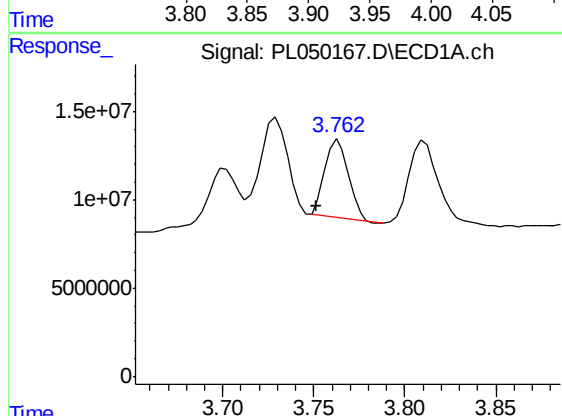


#2 alpha-BHC

R.T.: 3.763 min
Delta R.T.: 0.012 min
Response: 39820941
Conc: 2.12 ng/ml

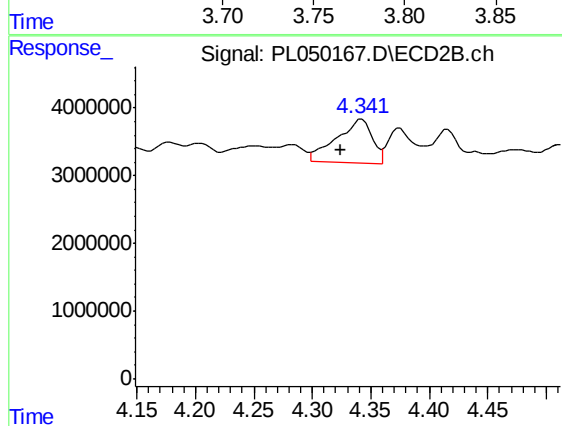

#2 alpha-BHC


R.T.: 4.342 min
Delta R.T.: 0.018 min
Response: 13942174
Conc: 3.11 ng/ml

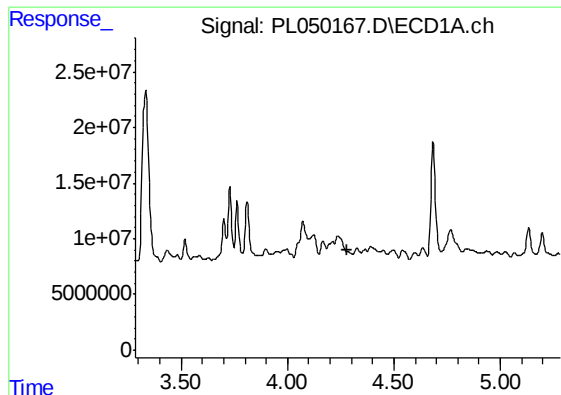

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

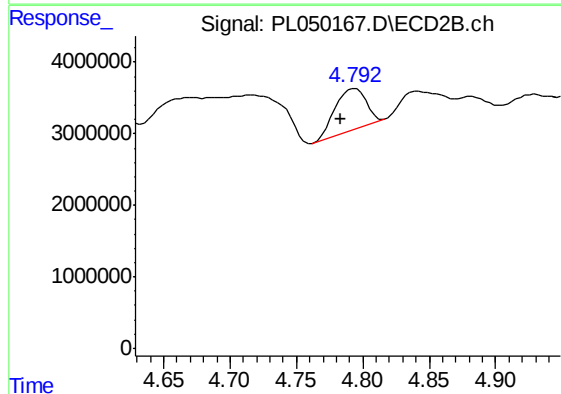


#6 beta-BHC

R.T.: 4.795 min
Delta R.T.: 0.012 min
Response: 9302858
Conc: 4.80 ng/ml

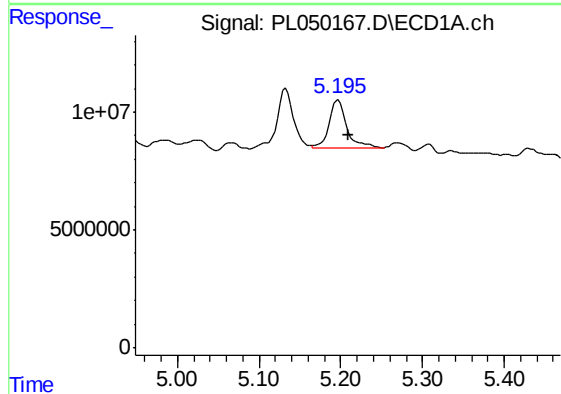


#10 gamma-Chlordane

R.T.: 5.197 min
Delta R.T.: -0.013 min
Response: 30506999
Conc: 1.79 ng/ml

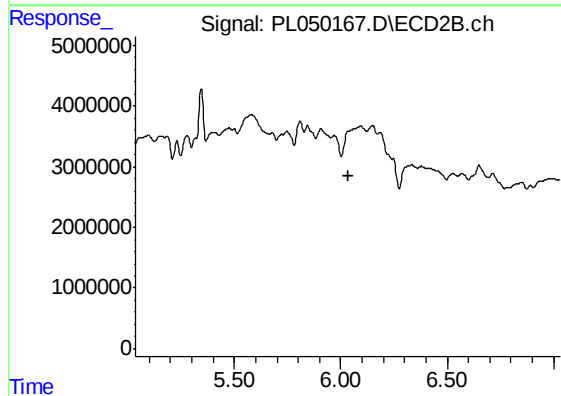

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.034 min
Response: 0
Conc: N.D.

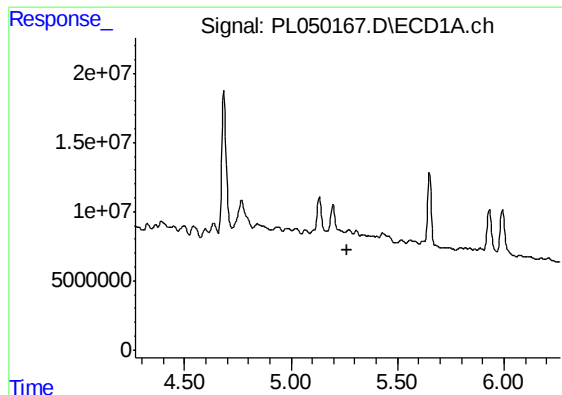

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

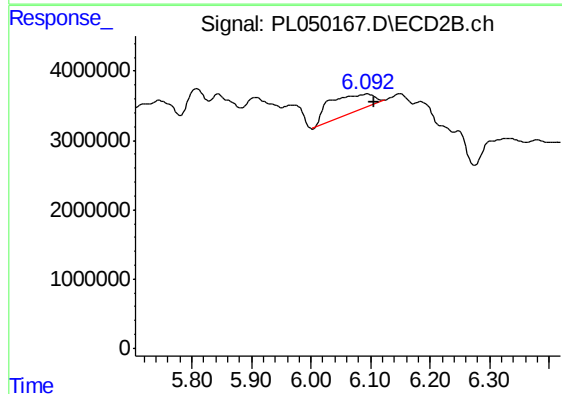


#11 alpha-Chlordane

R.T.: 6.094 min
Delta R.T.: -0.011 min
Response: 13672456
Conc: 3.70 ng/ml

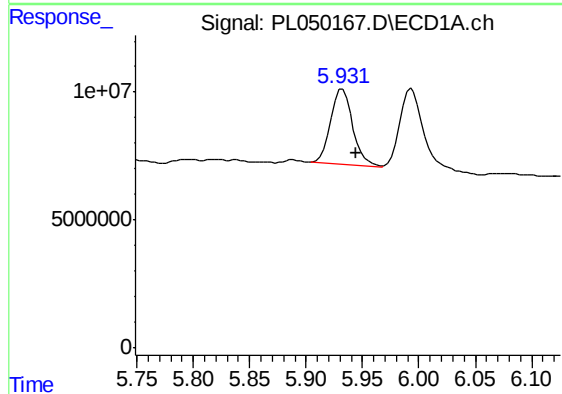


#16 4,4'-DDD

R.T.: 5.932 min
Delta R.T.: -0.013 min
Response: 40951624
Conc: 3.24 ng/ml

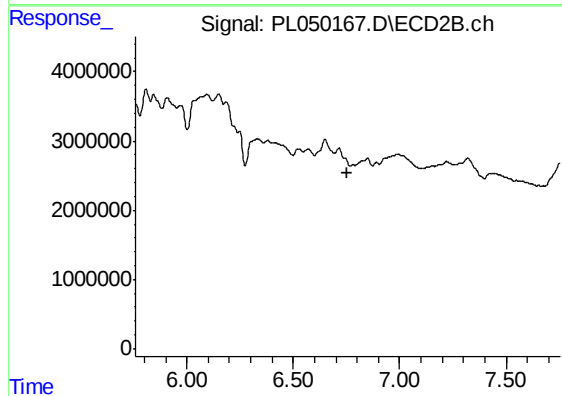

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

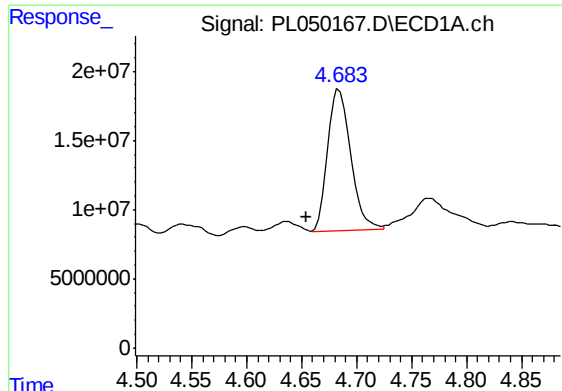

#24 Chlordane-2


R.T.: 4.684 min
Delta R.T.: 0.030 min
Response: 149980949
Conc: 256.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

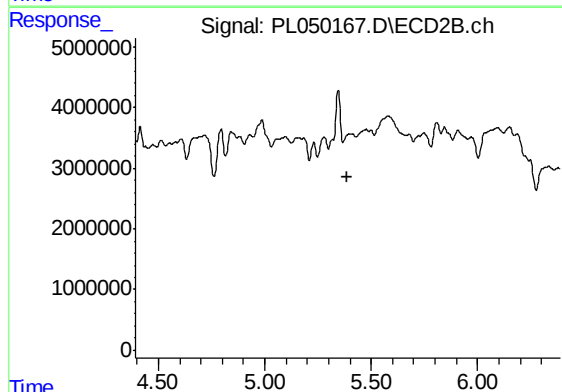


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

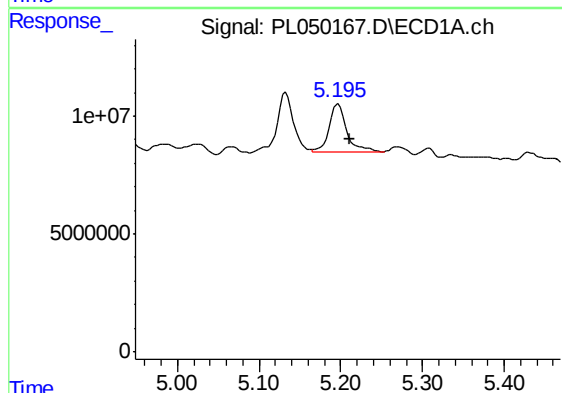


#25 Chlordane-3

R.T.: 5.197 min
Delta R.T.: -0.014 min
Response: 30506999
Conc: 16.24 ng/ml

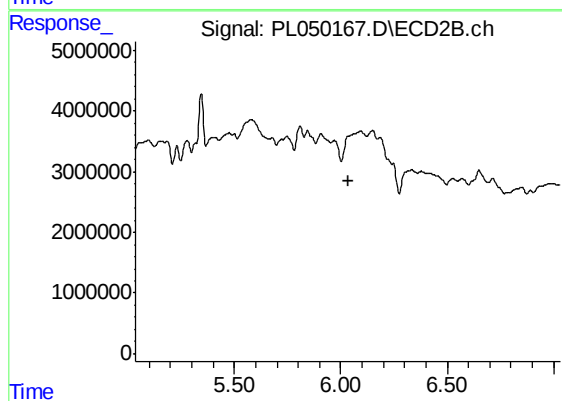

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

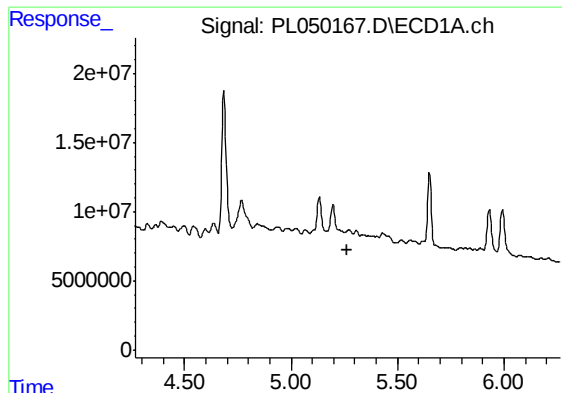

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-01-070219

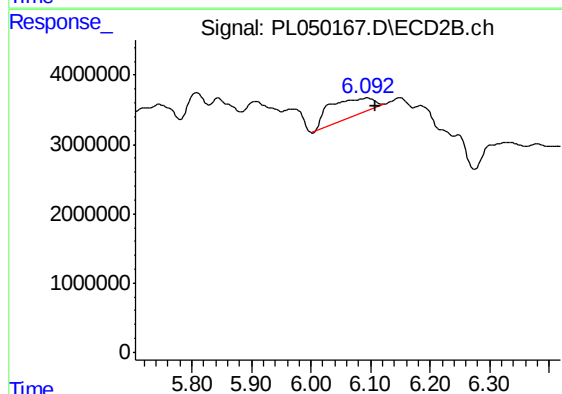


#26 Chlordane-4

R.T.: 6.094 min
Delta R.T.: -0.013 min
Response: 13672456
Conc: 23.00 ng/ml

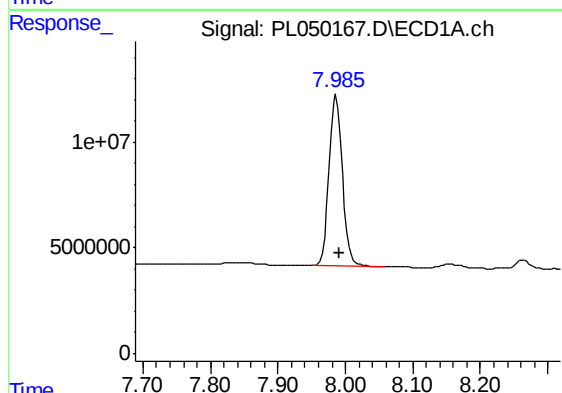

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 112078370
Conc: 8.82 ng/ml

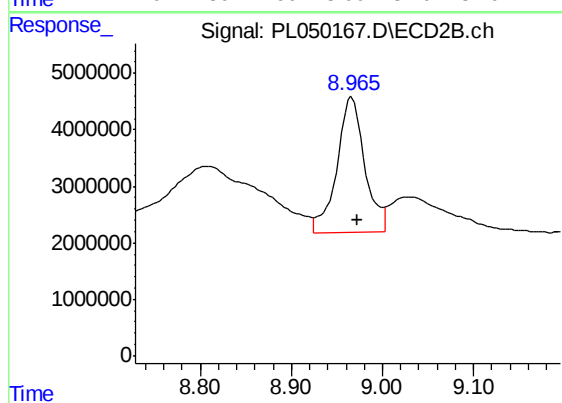

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 50869757
Conc: 15.15 ng/ml