

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070319\
 Data File : PL050181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 19:14
 Operator : SM\AJ
 Sample : K3650-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-051

Manual Integrations
 APPROVED

Ankita
 7/5/2019 10:02:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:22:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.933	195.3E6	55015399	17.322m	17.969
28)	SA Decachlor...	7.985	8.965	138.1E6	40961657	10.867	12.202m
Target Compounds							
10)	B gamma-Chl...	5.204	6.029	47712784	16511103	2.792m	4.431 #
11)	B alpha-Chl...	5.260	6.101	64707785	24766628	3.898m	6.697m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070319\
Data File : PL050181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 19:14
Operator : SM\AJ
Sample : K3650-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-051


Manual Integrations
APPROVED

Ankita
7/5/2019 10:02:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:22:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

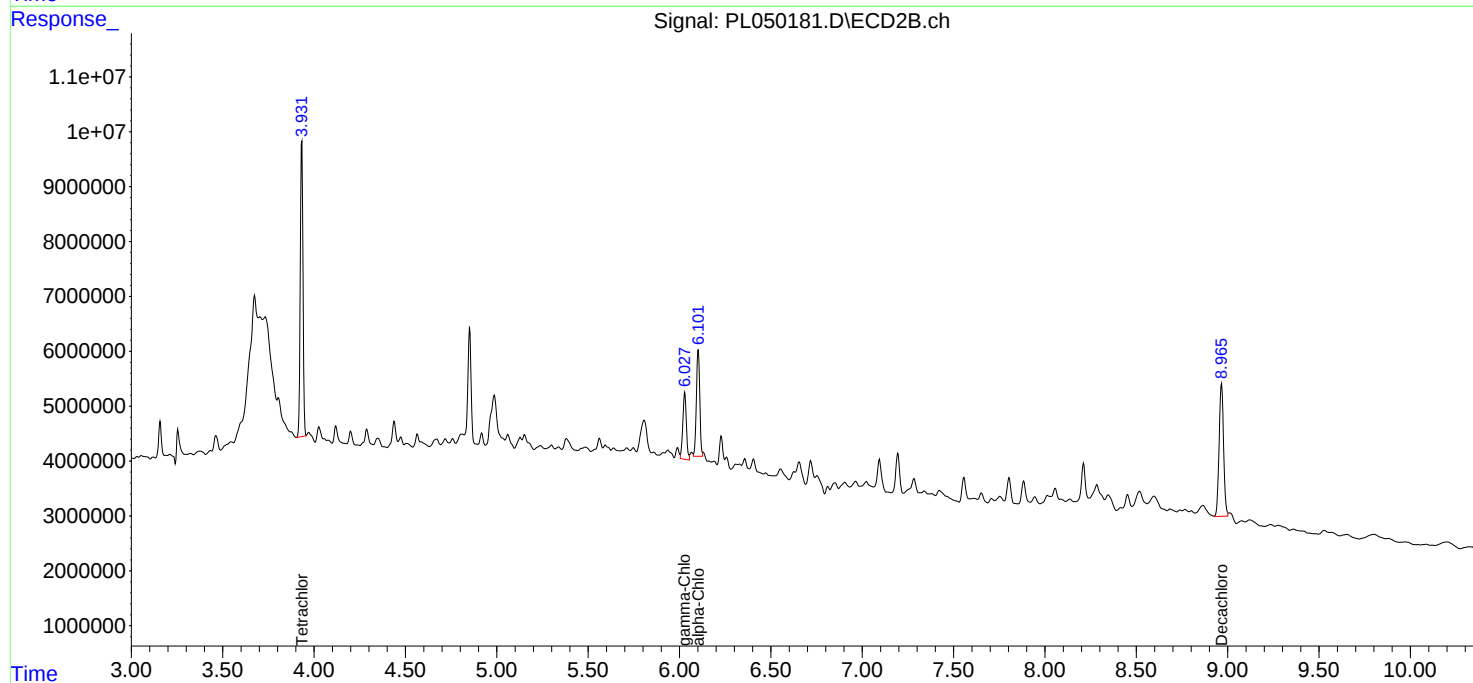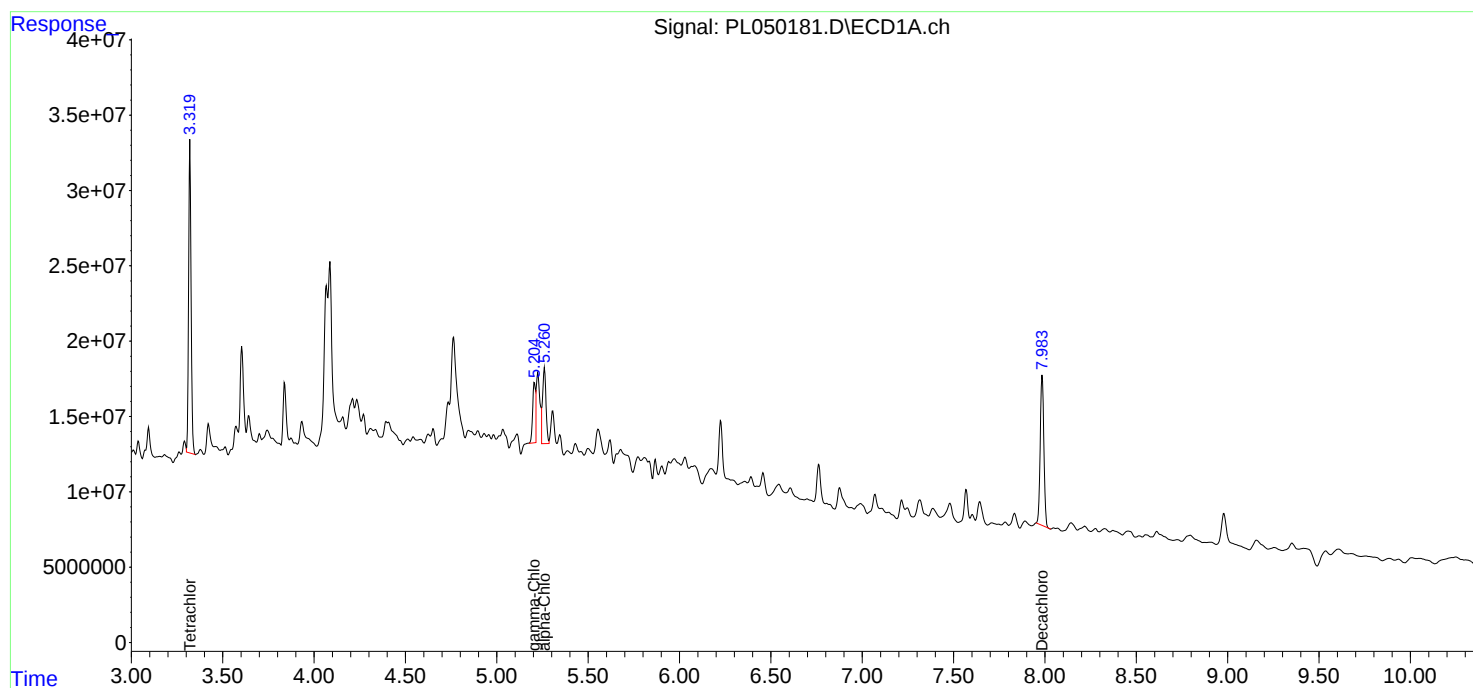

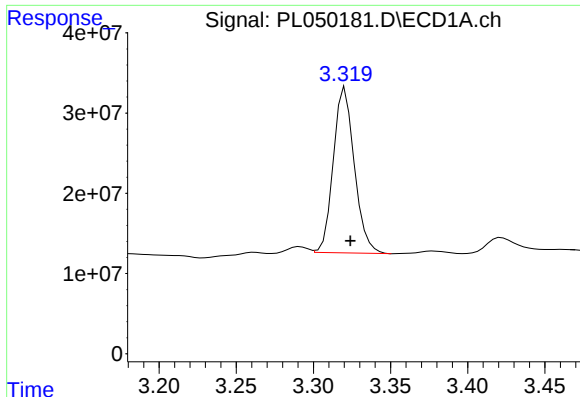


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.005 min
Response: 195349370
Conc: 17.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-051


Manual Integrations
APPROVED

Ankita
7/5/2019 10:02:40 AM

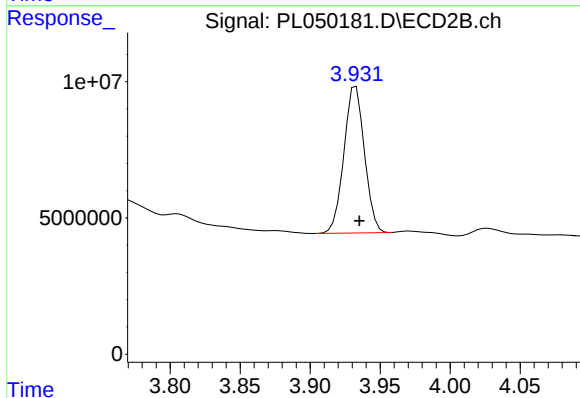


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 55015399
Conc: 17.97 ng/ml

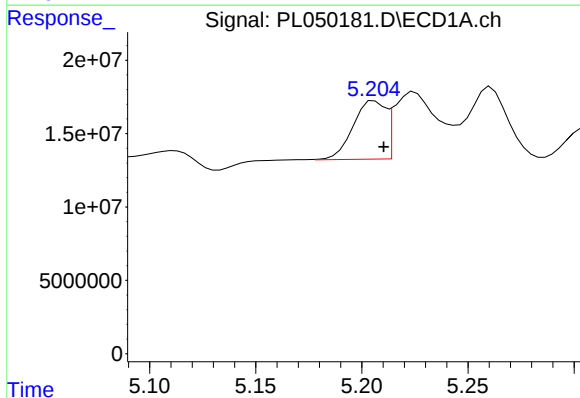


#10 gamma-Chlordane

R.T.: 5.204 min
Delta R.T.: -0.006 min
Response: 47712784
Conc: 2.79 ng/ml m

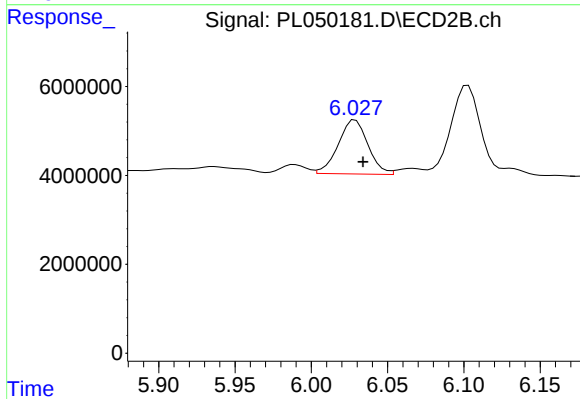

#10 gamma-Chlordane

R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 16511103
Conc: 4.43 ng/ml

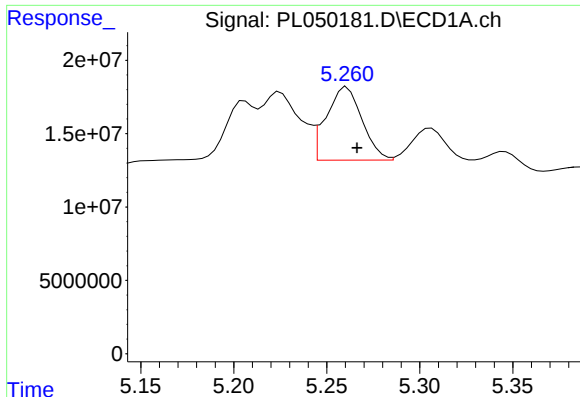


#11 alpha-Chlordane

R.T.: 5.260 min
Delta R.T.: -0.007 min
Response: 64707785
Conc: 3.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-051


Manual Integrations
APPROVED

Ankita
7/5/2019 10:02:40 AM

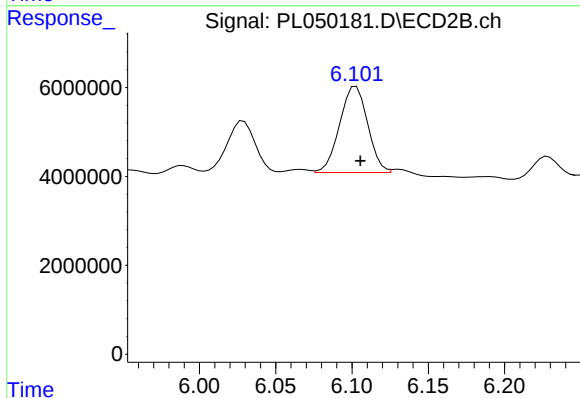


#11 alpha-Chlordane

R.T.: 6.101 min
Delta R.T.: -0.004 min
Response: 24766628
Conc: 6.70 ng/ml m

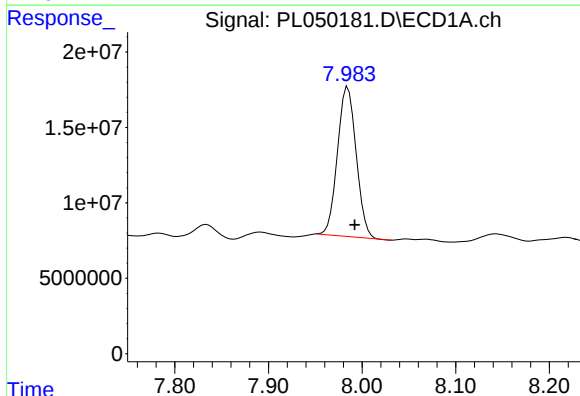

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 138086841
Conc: 10.87 ng/ml

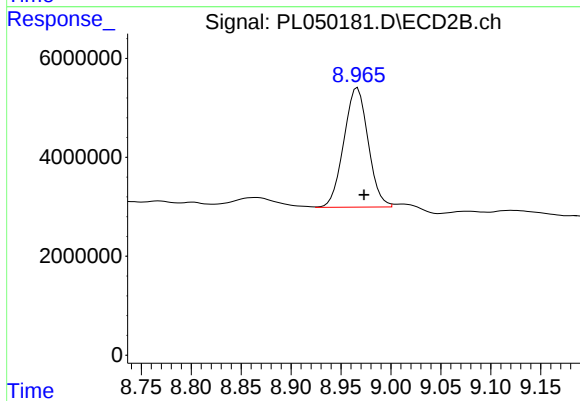

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 40961657
Conc: 12.20 ng/ml m