

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
 Data File : PL037691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2018 13:33
 Operator : UA\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 04:33:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
8) B	Heptachlo...	5.074f	0.000	228.0E6	0	24.338	N.D.	#
9) A	Endosulfan I	5.334	0.000	17004341	0	2.010	N.D.	#
10) B	gamma-Chl...	5.226	0.000	72362907	0	7.726	N.D.	#
11) B	alpha-Chl...	5.298	0.000	14901338	0	1.641	N.D.	#
14) MA	Endrin	5.816	0.000	43657861	0	5.542	N.D.	#
16) A	4,4'-DDD	5.974	0.000	12877264	0	1.961	N.D.	#
17) MA	4,4'-DDT	6.203	0.000	46597793	0	7.217	N.D.	#
19) B	Endosulfa...	6.549f	0.000	8508747	0	1.272	N.D.	#
20) A	Methoxychlor	6.760	0.000	4127656	0	1.214	N.D.	#
21) B	Endrin ke...	6.971	0.000	28866392	0	4.059	N.D.	#
25)	Chlordane-3	5.226	0.000	72362907	0	68.079	N.D.	#
26)	Chlordane-4	5.298	0.000	14901338	0	15.466	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
Data File : PL037691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2018 13:33
Operator : UA\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 04:33:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

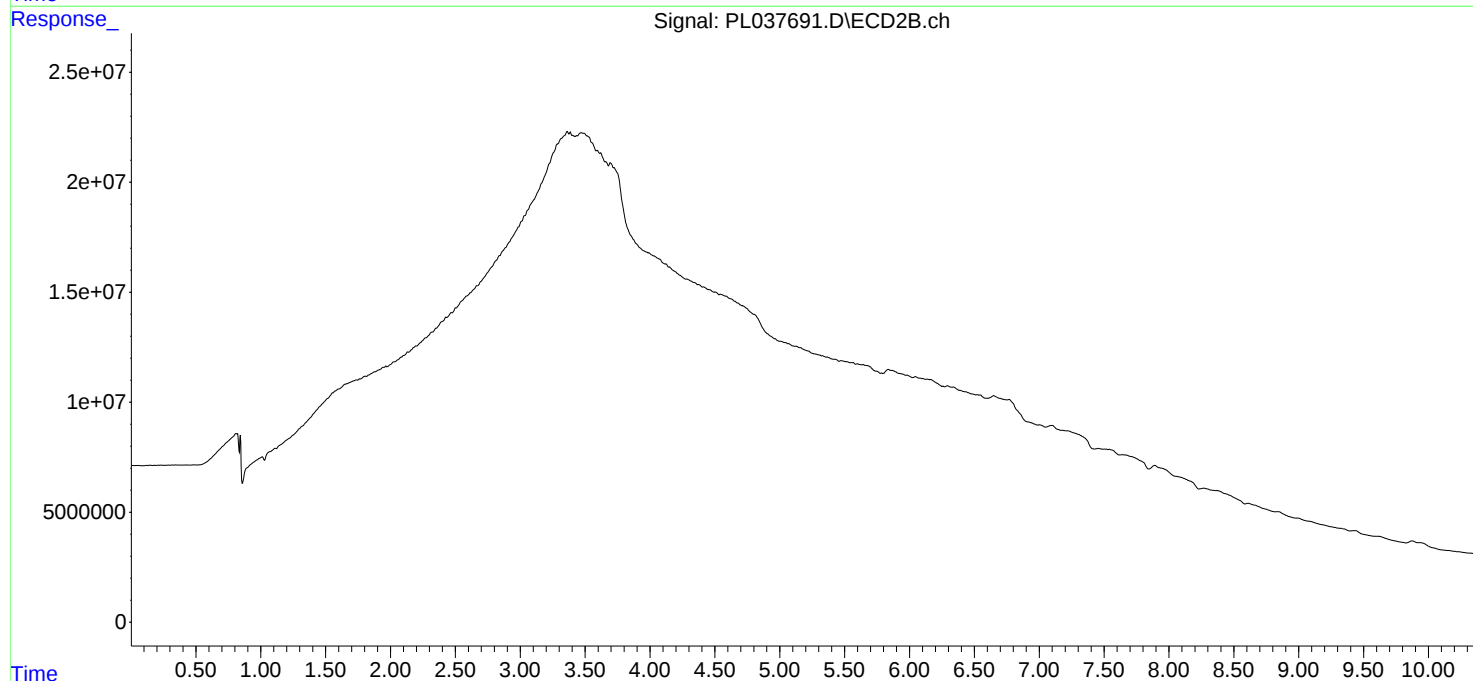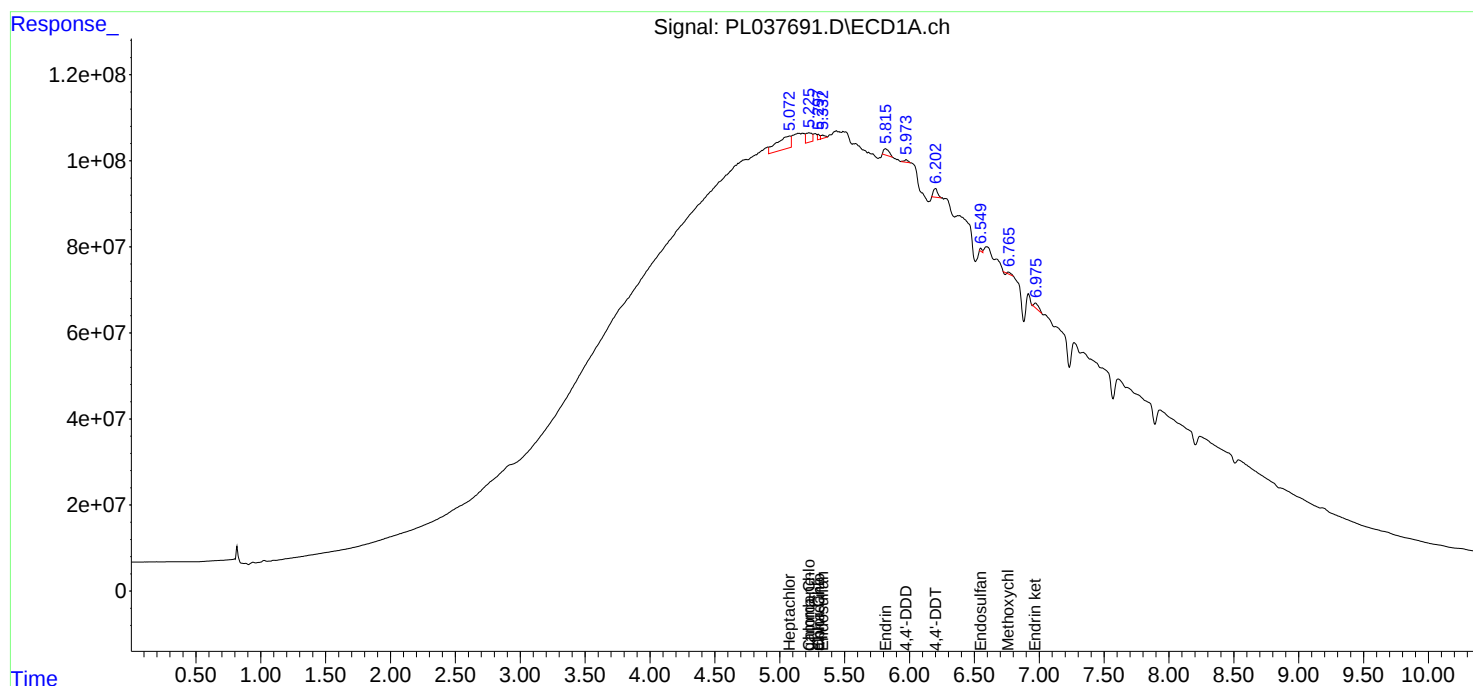


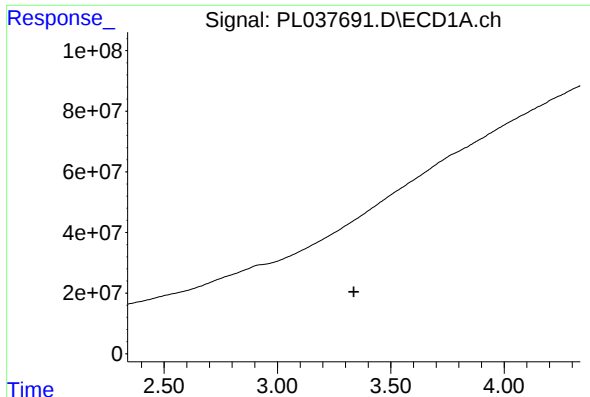

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

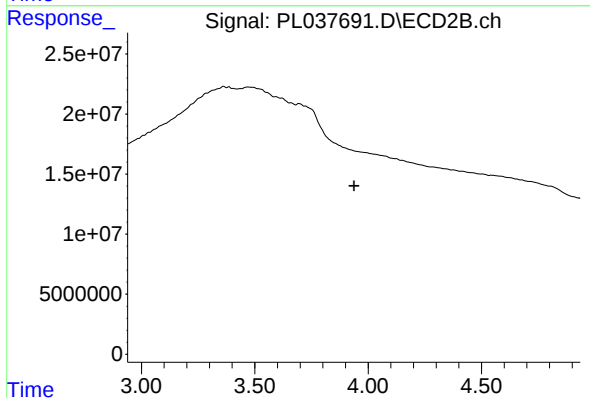


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.938 min
Response: 0
Conc: N.D.

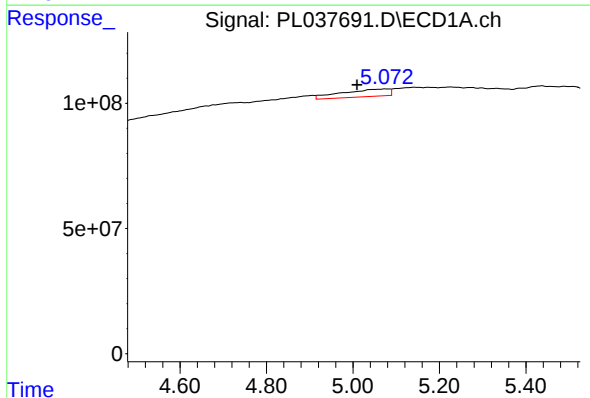


#8 Heptachlor epoxide

R.T.: 5.074 min
Delta R.T.: 0.065 min
Response: 227977297
Conc: 24.34 ng/ml

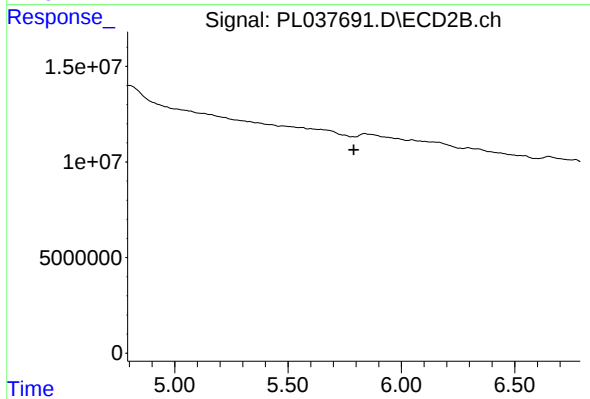

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.790 min
Response: 0
Conc: N.D.

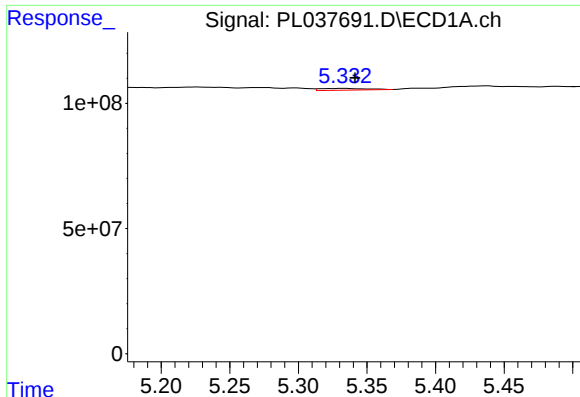

#9 Endosulfan I


R.T.: 5.334 min
Delta R.T.: -0.008 min
Response: 17004341
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

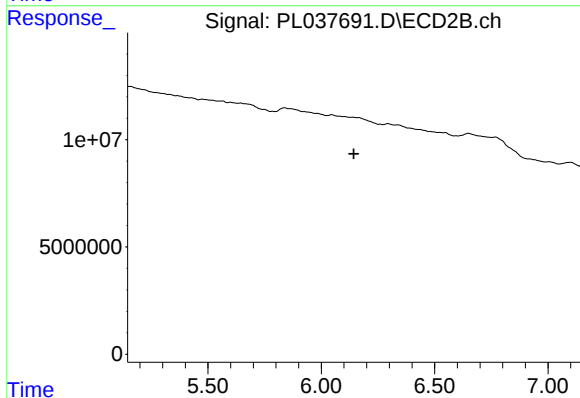


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

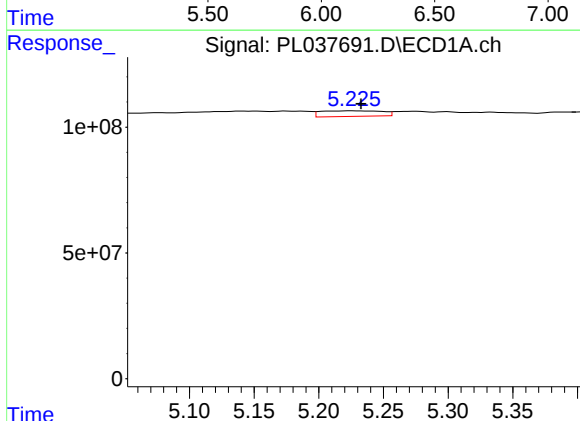


#10 gamma-Chlordane

R.T.: 5.226 min
Delta R.T.: -0.006 min
Response: 72362907
Conc: 7.73 ng/ml

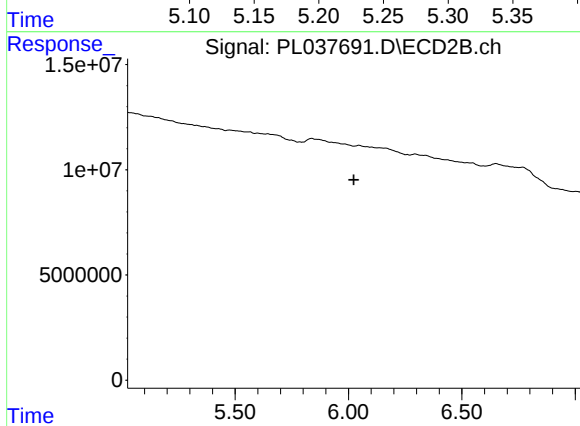

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

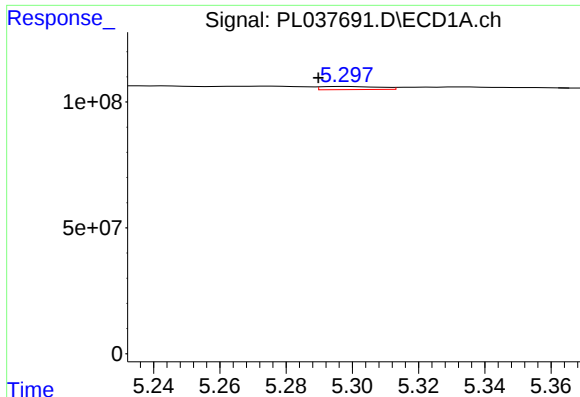

#11 alpha-Chlordane


R.T.: 5.298 min
Delta R.T.: 0.009 min
Response: 14901338
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

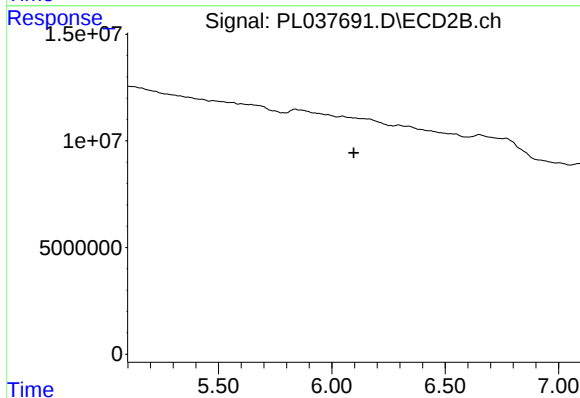


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

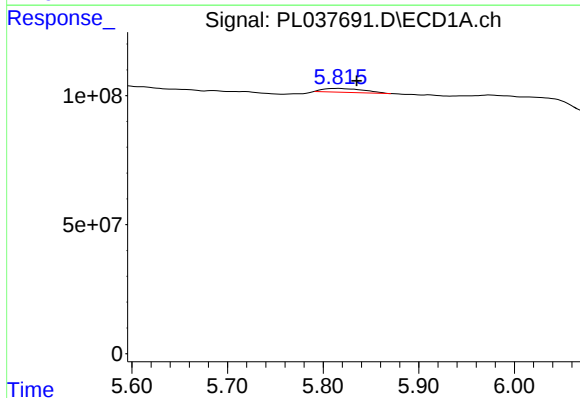


#14 Endrin

R.T.: 5.816 min
Delta R.T.: -0.019 min
Response: 43657861
Conc: 5.54 ng/ml

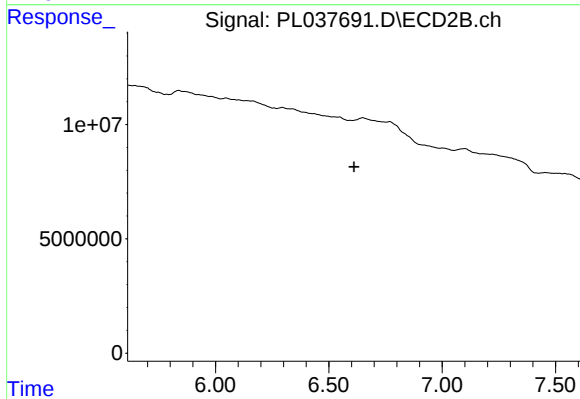

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

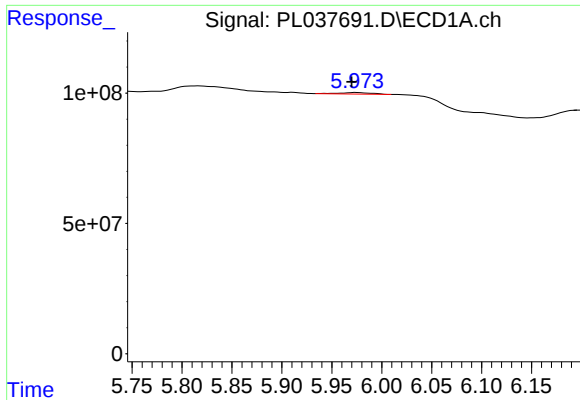

#16 4,4'-DDD


R.T.: 5.974 min
Delta R.T.: 0.004 min
Response: 12877264
Conc: 1.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

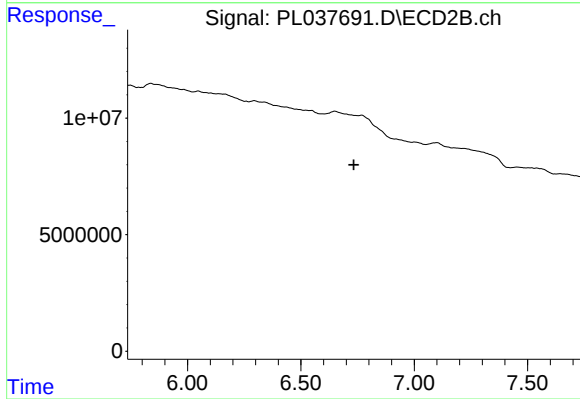


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

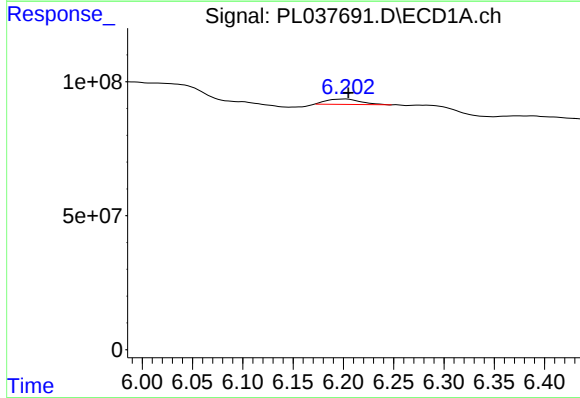


#17 4,4'-DDT

R.T.: 6.203 min
Delta R.T.: -0.002 min
Response: 46597793
Conc: 7.22 ng/ml

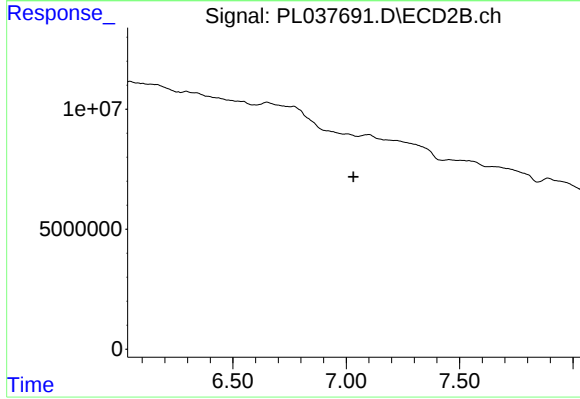

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

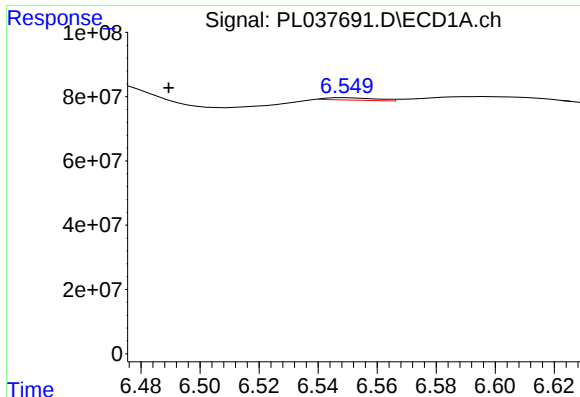

#19 Endosulfan Sulfate


R.T.: 6.549 min
Delta R.T.: 0.060 min
Response: 8508747
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

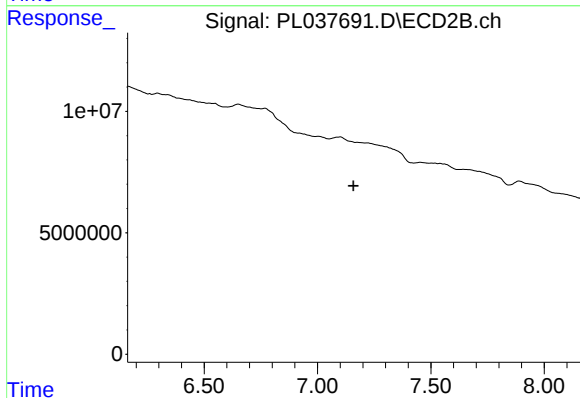


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.159 min
Response: 0
Conc: N.D.

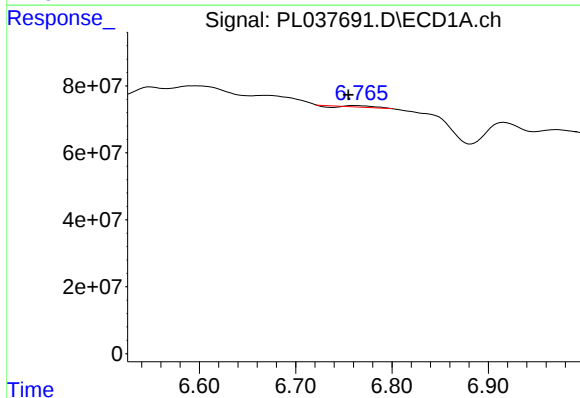


#20 Methoxychlor

R.T.: 6.760 min
Delta R.T.: 0.006 min
Response: 4127656
Conc: 1.21 ng/ml

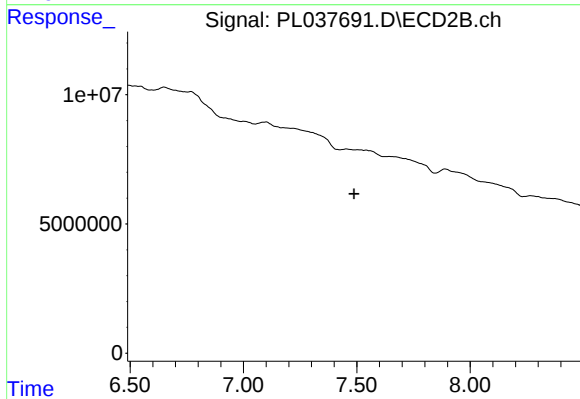

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

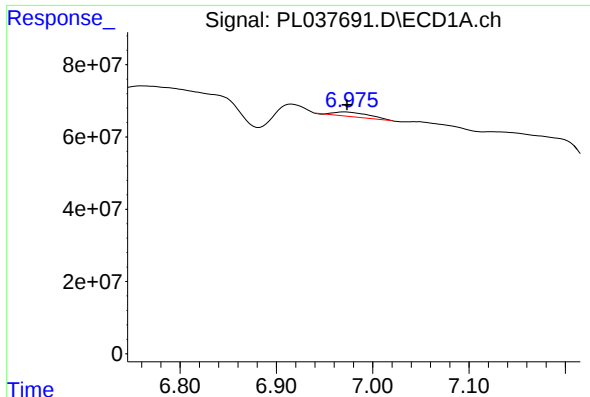

#21 Endrin ketone


R.T.: 6.971 min
Delta R.T.: -0.002 min
Response: 28866392
Conc: 4.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

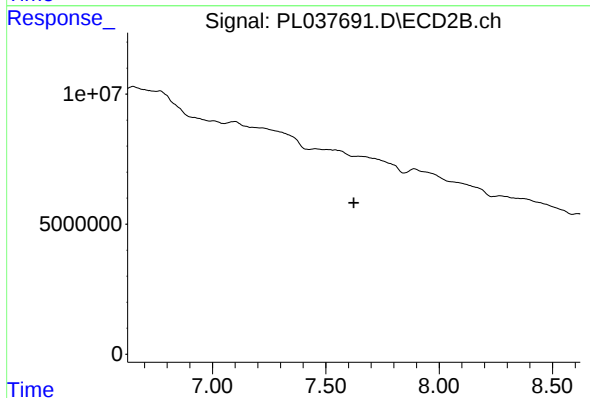


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

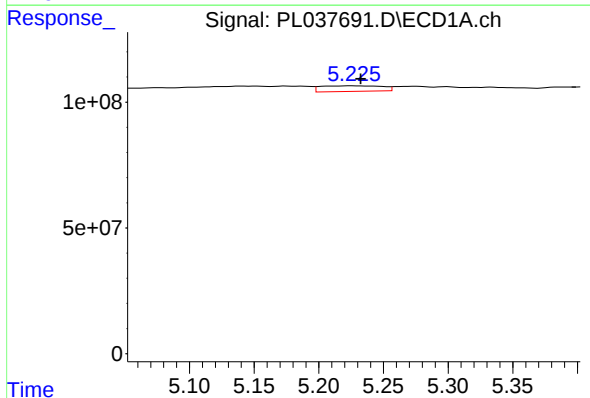


#25 Chlordane-3

R.T.: 5.226 min
Delta R.T.: -0.006 min
Response: 72362907
Conc: 68.08 ng/ml

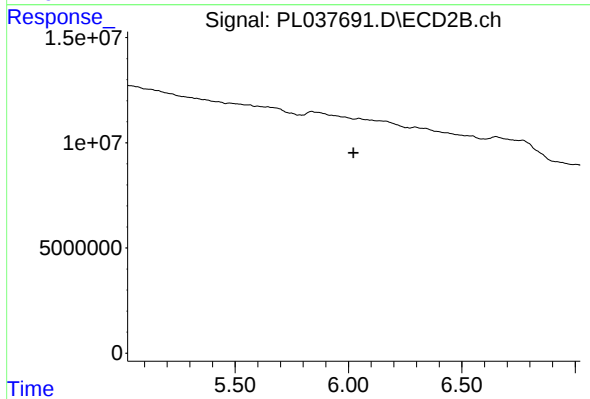

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

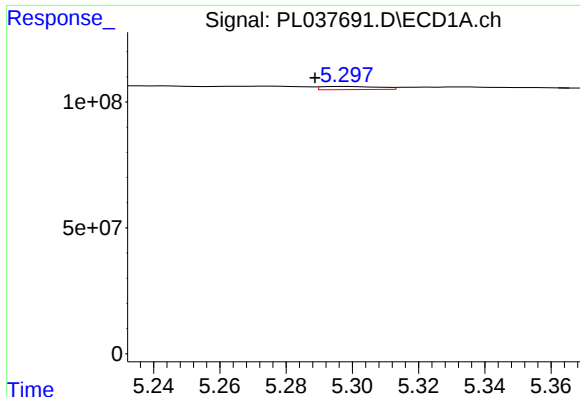

#26 Chlordane-4


R.T.: 5.298 min
Delta R.T.: 0.010 min
Response: 14901338
Conc: 15.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

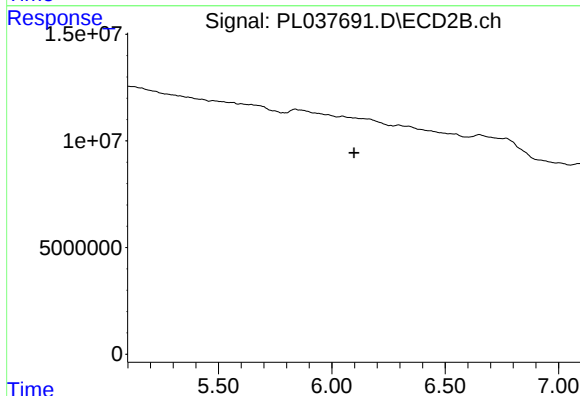


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

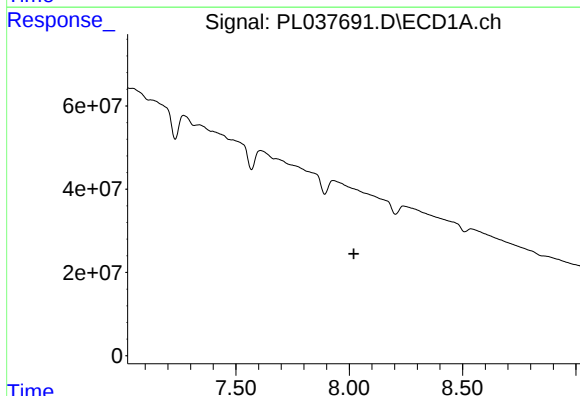

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.021 min
Response: 0
Conc: N.D.

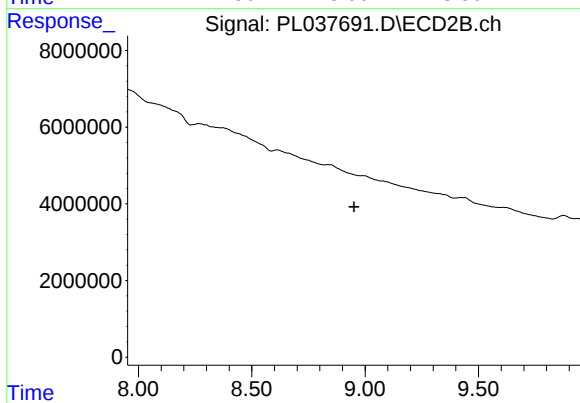

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.951 min
Response: 0
Conc: N.D.