

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
 Data File : PL037720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2018 20:25
 Operator : UA\AJ
 Sample : J3852-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 04:40:35 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.935	97350804	37319773	12.307	13.489
28)	SA Decachlor...	8.010	8.945	92202809	30989378	15.280	15.620
Target Compounds							
10)	B gamma-Chl...	5.163f	0.000	8725056	0	0.932	N.D. #
25)	Chlordane-3	5.163	0.000	8725056	0	8.209	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
Data File : PL037720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2018 20:25
Operator : UA\AJ
Sample : J3852-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 04:40:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

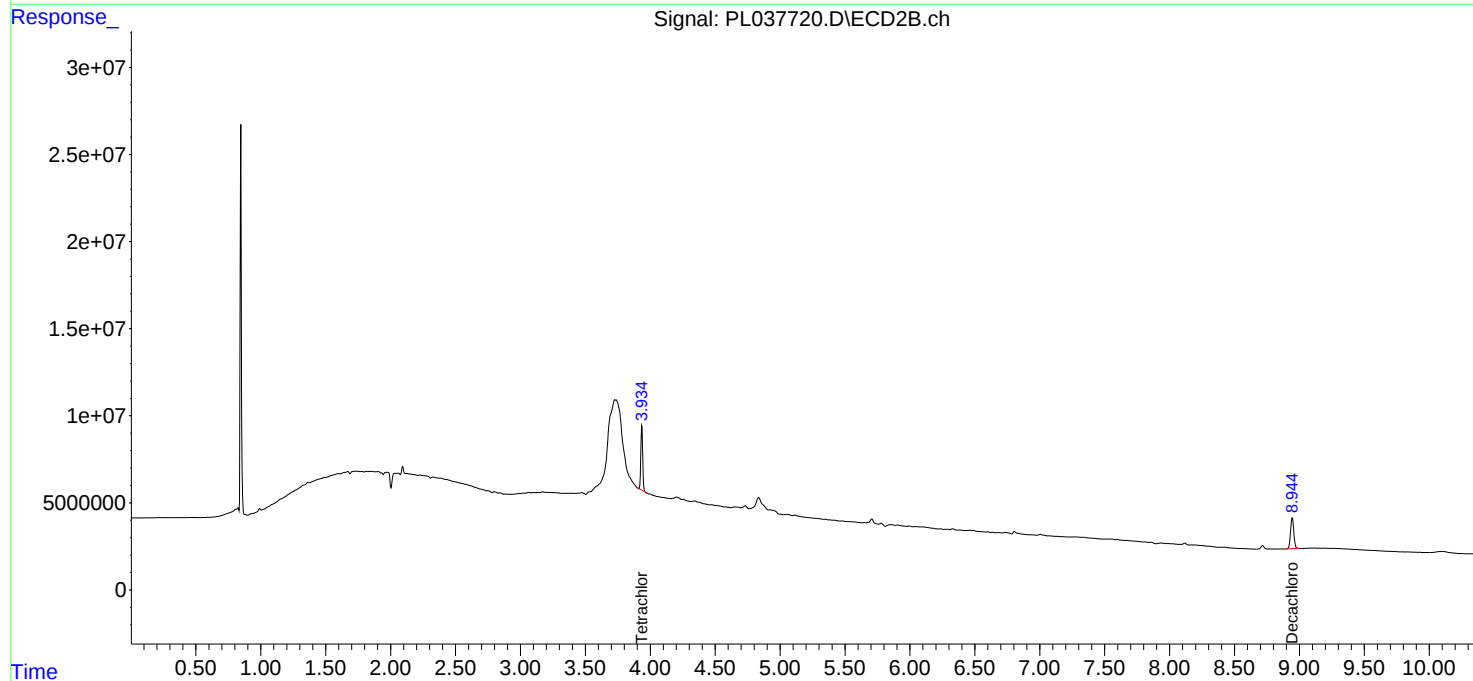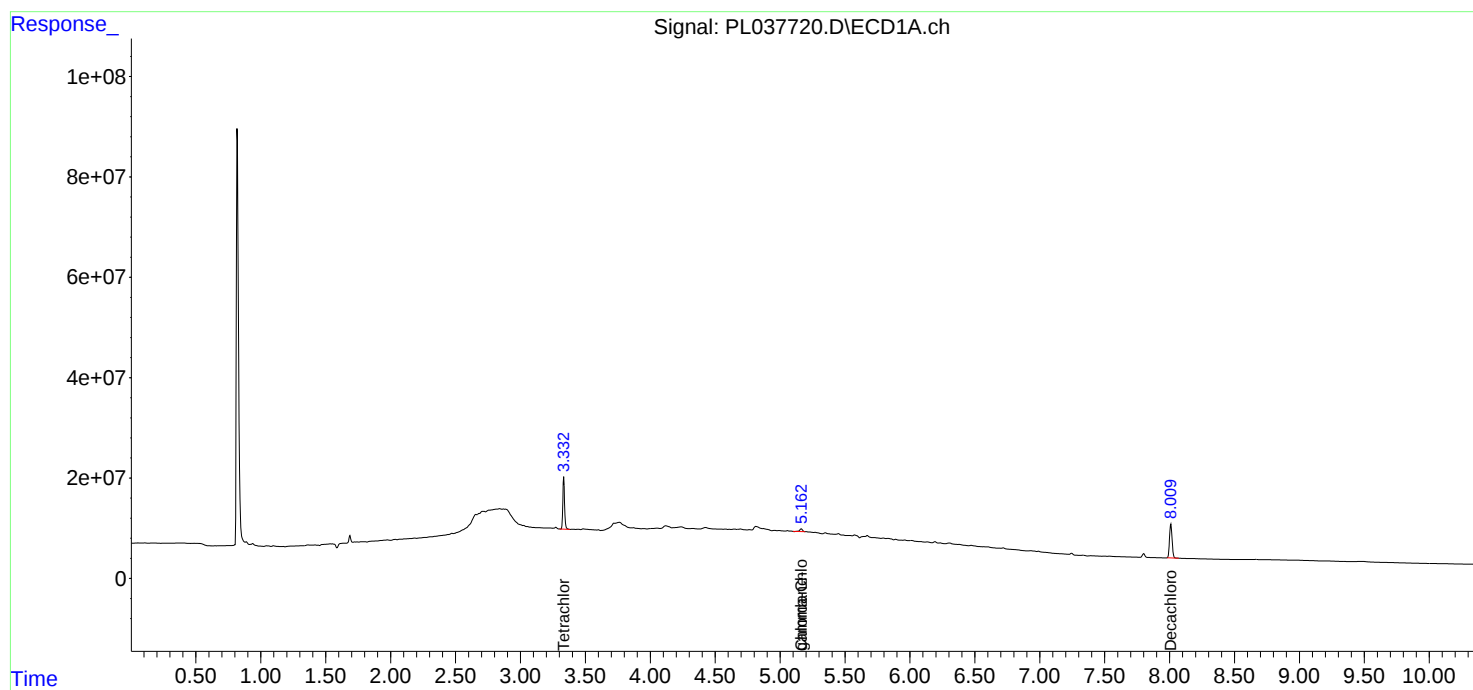


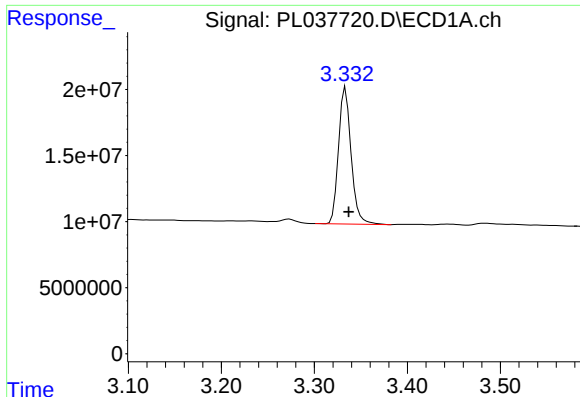

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 97350804
Conc: 12.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

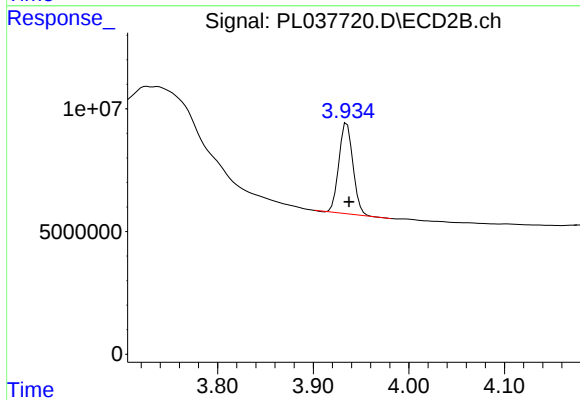


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 37319773
Conc: 13.49 ng/ml

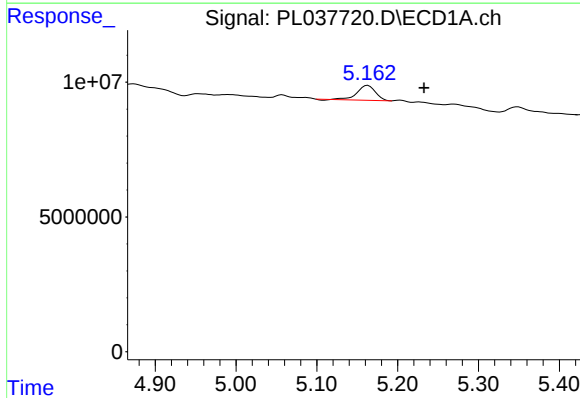


#10 gamma-Chlordane

R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 8725056
Conc: 0.93 ng/ml

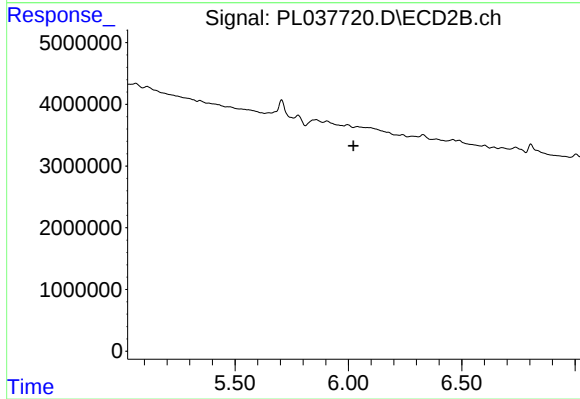

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

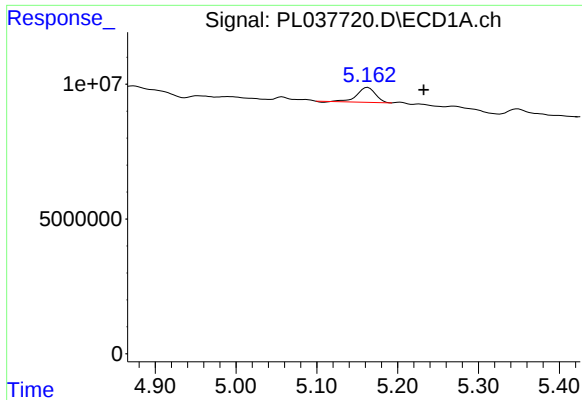

#25 Chlordane-3


R.T.: 5.163 min
Delta R.T.: -0.069 min
Response: 8725056
Conc: 8.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

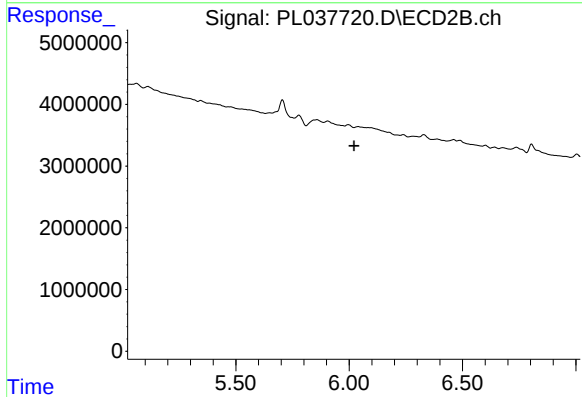


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

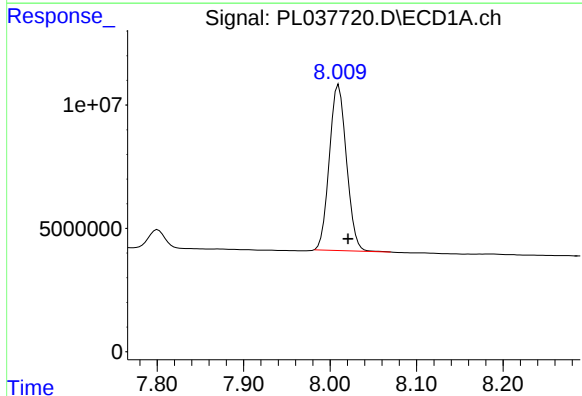

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 92202809
Conc: 15.28 ng/ml

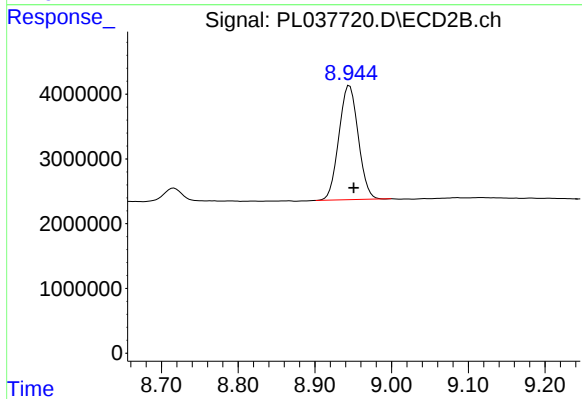

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 30989378
Conc: 15.62 ng/ml