

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
 Data File : PL037722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2018 20:53
 Operator : UA\AJ
 Sample : J3858-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 04:41:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	95684542	36676075	12.096	13.256
28)	SA Decachlor...	8.010	8.945	76607945	26026959	12.696	13.119
Target Compounds							
9)	A Endosulfan I	5.281f	6.096f	17240138	8464072	2.038	3.300 #
10)	B gamma-Chl...	5.226	0.000	13970113	0	1.492	N.D. #
11)	B alpha-Chl...	5.281	6.096	17240138	8464072	1.898	2.941 #
12)	B 4,4'-DDE	5.451	0.000	8520401	0	0.965	N.D. #
14)	MA Endrin	5.833	0.000	8905447	0	1.130	N.D. #
16)	A 4,4'-DDD	5.962	0.000	10589039	0	1.612	N.D. #
17)	MA 4,4'-DDT	6.197	7.029	70324638	24926321	10.892	11.768
23)	Chlordane-1	4.177	0.000	6889462	0	22.437	N.D. #
24)	Chlordane-2	4.670	0.000	9085612	0	25.521	N.D. #
25)	Chlordane-3	5.226	0.000	13970113	0	13.143	N.D. #
26)	Chlordane-4	5.281	6.096	17240138	8464072	17.893	17.663
27)	Chlordane-5	5.833	0.000	8905447	0	68.049	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
Data File : PL037722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2018 20:53
Operator : UA\AJ
Sample : J3858-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 04:41:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

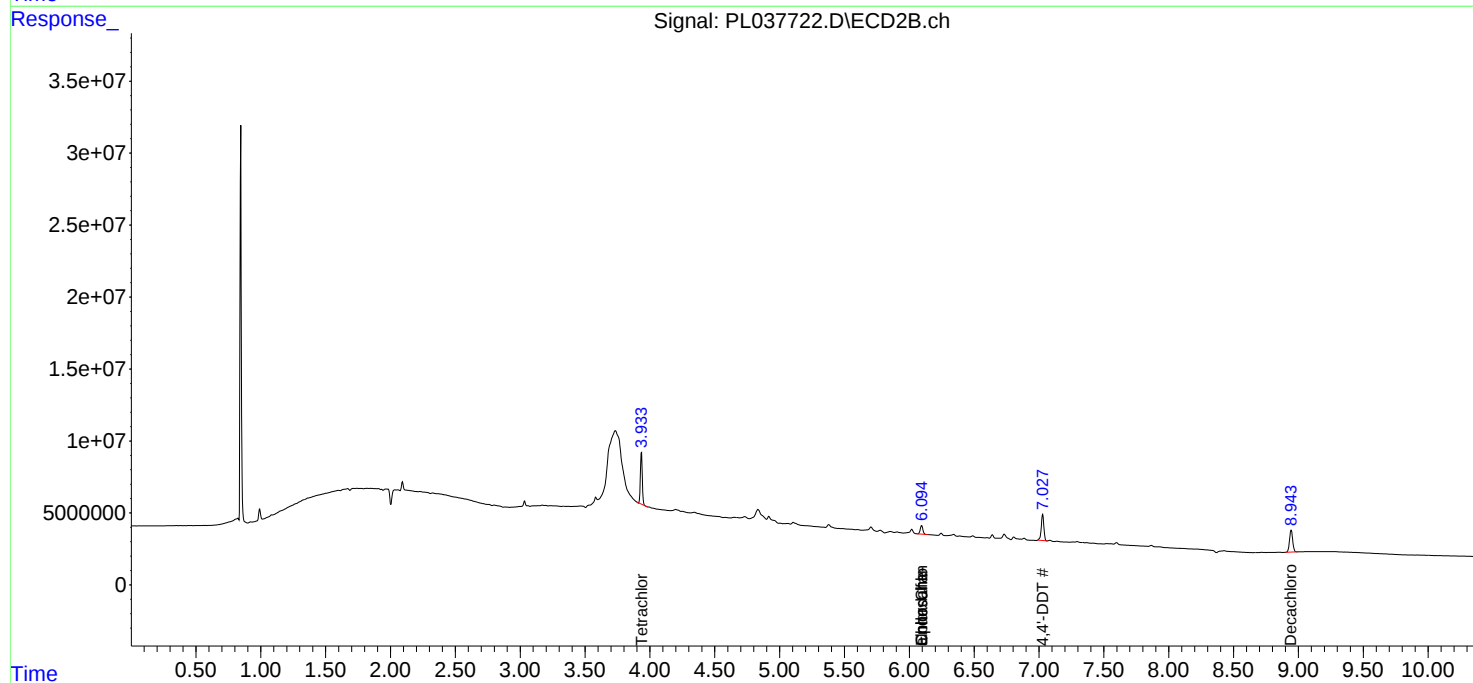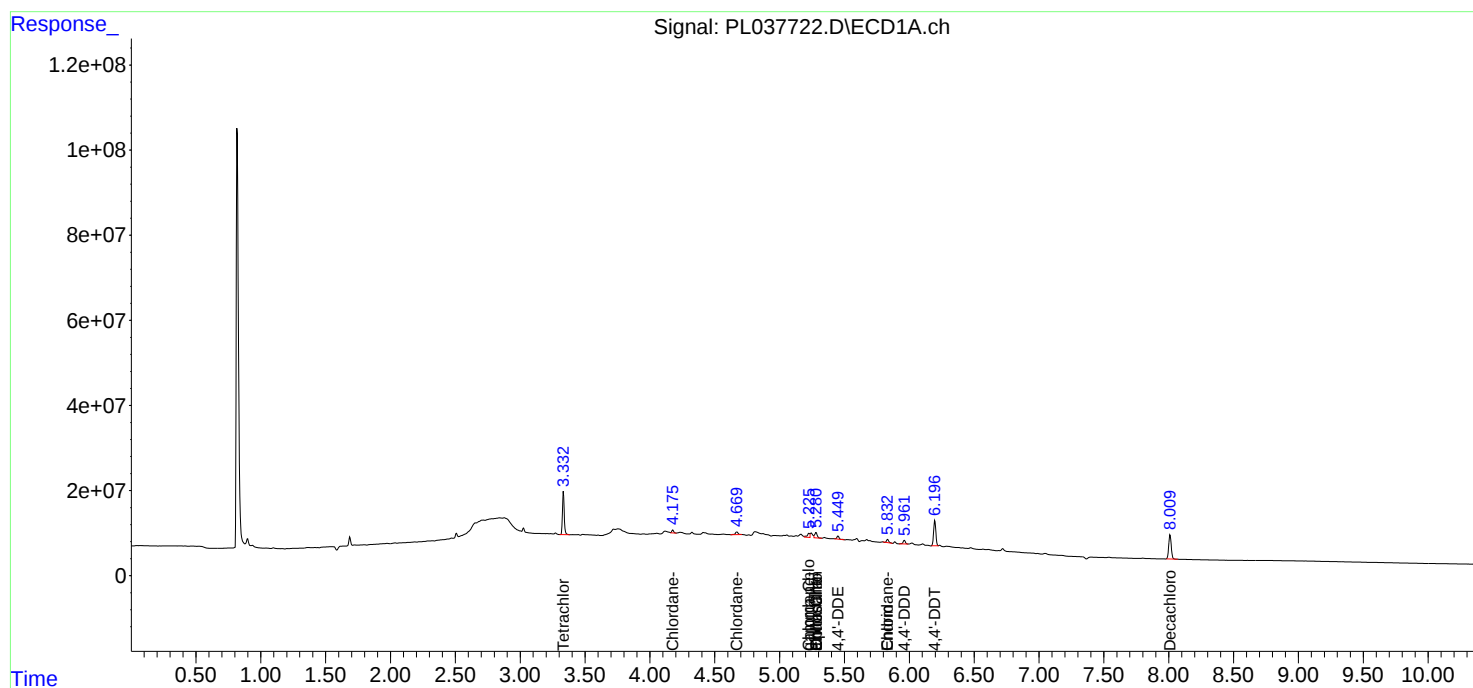


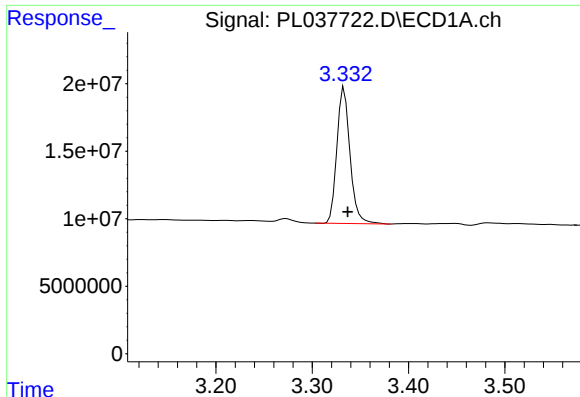

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 95684542
Conc: 12.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

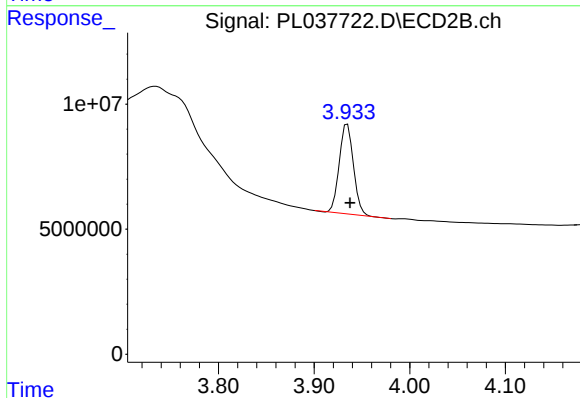


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 36676075
Conc: 13.26 ng/ml

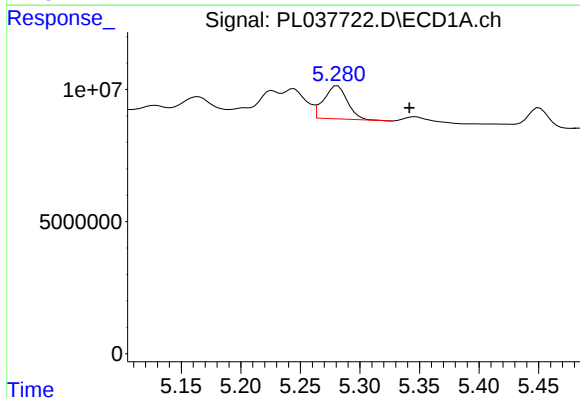


#9 Endosulfan I

R.T.: 5.281 min
Delta R.T.: -0.060 min
Response: 17240138
Conc: 2.04 ng/ml

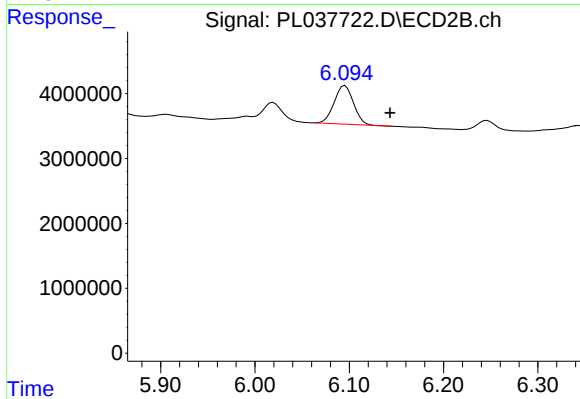

#9 Endosulfan I


R.T.: 6.096 min
Delta R.T.: -0.048 min
Response: 8464072
Conc: 3.30 ng/ml

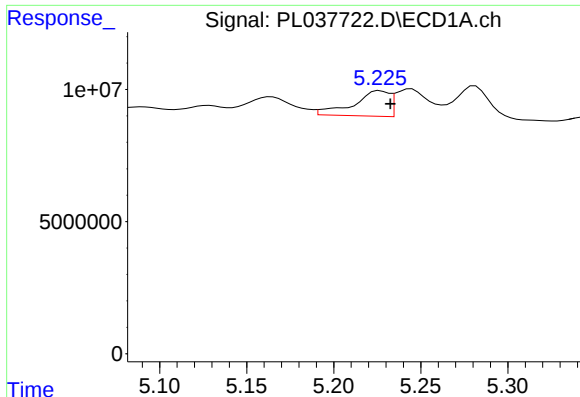

#10 gamma-Chlordane


R.T.: 5.226 min
Delta R.T.: -0.006 min
Response: 13970113
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

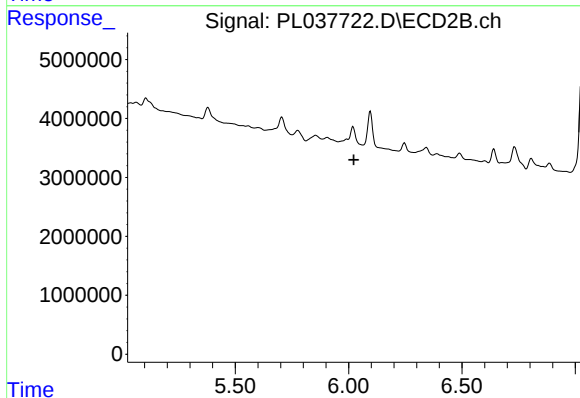


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

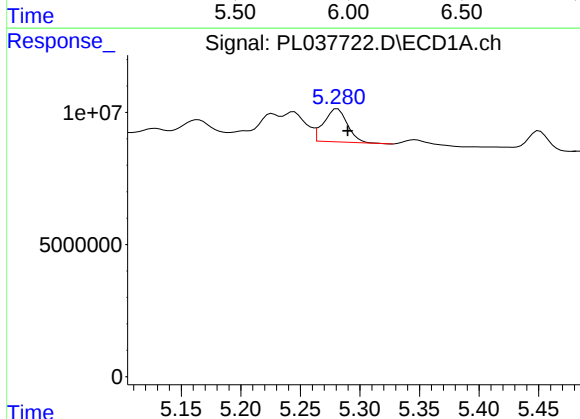


#11 alpha-Chlordane

R.T.: 5.281 min
Delta R.T.: -0.009 min
Response: 17240138
Conc: 1.90 ng/ml

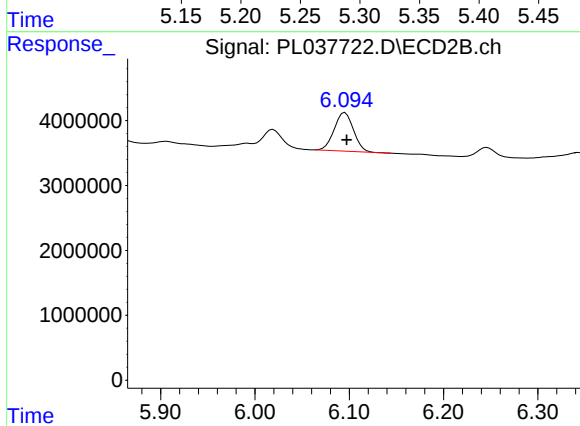

#11 alpha-Chlordane


R.T.: 6.096 min
Delta R.T.: -0.002 min
Response: 8464072
Conc: 2.94 ng/ml

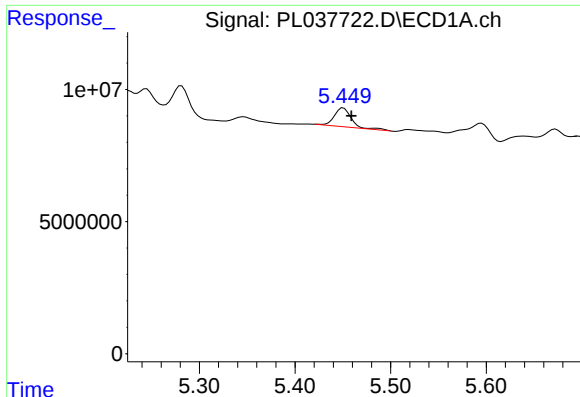

#12 4,4'-DDE


R.T.: 5.451 min
Delta R.T.: -0.008 min
Response: 8520401
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

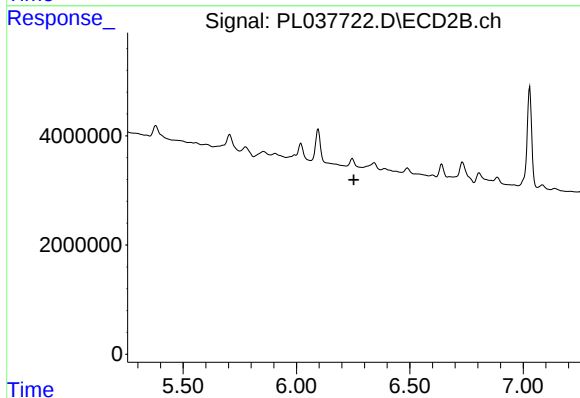


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

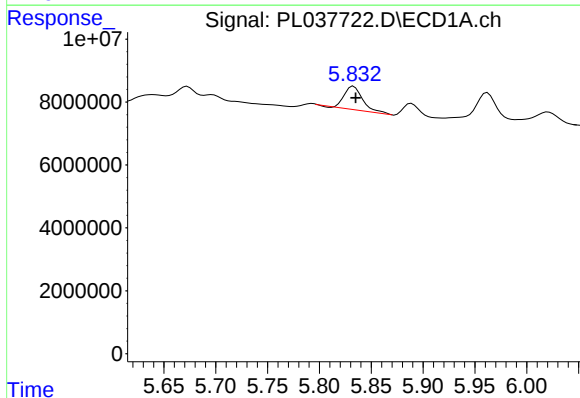


#14 Endrin

R.T.: 5.833 min
Delta R.T.: -0.002 min
Response: 8905447
Conc: 1.13 ng/ml

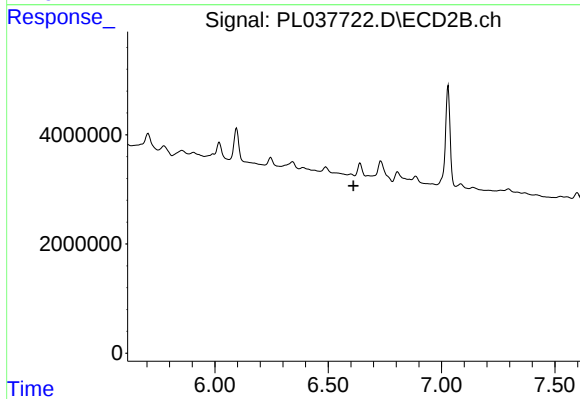

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

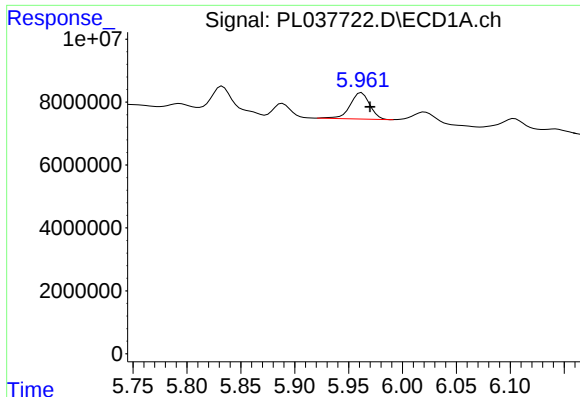

#16 4,4'-DDD


R.T.: 5.962 min
Delta R.T.: -0.008 min
Response: 10589039
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

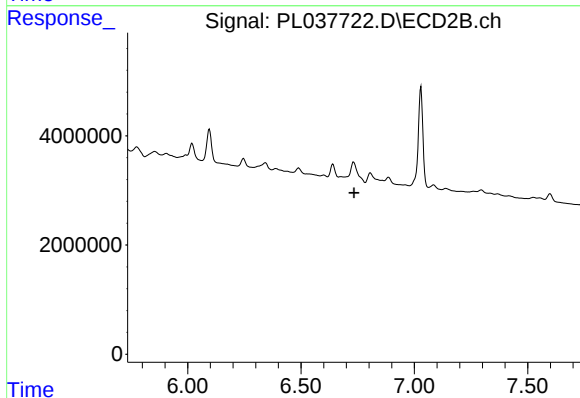


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.734 min
Response: 0
Conc: N.D.

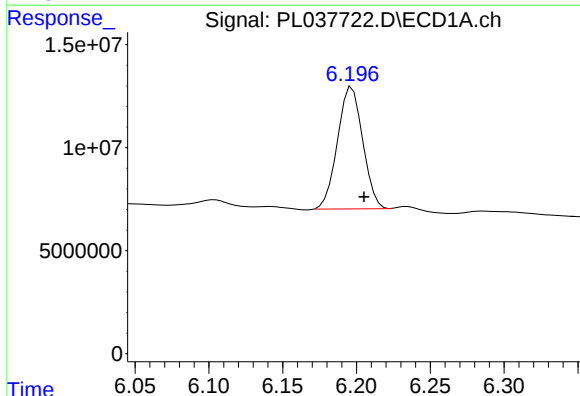


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: -0.008 min
Response: 70324638
Conc: 10.89 ng/ml

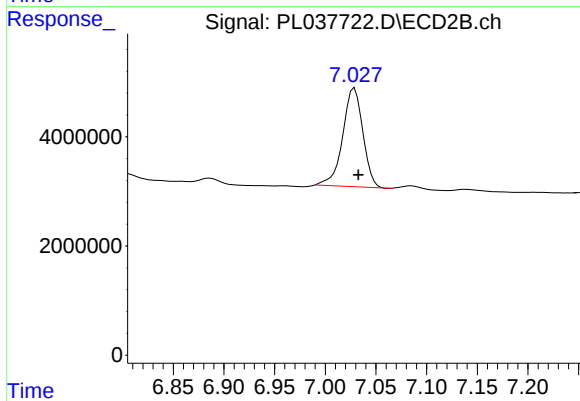

#17 4,4'-DDT


R.T.: 7.029 min
Delta R.T.: -0.004 min
Response: 24926321
Conc: 11.77 ng/ml

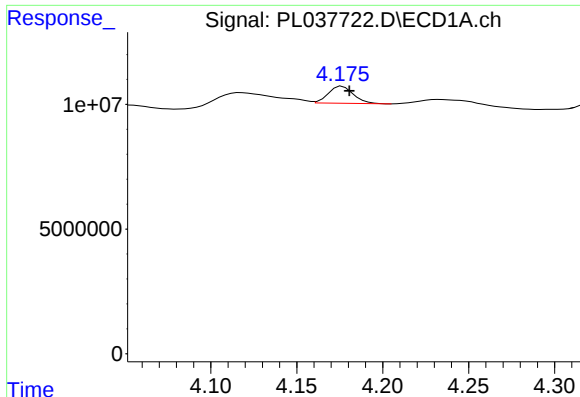

#23 Chlordane-1


R.T.: 4.177 min
Delta R.T.: -0.004 min
Response: 6889462
Conc: 22.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

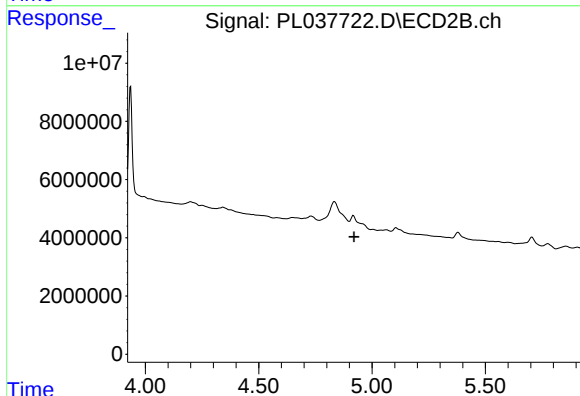


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

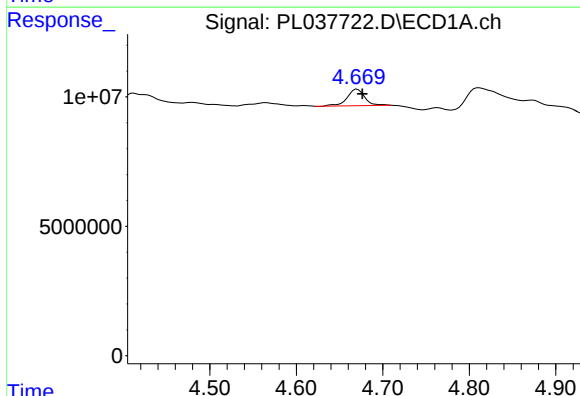


#24 Chlordane-2

R.T.: 4.670 min
Delta R.T.: -0.006 min
Response: 9085612
Conc: 25.52 ng/ml

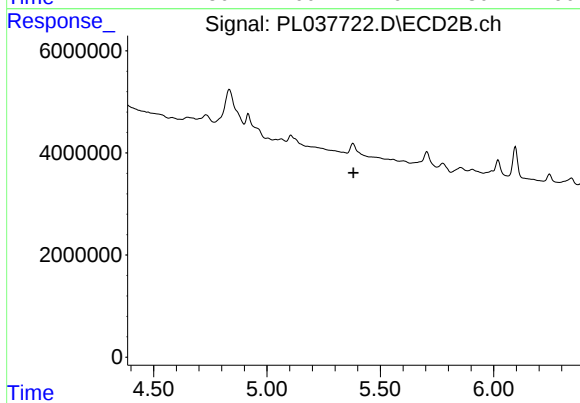

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

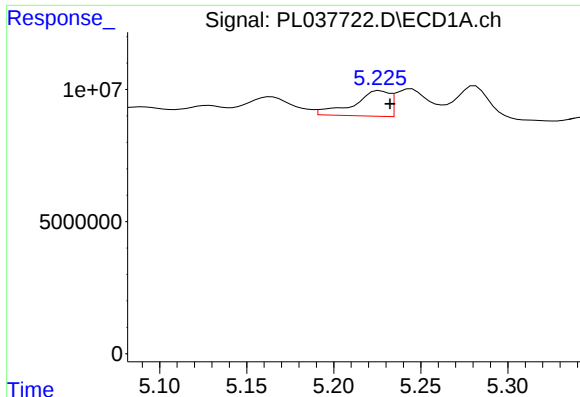

#25 Chlordane-3


R.T.: 5.226 min
Delta R.T.: -0.006 min
Response: 13970113
Conc: 13.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

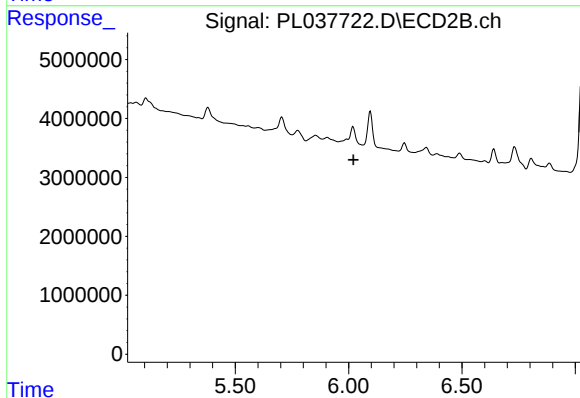


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

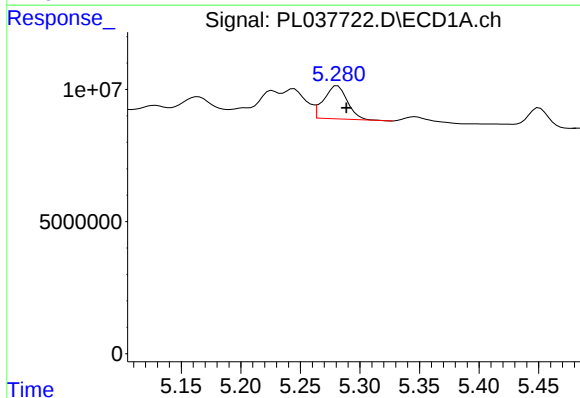


#26 Chlordane-4

R.T.: 5.281 min
Delta R.T.: -0.008 min
Response: 17240138
Conc: 17.89 ng/ml

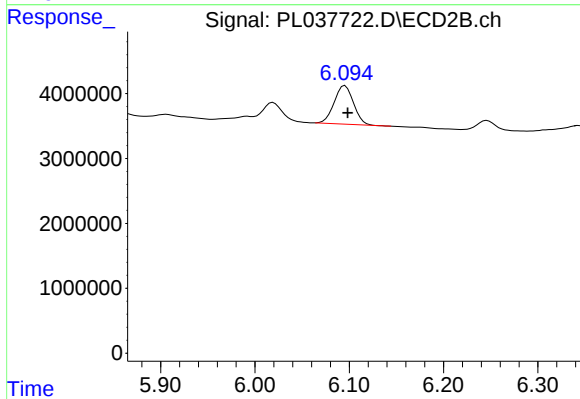

#26 Chlordane-4


R.T.: 6.096 min
Delta R.T.: -0.003 min
Response: 8464072
Conc: 17.66 ng/ml

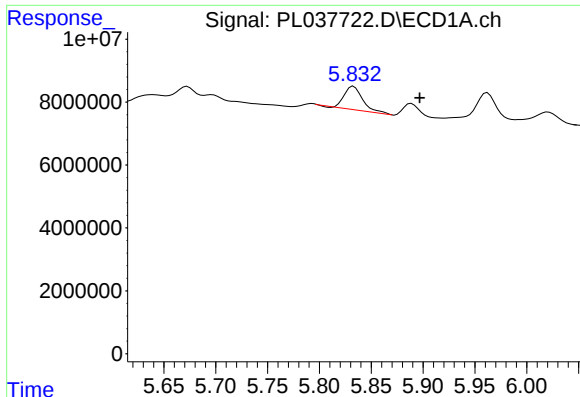

#27 Chlordane-5


R.T.: 5.833 min
Delta R.T.: -0.064 min
Response: 8905447
Conc: 68.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

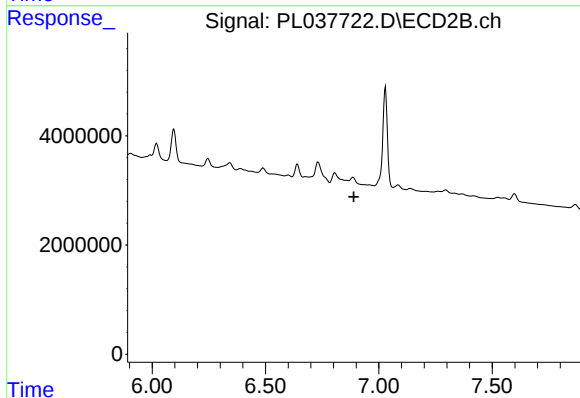


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

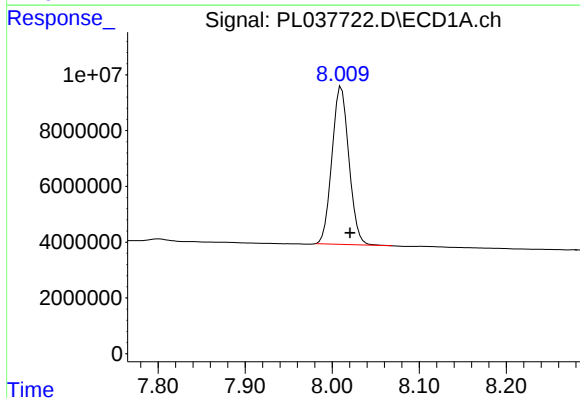

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.010 min
Response: 76607945
Conc: 12.70 ng/ml

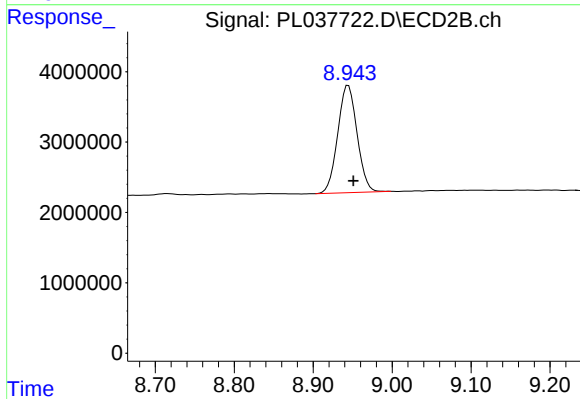

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 26026959
Conc: 13.12 ng/ml