

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
 Data File : PL037732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2018 23:14
 Operator : UA\AJ
 Sample : J3864-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 04:44:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	74926027	20054337	9.472	7.248
28)	SA Decachlor...	8.009	8.945	49426749	18279256	8.191	9.214
Target Compounds							
4)	MA Heptachlor	4.351	0.000	3294711	0	0.322	N.D. #
10)	B gamma-Chl...	5.164f	0.000	19908669	0	2.126	N.D. #
13)	MA Dieldrin	5.585	0.000	16225621	0	1.833	N.D. #
23)	Chlordane-1	4.182	0.000	17125467	0	55.774	N.D. #
24)	Chlordane-2	4.651	0.000	2161172	0	6.071	N.D. #
25)	Chlordane-3	5.164	0.000	19908669	0	18.730	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
Data File : PL037732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2018 23:14
Operator : UA\AJ
Sample : J3864-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 04:44:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

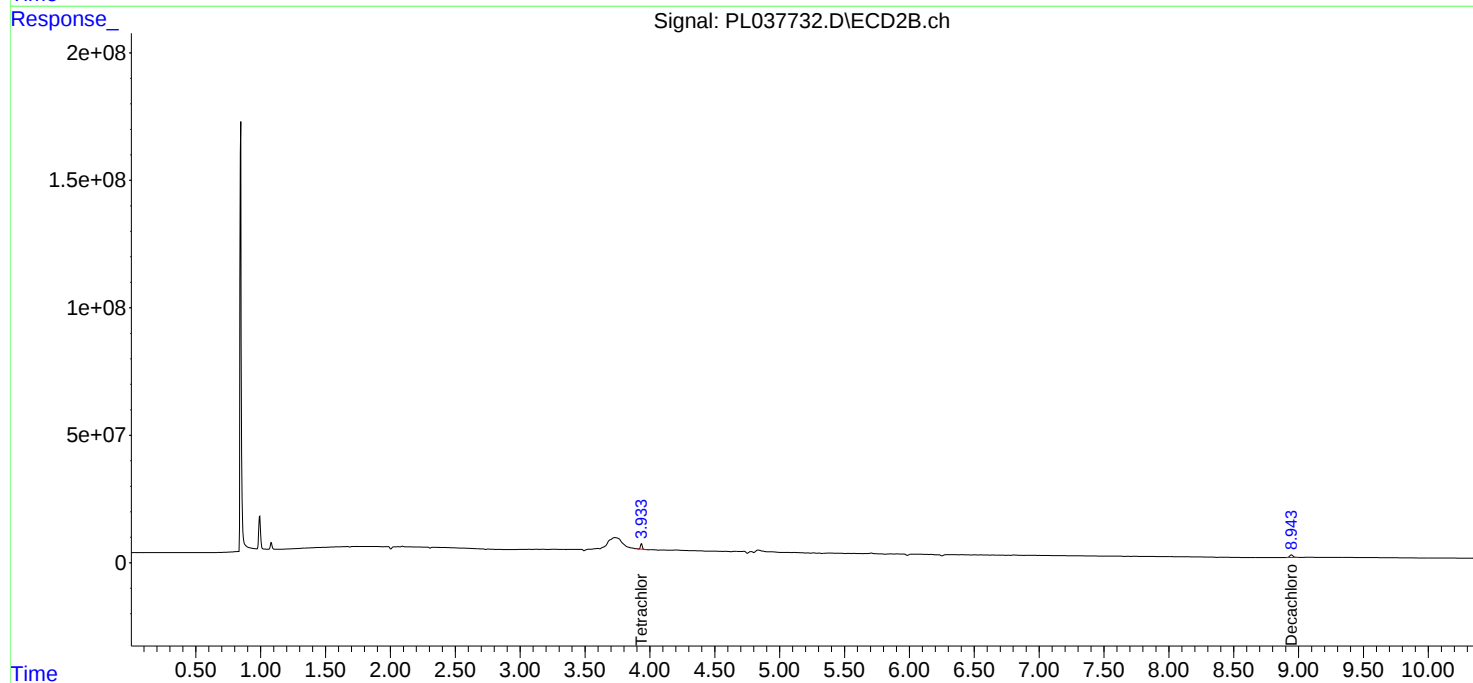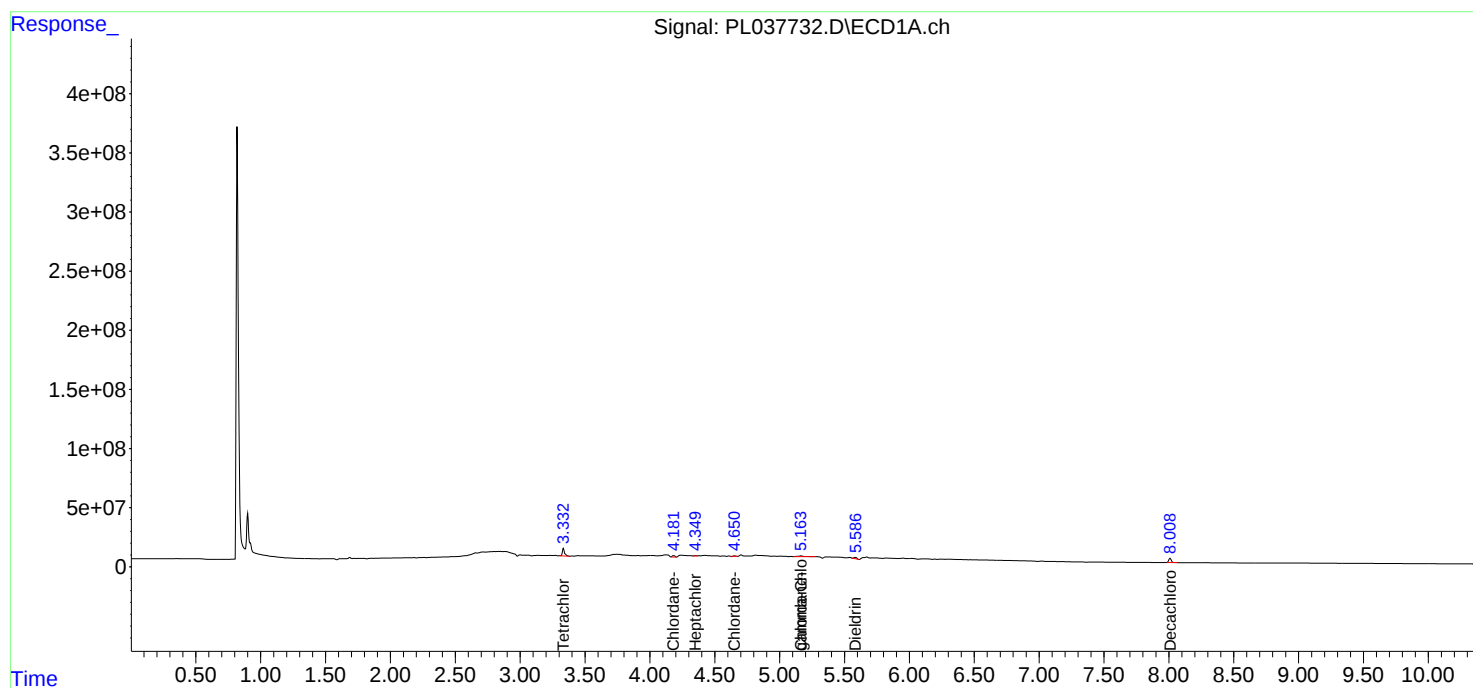


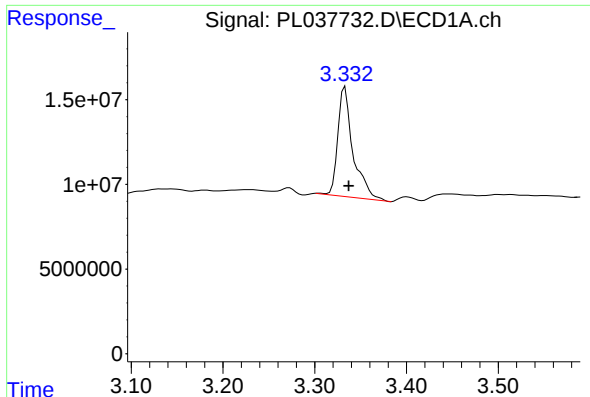

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 74926027
Conc: 9.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

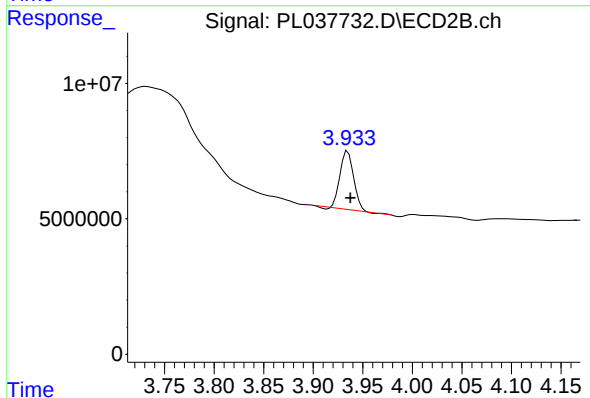


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 20054337
Conc: 7.25 ng/ml

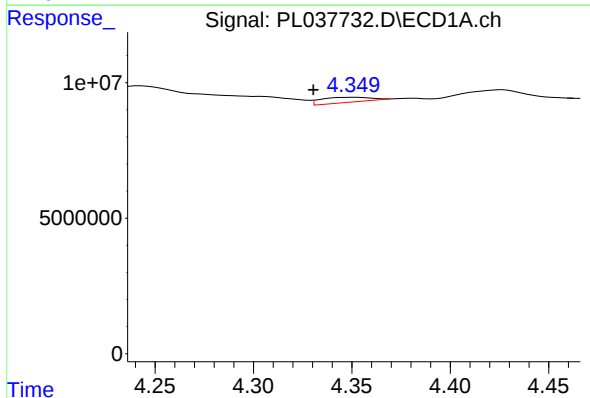


#4 Heptachlor

R.T.: 4.351 min
Delta R.T.: 0.020 min
Response: 3294711
Conc: 0.32 ng/ml

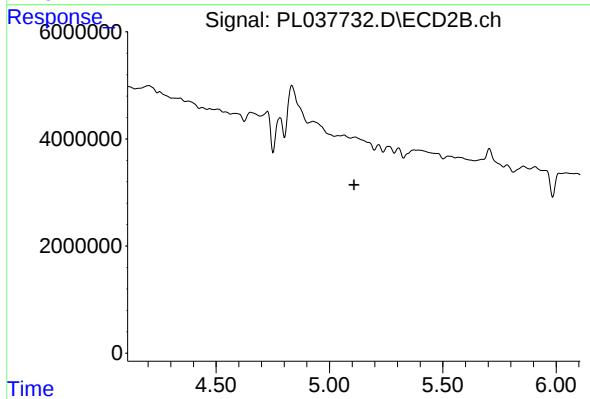

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

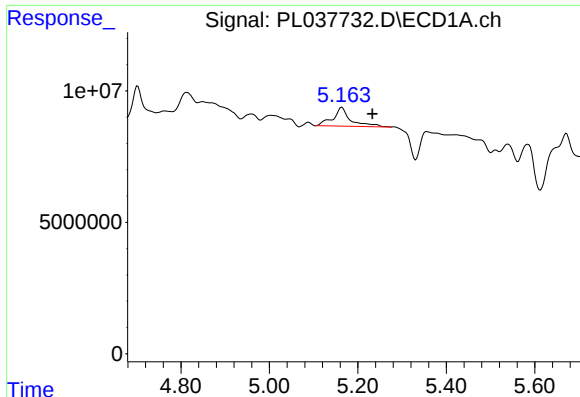

#10 gamma-Chlordane


R.T.: 5.164 min
Delta R.T.: -0.069 min
Response: 19908669
Conc: 2.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

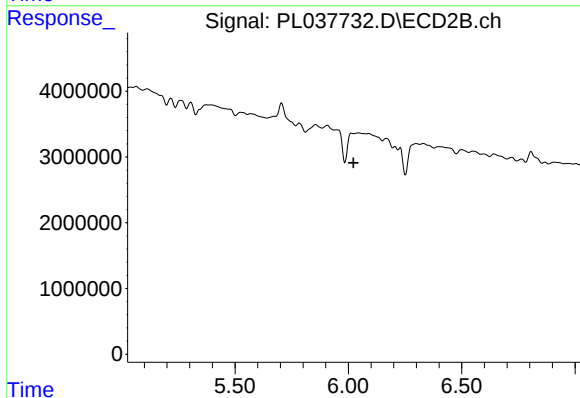


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

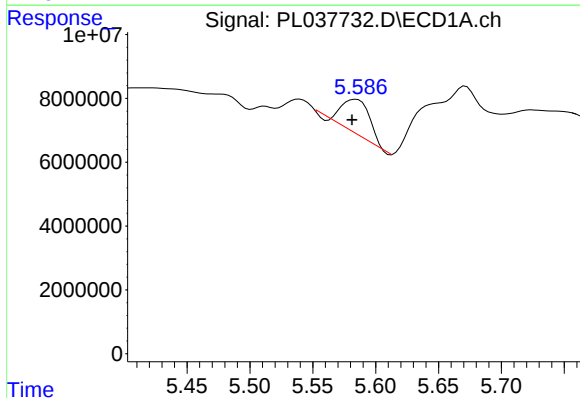


#13 Dieldrin

R.T.: 5.585 min
Delta R.T.: 0.003 min
Response: 16225621
Conc: 1.83 ng/ml

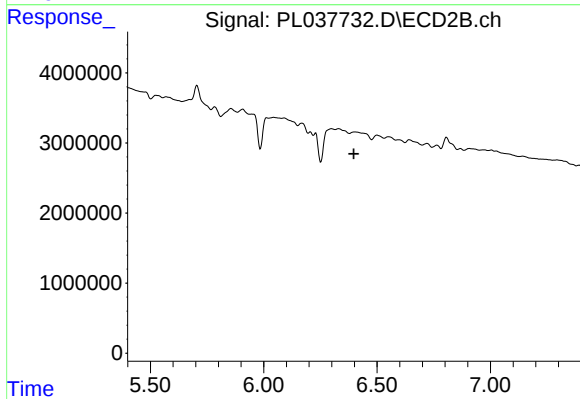

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

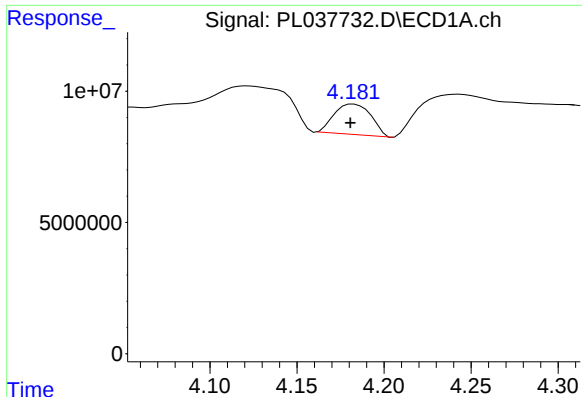

#23 Chlordane-1


R.T.: 4.182 min
Delta R.T.: 0.002 min
Response: 17125467
Conc: 55.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

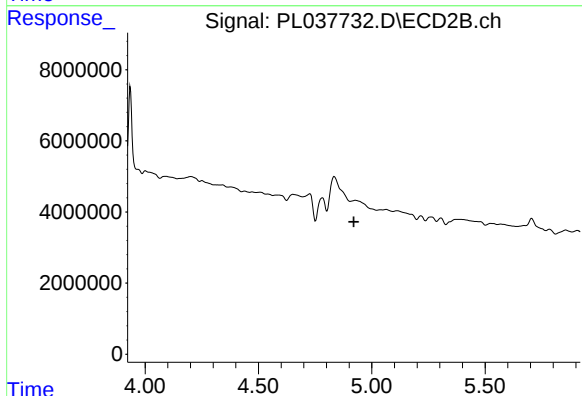


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

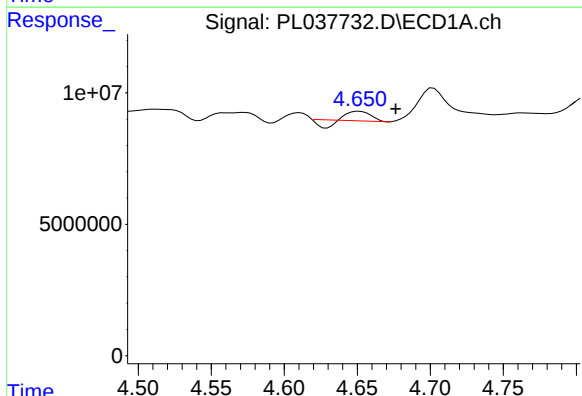


#24 Chlordane-2

R.T.: 4.651 min
Delta R.T.: -0.025 min
Response: 2161172
Conc: 6.07 ng/ml

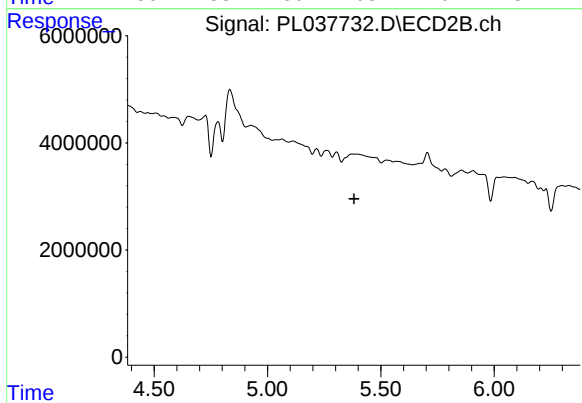

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

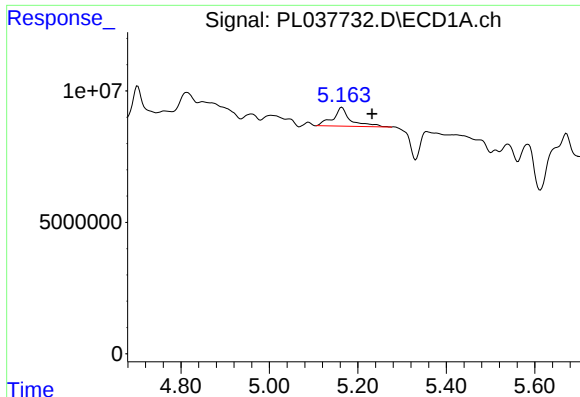

#25 Chlordane-3


R.T.: 5.164 min
Delta R.T.: -0.068 min
Response: 19908669
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

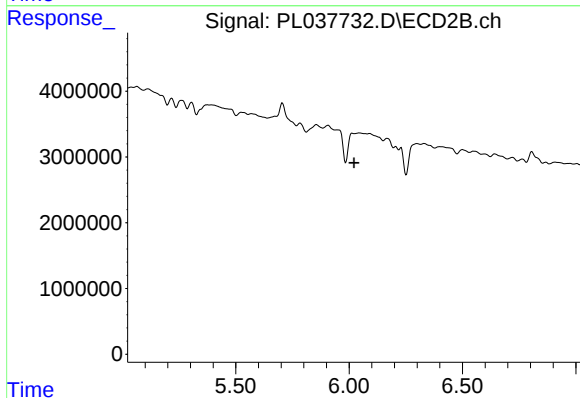


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

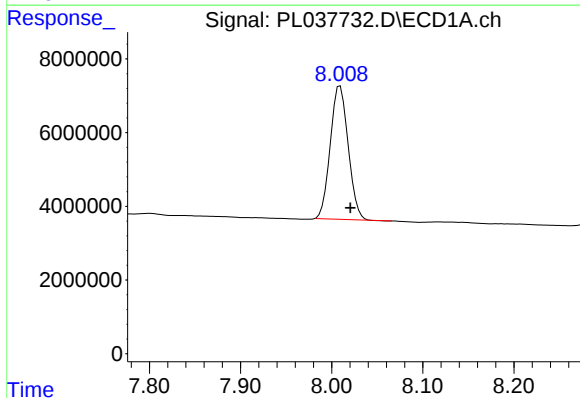

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: -0.011 min
Response: 49426749
Conc: 8.19 ng/ml

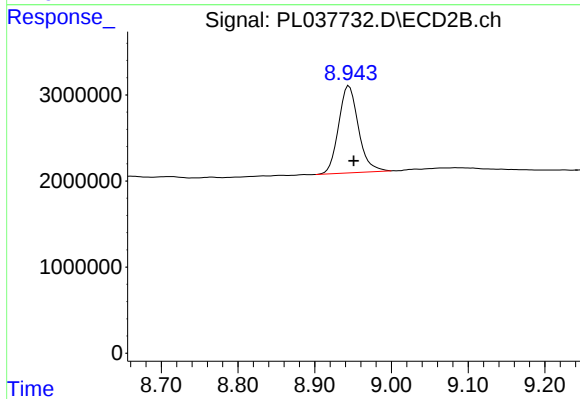

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 18279256
Conc: 9.21 ng/ml