

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
 Data File : PL037727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2018 22:04
 Operator : UA\AJ
 Sample : J3868-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-TP-5-S

Manual Integrations
 APPROVED

Sohil
 7/6/2018 3:09:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 04:42:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	97437395	35693371	12.318	12.901
28)	SA Decachlor...	8.010	8.945	85043484	28492021	14.094	14.361
Target Compounds							
12)	B 4,4'-DDE	5.451	6.249	265.0E6	70858863	30.007	27.846
17)	MA 4,4'-DDT	6.196	7.028	325.5E6	106.0E6	50.417	50.047m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070518\
Data File : PL037727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2018 22:04
Operator : UA\AJ
Sample : J3868-11
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-TP-5-S


Manual Integrations
APPROVED

Sohil
7/6/2018 3:09:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 04:42:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

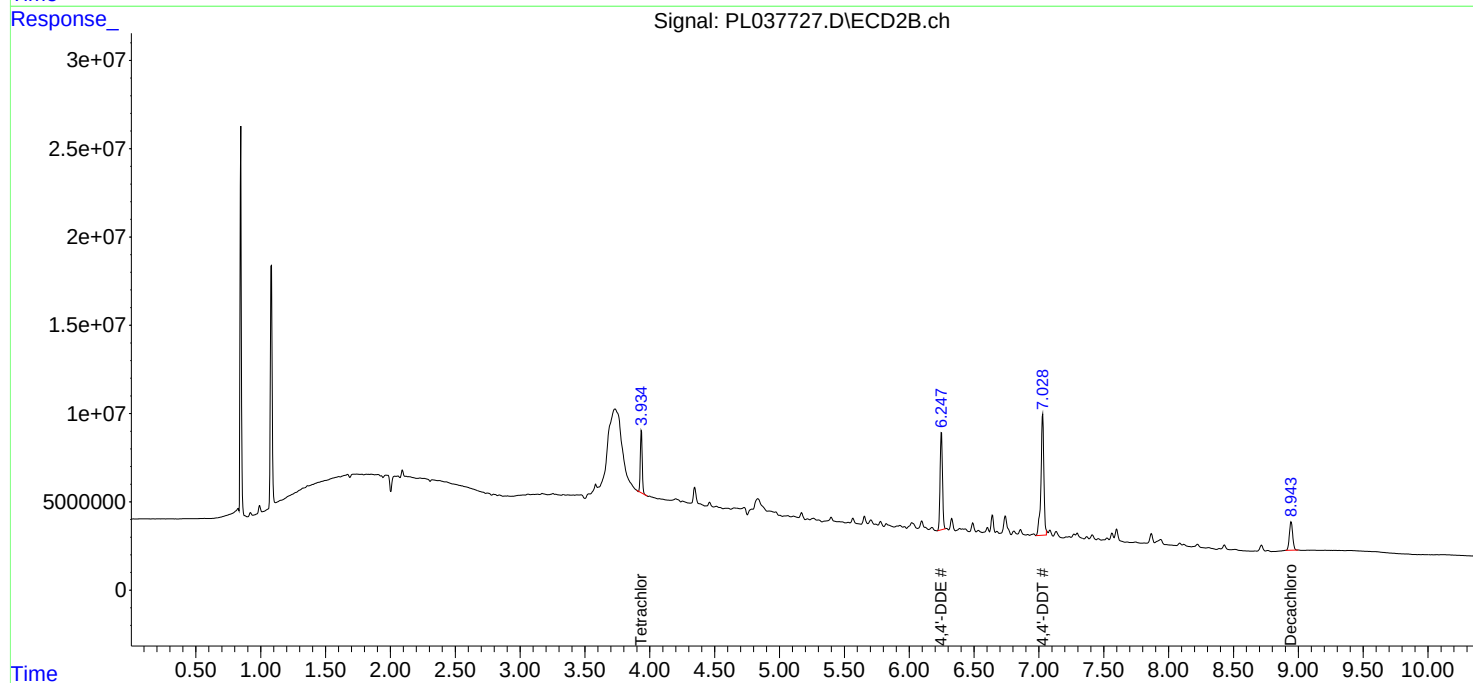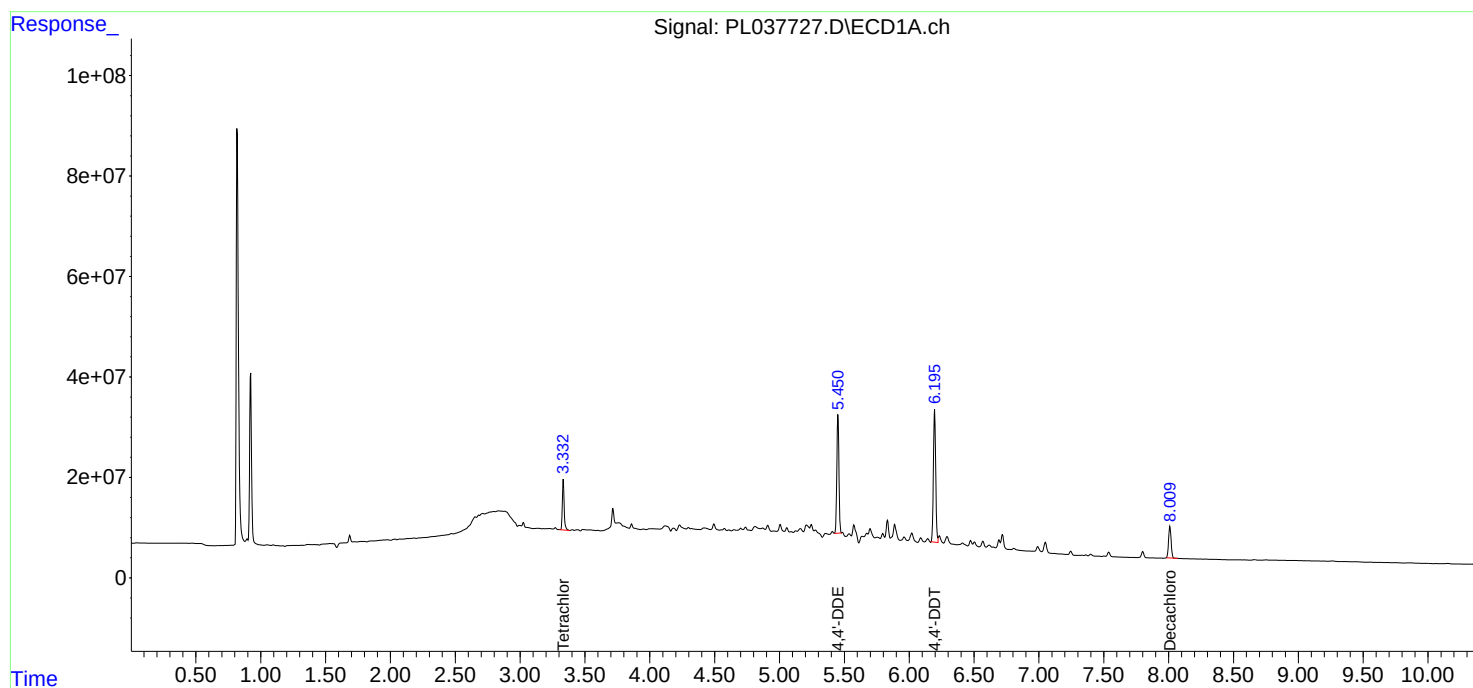

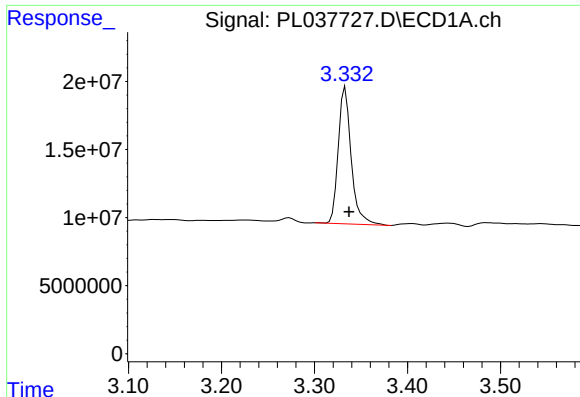


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 97437395
Conc: 12.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-TP-5-S


Manual Integrations
APPROVED

Sohil
7/6/2018 3:09:05 PM

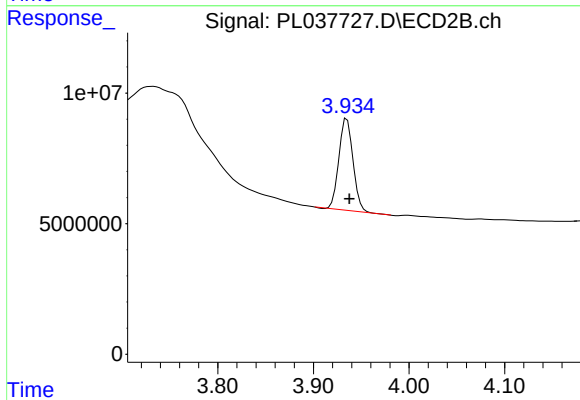


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 35693371
Conc: 12.90 ng/ml

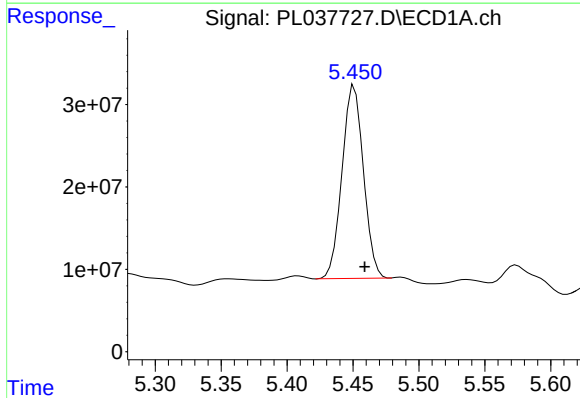


#12 4,4'-DDE

R.T.: 5.451 min
Delta R.T.: -0.008 min
Response: 265034068
Conc: 30.01 ng/ml

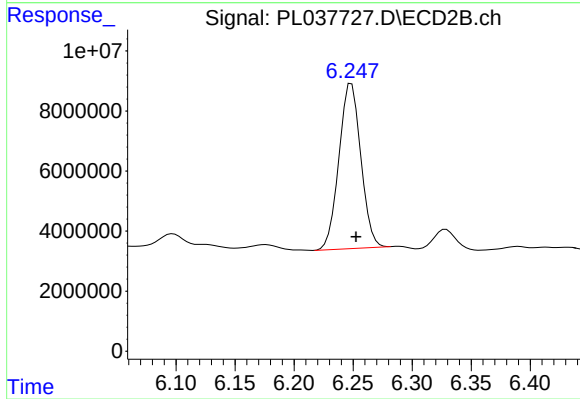

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.004 min
Response: 70858863
Conc: 27.85 ng/ml

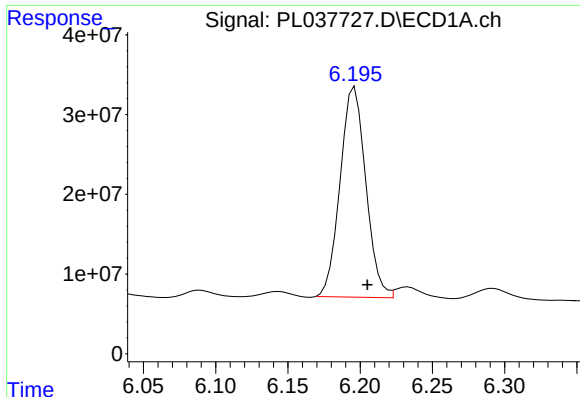


#17 4,4'-DDT

R.T.: 6.196 min
Delta R.T.: -0.009 min
Response: 325508353
Conc: 50.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-TP-5-S


Manual Integrations
APPROVED

Sohil
7/6/2018 3:09:05 PM

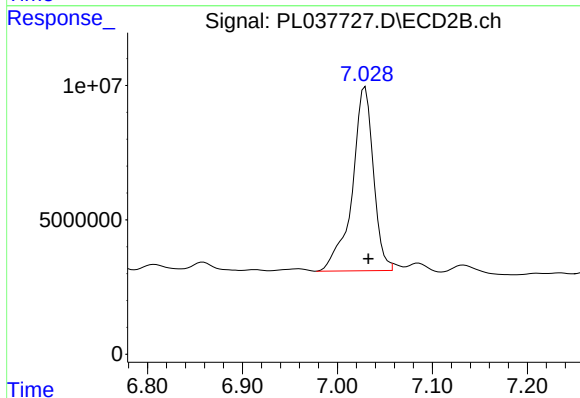


#17 4,4'-DDT

R.T.: 7.028 min
Delta R.T.: -0.005 min
Response: 106008608
Conc: 50.05 ng/ml m

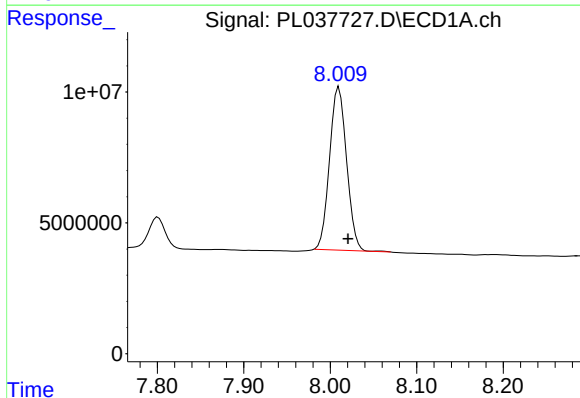

#28 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.011 min
Response: 85043484
Conc: 14.09 ng/ml

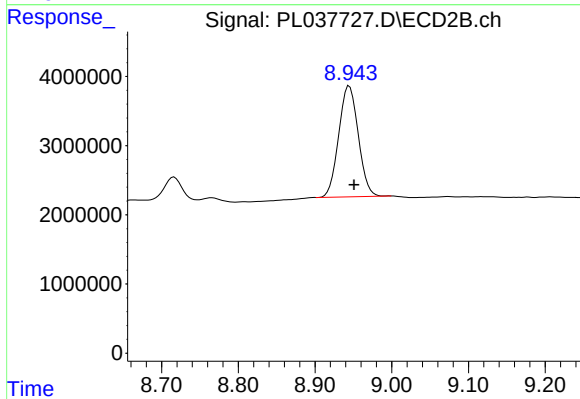

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.006 min
Response: 28492021
Conc: 14.36 ng/ml