

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
 Data File : PL050194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2019 09:44
 Operator : SM\AJ
 Sample : K3622-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 23:04:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.932	158.2E6	37597009	14.029	12.280
28)	SA Decachlor...	7.984	8.963	116.9E6	35486006	9.201	10.571
Target Compounds							
6)	B beta-BHC	0.000	4.798	0	5286675	N.D.	2.729 #
10)	B gamma-Chl...	5.206	6.028	67297340	24387806	3.938	6.545 #
11)	B alpha-Chl...	5.261	6.101	111.5E6	43987078	6.716	11.893 #
15)	B Endosulfa...	6.082	0.000	32045528	0	2.199	N.D. #
24)	Chlordane-2	4.683f	0.000	29880555	0	51.162	N.D. #
25)	Chlordane-3	5.206	6.028	67297340	24387806	35.830	49.008 #
26)	Chlordane-4	5.261	6.101	111.5E6	43987078	63.877	74.010
27)	Chlordane-5	6.082	6.903	32045528	7383497	57.101	65.046



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
Data File : PL050194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2019 09:44
Operator : SM\AJ
Sample : K3622-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 23:04:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

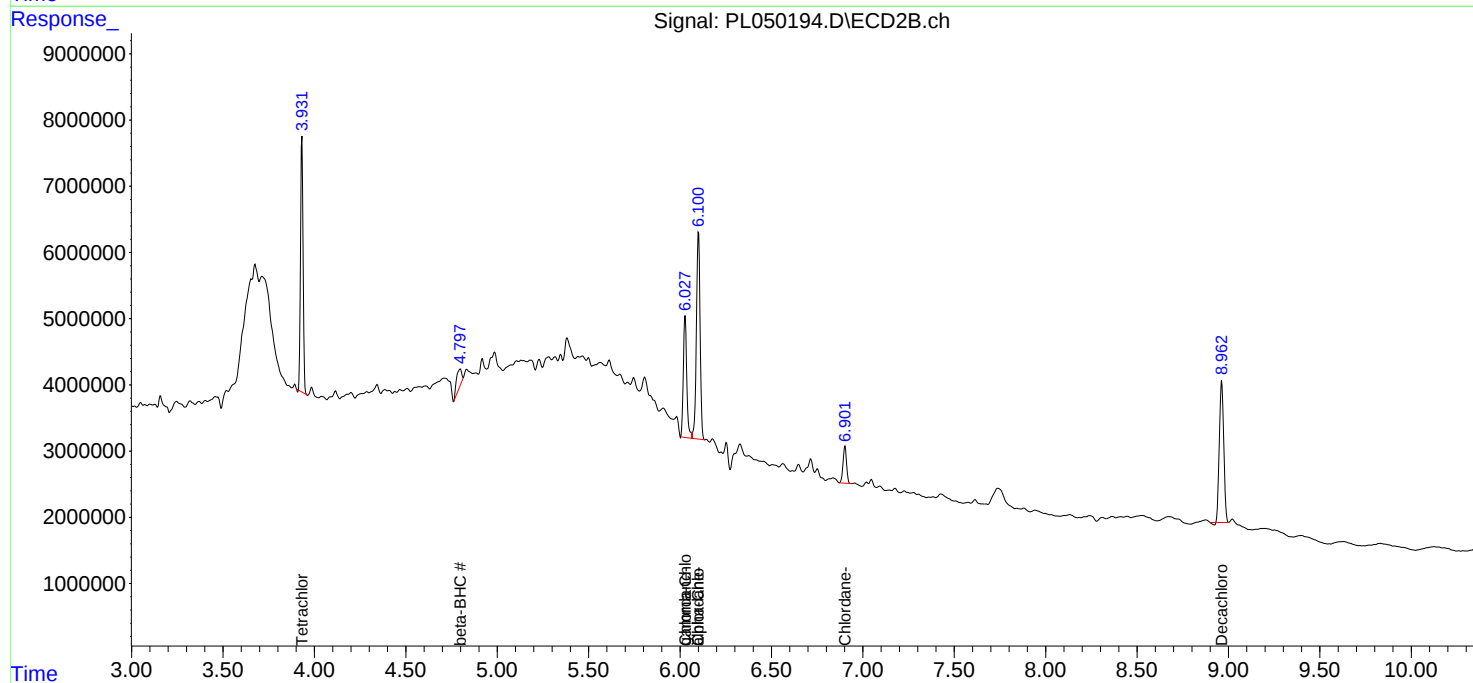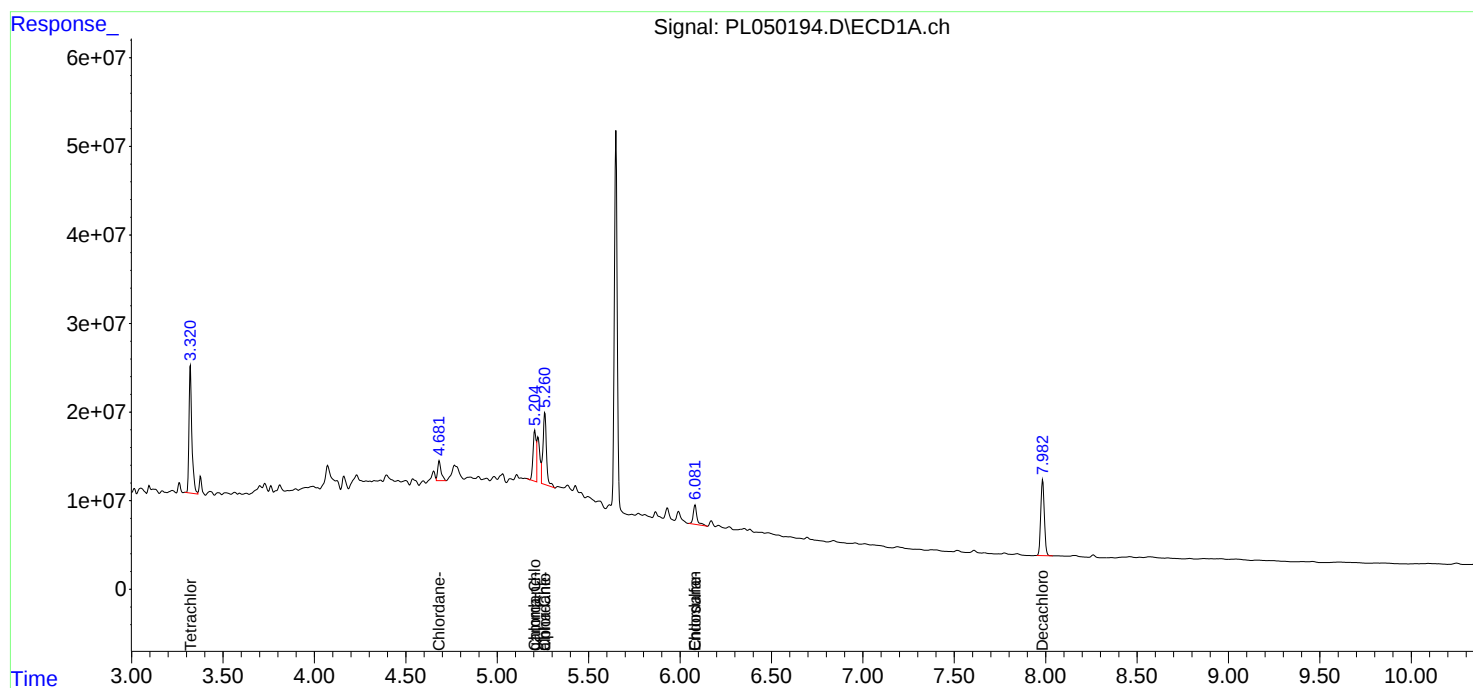


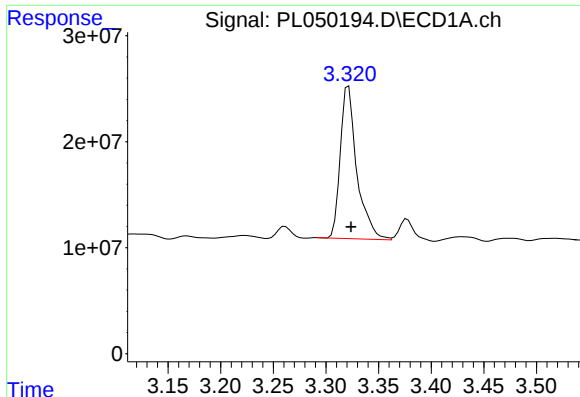

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 158217018
Conc: 14.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

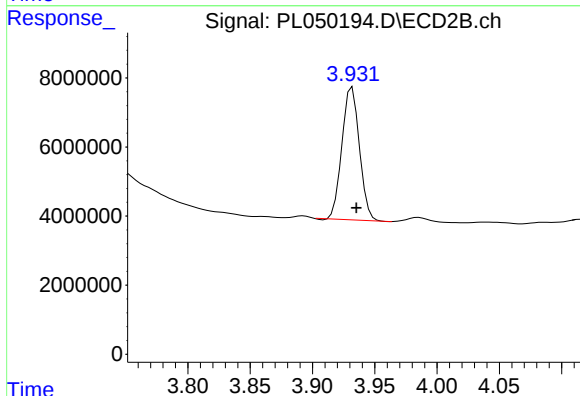


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 37597009
Conc: 12.28 ng/ml

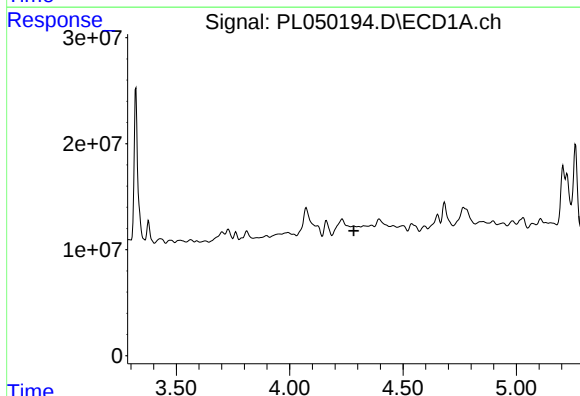


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

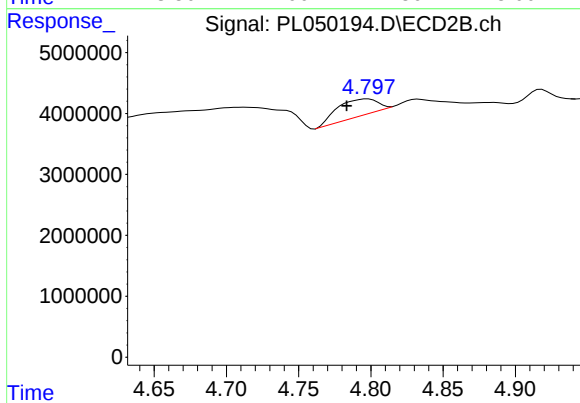

#6 beta-BHC


R.T.: 4.798 min
Delta R.T.: 0.015 min
Response: 5286675
Conc: 2.73 ng/ml

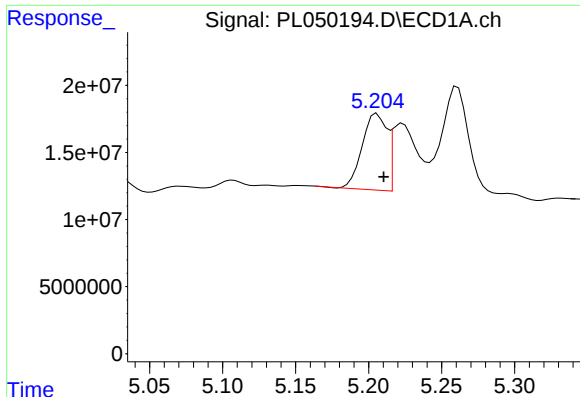

#10 gamma-Chlordane


R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 67297340
Conc: 3.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

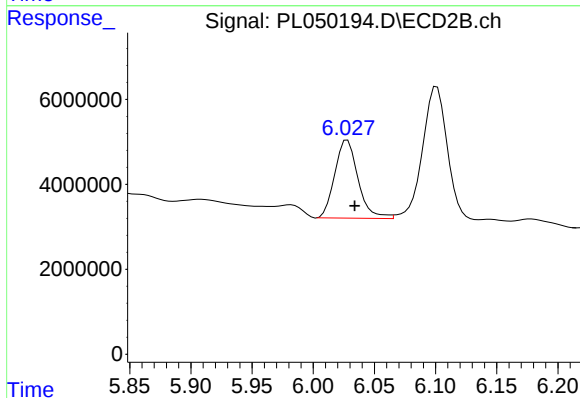


#10 gamma-Chlordane

R.T.: 6.028 min
Delta R.T.: -0.006 min
Response: 24387806
Conc: 6.54 ng/ml

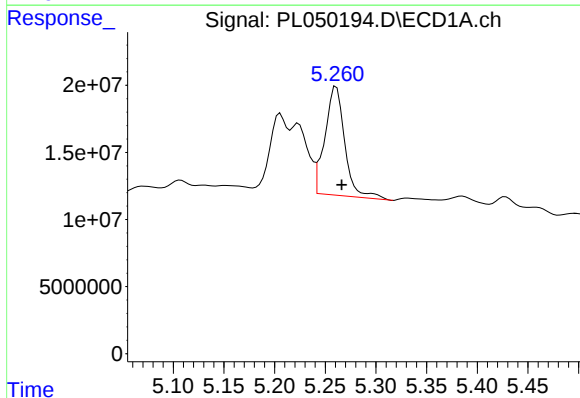


#11 alpha-Chlordane

R.T.: 5.261 min
Delta R.T.: -0.005 min
Response: 111474314
Conc: 6.72 ng/ml

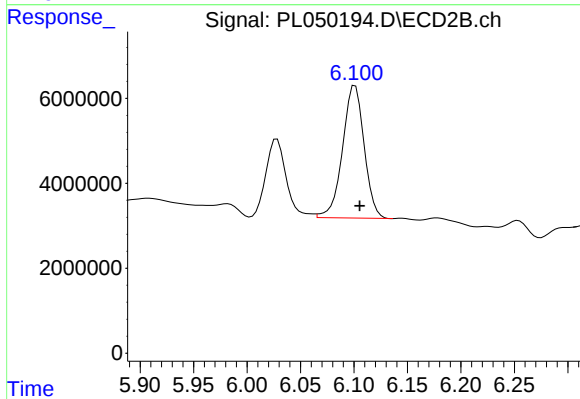

#11 alpha-Chlordane


R.T.: 6.101 min
Delta R.T.: -0.004 min
Response: 43987078
Conc: 11.89 ng/ml

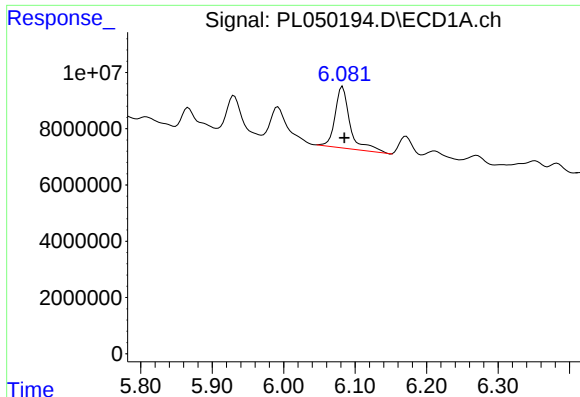

#15 Endosulfan II


R.T.: 6.082 min
Delta R.T.: -0.003 min
Response: 32045528
Conc: 2.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

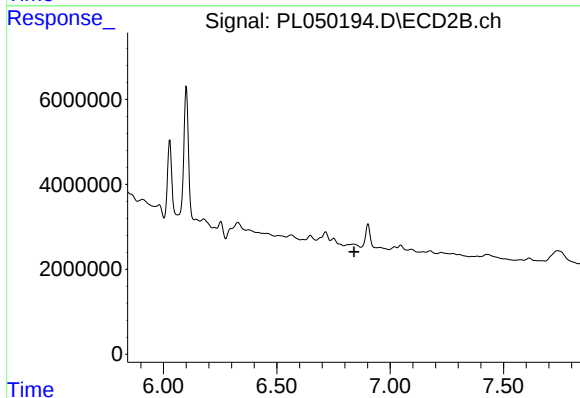


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.841 min
Response: 0
Conc: N.D.

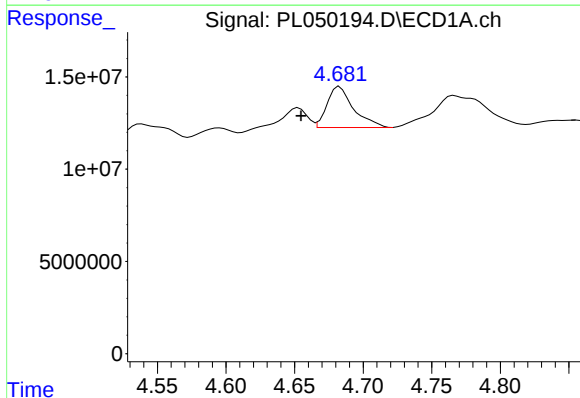


#24 Chlordane-2

R.T.: 4.683 min
Delta R.T.: 0.028 min
Response: 29880555
Conc: 51.16 ng/ml

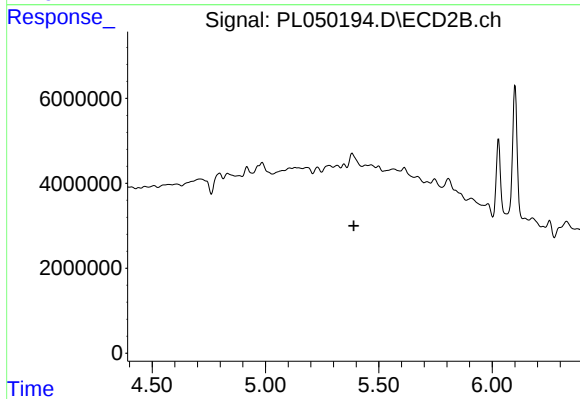

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

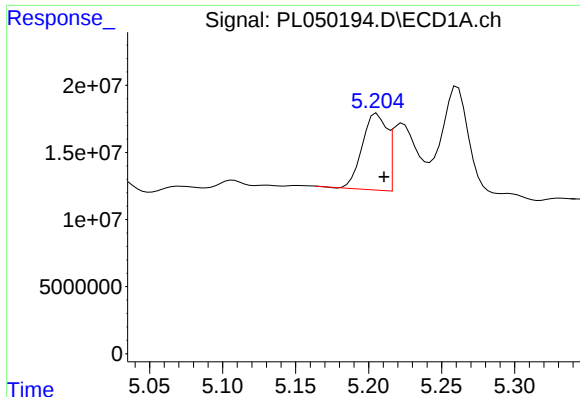

#25 Chlordane-3


R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 67297340
Conc: 35.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

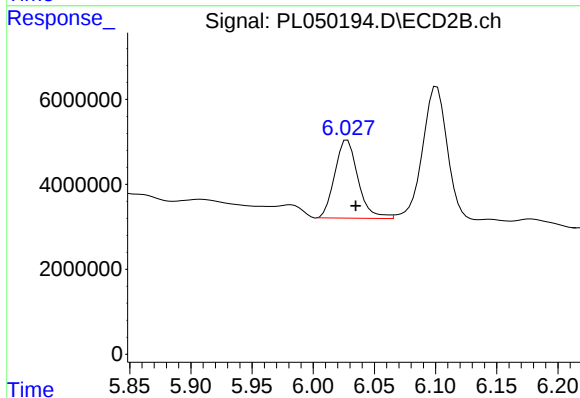


#25 Chlordane-3

R.T.: 6.028 min
Delta R.T.: -0.007 min
Response: 24387806
Conc: 49.01 ng/ml

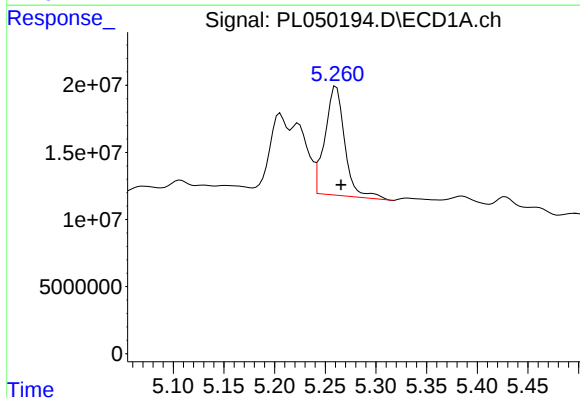


#26 Chlordane-4

R.T.: 5.261 min
Delta R.T.: -0.005 min
Response: 111474314
Conc: 63.88 ng/ml

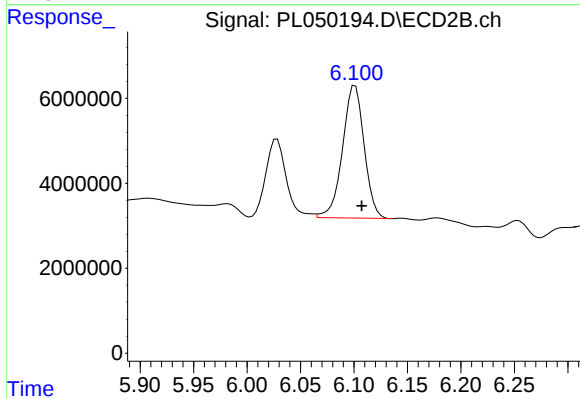

#26 Chlordane-4


R.T.: 6.101 min
Delta R.T.: -0.006 min
Response: 43987078
Conc: 74.01 ng/ml

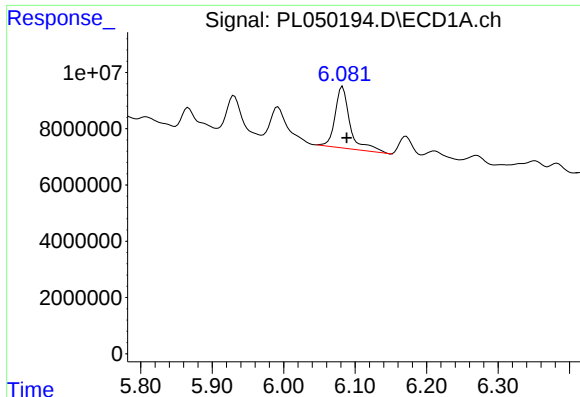

#27 Chlordane-5


R.T.: 6.082 min
Delta R.T.: -0.006 min
Response: 32045528
Conc: 57.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

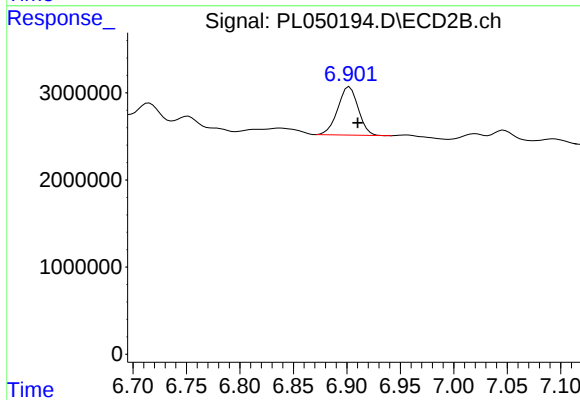


#27 Chlordane-5

R.T.: 6.903 min
Delta R.T.: -0.008 min
Response: 7383497
Conc: 65.05 ng/ml

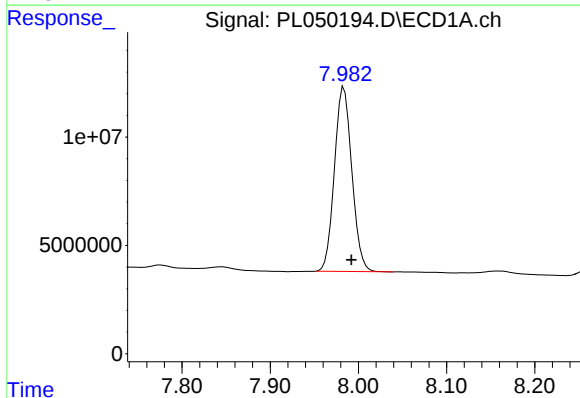

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: -0.008 min
Response: 116910698
Conc: 9.20 ng/ml

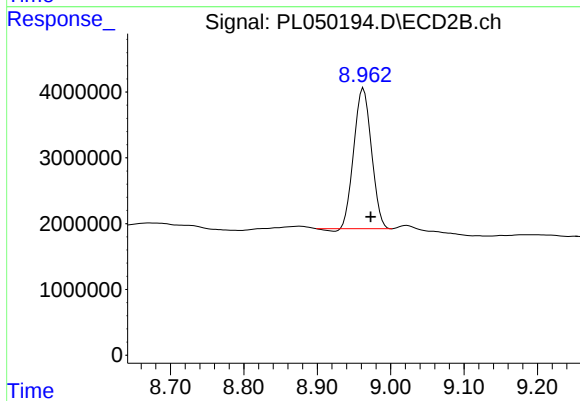

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: -0.010 min
Response: 35486006
Conc: 10.57 ng/ml