

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
 Data File : PL050198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2019 10:43
 Operator : SM\AJ
 Sample : K3624-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 23:05:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.932	169.0E6	41992402	14.988	13.715
28)	SA Decachlor...	7.984	8.962	130.5E6	40135701	10.272	11.956
Target Compounds							
6)	B beta-BHC	0.000	4.797	0	5176285	N.D.	2.672 #
10)	B gamma-Chl...	5.205	6.028	64819181	11231894	3.793	3.014
11)	B alpha-Chl...	5.260	6.101	68906126	14774067	4.151	3.995
12)	B 4,4'-DDE	5.427	0.000	17130763	0	1.028	N.D. #
17)	MA 4,4'-DDT	6.171	0.000	35114455	0	2.645	N.D. #
24)	Chlordane-2	4.654	0.000	25444569	0	43.567	N.D. #
25)	Chlordane-3	5.205	6.028	64819181	11231894	34.511	22.571 #
26)	Chlordane-4	5.260	6.101	68906126	14774067	39.485	24.858 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
Data File : PL050198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2019 10:43
Operator : SM\AJ
Sample : K3624-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 23:05:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

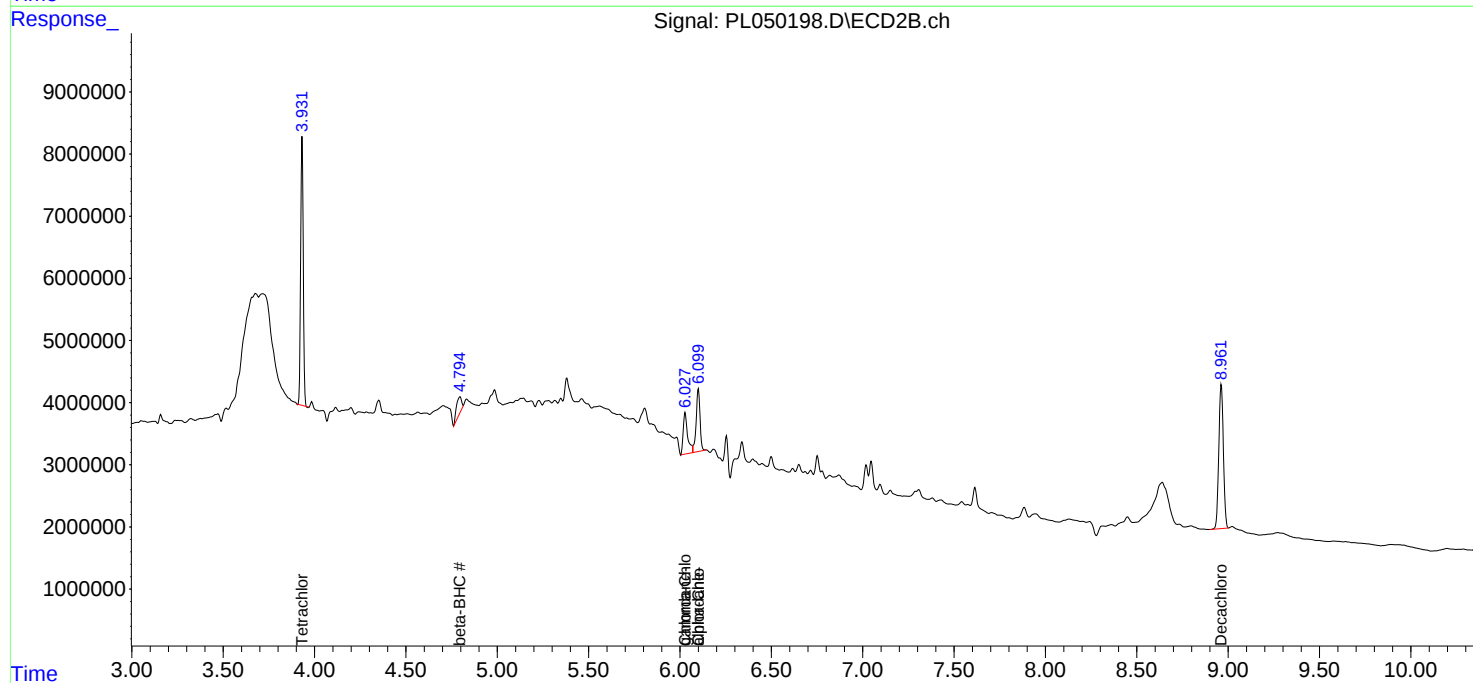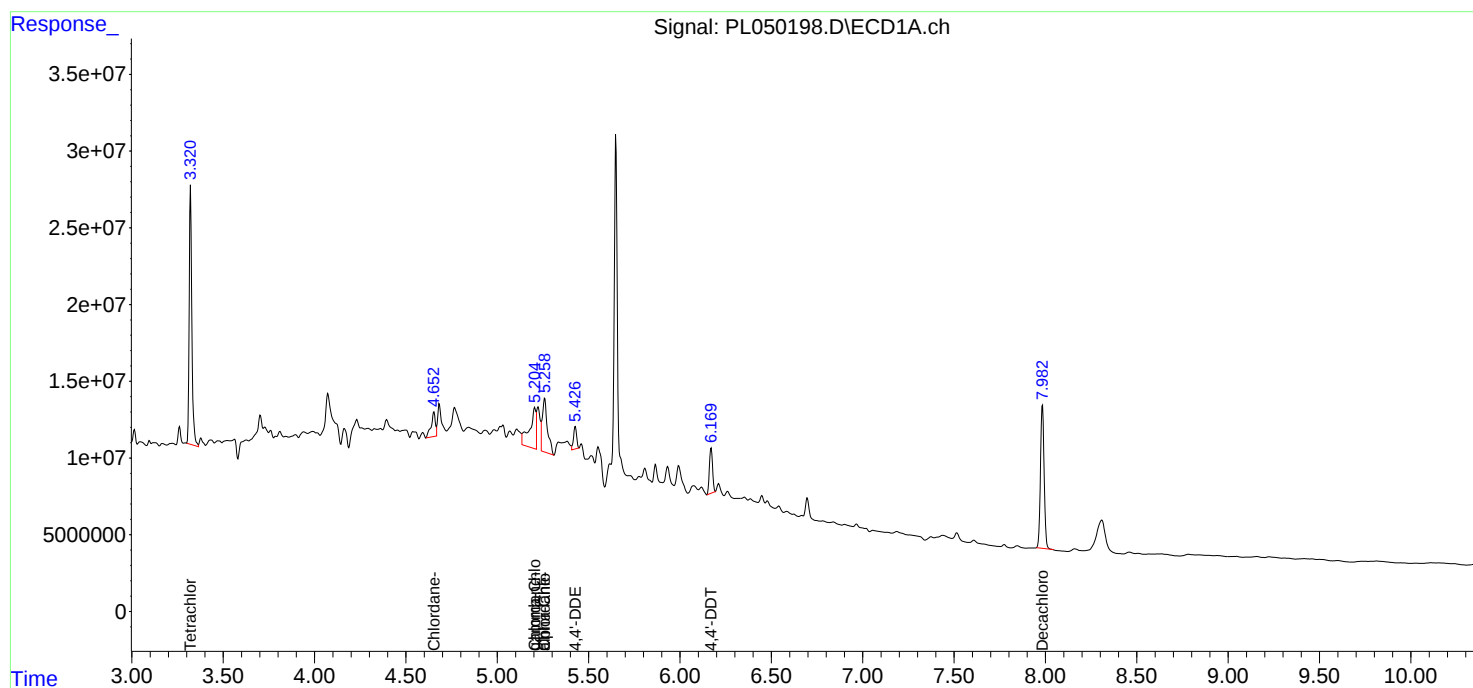


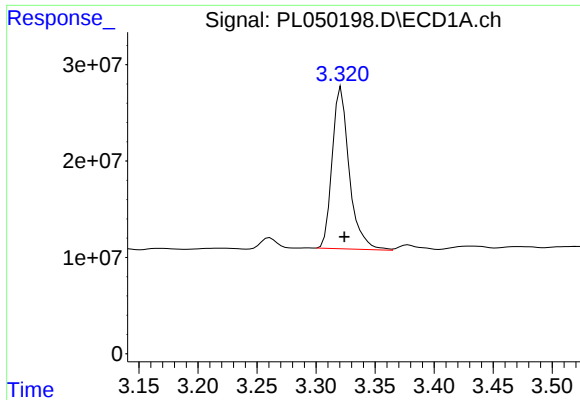

#1 Tetrachloro-m-xylene


R.T.: 3.321 min
Delta R.T.: -0.003 min
Response: 169029340
Conc: 14.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

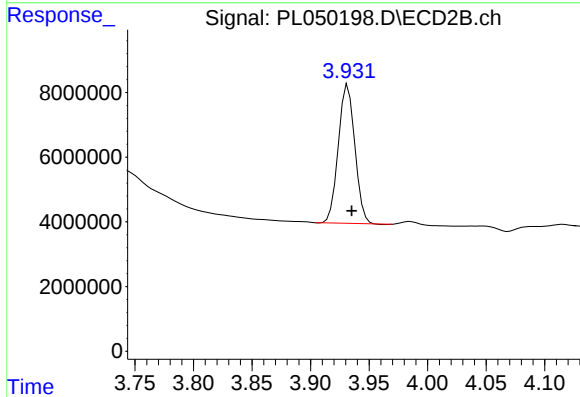


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 41992402
Conc: 13.72 ng/ml

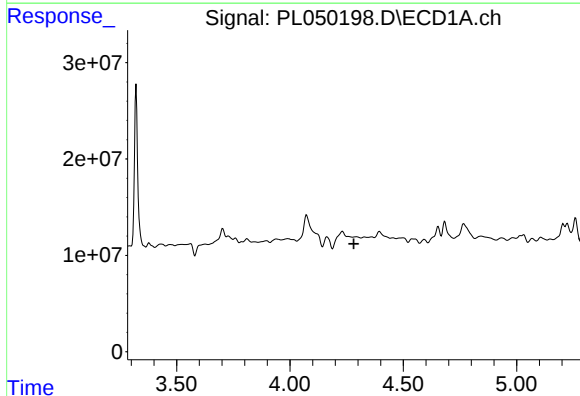


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

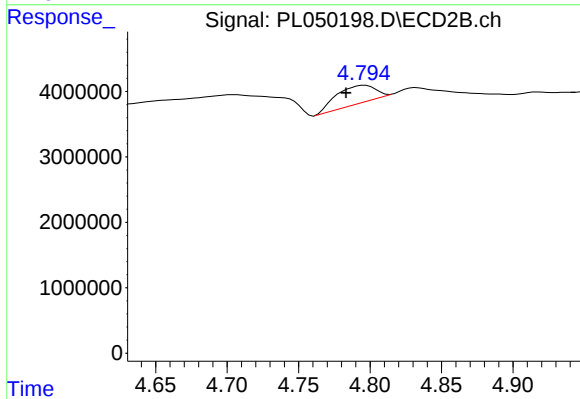

#6 beta-BHC


R.T.: 4.797 min
Delta R.T.: 0.013 min
Response: 5176285
Conc: 2.67 ng/ml

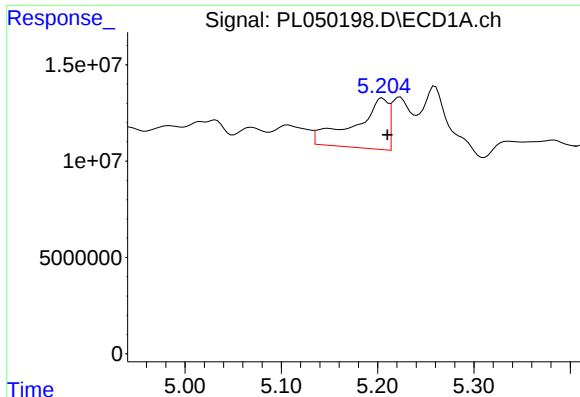

#10 gamma-Chlordane


R.T.: 5.205 min
Delta R.T.: -0.005 min
Response: 64819181
Conc: 3.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

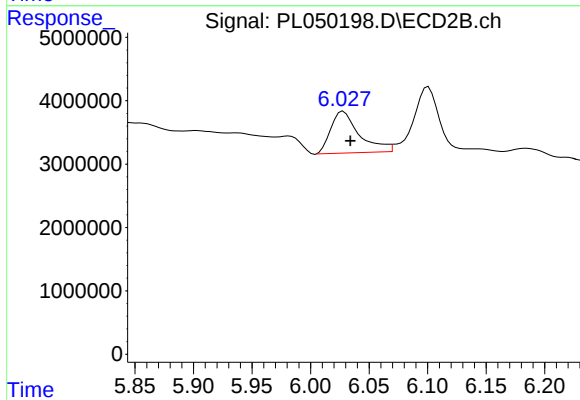


#10 gamma-Chlordane

R.T.: 6.028 min
Delta R.T.: -0.006 min
Response: 11231894
Conc: 3.01 ng/ml

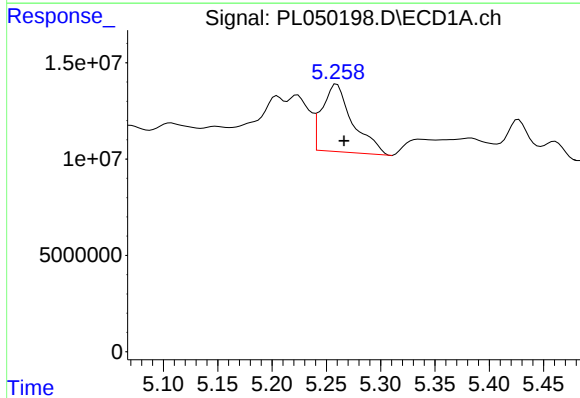


#11 alpha-Chlordane

R.T.: 5.260 min
Delta R.T.: -0.007 min
Response: 68906126
Conc: 4.15 ng/ml

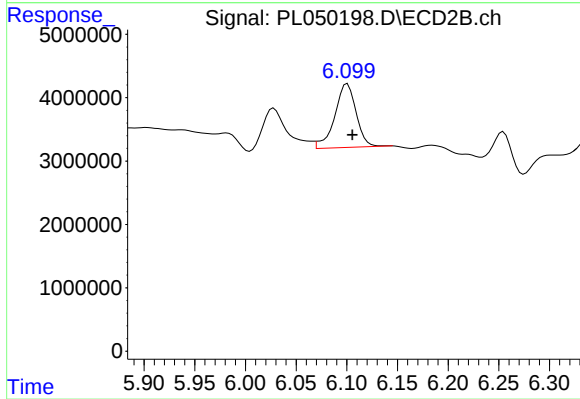

#11 alpha-Chlordane


R.T.: 6.101 min
Delta R.T.: -0.005 min
Response: 14774067
Conc: 3.99 ng/ml

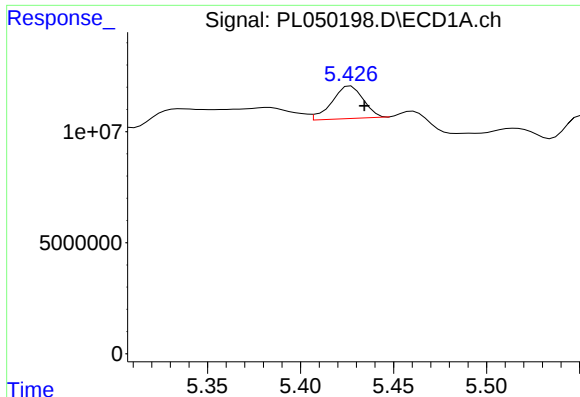

#12 4,4'-DDE


R.T.: 5.427 min
Delta R.T.: -0.007 min
Response: 17130763
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

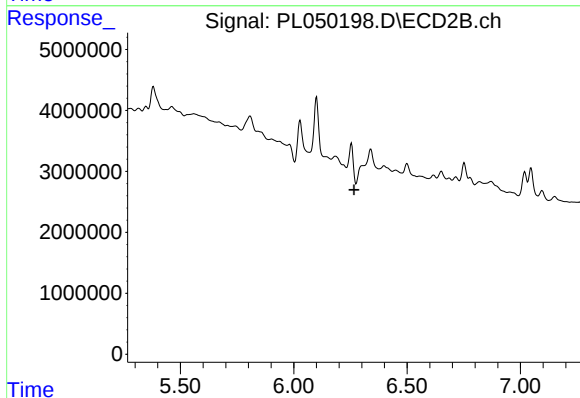


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

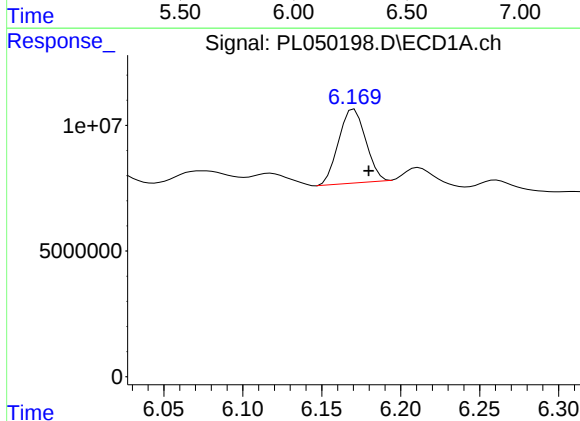


#17 4,4'-DDT

R.T.: 6.171 min
Delta R.T.: -0.009 min
Response: 35114455
Conc: 2.64 ng/ml

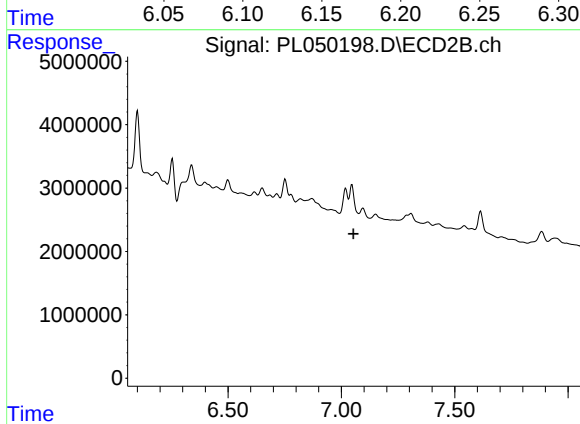

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

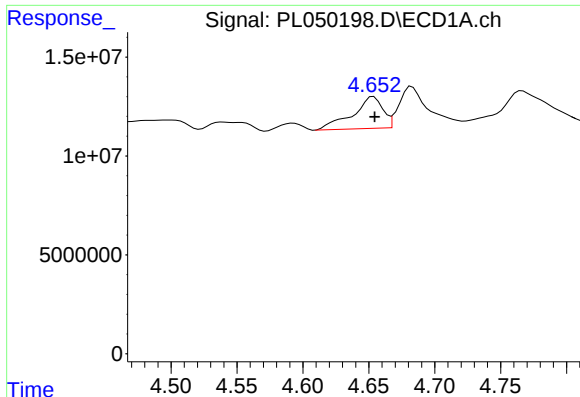

#24 Chlordane-2


R.T.: 4.654 min
Delta R.T.: -0.001 min
Response: 25444569
Conc: 43.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

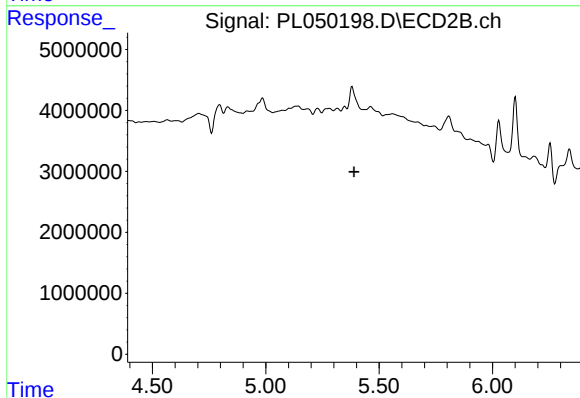


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

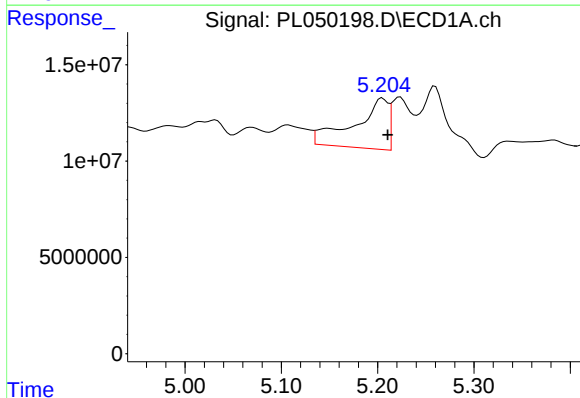


#25 Chlordane-3

R.T.: 5.205 min
Delta R.T.: -0.006 min
Response: 64819181
Conc: 34.51 ng/ml

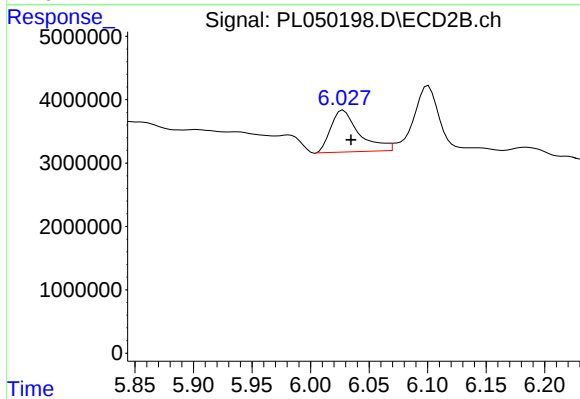

#25 Chlordane-3


R.T.: 6.028 min
Delta R.T.: -0.007 min
Response: 11231894
Conc: 22.57 ng/ml

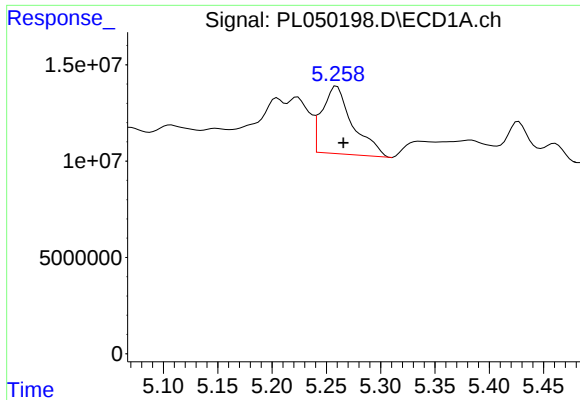

#26 Chlordane-4


R.T.: 5.260 min
Delta R.T.: -0.006 min
Response: 68906126
Conc: 39.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

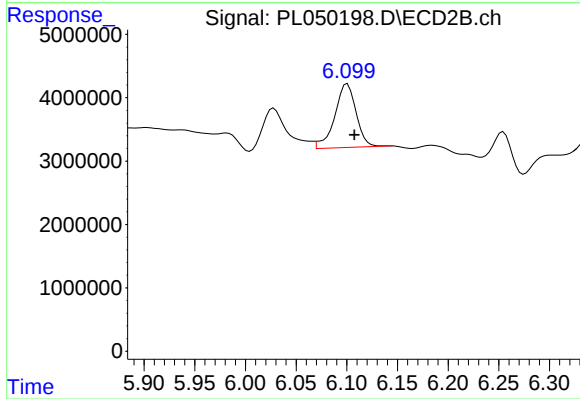


#26 Chlordane-4

R.T.: 6.101 min
Delta R.T.: -0.007 min
Response: 14774067
Conc: 24.86 ng/ml

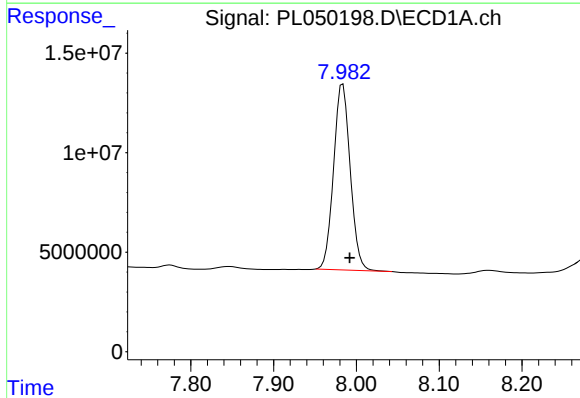

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: -0.008 min
Response: 130517952
Conc: 10.27 ng/ml

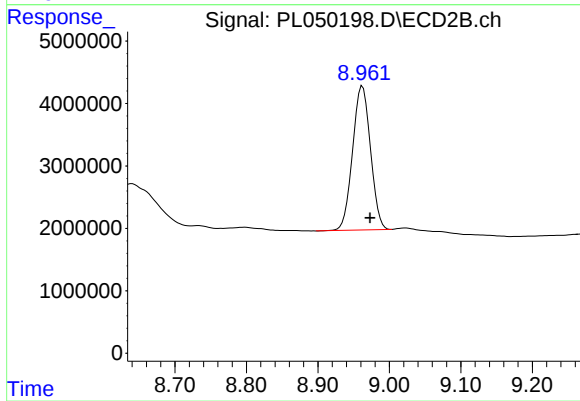

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: -0.011 min
Response: 40135701
Conc: 11.96 ng/ml