

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
 Data File : PL050201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2019 11:56
 Operator : SM\AJ
 Sample : K3668-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TRANSFORMER-T2

Manual Integrations
 APPROVED

Ankita
 7/8/2019 9:58:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 05 23:05:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.933	221.4E6	57939035	19.636m	18.923
28)	SA Decachlor...	7.984	8.963	142.2E6	42035152	11.188	12.521

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070519\
Data File : PL050201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2019 11:56
Operator : SM\AJ
Sample : K3668-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-T2


Manual Integrations
APPROVED

Ankita
7/8/2019 9:58:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 05 23:05:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

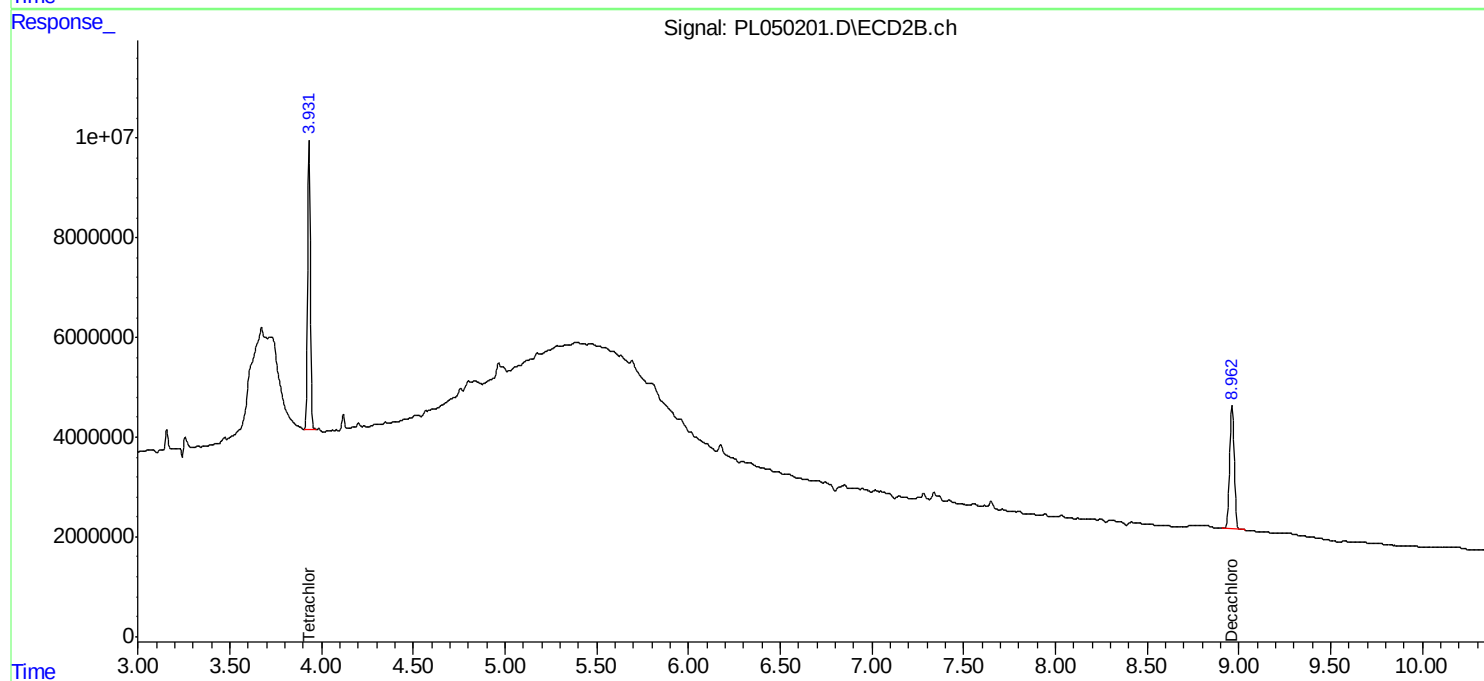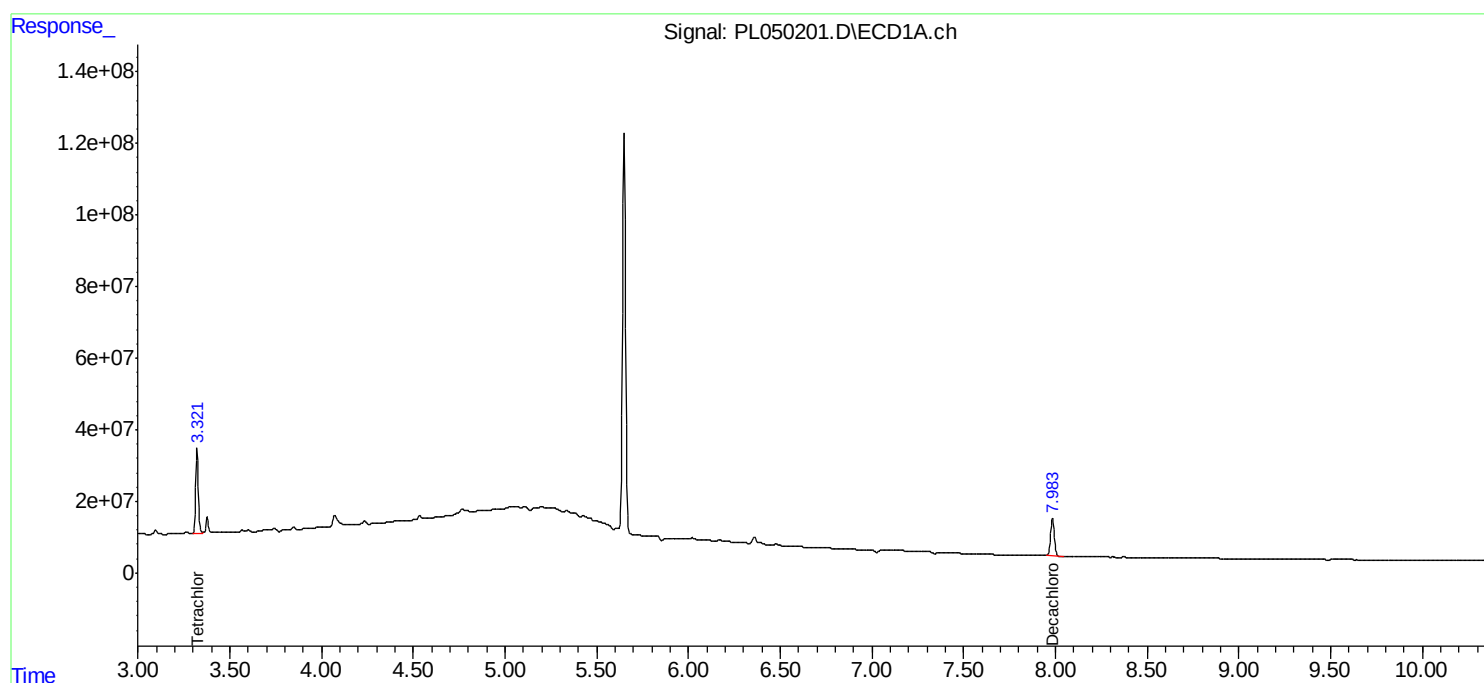

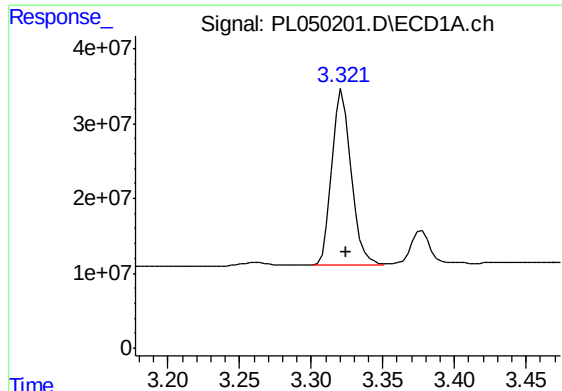


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.003 min
Response: 221447359
Conc: 19.64 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TRANSFORMER-T2


Manual Integrations
APPROVED

Ankita
7/8/2019 9:58:51 AM

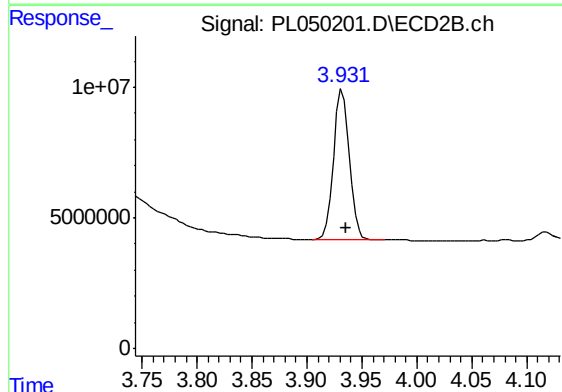


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 57939035
Conc: 18.92 ng/ml

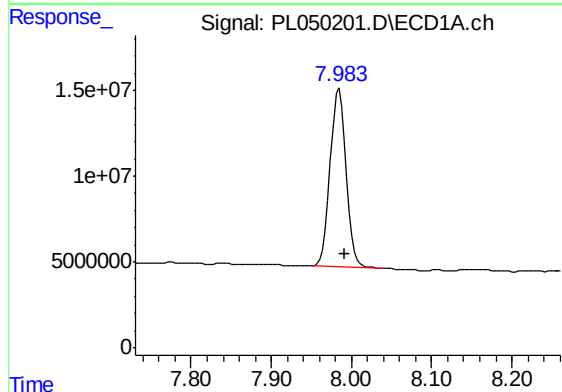

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: -0.008 min
Response: 142157144
Conc: 11.19 ng/ml

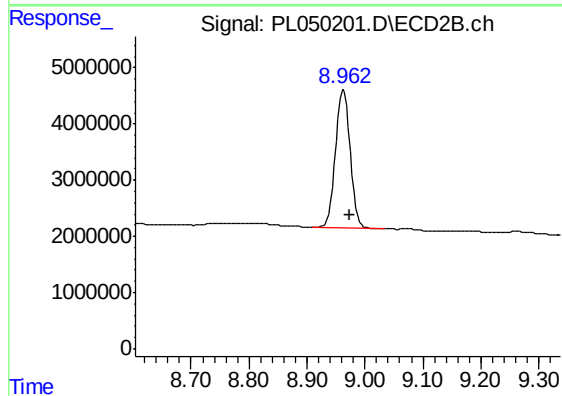

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: -0.010 min
Response: 42035152
Conc: 12.52 ng/ml