

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070522\
 Data File : PL076246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 12:46
 Operator : AR\AJ
 Sample : N3564-26 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-16-2-4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/06/2022
 Supervised By : Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 02:52:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.635	4.626	1589732	5281699	2.102m	2.785 #
28)	SA Decachlor...	11.628	10.361	3242617	5082116	5.153	3.309 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070522\
Data File : PL076246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 12:46
Operator : AR\AJ
Sample : N3564-26 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-16-2-4


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/06/2022
Supervised By : Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 02:52:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

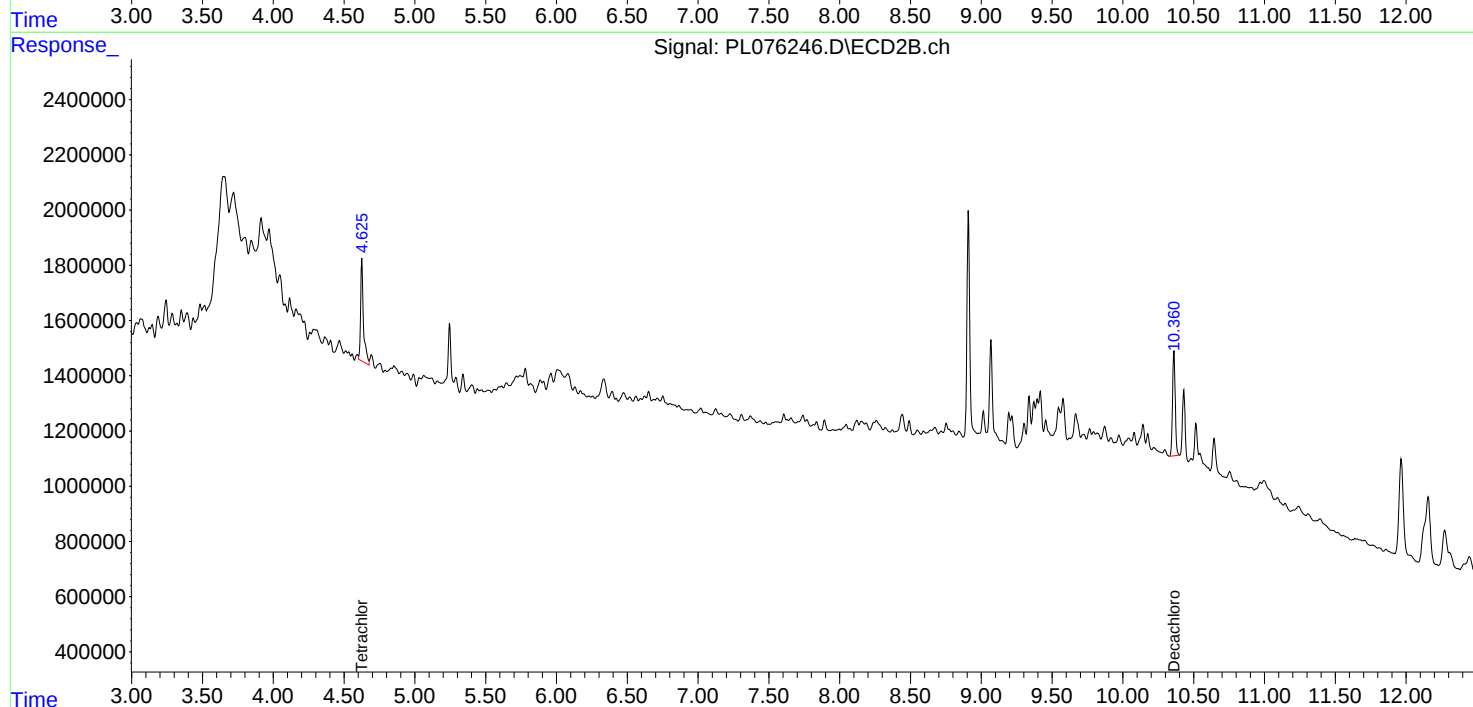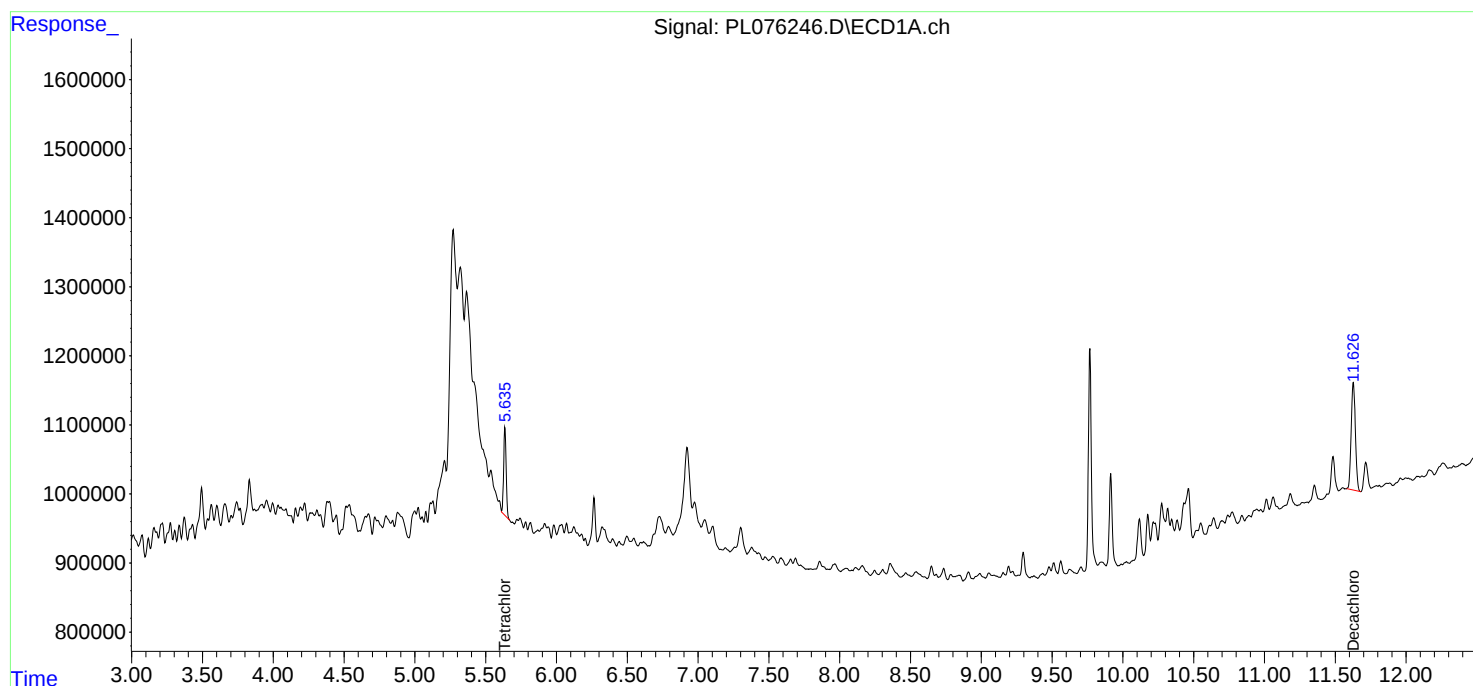

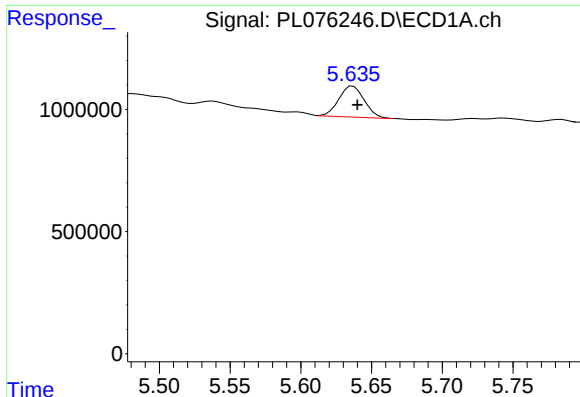


#1 Tetrachloro-m-xylene

R.T.: 5.635 min
Delta R.T.: -0.005 min
Response: 1589732
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-16-2-4


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/06/2022
Supervised By :Ankita Jodhani 07/06/2022

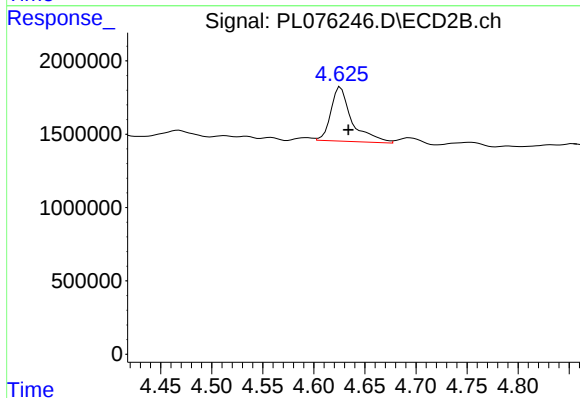


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.008 min
Response: 5281699
Conc: 2.78 ng/ml

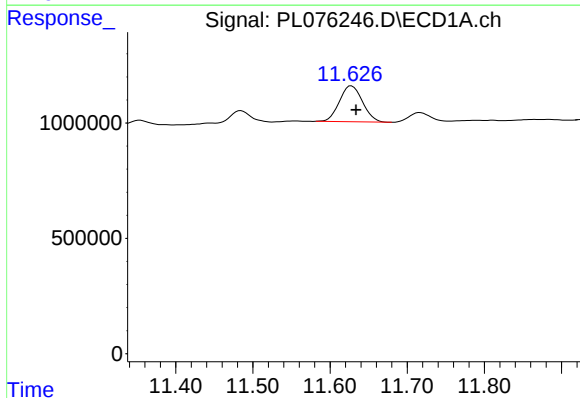

#28 Decachlorobiphenyl

R.T.: 11.628 min
Delta R.T.: -0.006 min
Response: 3242617
Conc: 5.15 ng/ml

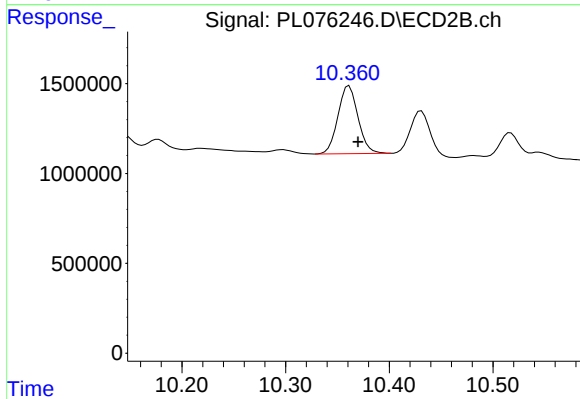

#28 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.009 min
Response: 5082116
Conc: 3.31 ng/ml