

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070522\
 Data File : PL076249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 13:36
 Operator : AR\AJ
 Sample : N3564-16 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-16-2-6

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/06/2022
 Supervised By :Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 02:53:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.634	4.625	887562	2379118	1.174m	1.254
2) SA Decachlor...	11.624	10.361	1421024	3749349	2.258	2.441

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070522\
Data File : PL076249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 13:36
Operator : AR\AJ
Sample : N3564-16 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-16-2-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/06/2022
Supervised By : Ankita Jodhani 07/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 02:53:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

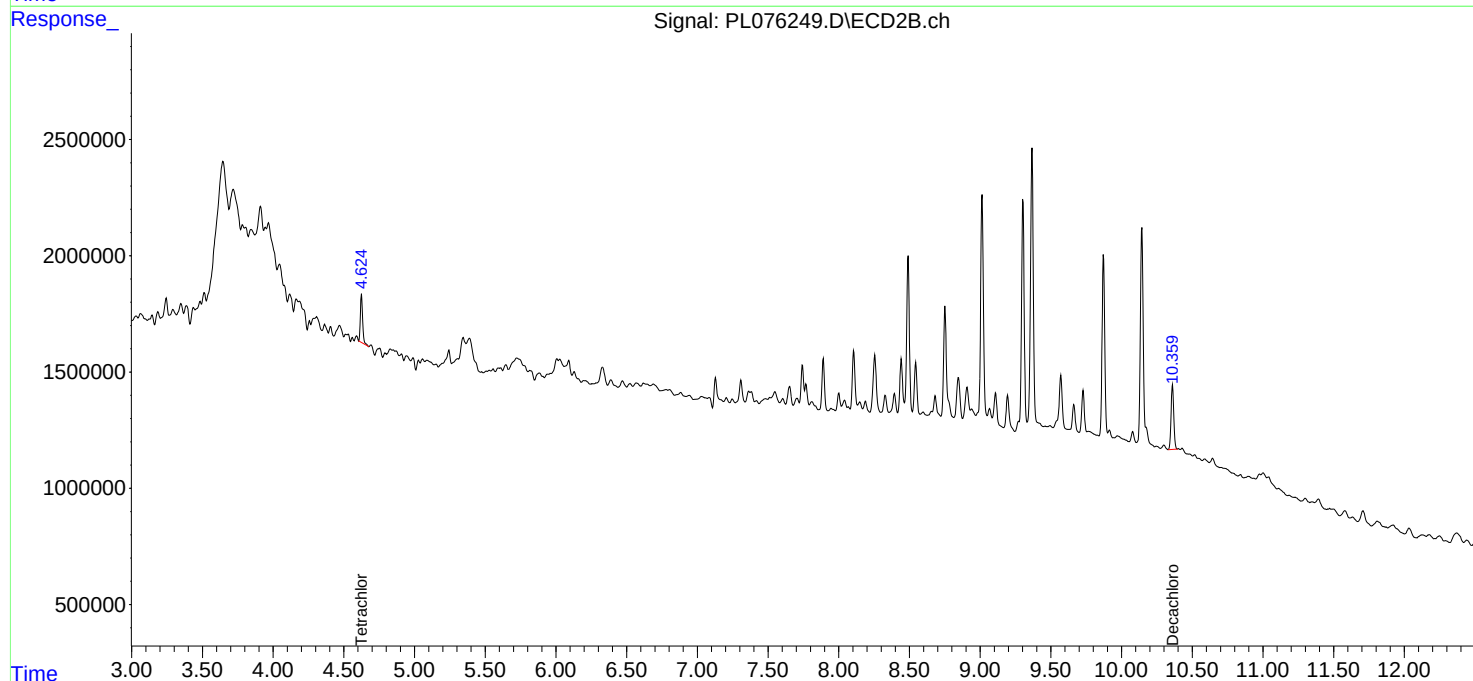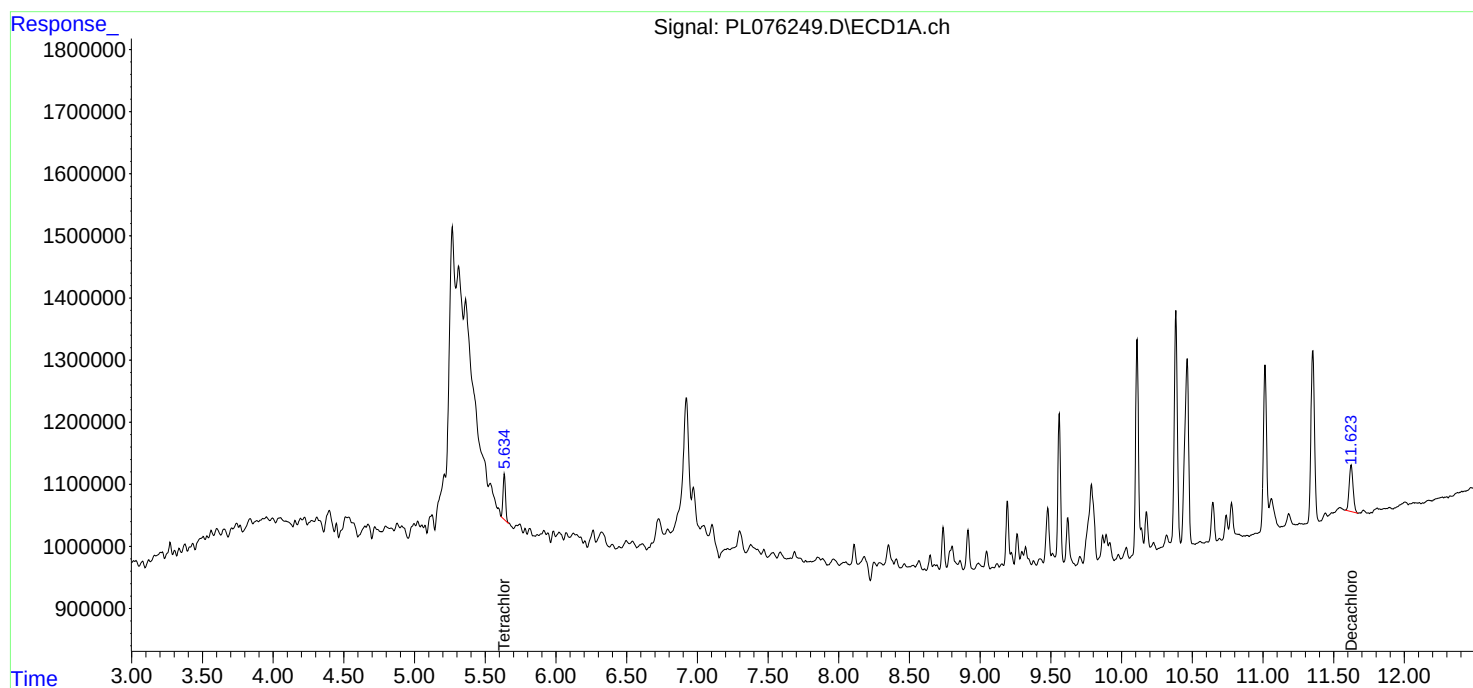

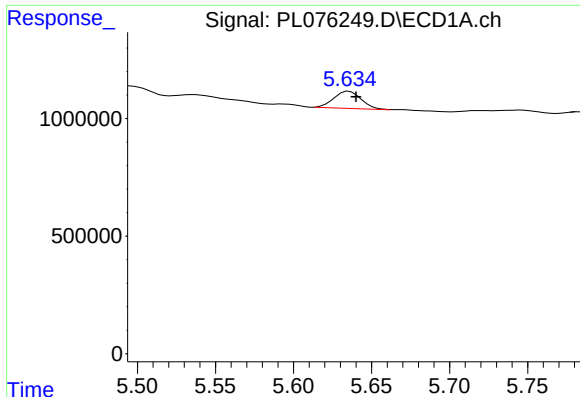


#1 Tetrachloro-m-xylene

R.T.: 5.634 min
Delta R.T.: -0.006 min
Response: 887562
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-16-2-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/06/2022
Supervised By :Ankita Jodhani 07/06/2022

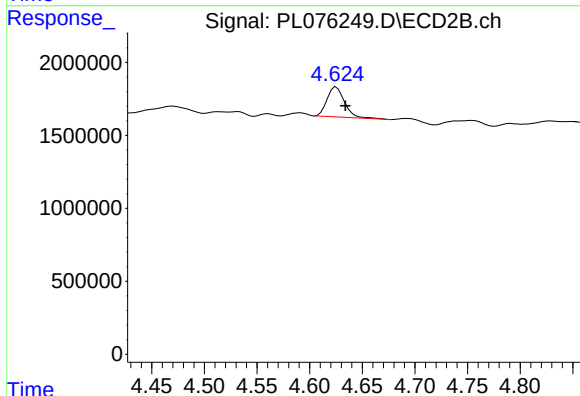


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.009 min
Response: 2379118
Conc: 1.25 ng/ml

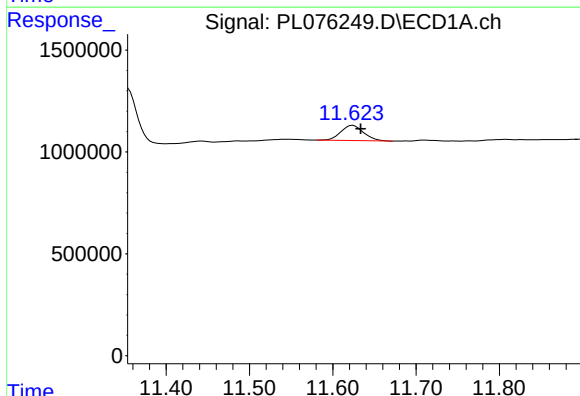

#28 Decachlorobiphenyl

R.T.: 11.624 min
Delta R.T.: -0.010 min
Response: 1421024
Conc: 2.26 ng/ml

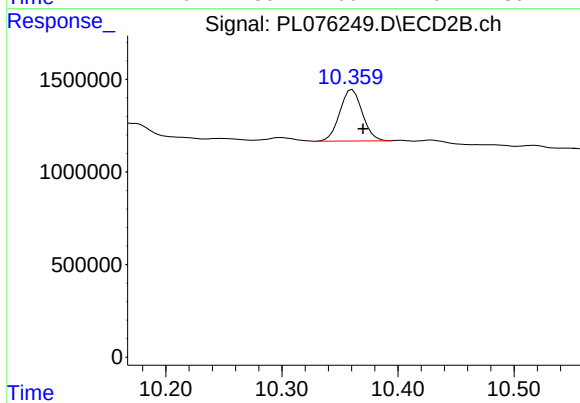

#28 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.009 min
Response: 3749349
Conc: 2.44 ng/ml