

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 16:45
 Operator : AJ\MA
 Sample : J3874-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:33:58 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	62891916	23199983	7.951	8.385
28)	SA Decachlor...	8.011	8.947	40155439	14589317	6.655	7.354
Target Compounds							
24)	Chlordane-2	4.698	0.000	16294592	0	45.771	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 16:45
Operator : AJ\MA
Sample : J3874-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:33:58 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

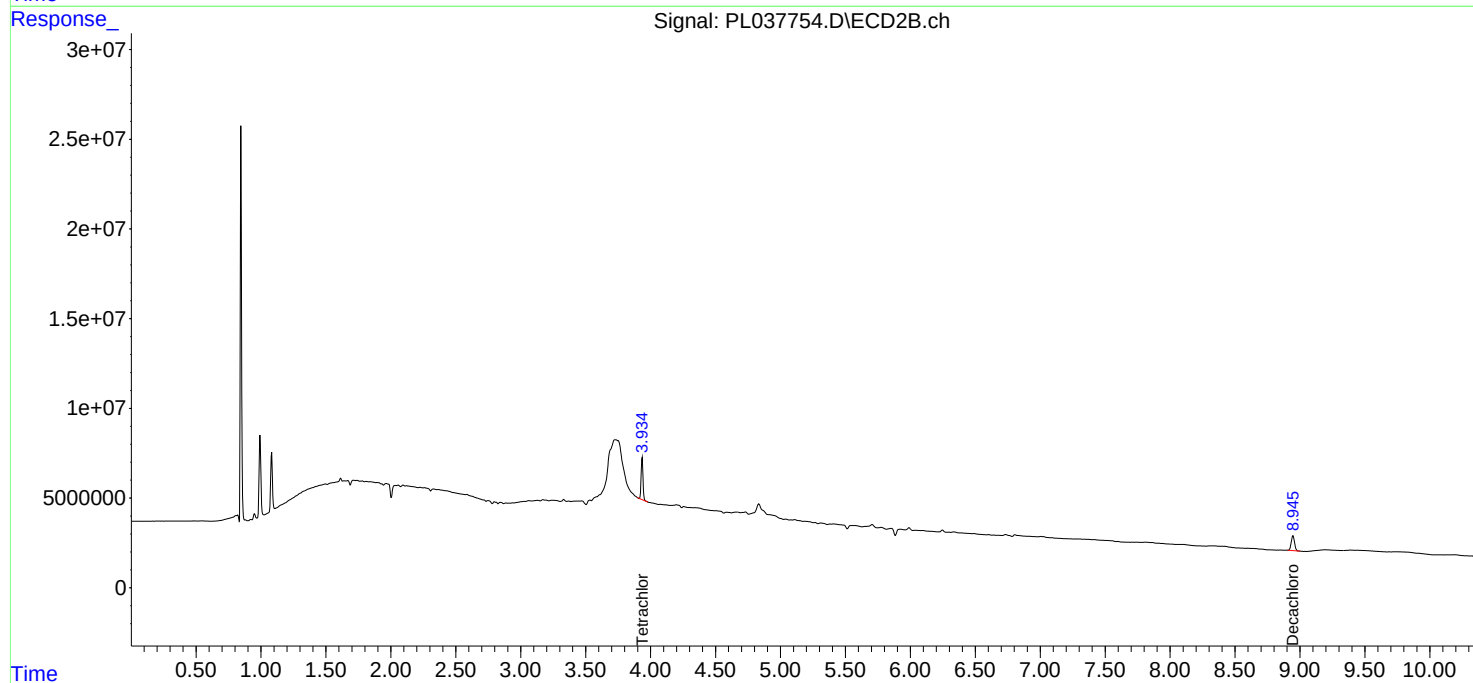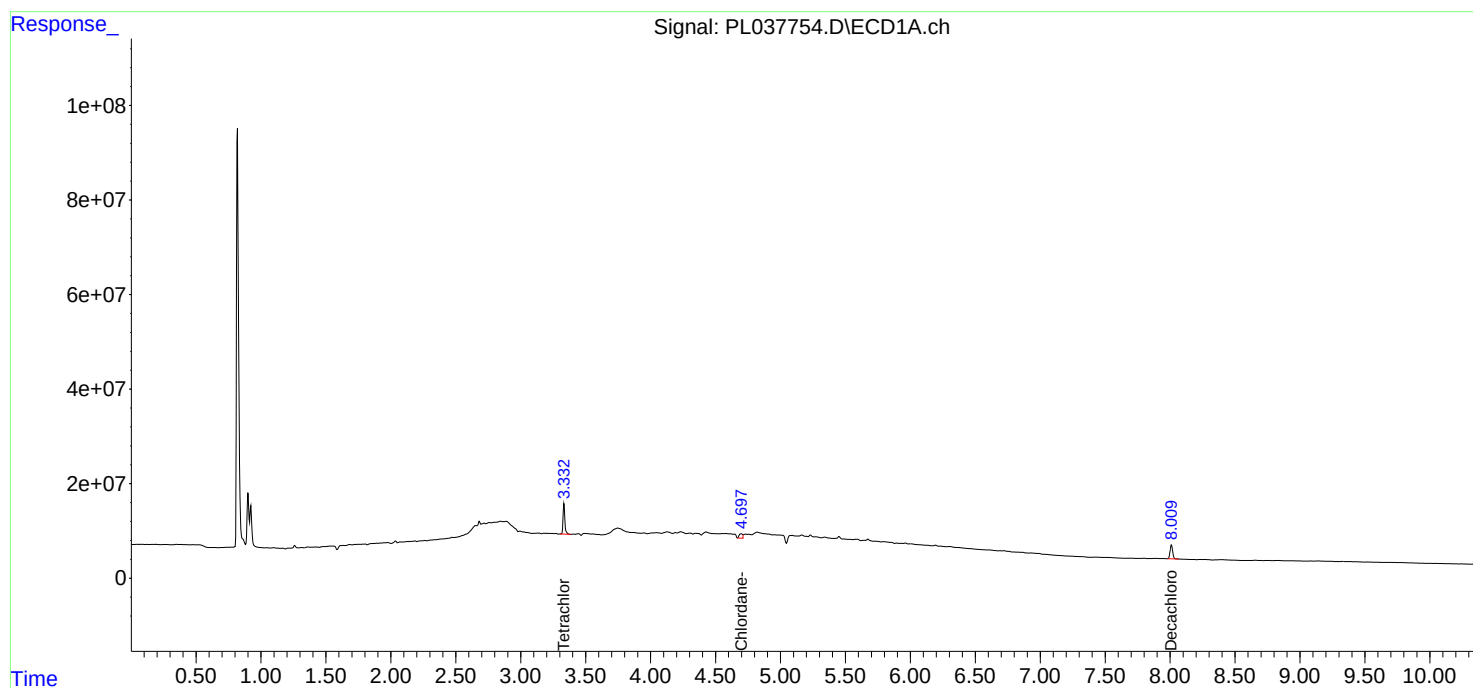


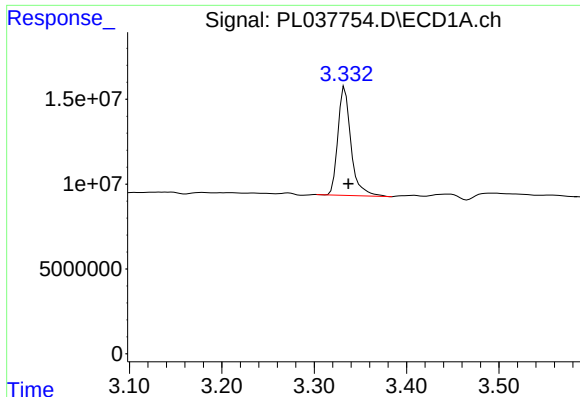

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 62891916
Conc: 7.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

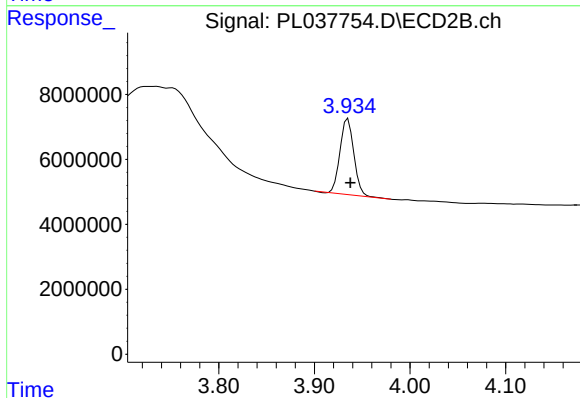


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 23199983
Conc: 8.39 ng/ml

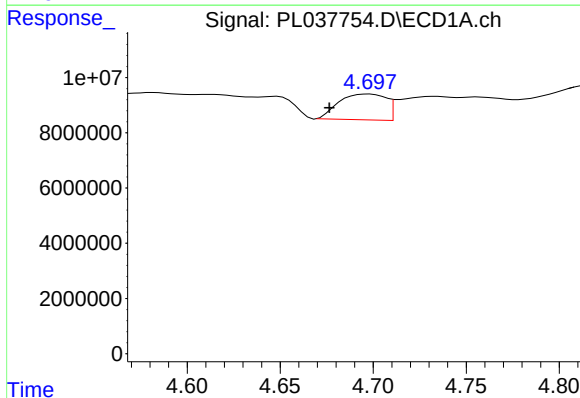


#24 Chlordane-2

R.T.: 4.698 min
Delta R.T.: 0.022 min
Response: 16294592
Conc: 45.77 ng/ml

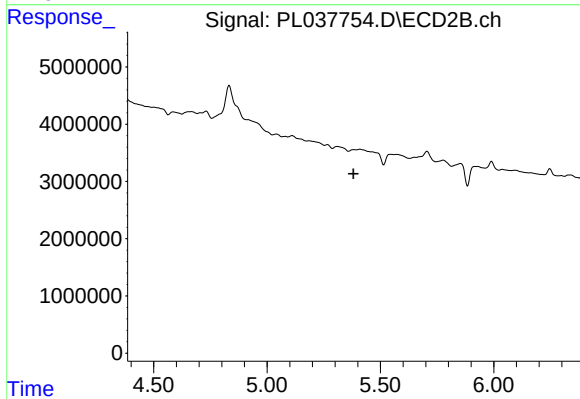

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

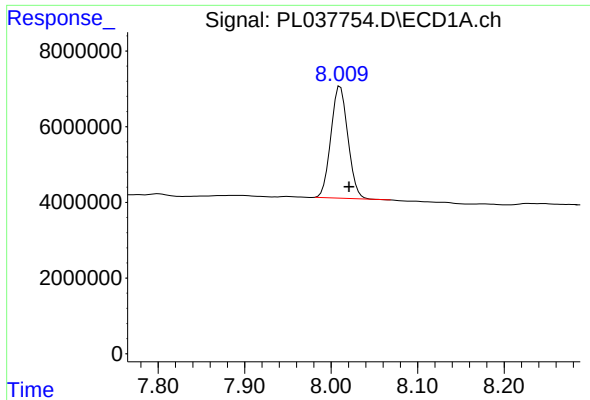

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.010 min
Response: 40155439
Conc: 6.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

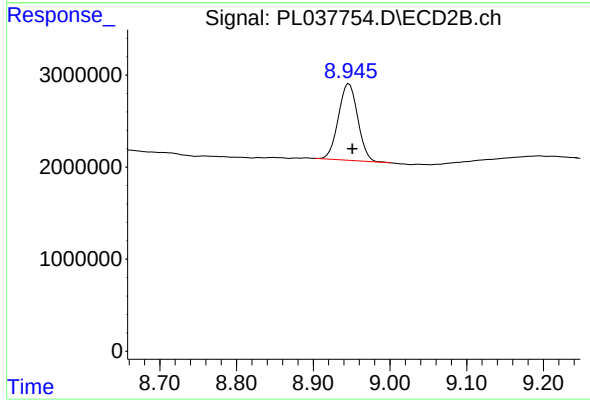

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 14589317
Conc: 7.35 ng/ml