

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 17:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:35:03 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.936	132.7E6	50365215	16.776	18.204
28)	SA Decachlor...	8.011	8.946	125.4E6	44832160	20.783	22.597
Target Compounds							
8)	B Heptachlo...	0.000	5.780	0	24072198	N.D.	8.444 #
13)	MA Dieldrin	5.537f	0.000	9320132	0	1.053	N.D. #
14)	MA Endrin	5.847	0.000	29461808	0	3.740	N.D. #
21)	B Endrin ke...	6.932f	0.000	436.6E6	0	61.386	N.D. #
23)	Chlordane-1	4.120	0.000	12242046	0	39.870	N.D. #
27)	Chlordane-5	5.847	0.000	29461808	0	225.126	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 17:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:35:03 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

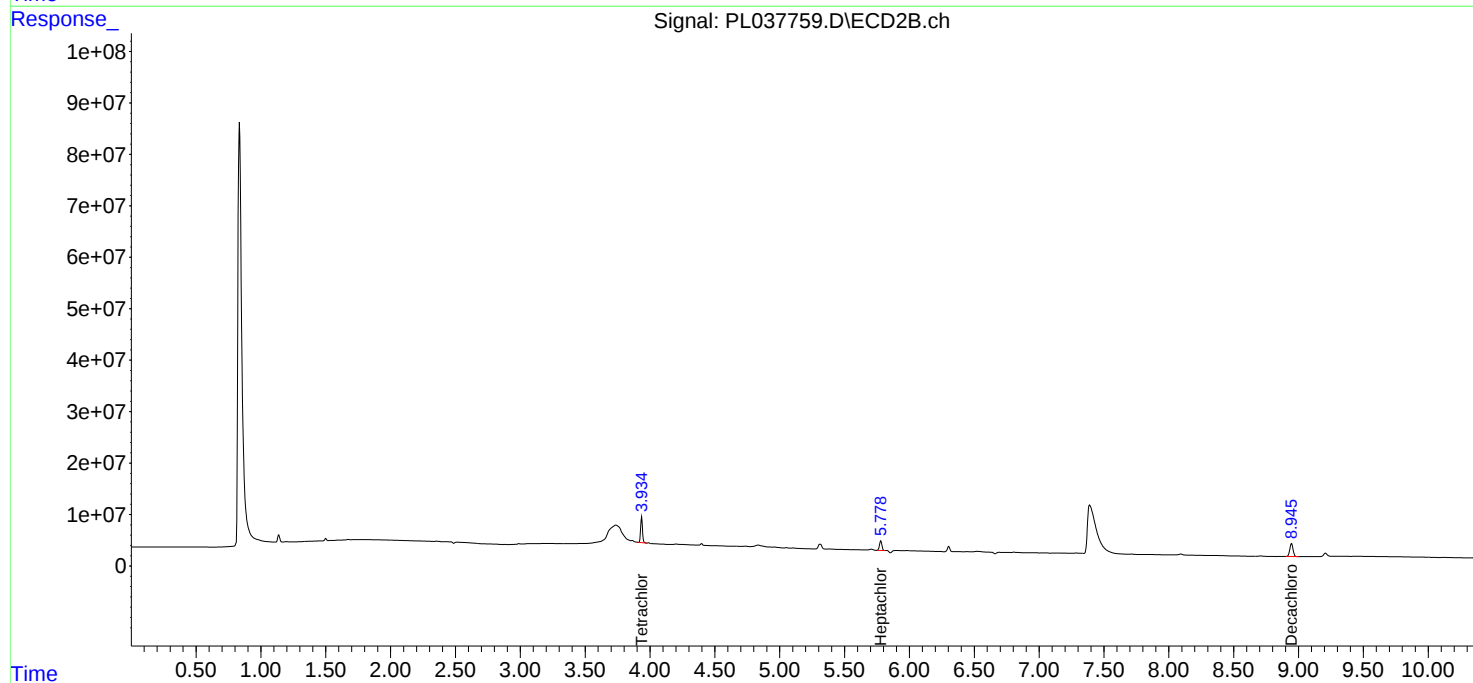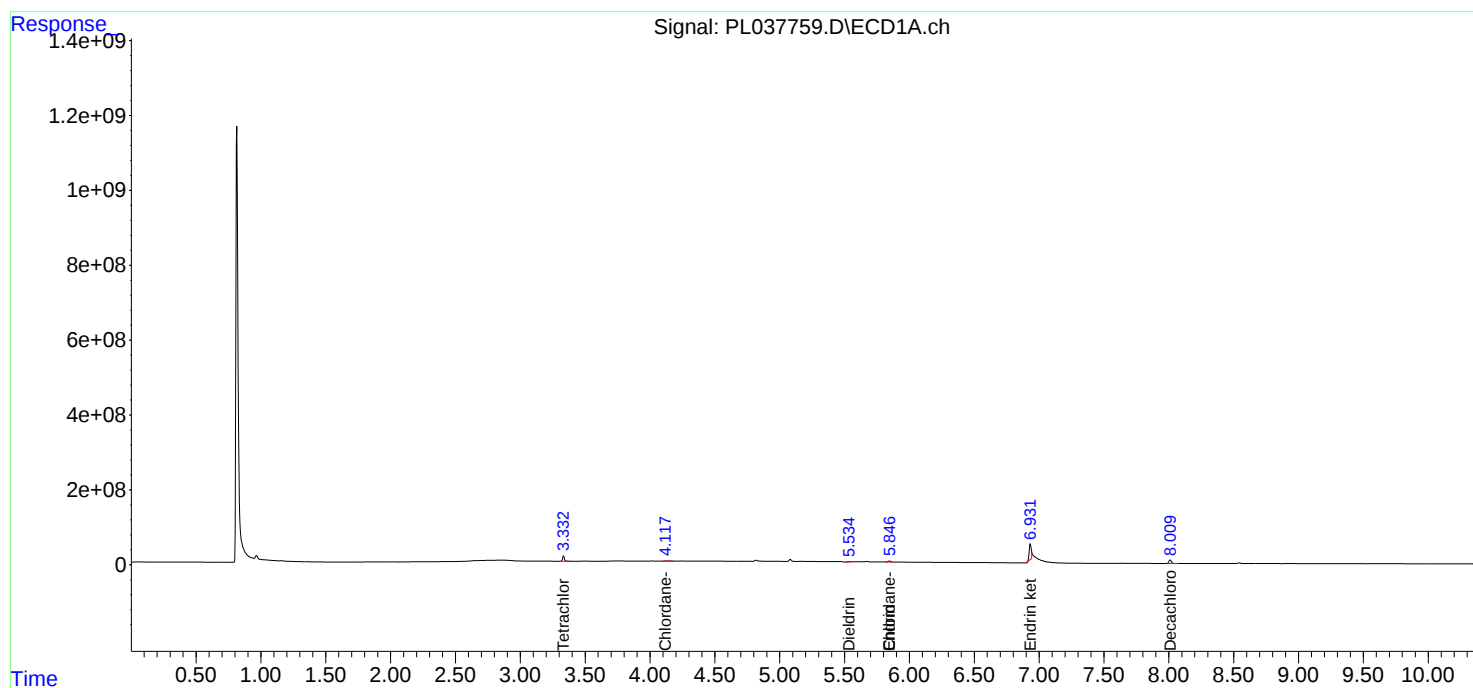


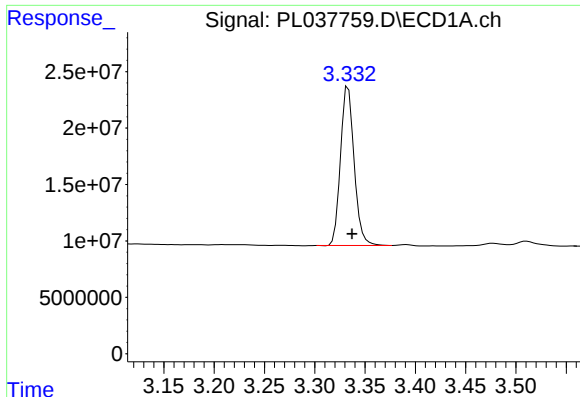

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 132702445
Conc: 16.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

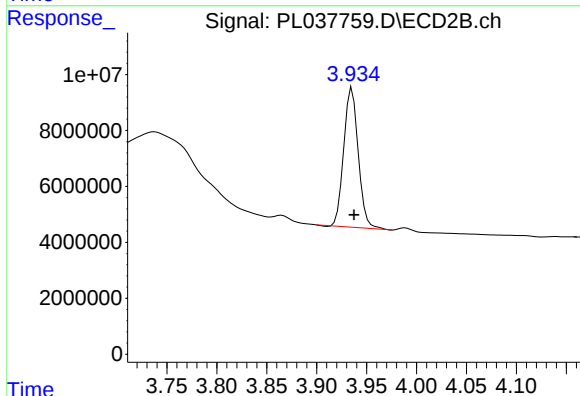


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 50365215
Conc: 18.20 ng/ml

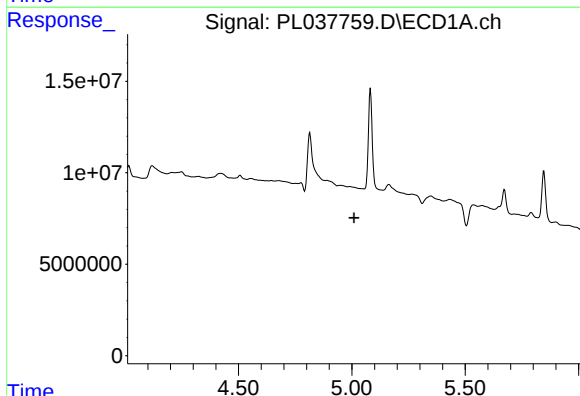


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.010 min
Response: 0
Conc: N.D.

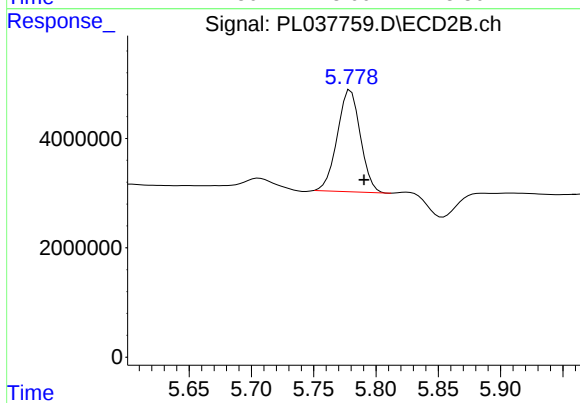

#8 Heptachlor epoxide


R.T.: 5.780 min
Delta R.T.: -0.011 min
Response: 24072198
Conc: 8.44 ng/ml

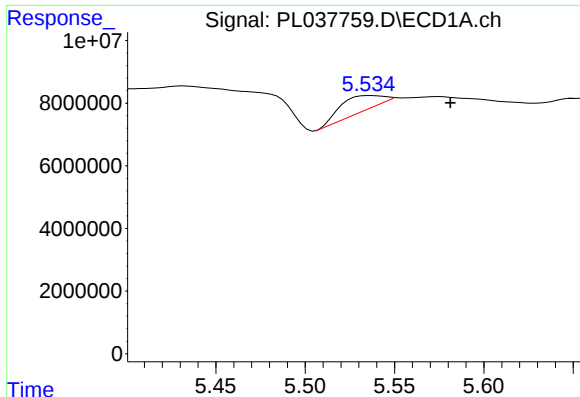

#13 Dieldrin


R.T.: 5.537 min
Delta R.T.: -0.045 min
Response: 9320132
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

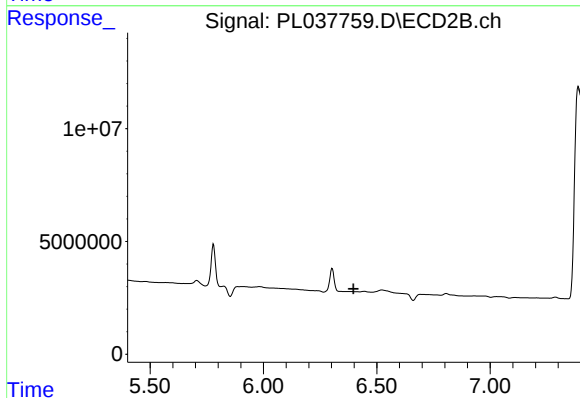


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

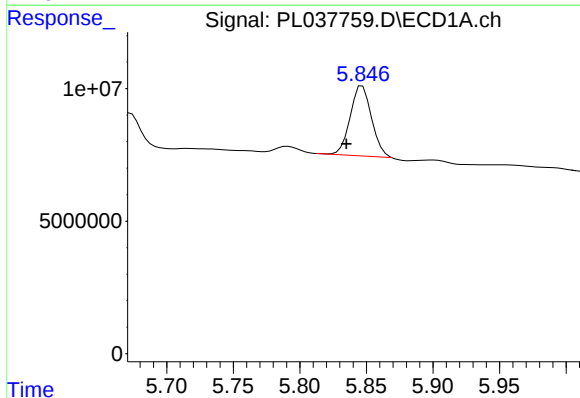


#14 Endrin

R.T.: 5.847 min
Delta R.T.: 0.012 min
Response: 29461808
Conc: 3.74 ng/ml

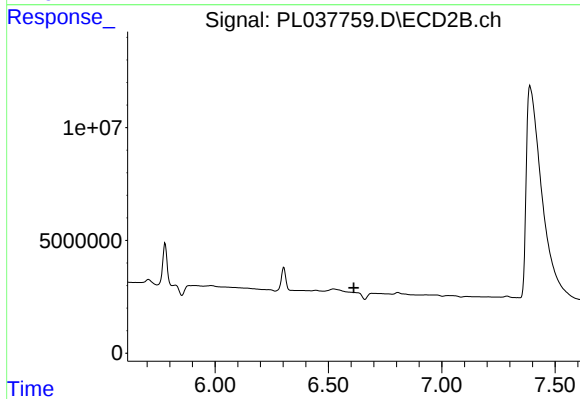

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

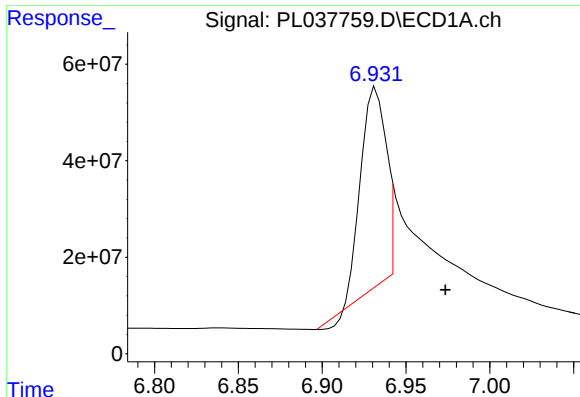

#21 Endrin ketone


R.T.: 6.932 min
Delta R.T.: -0.041 min
Response: 436553189
Conc: 61.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

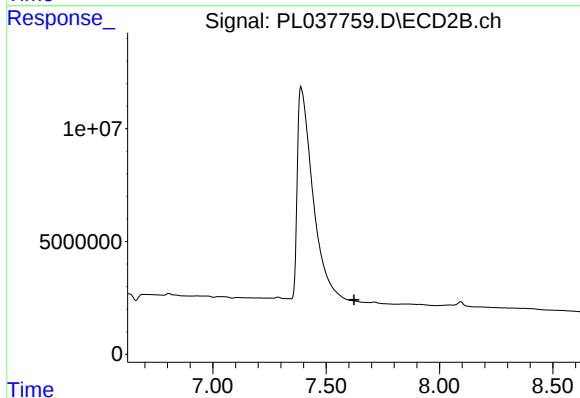


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

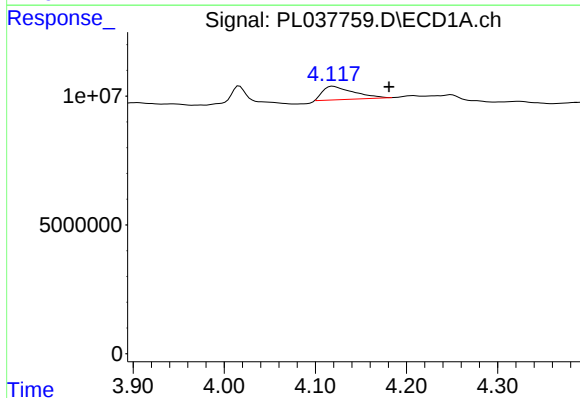


#23 Chlordane-1

R.T.: 4.120 min
Delta R.T.: -0.061 min
Response: 12242046
Conc: 39.87 ng/ml

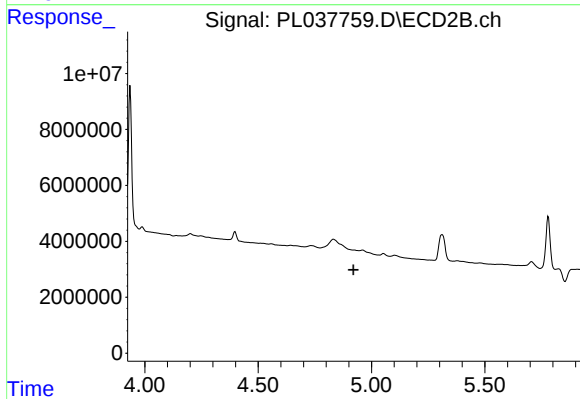

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

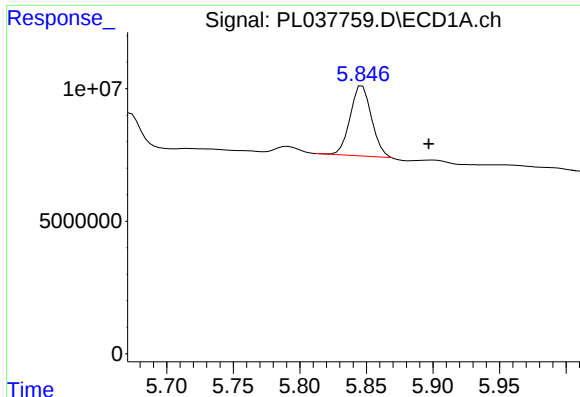

#27 Chlordane-5


R.T.: 5.847 min
Delta R.T.: -0.050 min
Response: 29461808
Conc: 225.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

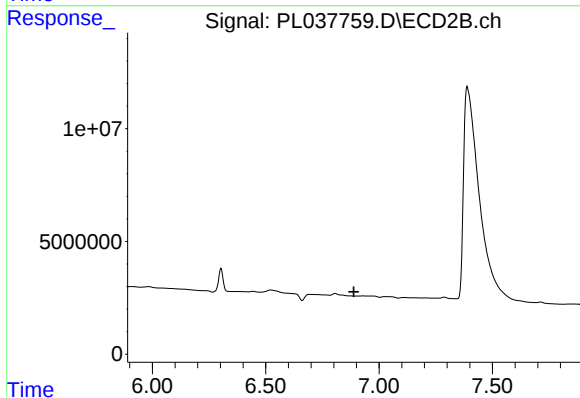


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

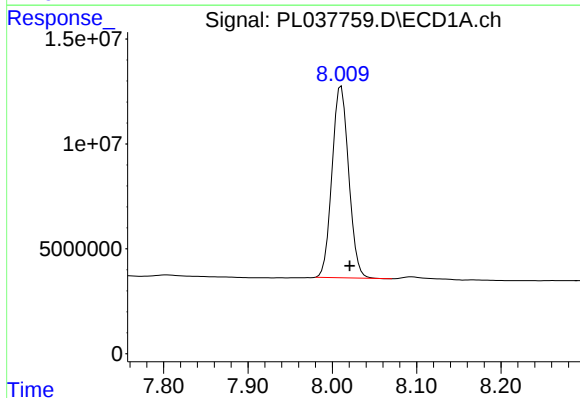

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.010 min
Response: 125404589
Conc: 20.78 ng/ml

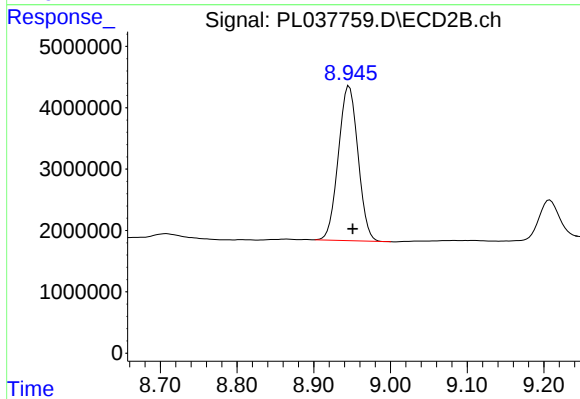

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.005 min
Response: 44832160
Conc: 22.60 ng/ml