

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 16:59
 Operator : AJ\MA
 Sample : J3874-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2018-NYSEG-MCMaster-PH4-5(3-

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:45:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:34:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.934	59851418	23261584	7.566	8.408m
28)	SA Decachlor...	8.011	8.947	54607976	19648982	9.050	9.904
Target Compounds							
17)	MA 4,4'-DDT	6.193	7.028	7426915	1889025	1.150m	0.892m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 16:59
Operator : AJ\MA
Sample : J3874-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-MCMaster-PH4-5(3-


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:34:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

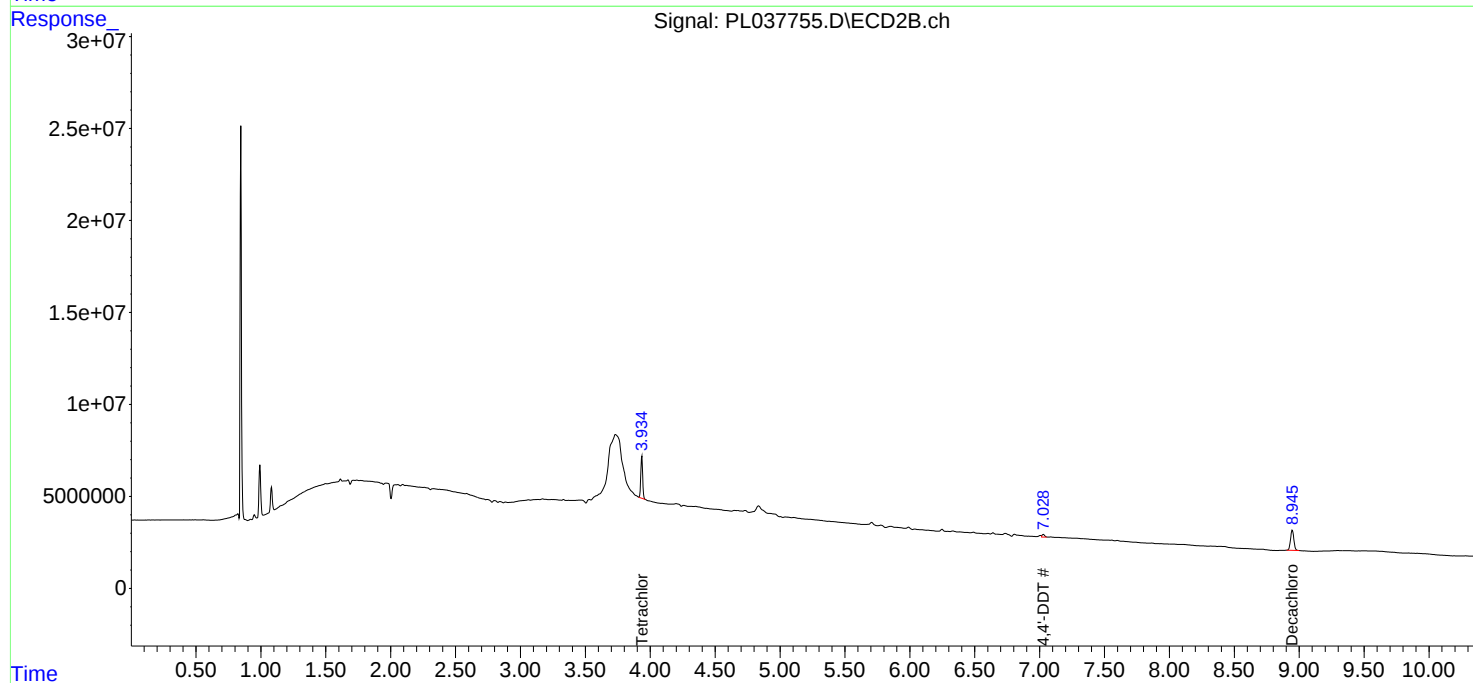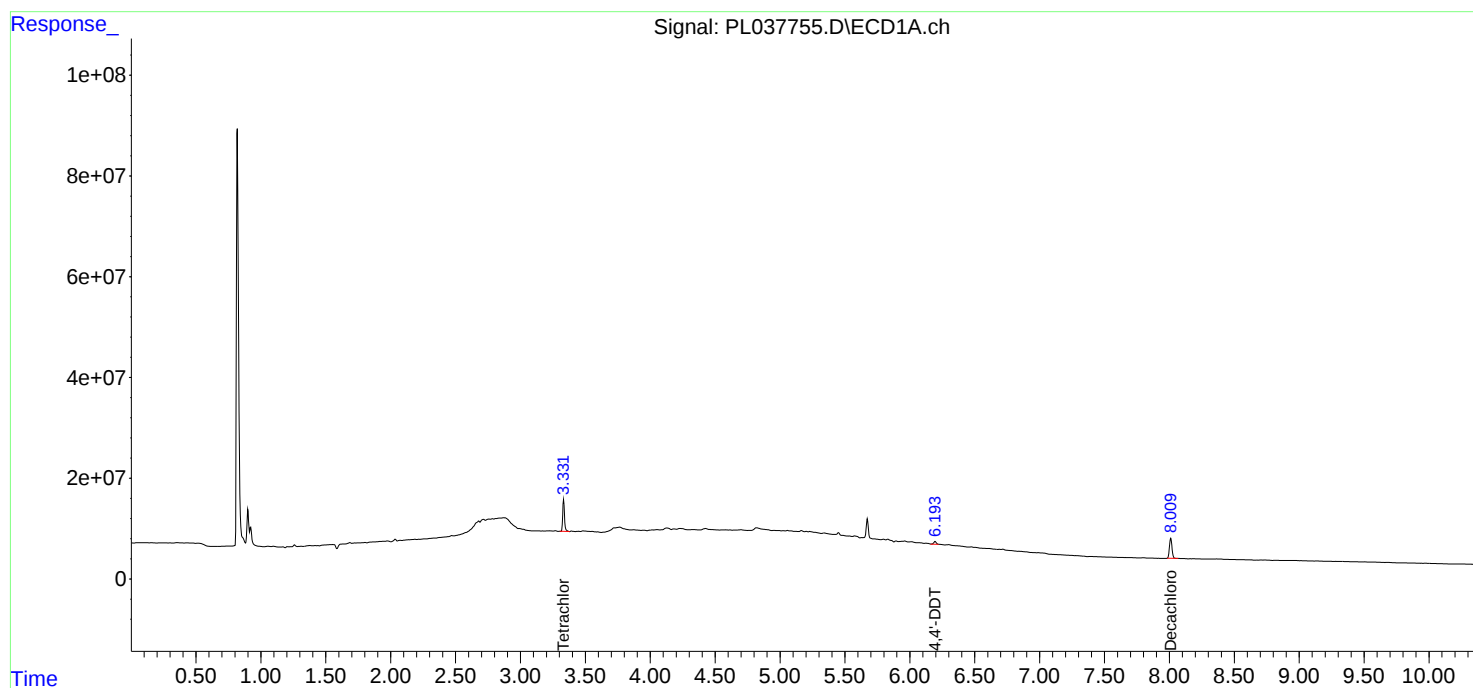

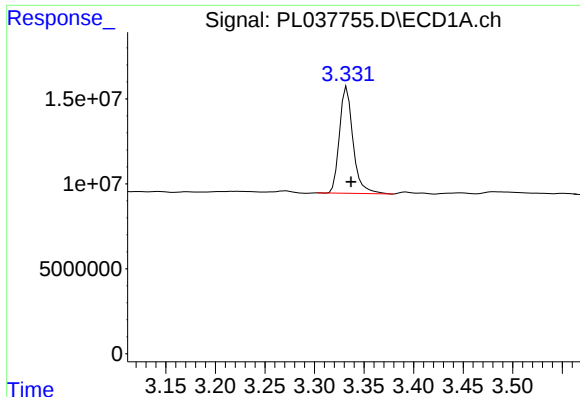


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 59851418
Conc: 7.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-MCMaster-PH4-5(3-


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:04 PM

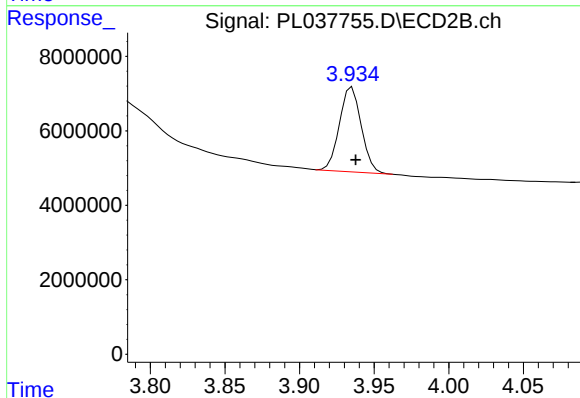


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.004 min
Response: 23261584
Conc: 8.41 ng/ml m

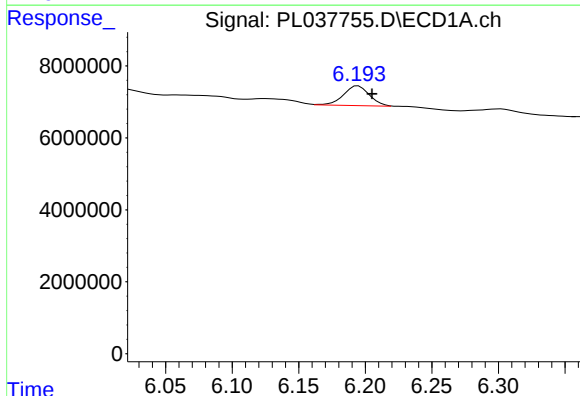


#17 4,4'-DDT

R.T.: 6.193 min
Delta R.T.: -0.012 min
Response: 7426915
Conc: 1.15 ng/ml m

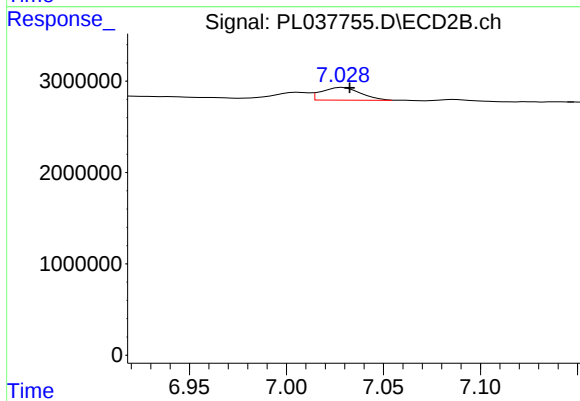

#17 4,4'-DDT

R.T.: 7.028 min
Delta R.T.: -0.005 min
Response: 1889025
Conc: 0.89 ng/ml m

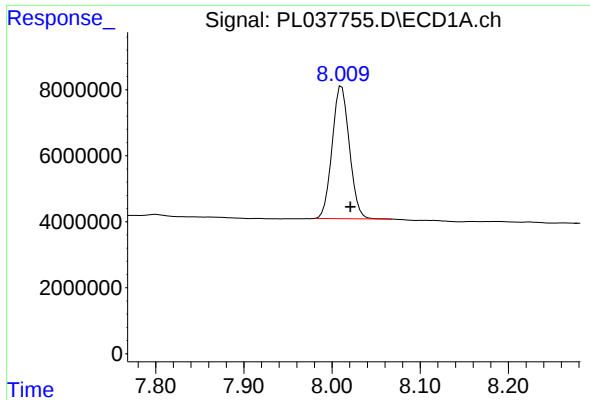


#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.010 min
Response: 54607976
Conc: 9.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-MCMaster-PH4-5(3-

Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:04 PM

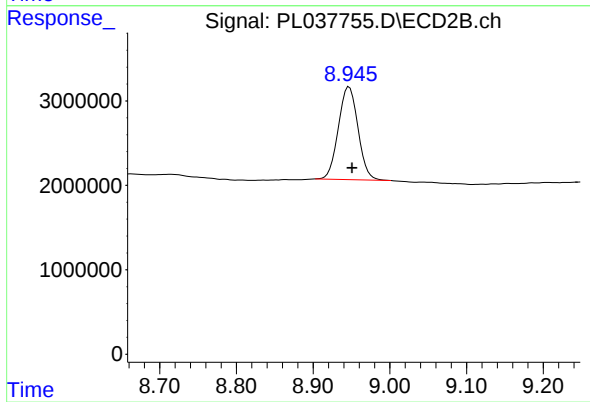

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 19648982
Conc: 9.90 ng/ml