

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 18:51
 Operator : AJ\MA
 Sample : J3880-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURCHARGE-SP-14

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:45:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:35:48 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.936	104.9E6	38053090	13.260	13.754
28)	SA Decachlor...	8.012	8.947	98845885	33247760	16.381	16.758
Target Compounds							
12)	B 4,4'-DDE	5.451	6.248	70506241	22604816	7.983	8.883

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 18:51
Operator : AJ\MA
Sample : J3880-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-14


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:35:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

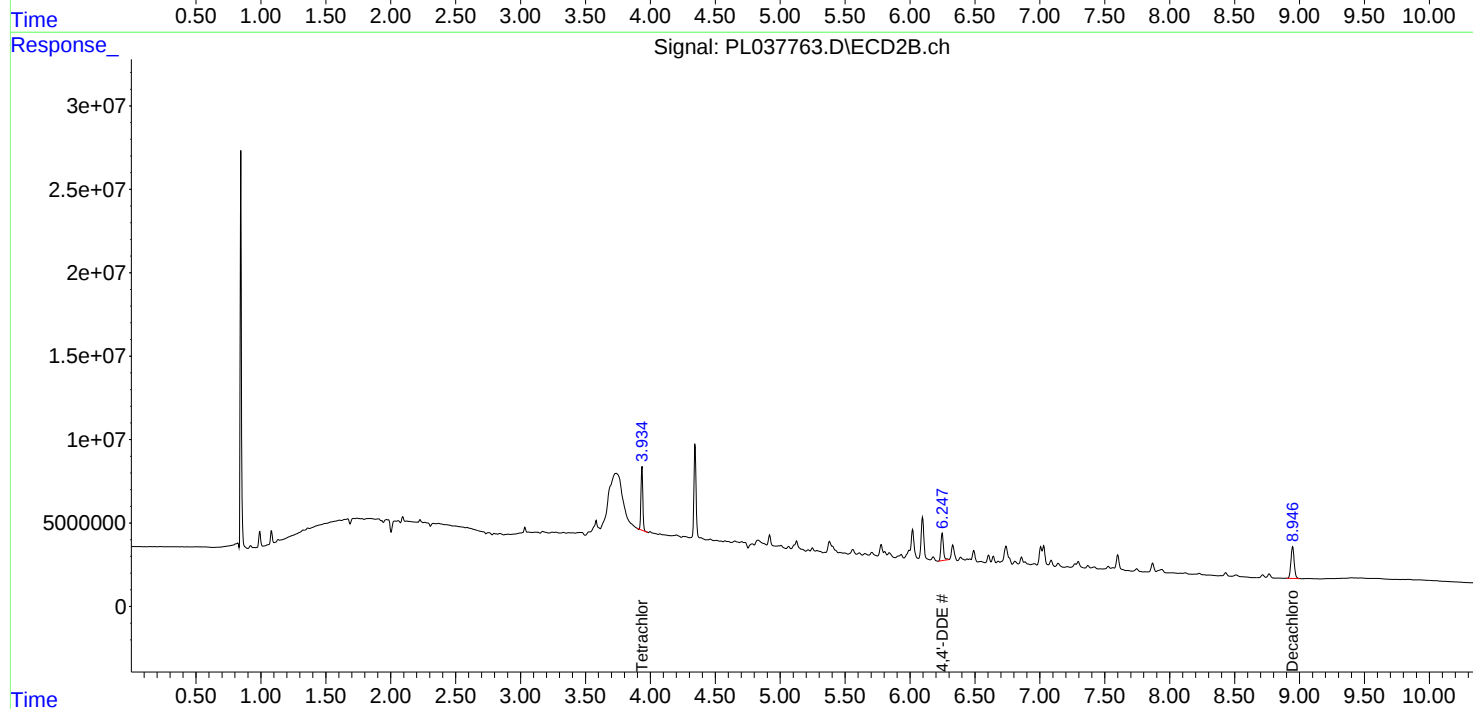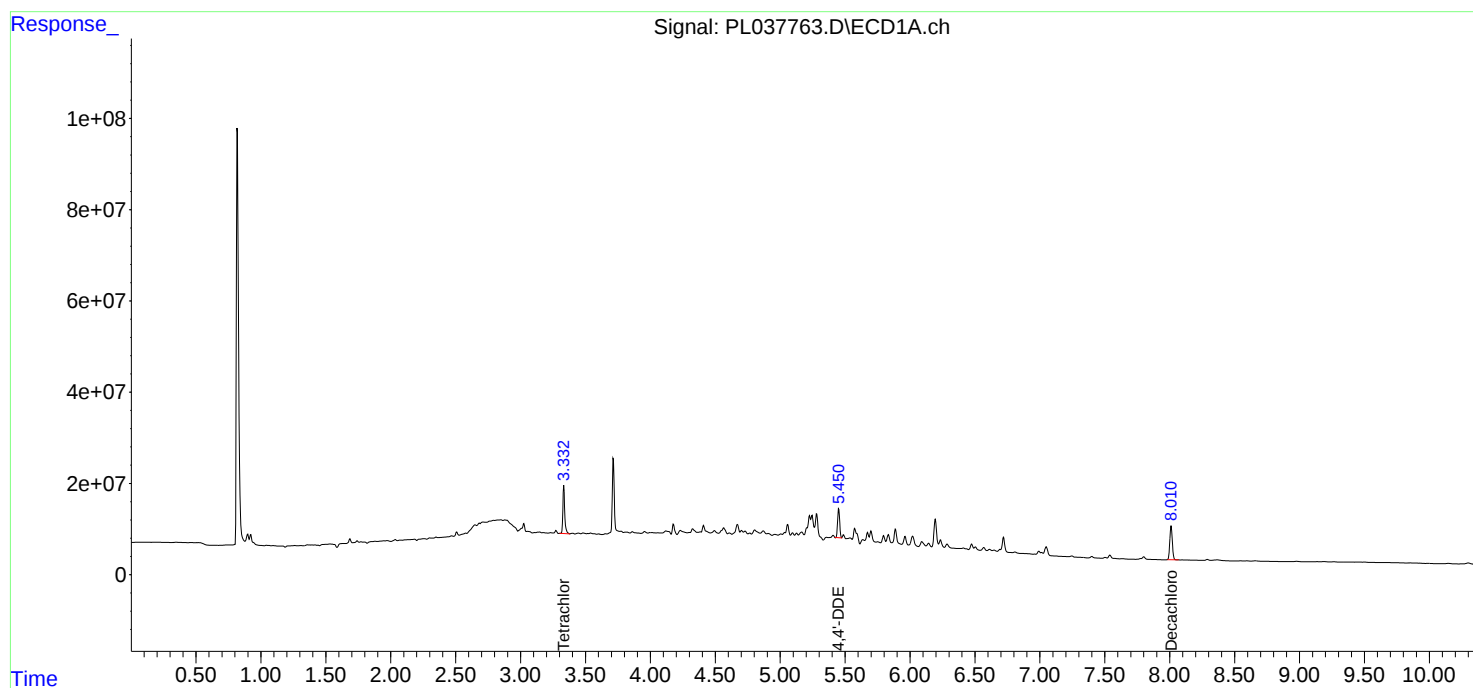

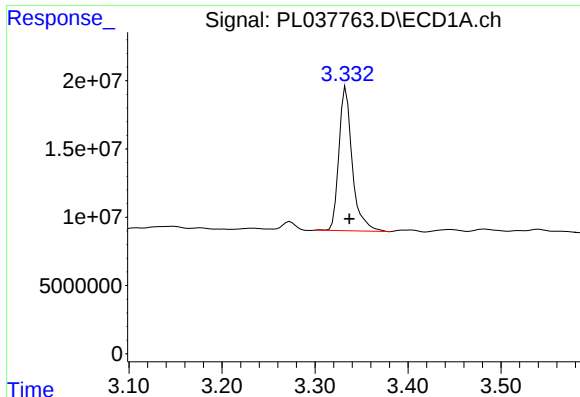


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 104894239
Conc: 13.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-14


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:19 PM

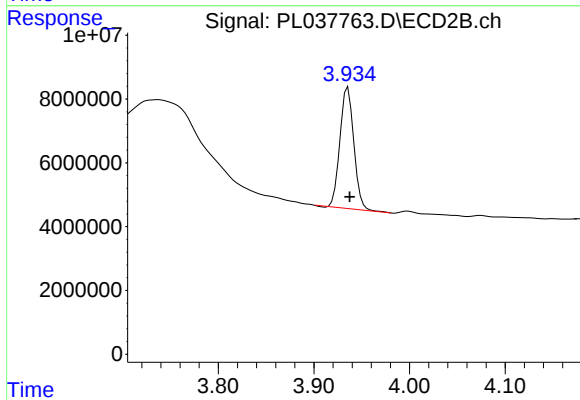


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 38053090
Conc: 13.75 ng/ml

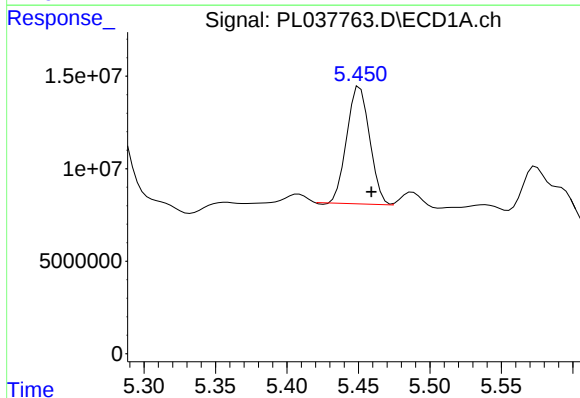


#12 4,4'-DDE

R.T.: 5.451 min
Delta R.T.: -0.008 min
Response: 70506241
Conc: 7.98 ng/ml

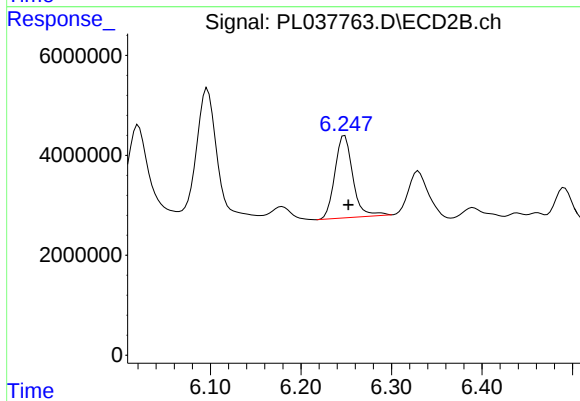

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.004 min
Response: 22604816
Conc: 8.88 ng/ml

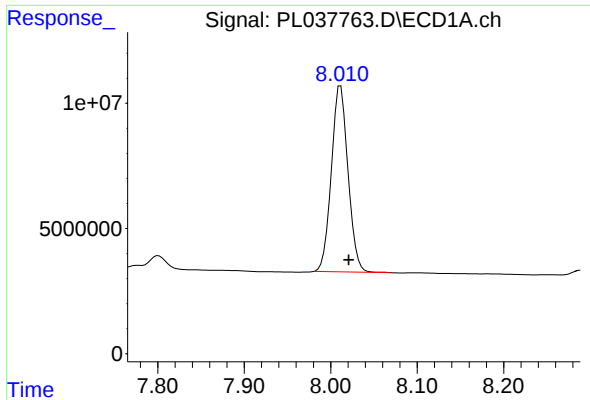


#28 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.009 min
Response: 98845885
Conc: 16.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-14

Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:19 PM

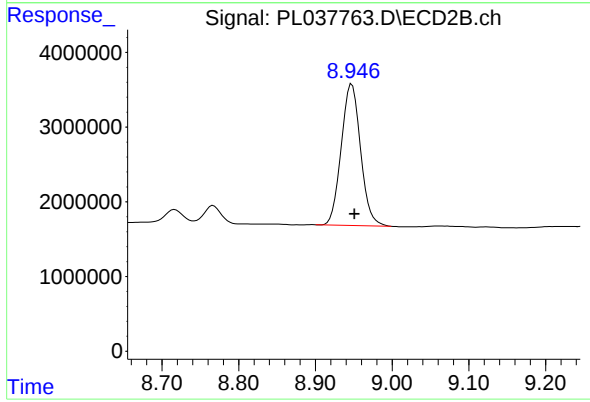

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.003 min
Response: 33247760
Conc: 16.76 ng/ml