

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 19:19
 Operator : AJ\MA
 Sample : J3880-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURCHARGE-SP-16

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:45:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:36:09 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.936	122.8E6	43479264	15.526	15.715
28)	SA Decachlor...	8.010	8.947	101.6E6	36224942	16.835	18.259
Target Compounds							
12)	B 4,4'-DDE	5.450	6.249	88339983	27418065	10.002m	10.775

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 19:19
Operator : AJ\MA
Sample : J3880-11
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-16


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:36:09 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

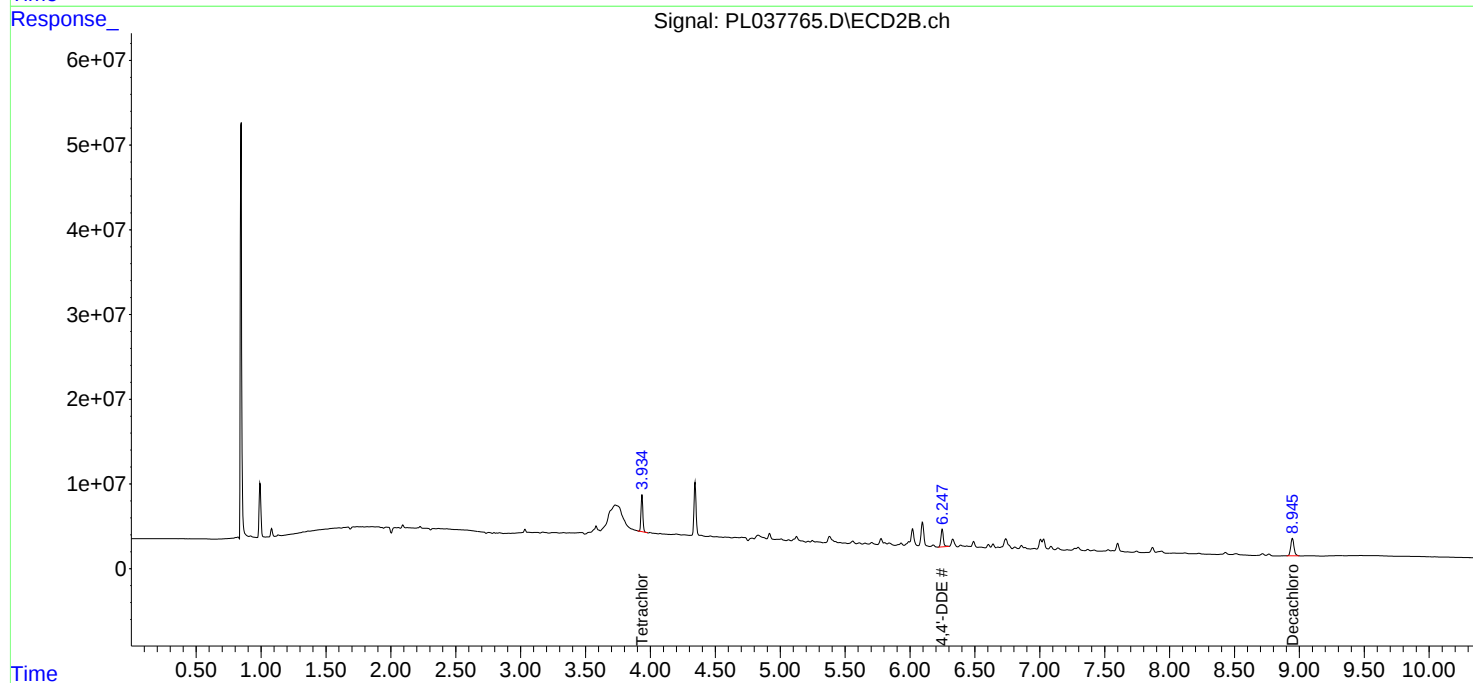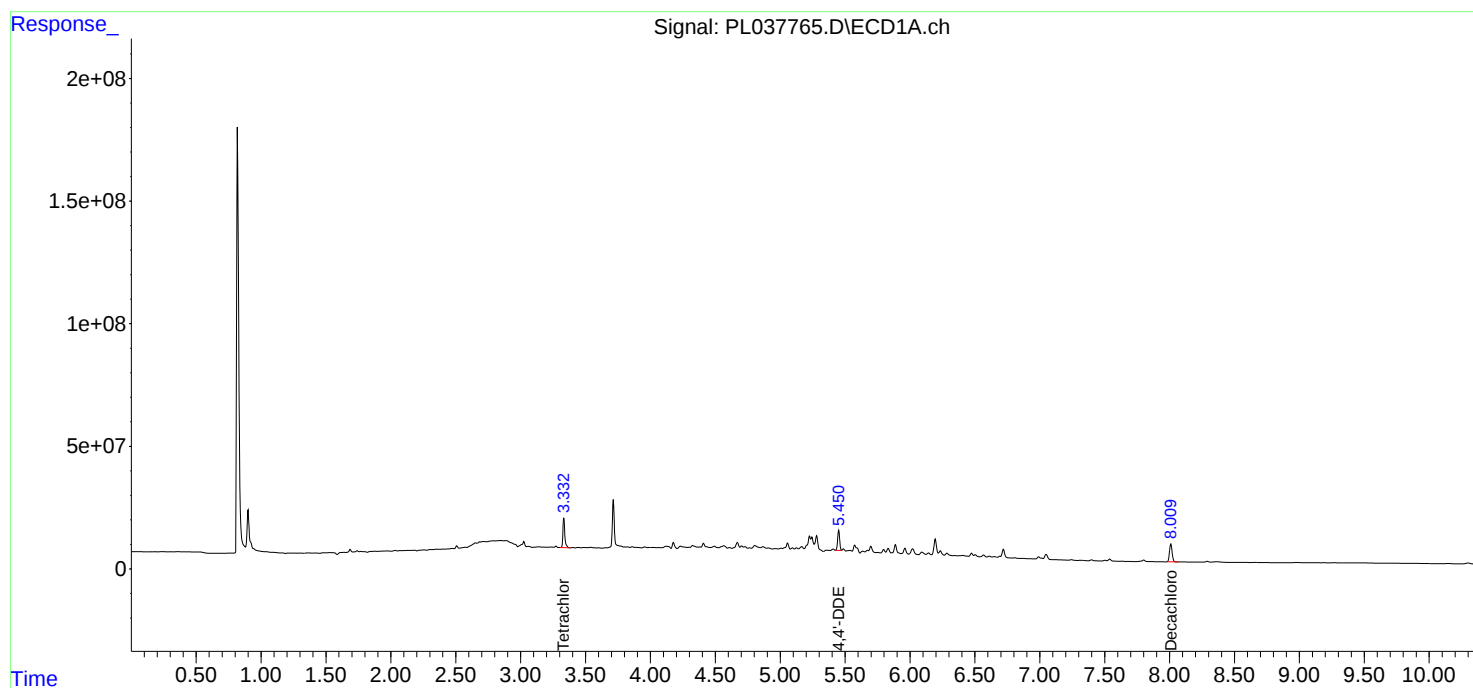

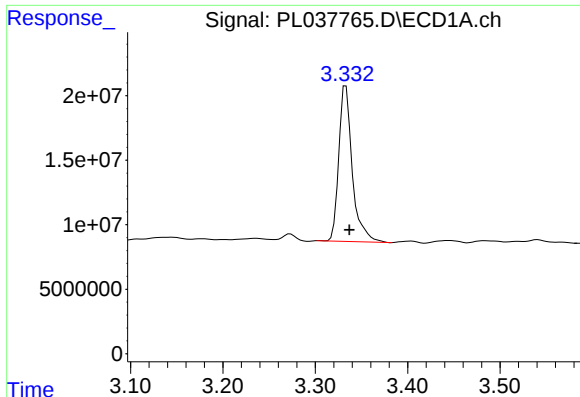


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 122814581
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-16


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:22 PM

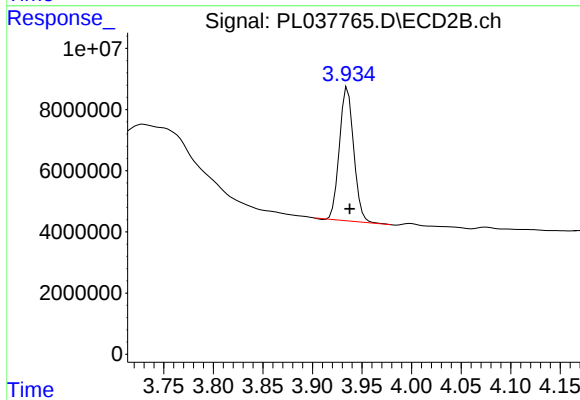


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 43479264
Conc: 15.72 ng/ml

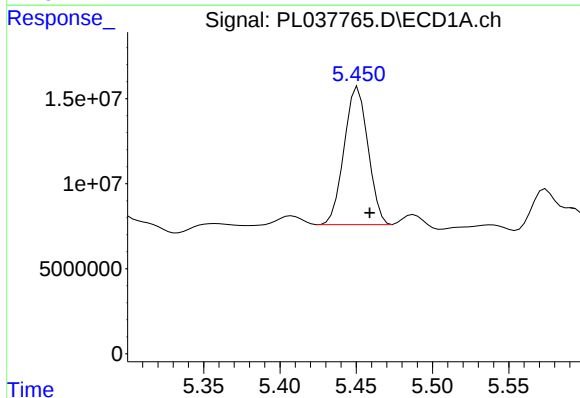


#12 4,4'-DDE

R.T.: 5.450 min
Delta R.T.: -0.009 min
Response: 88339983
Conc: 10.00 ng/ml m

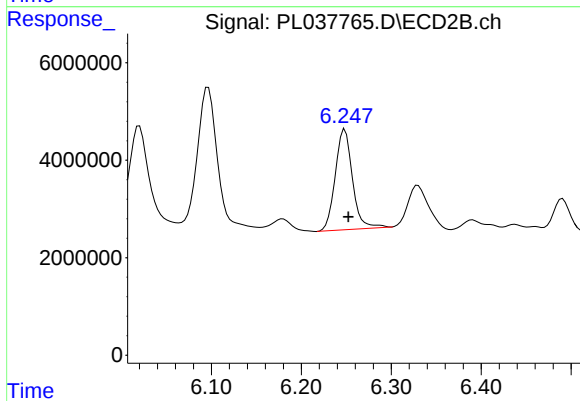

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.004 min
Response: 27418065
Conc: 10.77 ng/ml

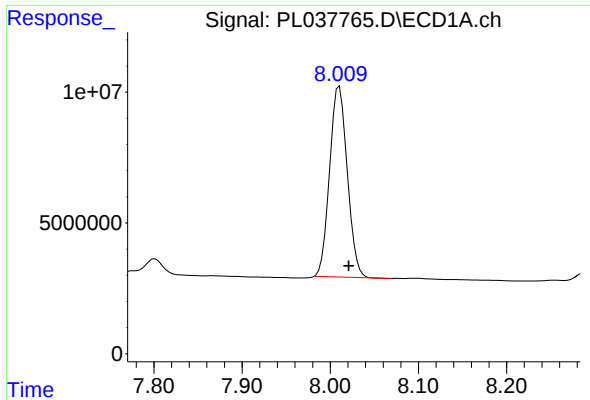

#28 Decachlorobiphenyl

R.T.: 8.010 min

Delta R.T.: -0.010 min


Response: 101585635

Conc: 16.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-16

Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:22 PM

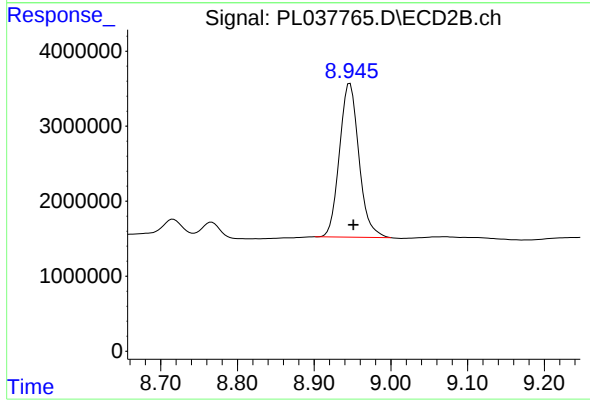

#28 Decachlorobiphenyl

R.T.: 8.947 min

Delta R.T.: -0.004 min

Response: 36224942

Conc: 18.26 ng/ml