

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
 Data File : PL037772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 20:57
 Operator : AJ\MA
 Sample : J3881-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SURCHARGE-SP-23

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:45:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:37:44 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.934	106.7E6	32768430	13.486	11.844m
28)	SA Decachlor...	8.011	8.947	104.5E6	35573881	17.322	17.931
Target Compounds							
12)	B 4,4'-DDE	5.450	6.249	149.2E6	65077397	16.897m	25.574 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070618\
Data File : PL037772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 20:57
Operator : AJ\MA
Sample : J3881-05
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-23


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:37:44 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

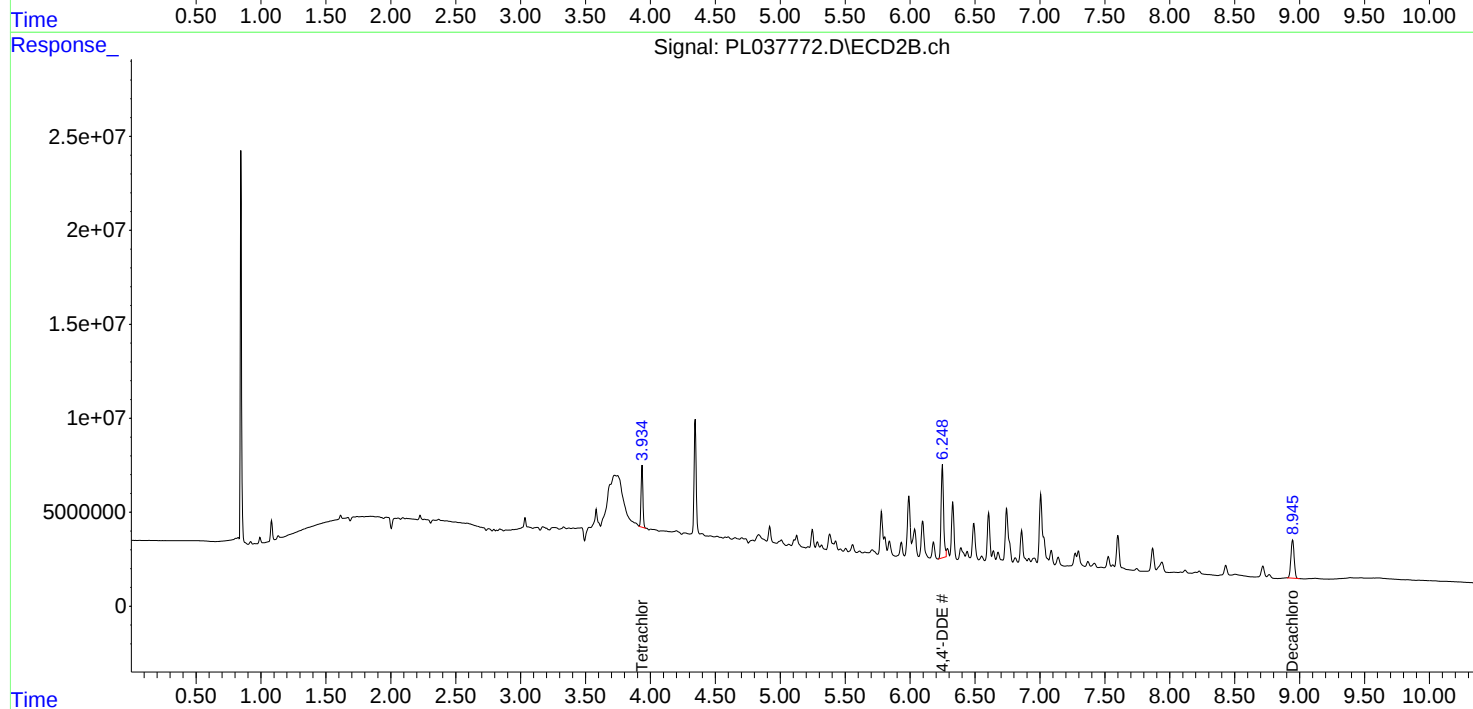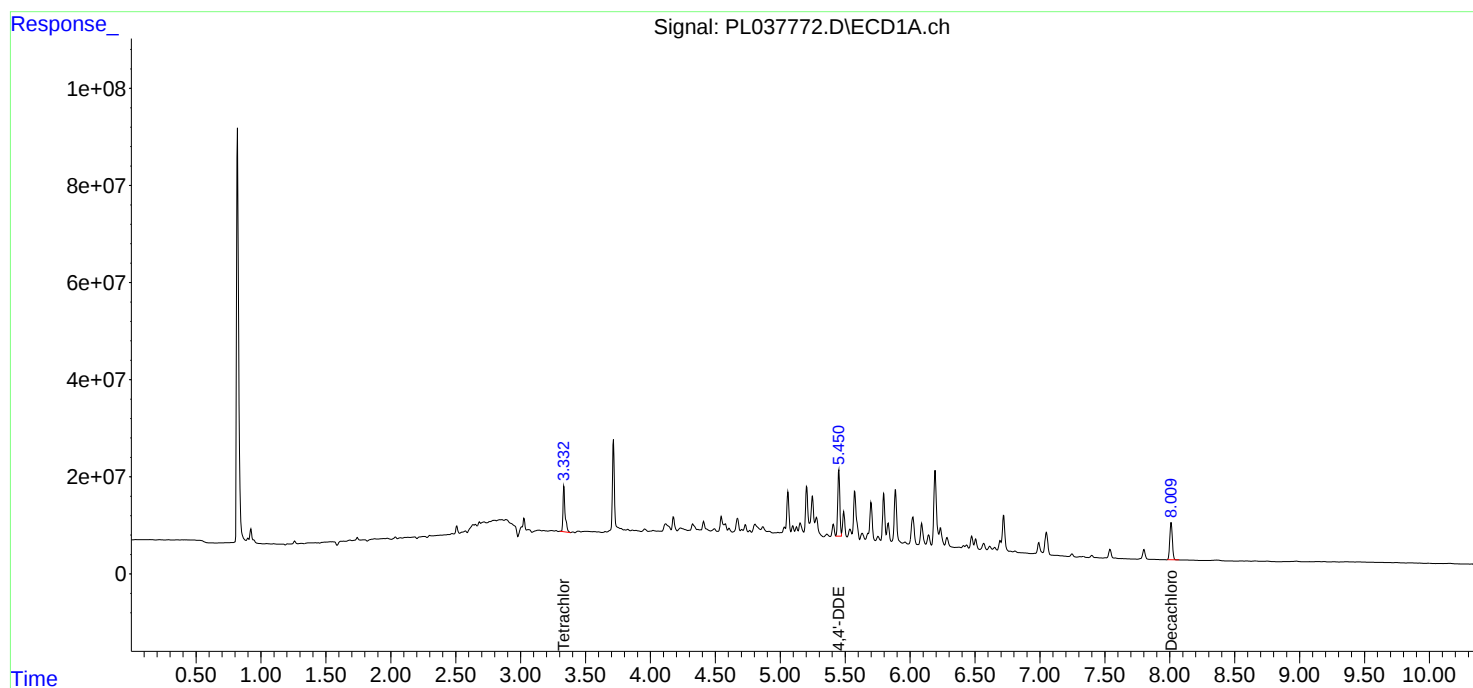

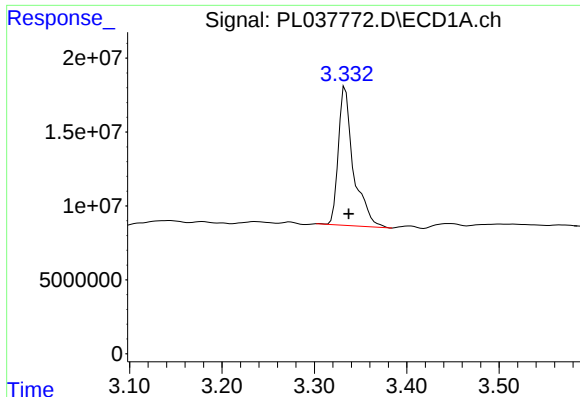


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 106681630
Conc: 13.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-23


Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:34 PM

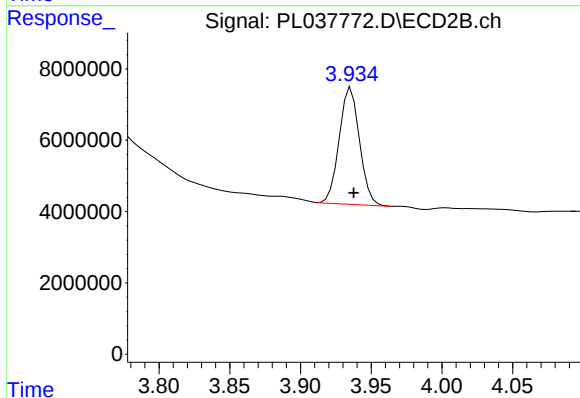


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 32768430
Conc: 11.84 ng/ml m

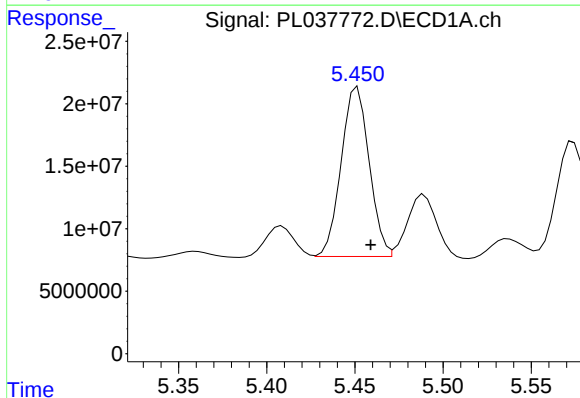


#12 4,4'-DDE

R.T.: 5.450 min
Delta R.T.: -0.009 min
Response: 149243322
Conc: 16.90 ng/ml m

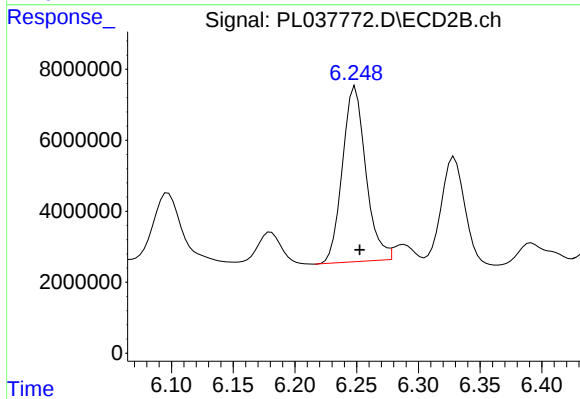

#12 4,4'-DDE

R.T.: 6.249 min
Delta R.T.: -0.003 min
Response: 65077397
Conc: 25.57 ng/ml

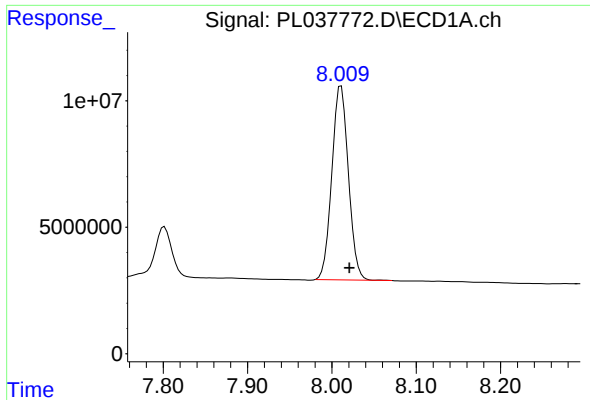


#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.010 min
Response: 104522340
Conc: 17.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
SURCHARGE-SP-23

Manual Integrations
APPROVED

Sohil
7/9/2018 4:45:34 PM

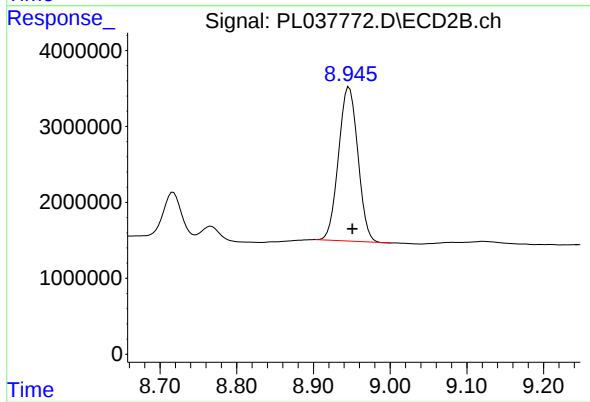

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 35573881
Conc: 17.93 ng/ml