

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
 Data File : PL059732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2020 14:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 16:44:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.070	40345782	60018644	22.463	22.568
28)	SA Decachlor...	8.285	9.181	31664958	44395588	20.626	20.424
Target Compounds							
2)	A alpha-BHC	3.962	0.000	1193591	0	0.464	N.D. #
4)	MA Heptachlor	0.000	5.265	0	852070	N.D.	0.243 #
9)	A Endosulfan I	5.604f	0.000	124799	0	0.081	N.D. #
13)	MA Dieldrin	0.000	6.552f	0	385317	N.D.	0.137 #
15)	B Endosulfa...	6.358	7.008	222056	425618	0.146	0.166
18)	B Endrin al...	0.000	7.139	0	353459	N.D.	0.160 #
20)	A Methoxychlor	0.000	7.676	0	509953	N.D.	0.395 #
23)	Chlordane-1	4.419f	5.102f	1626780	2666444	31.216	24.698
27)	Chlordane-5	6.358	7.075	222056	145326	4.322	1.670 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
Data File : PL059732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2020 14:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 16:44:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

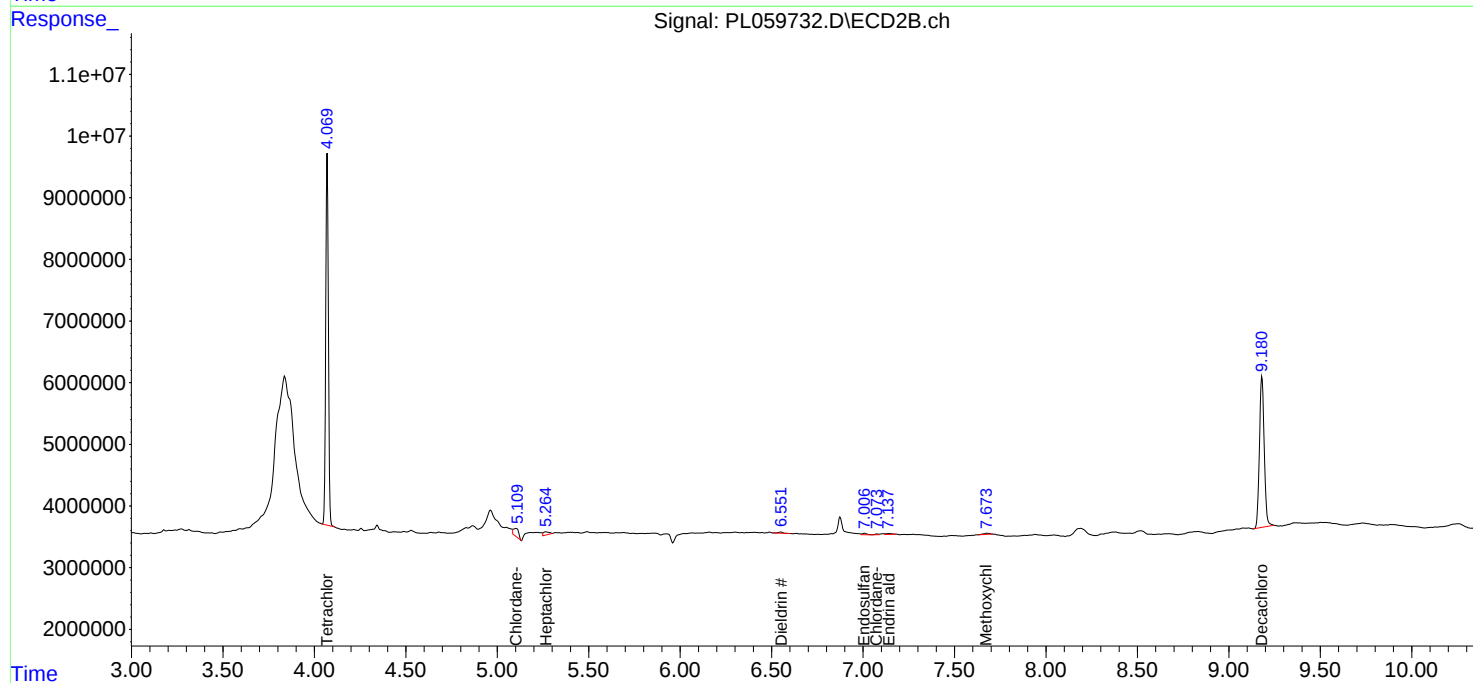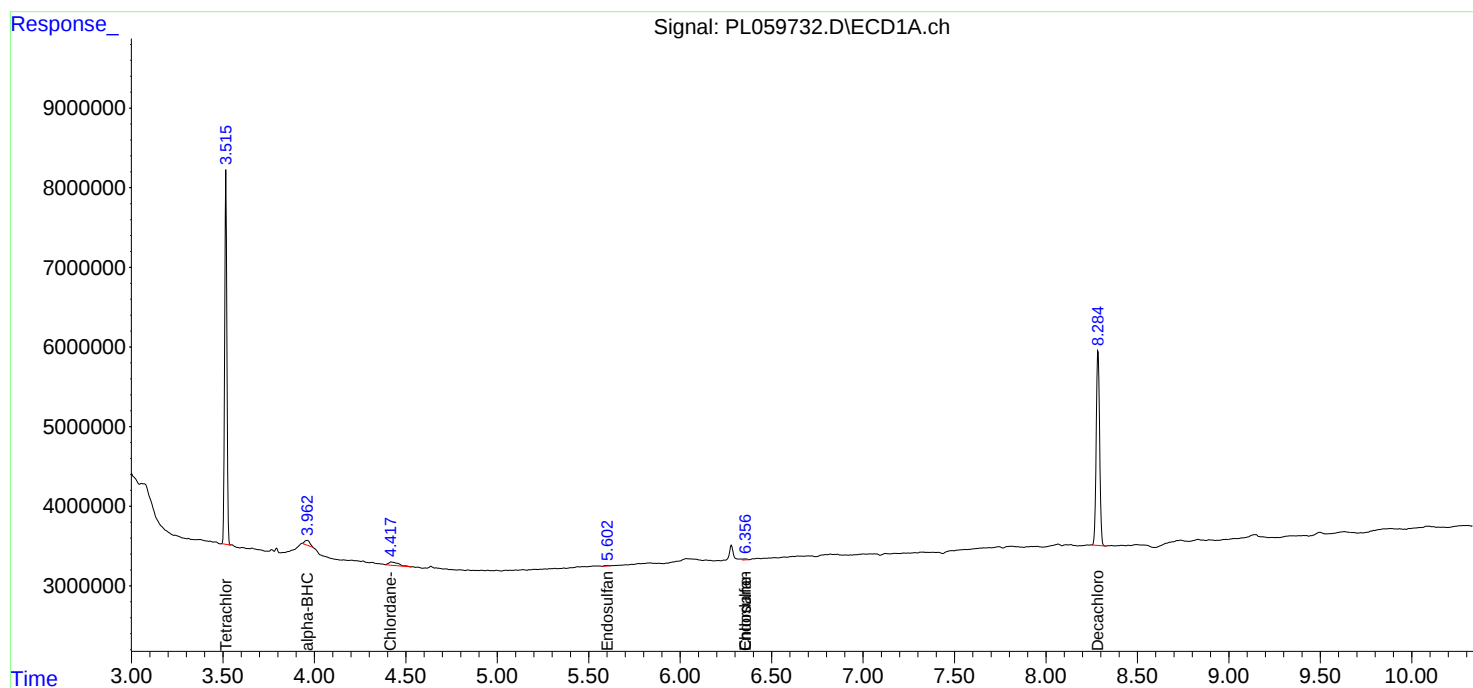


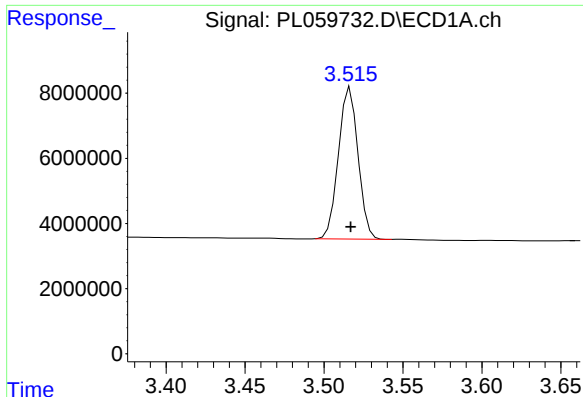

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 40345782
Conc: 22.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

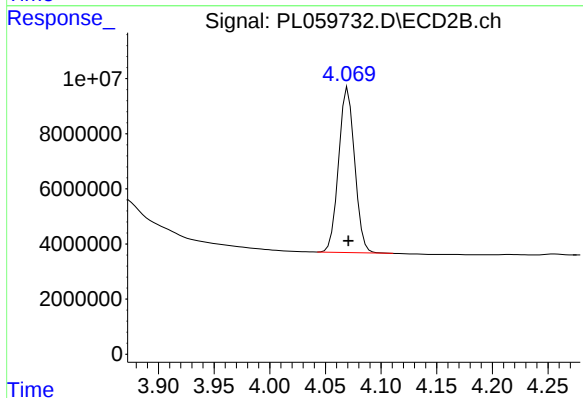


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 60018644
Conc: 22.57 ng/ml

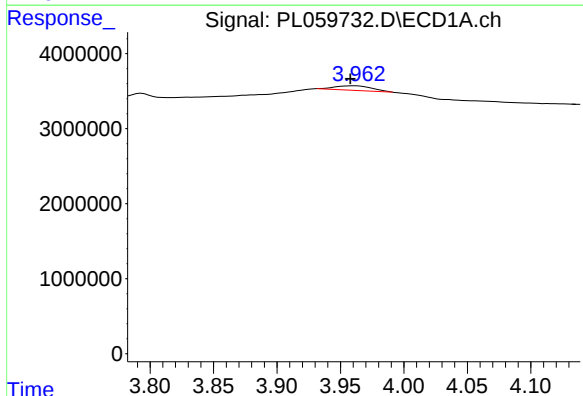


#2 alpha-BHC

R.T.: 3.962 min
Delta R.T.: 0.004 min
Response: 1193591
Conc: 0.46 ng/ml

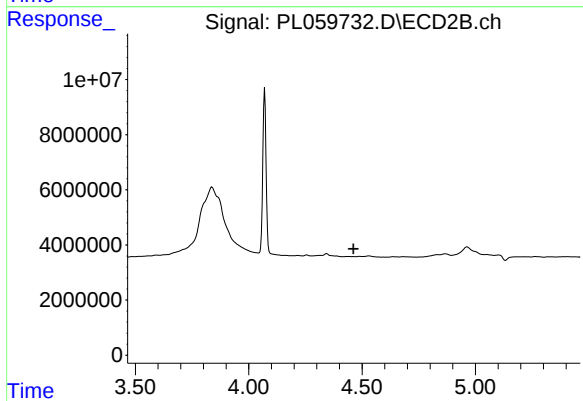

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

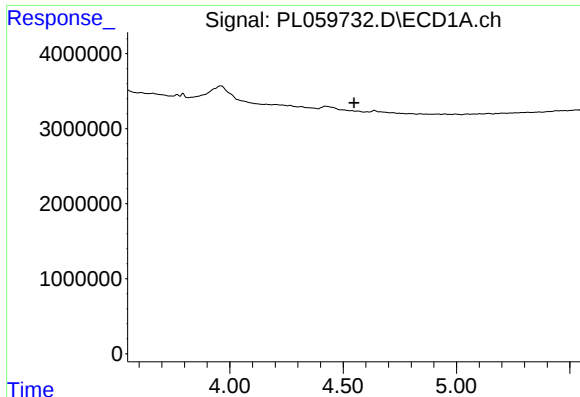

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

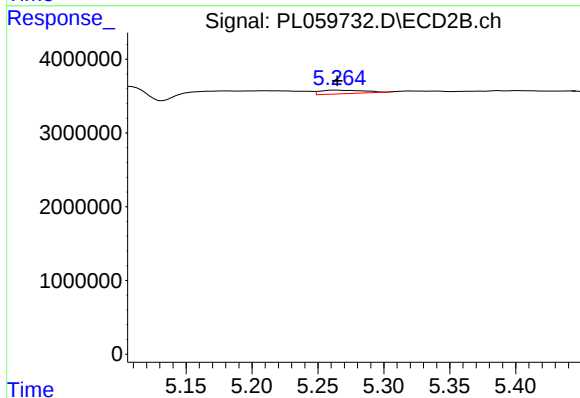


#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 852070
Conc: 0.24 ng/ml

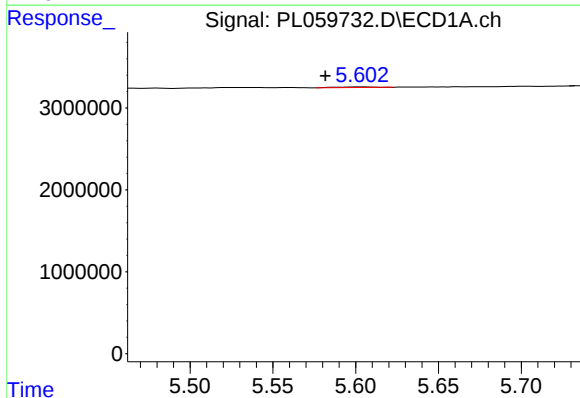


#9 Endosulfan I

R.T.: 5.604 min
Delta R.T.: 0.022 min
Response: 124799
Conc: 0.08 ng/ml

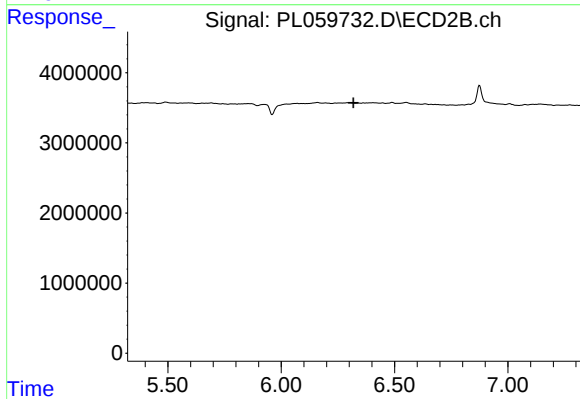

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

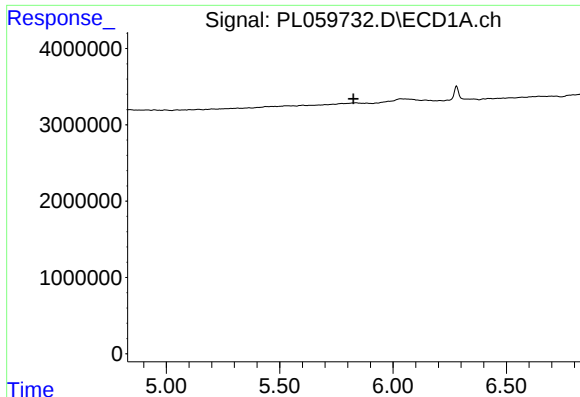

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

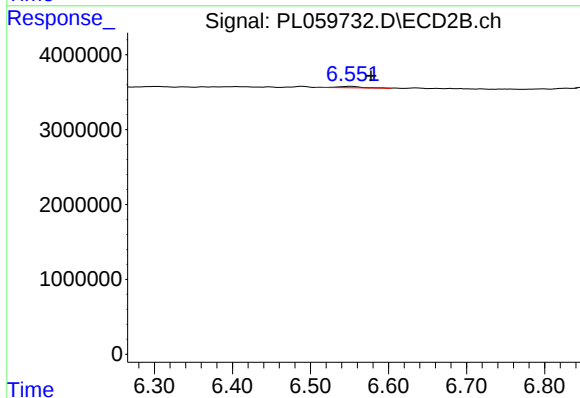


#13 Dieldrin

R.T.: 6.552 min
Delta R.T.: -0.025 min
Response: 385317
Conc: 0.14 ng/ml

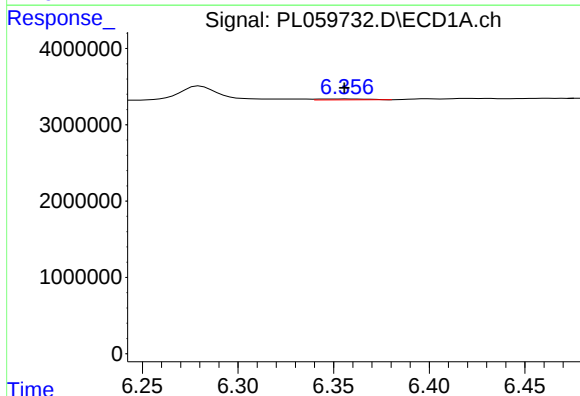


#15 Endosulfan II

R.T.: 6.358 min
Delta R.T.: 0.003 min
Response: 222056
Conc: 0.15 ng/ml

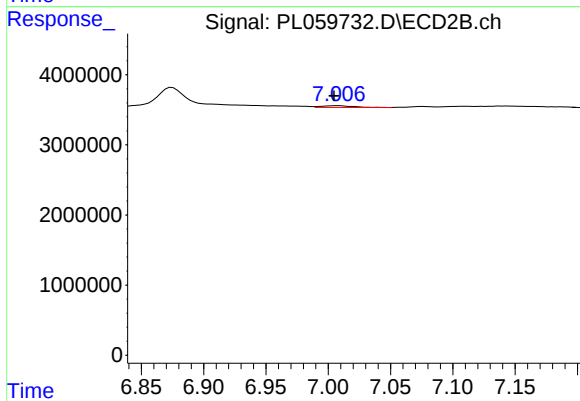

#15 Endosulfan II


R.T.: 7.008 min
Delta R.T.: 0.003 min
Response: 425618
Conc: 0.17 ng/ml

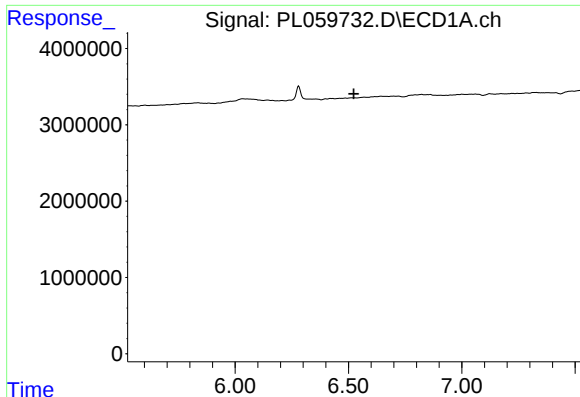

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

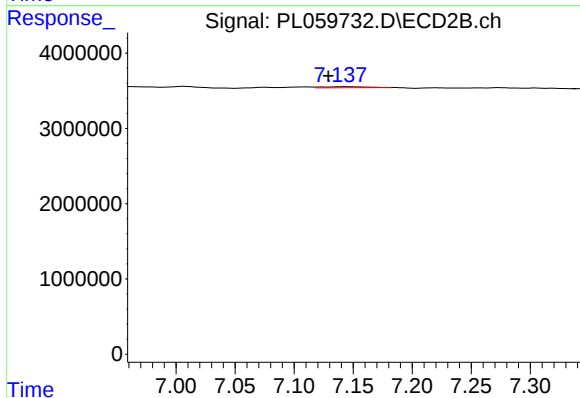


#18 Endrin aldehyde

R.T.: 7.139 min
Delta R.T.: 0.010 min
Response: 353459
Conc: 0.16 ng/ml

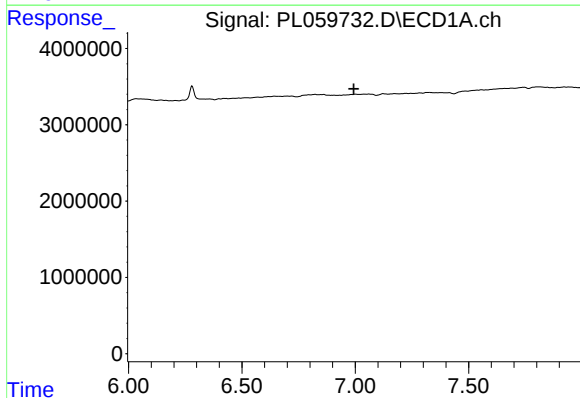


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.994 min
Response: 0
Conc: N.D.

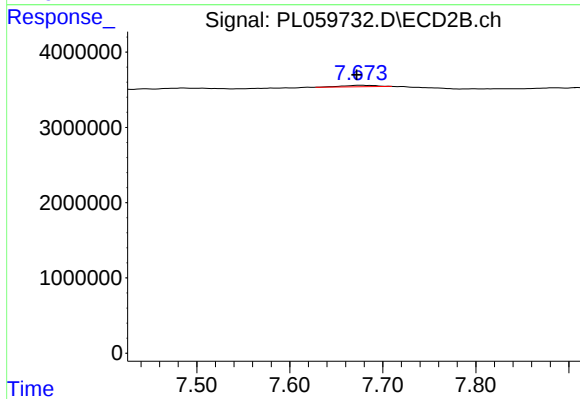

#20 Methoxychlor


R.T.: 7.676 min
Delta R.T.: 0.004 min
Response: 509953
Conc: 0.39 ng/ml

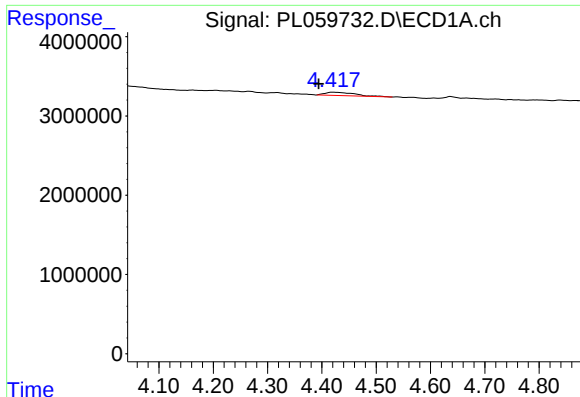

#23 Chlordane-1


R.T.: 4.419 min
Delta R.T.: 0.025 min
Response: 1626780
Conc: 31.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

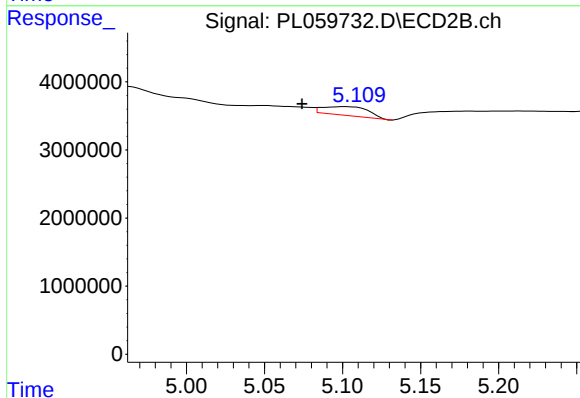


#23 Chlordane-1

R.T.: 5.102 min
Delta R.T.: 0.028 min
Response: 2666444
Conc: 24.70 ng/ml

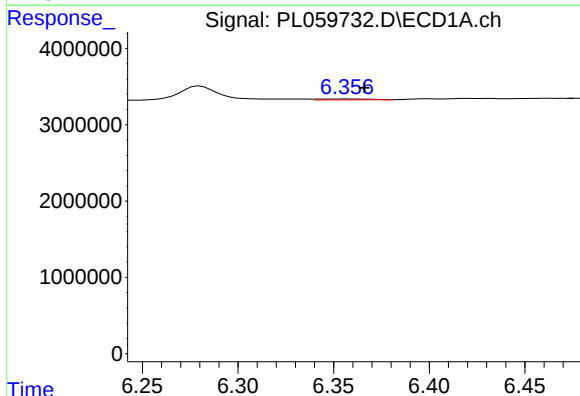


#27 Chlordane-5

R.T.: 6.358 min
Delta R.T.: -0.008 min
Response: 222056
Conc: 4.32 ng/ml

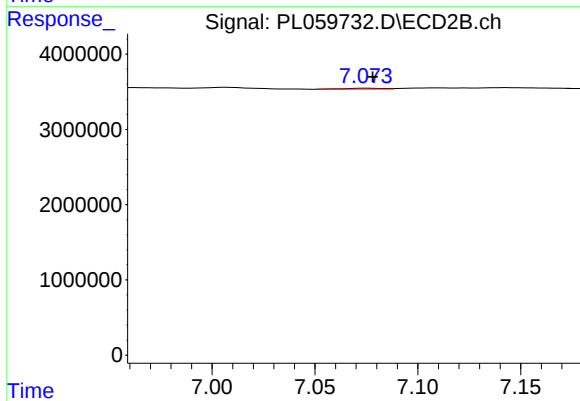

#27 Chlordane-5


R.T.: 7.075 min
Delta R.T.: -0.003 min
Response: 145326
Conc: 1.67 ng/ml

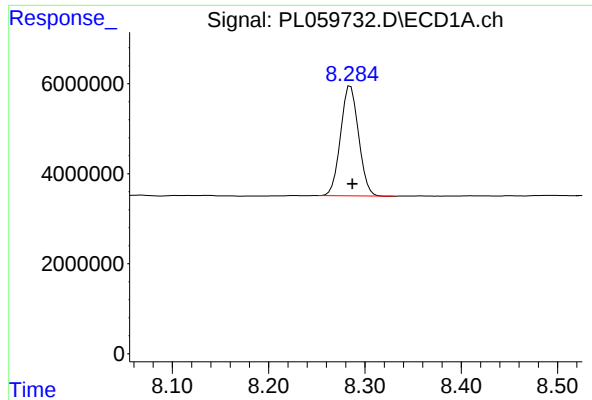

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 31664958
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

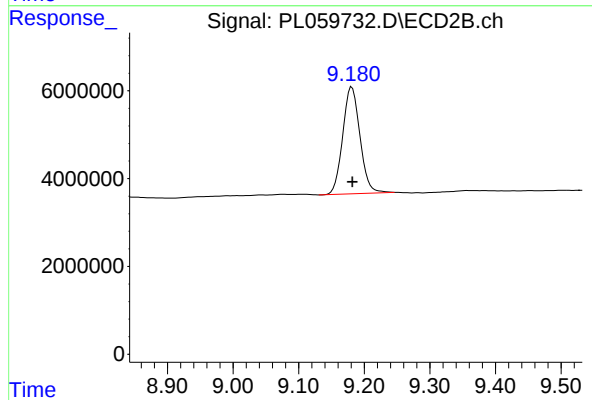

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: 0.000 min
Response: 44395588
Conc: 20.42 ng/ml