

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
 Data File : PL059736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2020 15:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 16:45:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.516	4.070	40193030	59868312	22.378	22.512
28)	SA Decachlor...	8.285	9.181	29607237	41642725	19.285	19.158
Target Compounds							
2)	A alpha-BHC	3.959	0.000	1592600	0	0.619	N.D. #
4)	MA Heptachlor	0.000	5.267	0	938958	N.D.	0.268 #
7)	B delta-BHC	0.000	5.160f	0	1059522	N.D.	0.362 #
8)	B Heptachlo...	0.000	5.934f	0	3029756	N.D.	1.247 #
15)	B Endosulfa...	6.357	0.000	52256	0	0.034	N.D. #
18)	B Endrin al...	6.524	7.127	170072	1415440	0.135	0.639 #
22)	Mirex	7.420	8.309f	169637	590578	0.131	0.309 #
23)	Chlordane-1	4.423f	0.000	771761	0	14.809	N.D. #
27)	Chlordane-5	6.357	7.078	52256	205358	1.017	2.360 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
Data File : PL059736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2020 15:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 16:45:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

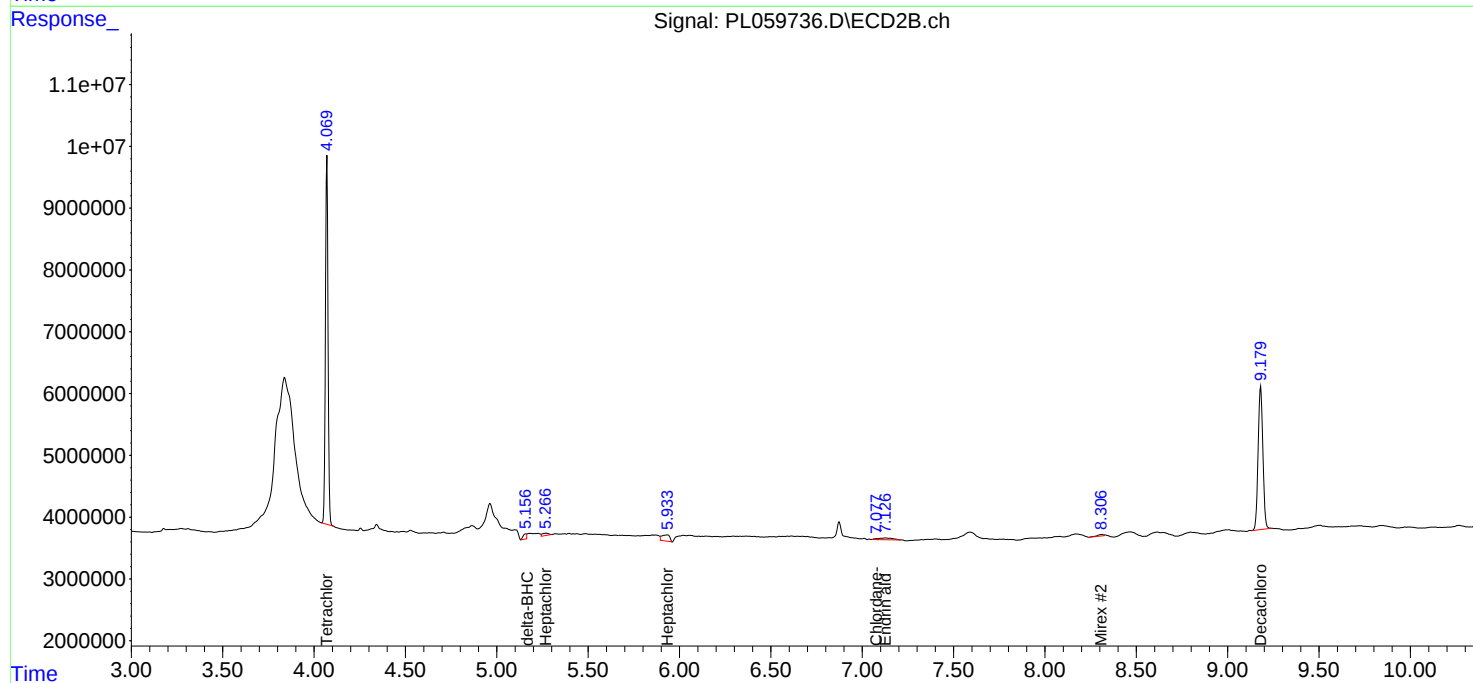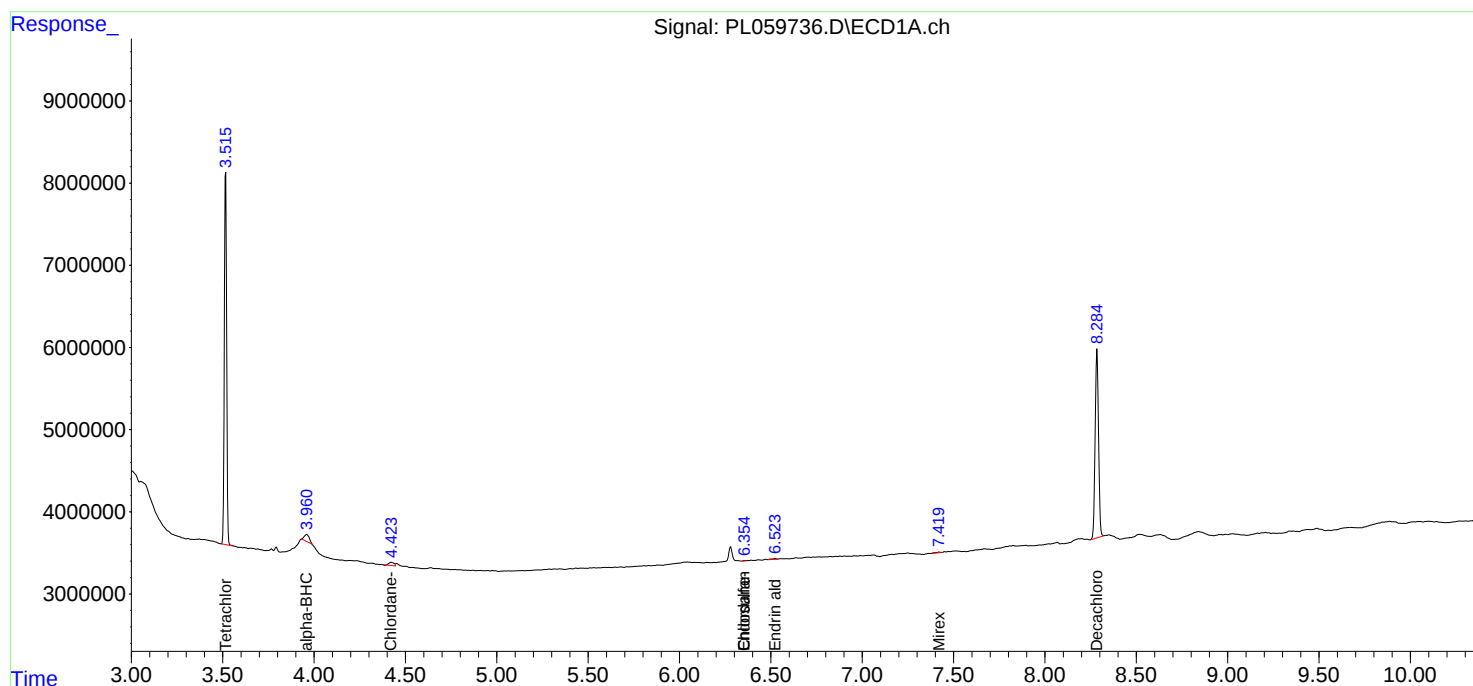


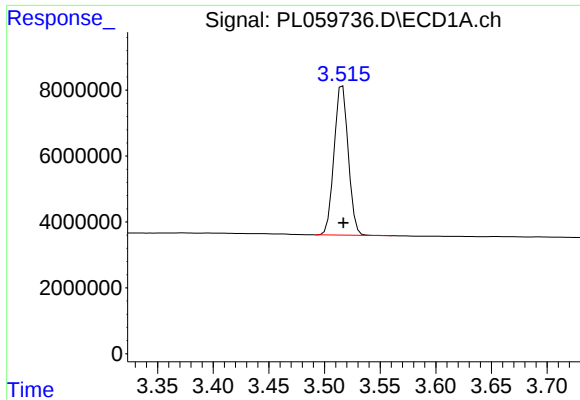

#1 Tetrachloro-m-xylene


R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 40193030
Conc: 22.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

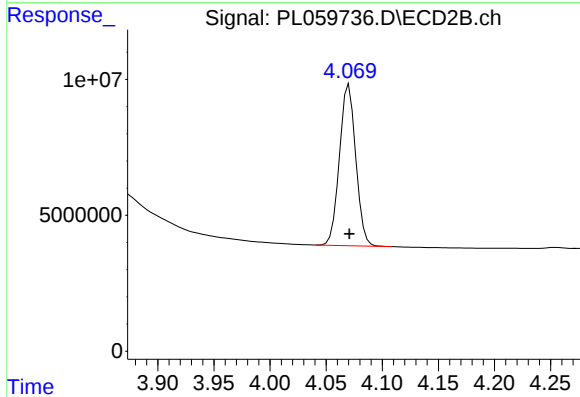


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 59868312
Conc: 22.51 ng/ml

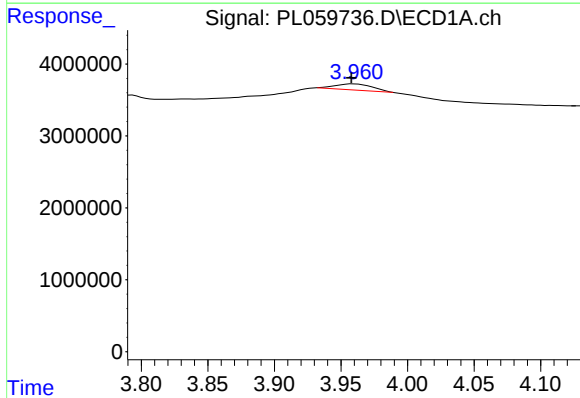


#2 alpha-BHC

R.T.: 3.959 min
Delta R.T.: 0.001 min
Response: 1592600
Conc: 0.62 ng/ml

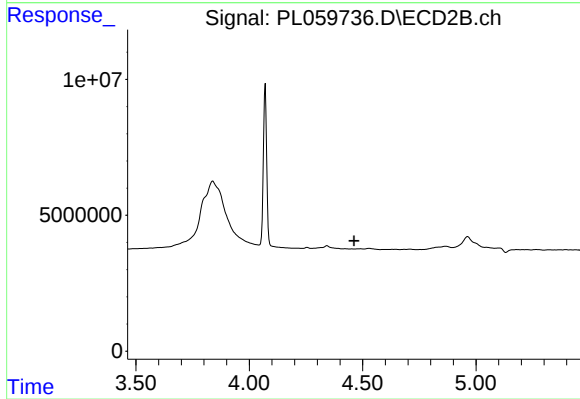

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

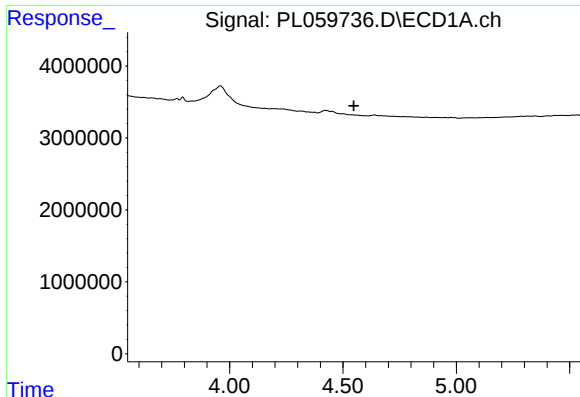

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

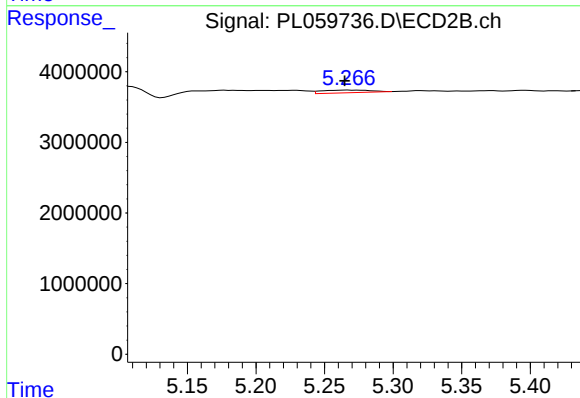


#4 Heptachlor

R.T.: 5.267 min
Delta R.T.: 0.003 min
Response: 938958
Conc: 0.27 ng/ml

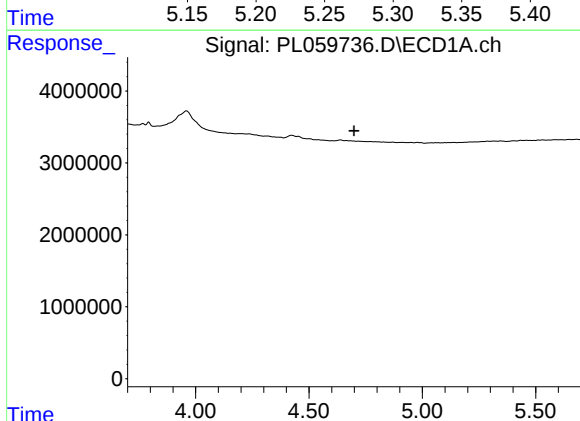


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.699 min
Response: 0
Conc: N.D.

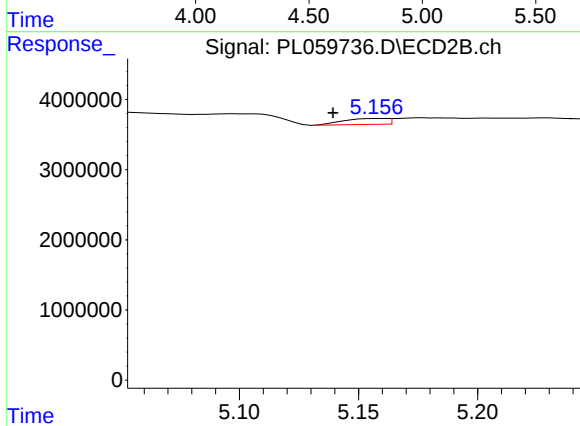

#7 delta-BHC


R.T.: 5.160 min
Delta R.T.: 0.020 min
Response: 1059522
Conc: 0.36 ng/ml

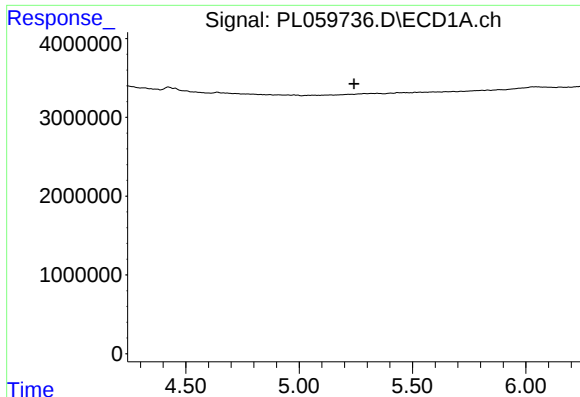

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

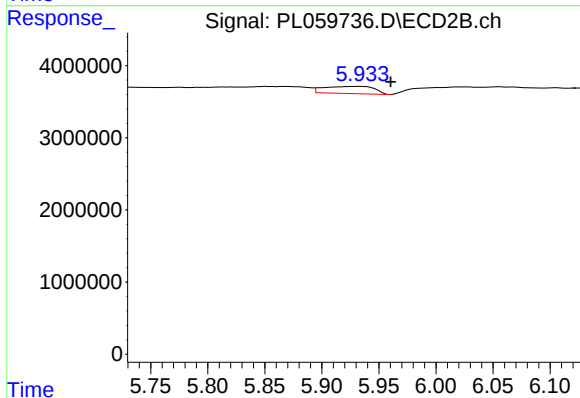


#8 Heptachlor epoxide

R.T.: 5.934 min
Delta R.T.: -0.026 min
Response: 3029756
Conc: 1.25 ng/ml

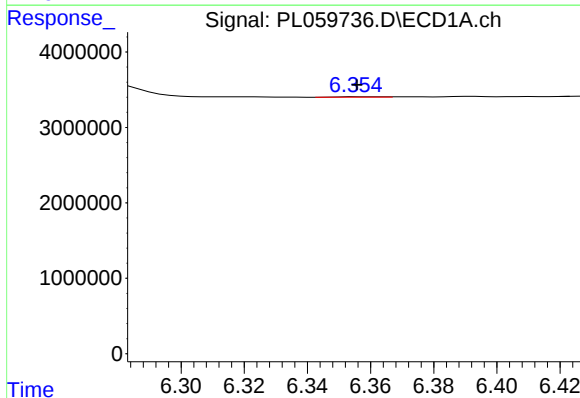


#15 Endosulfan II

R.T.: 6.357 min
Delta R.T.: 0.002 min
Response: 52256
Conc: 0.03 ng/ml

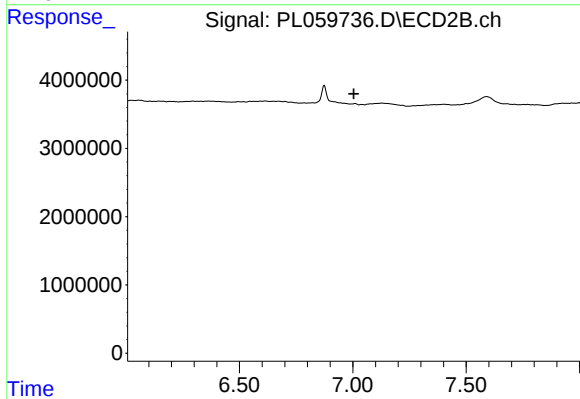

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.005 min
Response: 0
Conc: N.D.

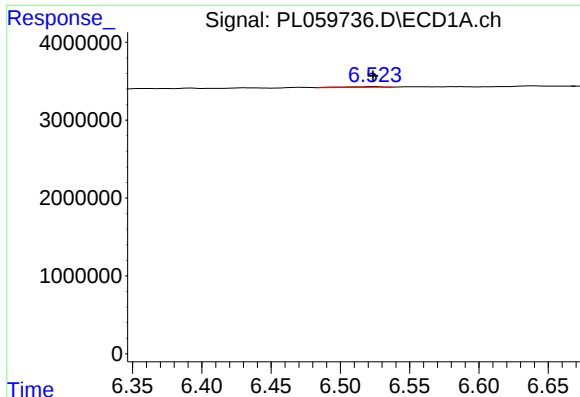

#18 Endrin aldehyde


R.T.: 6.524 min
Delta R.T.: 0.000 min
Response: 170072
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

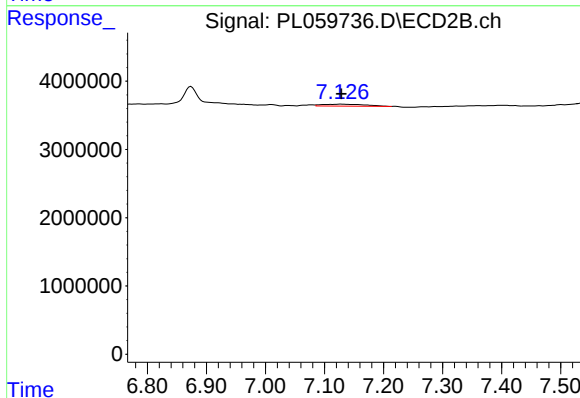


#18 Endrin aldehyde

R.T.: 7.127 min
Delta R.T.: -0.002 min
Response: 1415440
Conc: 0.64 ng/ml

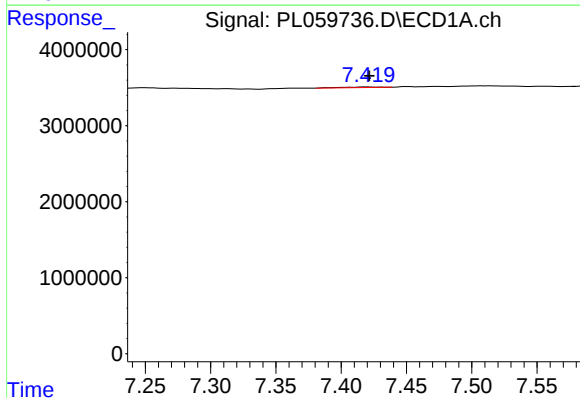


#22 Mirex

R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 169637
Conc: 0.13 ng/ml

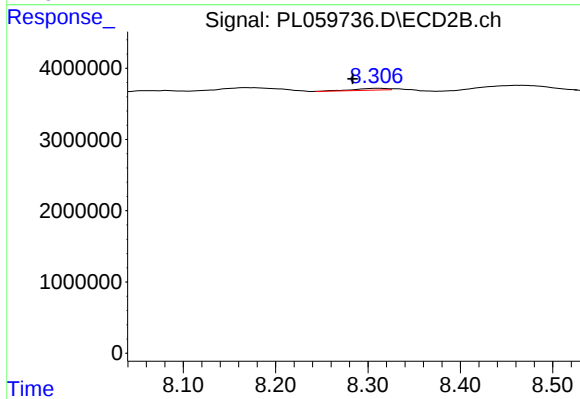

#22 Mirex


R.T.: 8.309 min
Delta R.T.: 0.025 min
Response: 590578
Conc: 0.31 ng/ml

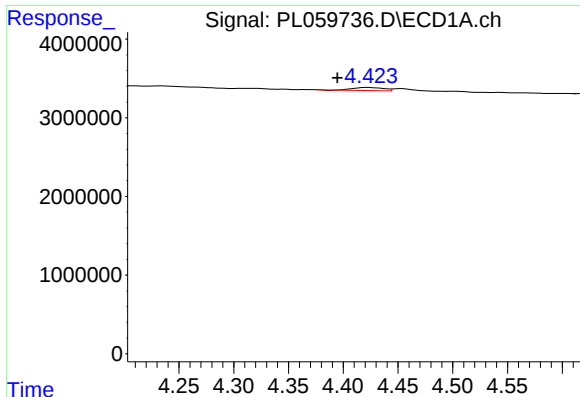

#23 Chlordane-1


R.T.: 4.423 min
Delta R.T.: 0.028 min
Response: 771761
Conc: 14.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

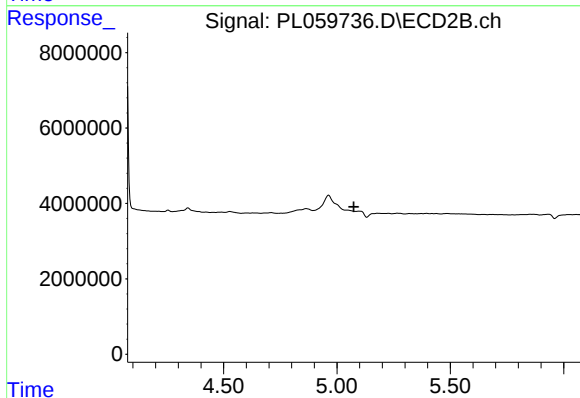


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

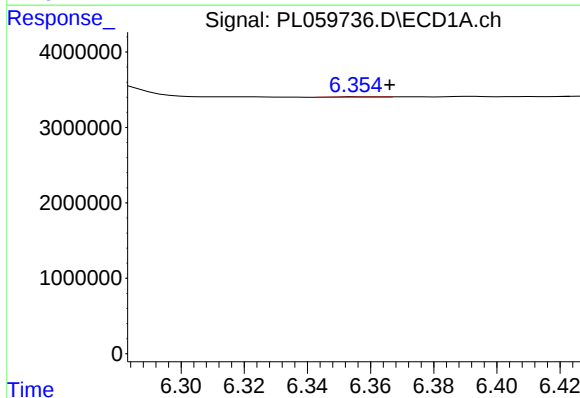


#27 Chlordane-5

R.T.: 6.357 min
Delta R.T.: -0.009 min
Response: 52256
Conc: 1.02 ng/ml

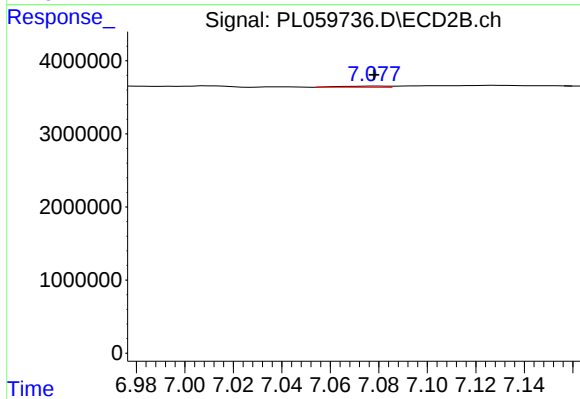

#27 Chlordane-5


R.T.: 7.078 min
Delta R.T.: 0.000 min
Response: 205358
Conc: 2.36 ng/ml

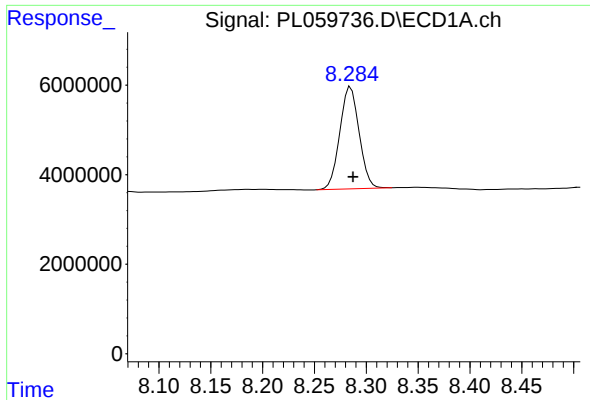

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 29607237
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

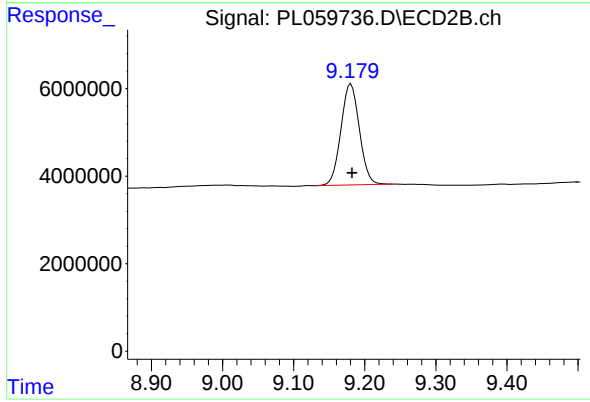

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.001 min
Response: 41642725
Conc: 19.16 ng/ml