

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
 Data File : PL059729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2020 13:06
 Operator : DD\AJ
 Sample : L3202-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-COMP

Manual Integrations
 APPROVED

Ankita
 7/7/2020 1:13:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 17:31:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.516	4.070	26640658	40376370	14.833	15.182
28)	SA Decachlor...	8.285	9.180	23104636	31595265	15.050	14.536
Target Compounds							
10)	B gamma-Chl...	5.467	6.192	852662	1863059	0.521m	0.632m
11)	B alpha-Chl...	5.527	6.268	1102662	1371005	0.672	0.464 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070620\
Data File : PL059729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2020 13:06
Operator : DD\AJ
Sample : L3202-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
7/7/2020 1:13:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 17:31:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

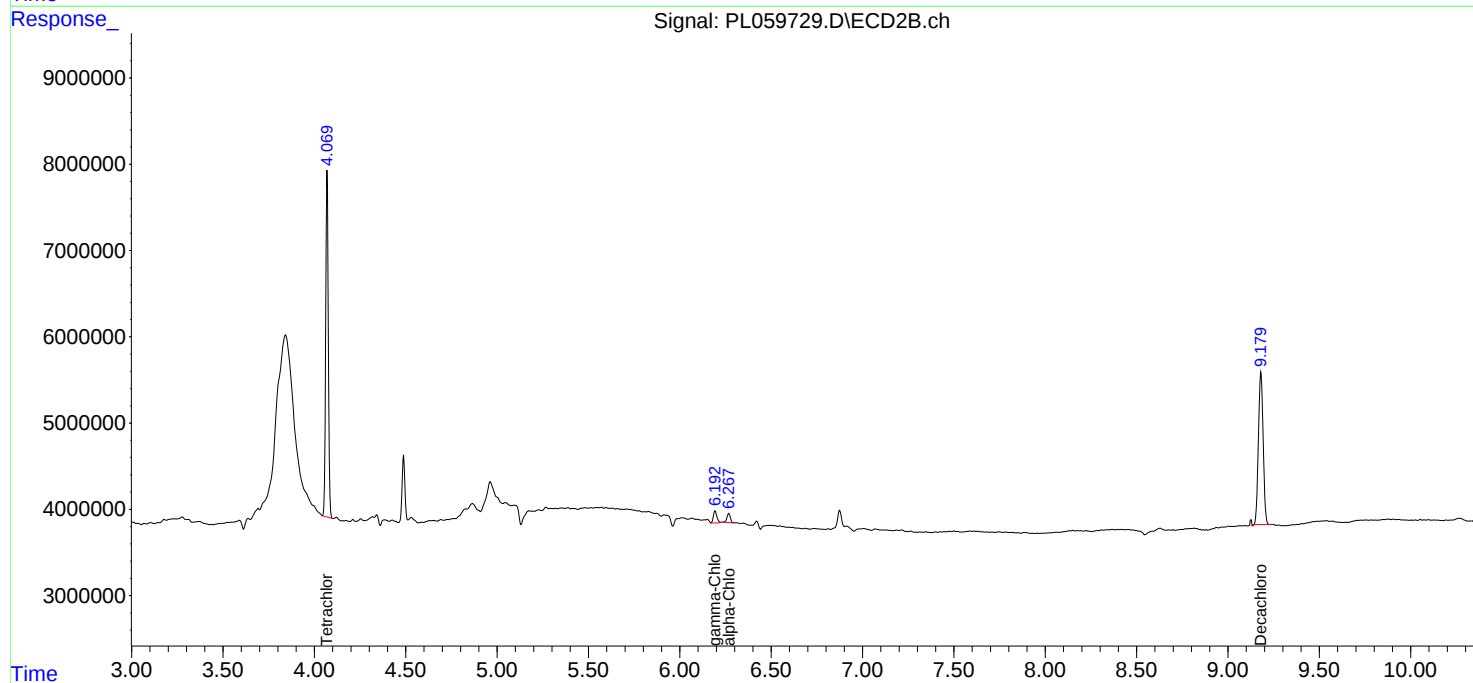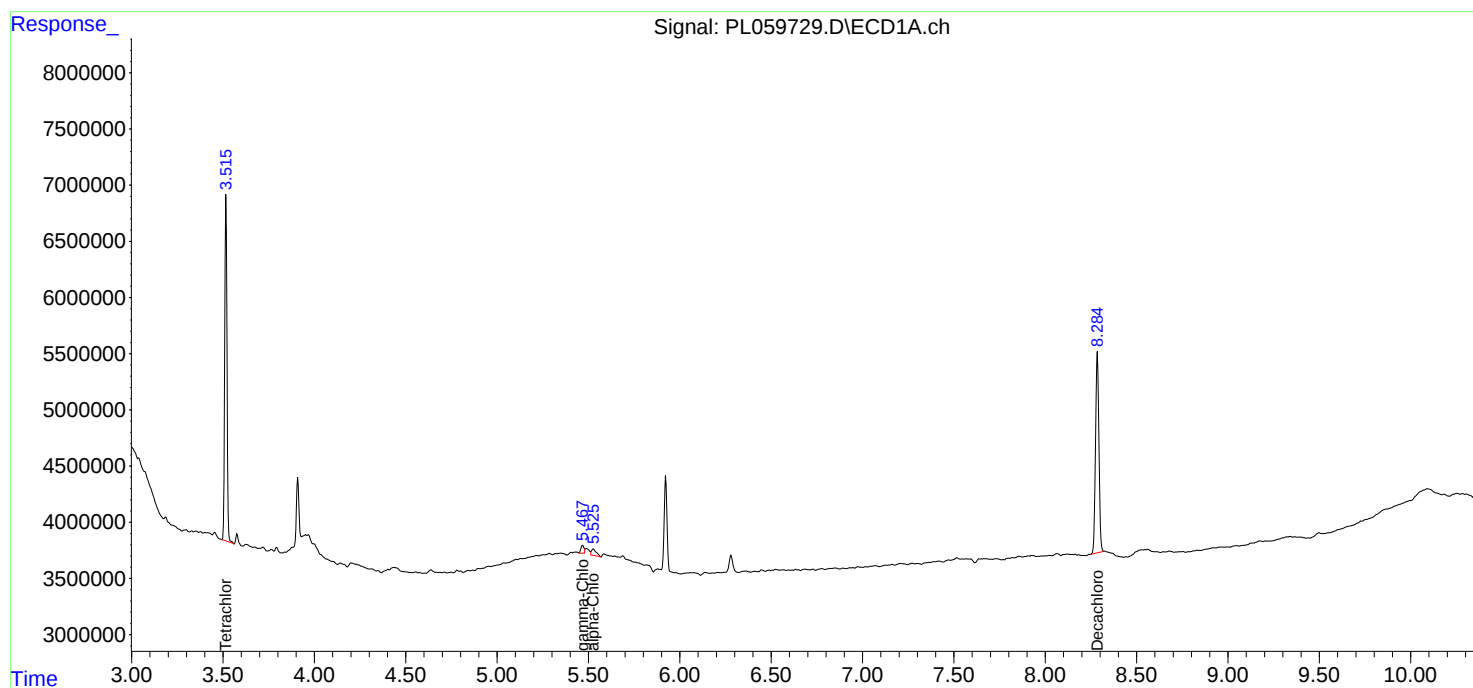

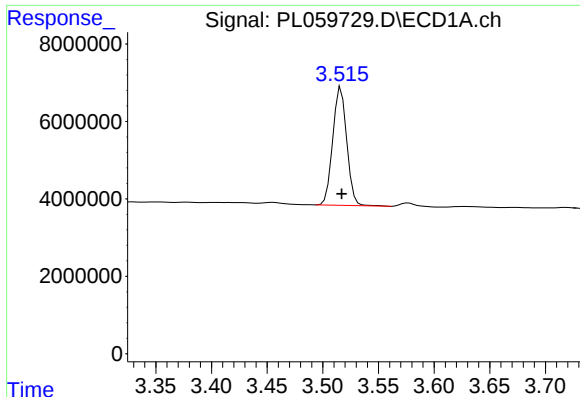


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 26640658
Conc: 14.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
7/7/2020 1:13:11 PM

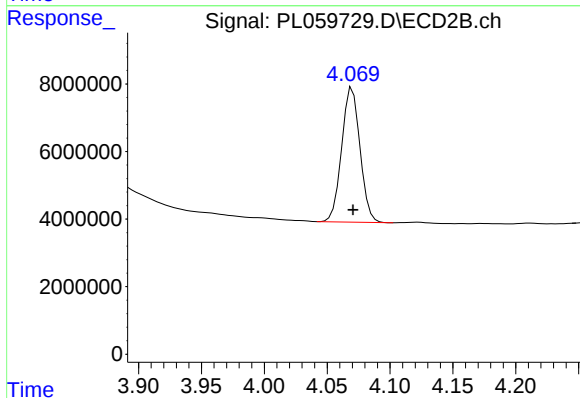


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 40376370
Conc: 15.18 ng/ml

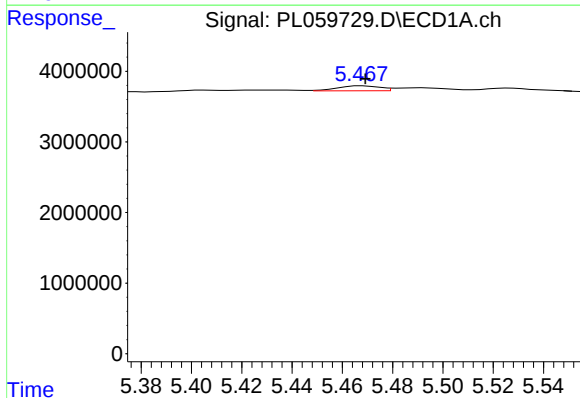


#10 gamma-Chlordane

R.T.: 5.467 min
Delta R.T.: -0.003 min
Response: 852662
Conc: 0.52 ng/ml m

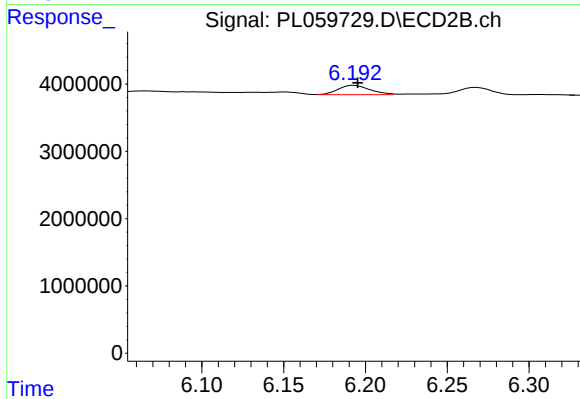

#10 gamma-Chlordane

R.T.: 6.192 min
Delta R.T.: -0.003 min
Response: 1863059
Conc: 0.63 ng/ml m

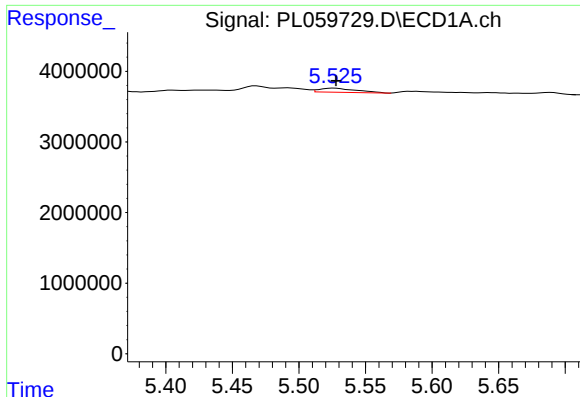


#11 alpha-Chlordane

R.T.: 5.527 min
Delta R.T.: -0.001 min
Response: 1102662
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
7/7/2020 1:13:11 PM

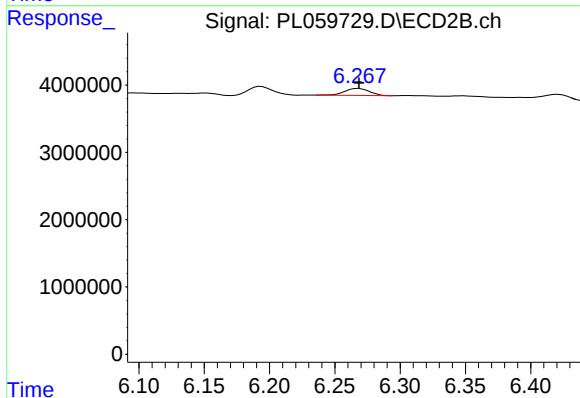


#11 alpha-Chlordane

R.T.: 6.268 min
Delta R.T.: 0.000 min
Response: 1371005
Conc: 0.46 ng/ml

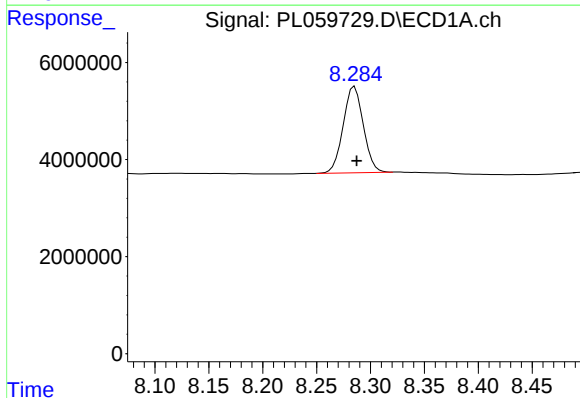

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 23104636
Conc: 15.05 ng/ml

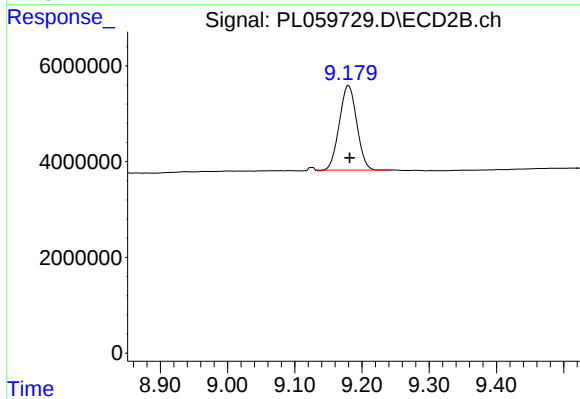

#28 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.001 min
Response: 31595265
Conc: 14.54 ng/ml