

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070621\
 Data File : PL067973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2021 16:07
 Operator : AR\AJ
 Sample : M2932-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DRUM-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 02:00:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.527	9832528	17286025	17.884	18.336
28)	SA Decachlor...	10.216	11.423	7909254	10538596	11.160	10.580
Target Compounds							
2)	A alpha-BHC	0.000	6.131f	0	506145	N.D.	0.409 #
3)	MA gamma-BHC...	5.606	0.000	446422	0	0.596	N.D. #
14)	MA Endrin	7.892	0.000	190973	0	0.291	N.D. #
15)	B Endosulfa...	8.171f	9.176f	222579	356100	0.361	0.447
21)	B Endrin ke...	0.000	10.002f	0	57346	N.D.	0.063 #
22)	Mirex	9.294	0.000	308774	0	0.490	N.D. #
23)	Chlordane-1	0.000	6.940f	0	165986	N.D.	5.878 #
27)	Chlordane-5	8.171f	0.000	222579	0	10.173	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070621\
Data File : PL067973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2021 16:07
Operator : AR\AJ
Sample : M2932-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
DRUM-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 02:00:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

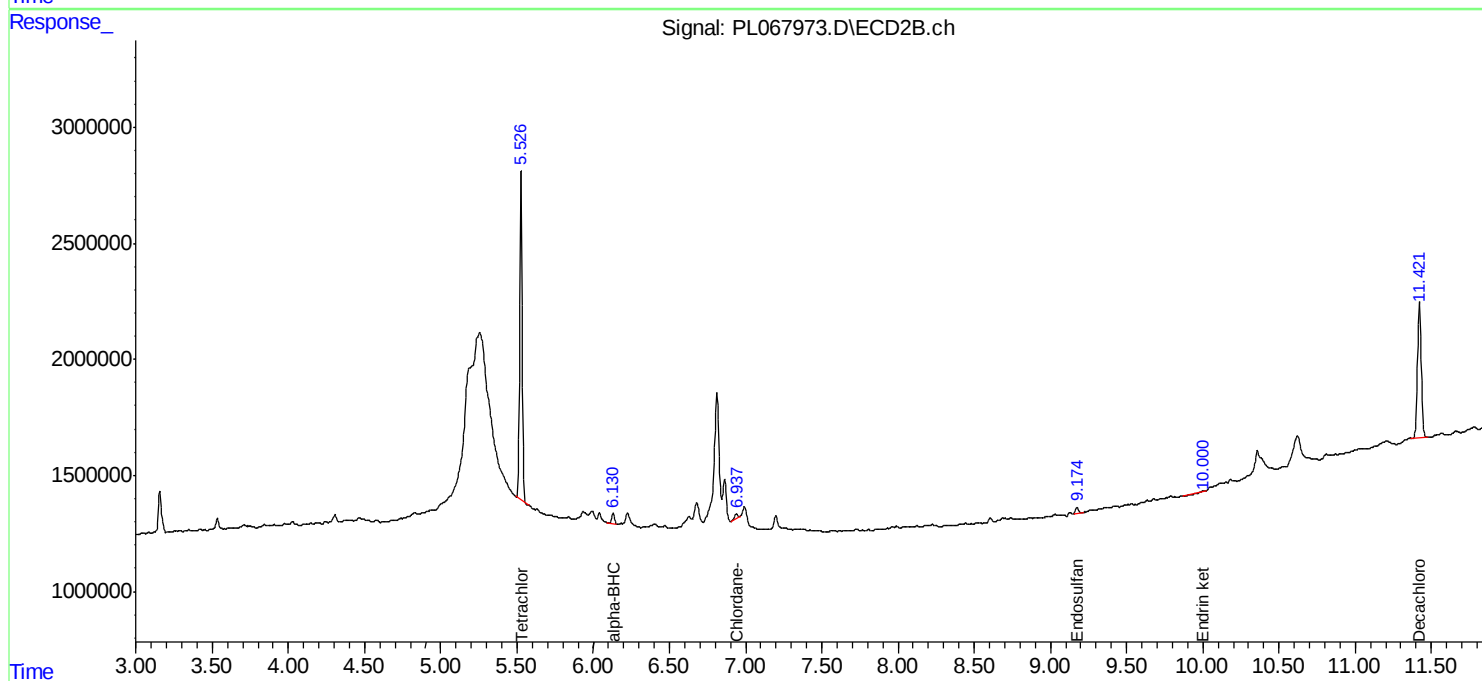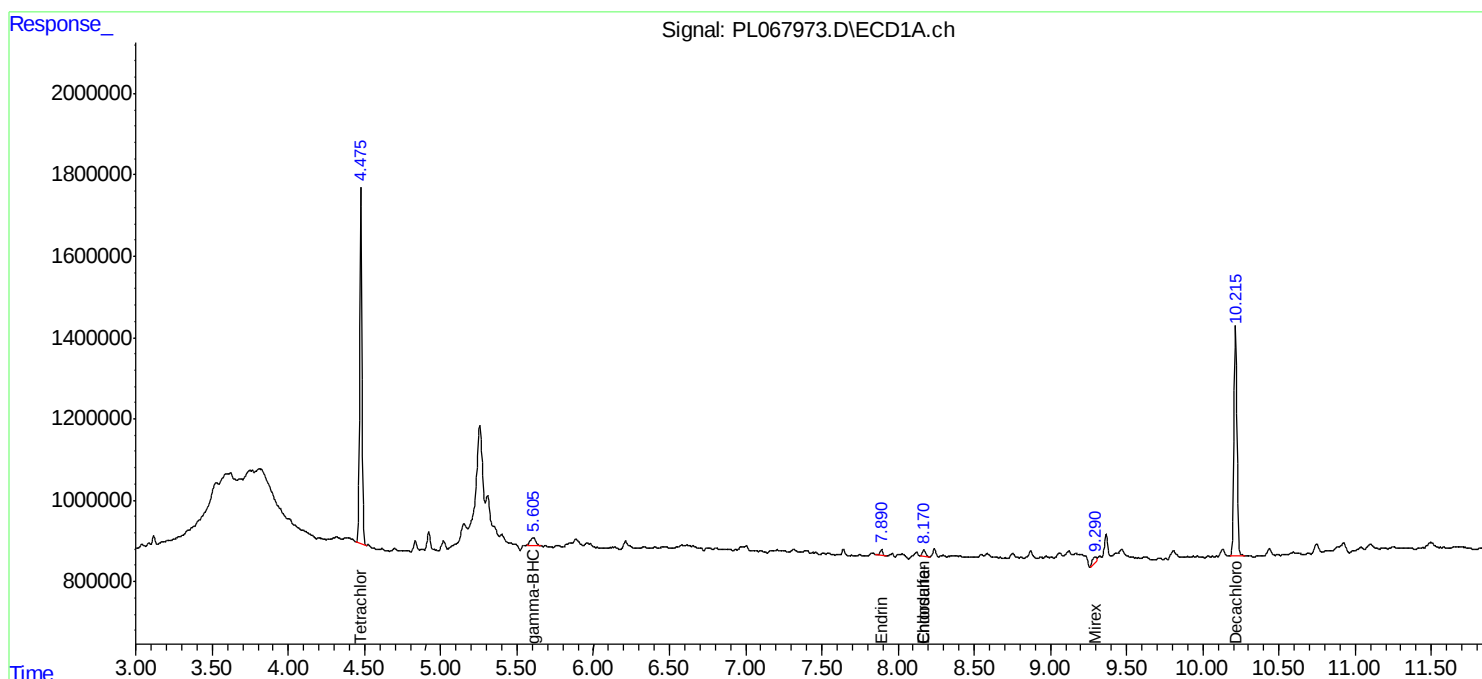


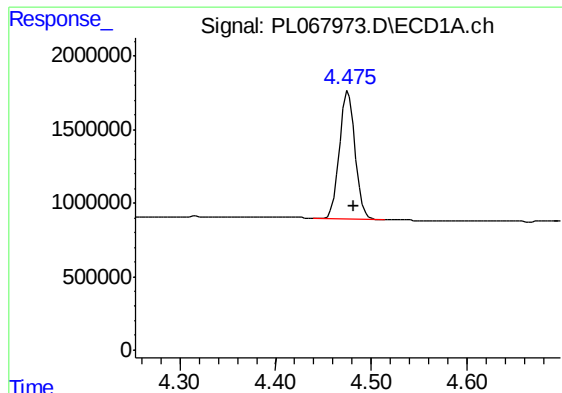

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 9832528
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

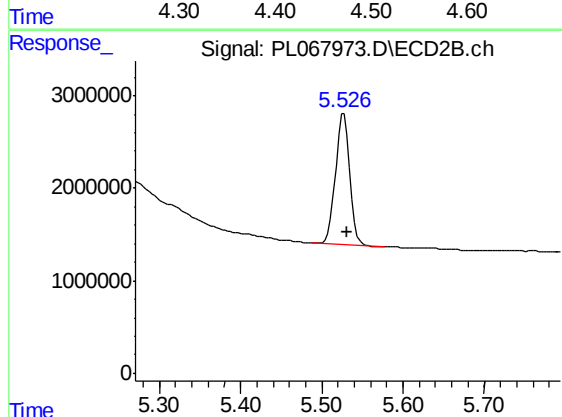


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 17286025
Conc: 18.34 ng/ml

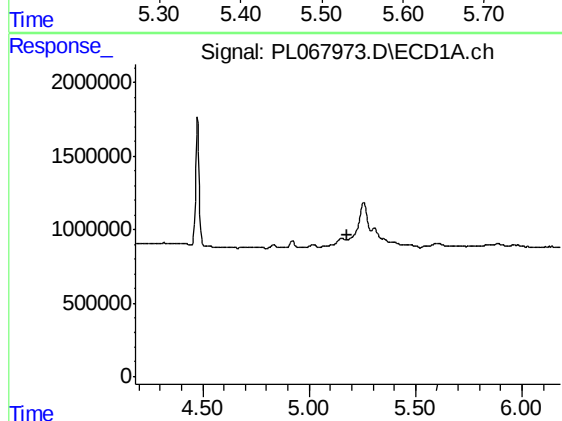


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

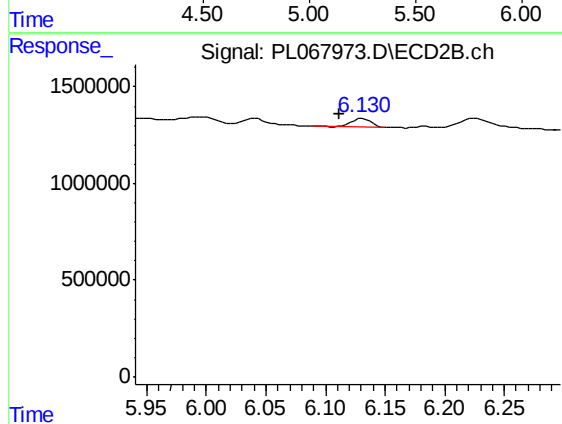

#2 alpha-BHC


R.T.: 6.131 min
Delta R.T.: 0.019 min
Response: 506145
Conc: 0.41 ng/ml

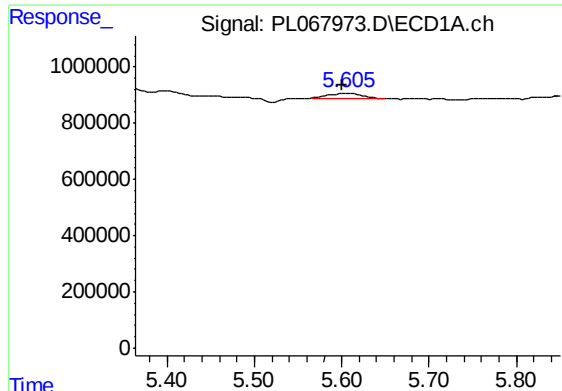

#3 gamma-BHC (Lindane)


R.T.: 5.606 min
Delta R.T.: 0.006 min
Response: 446422
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

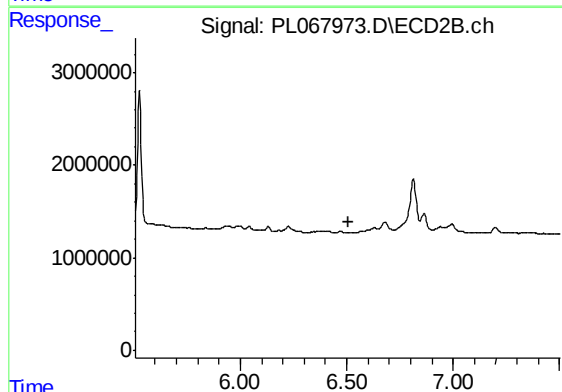


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

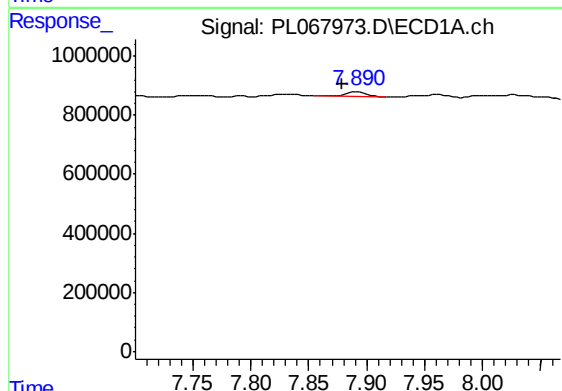


#14 Endrin

R.T.: 7.892 min
Delta R.T.: 0.013 min
Response: 190973
Conc: 0.29 ng/ml

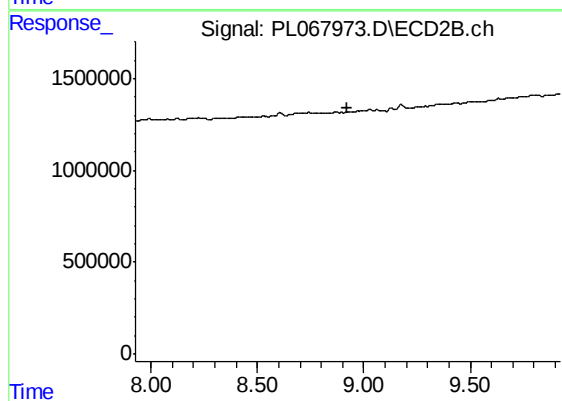

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

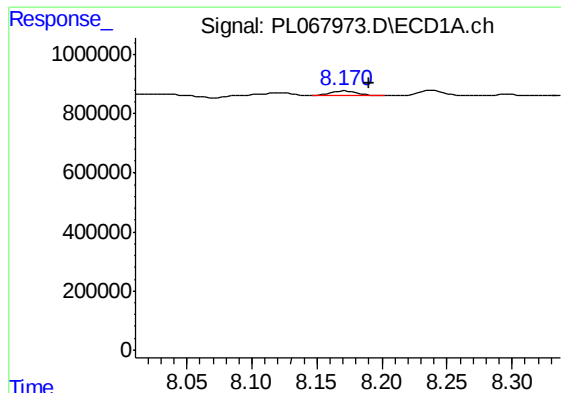

#15 Endosulfan II


R.T.: 8.171 min
Delta R.T.: -0.018 min
Response: 222579
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

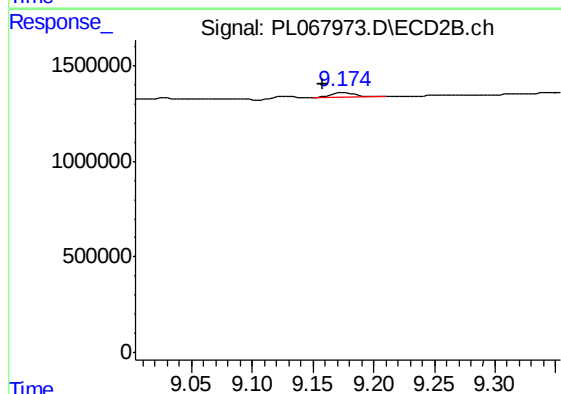


#15 Endosulfan II

R.T.: 9.176 min
Delta R.T.: 0.017 min
Response: 356100
Conc: 0.45 ng/ml

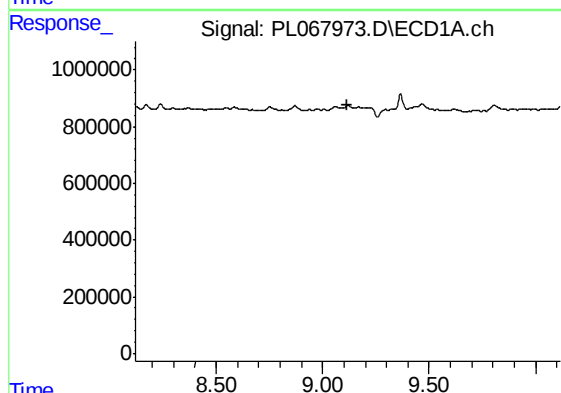


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

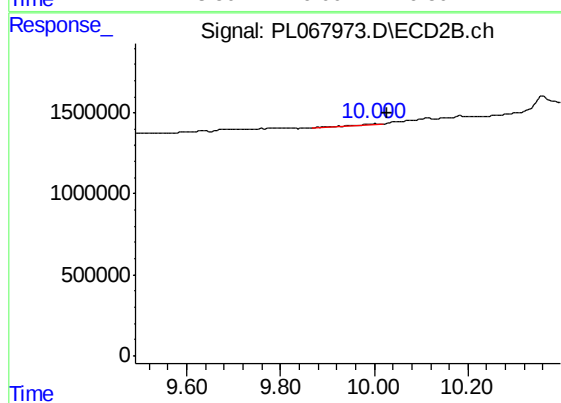

#21 Endrin ketone


R.T.: 10.002 min
Delta R.T.: -0.025 min
Response: 57346
Conc: 0.06 ng/ml

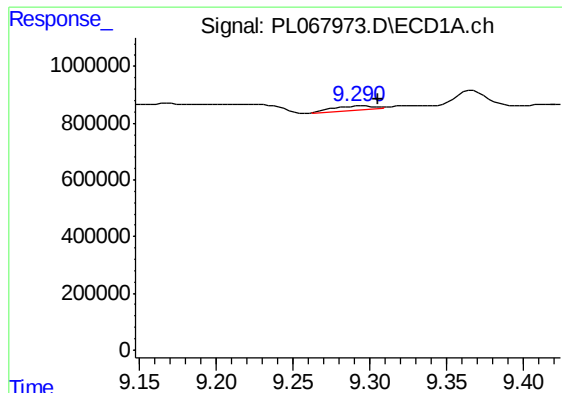

#22 Mirex


R.T.: 9.294 min
Delta R.T.: -0.012 min
Response: 308774
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

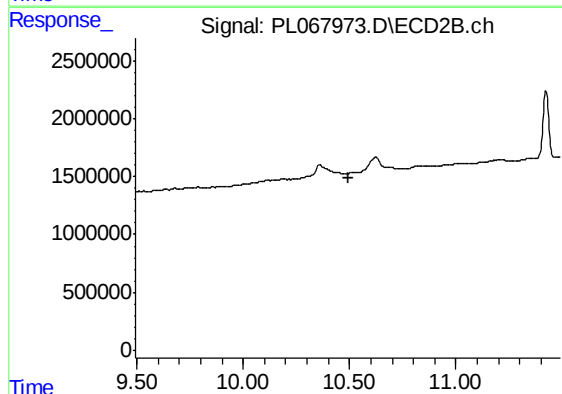


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.492 min
Response: 0
Conc: N.D.

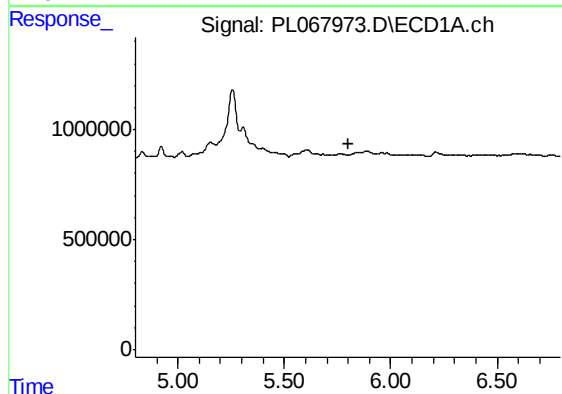


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.800 min
Response: 0
Conc: N.D.

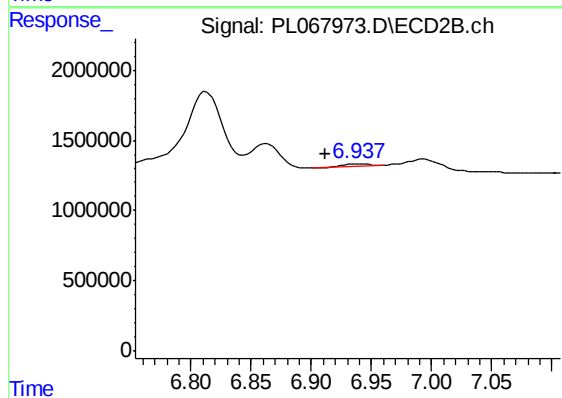

#23 Chlordane-1


R.T.: 6.940 min
Delta R.T.: 0.028 min
Response: 165986
Conc: 5.88 ng/ml

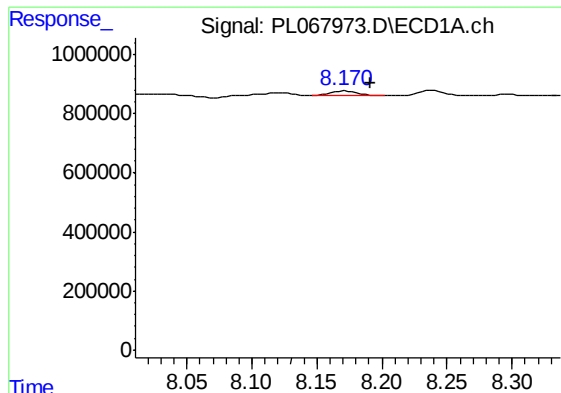

#27 Chlordane-5


R.T.: 8.171 min
Delta R.T.: -0.019 min
Response: 222579
Conc: 10.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

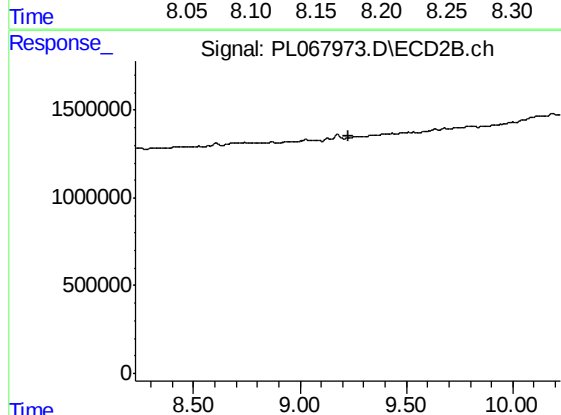


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

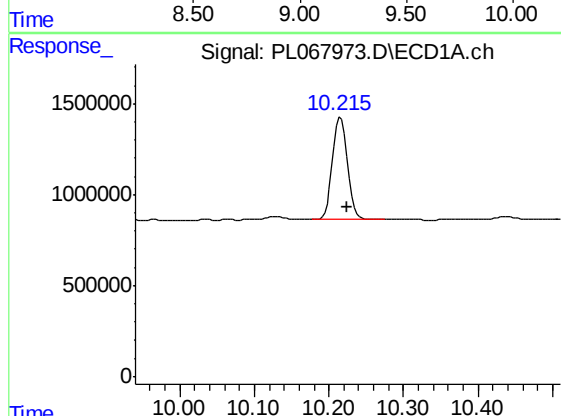

#28 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.008 min
Response: 7909254
Conc: 11.16 ng/ml

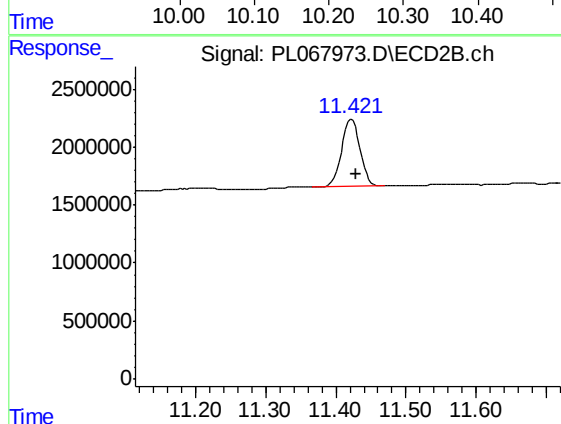

#28 Decachlorobiphenyl

R.T.: 11.423 min
Delta R.T.: -0.006 min
Response: 10538596
Conc: 10.58 ng/ml