

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070622\
 Data File : PL076261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2022 10:17
 Operator : AR\AJ
 Sample : N3564-21RE 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-16-2-5RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/07/2022
 Supervised By : Ankita Jodhani 07/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 00:07:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.637	4.625	995159	2110162	1.316m	1.113
28) SA Decachlor...	11.624	10.362	11988138	27519930	19.051m	17.918

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070622\
Data File : PL076261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2022 10:17
Operator : AR\AJ
Sample : N3564-21RE 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-16-2-5RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/07/2022
Supervised By : Ankita Jodhani 07/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 00:07:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

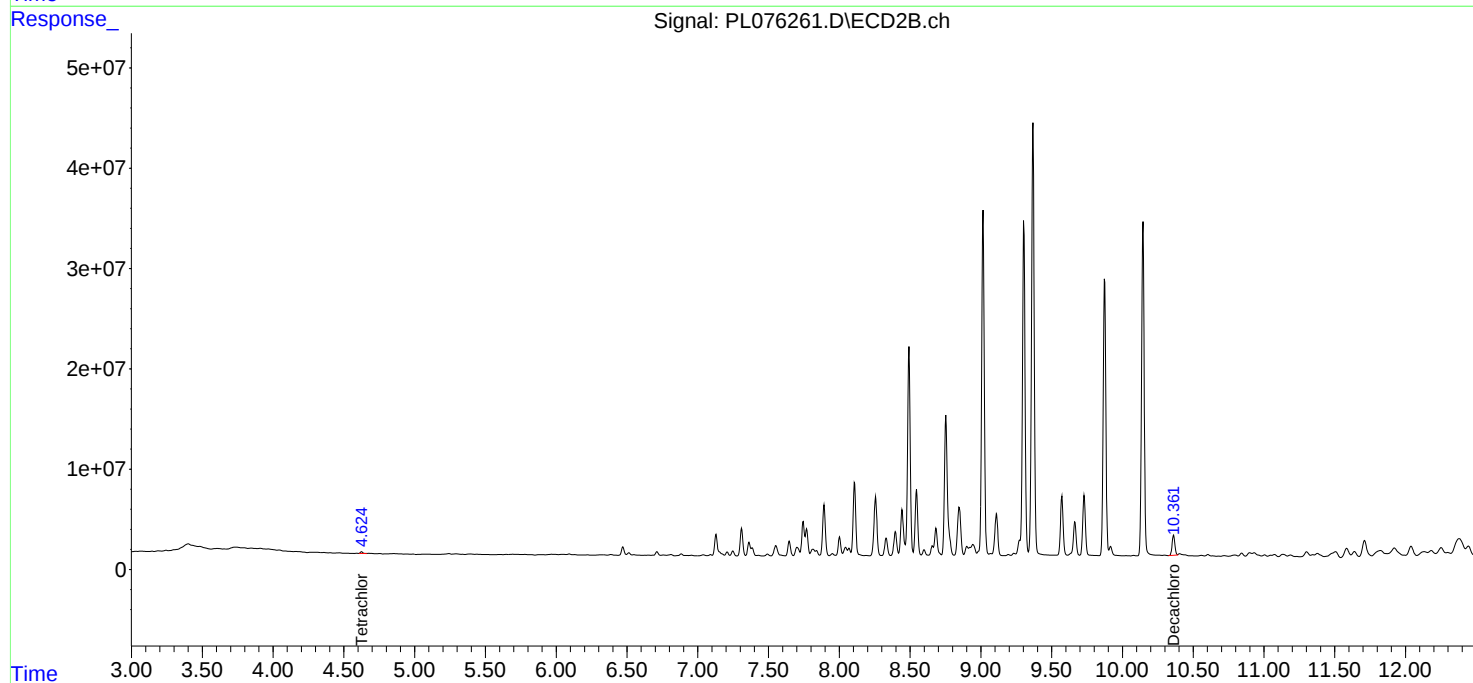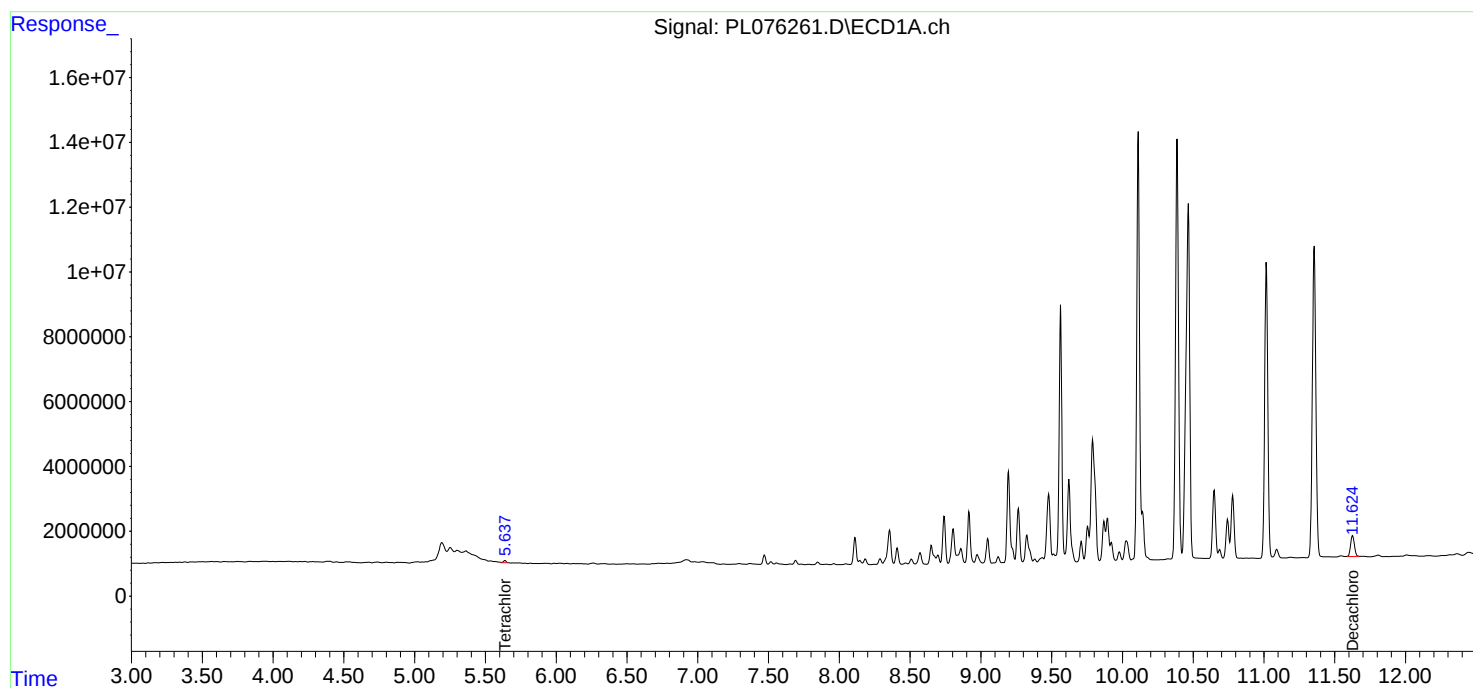

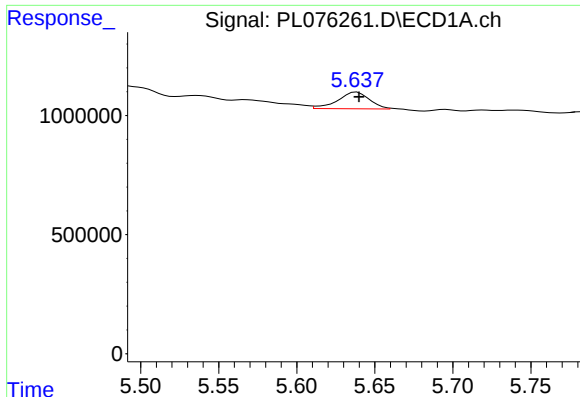


#1 Tetrachloro-m-xylene

R.T.: 5.637 min
Delta R.T.: -0.003 min
Response: 995159
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-16-2-5RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/07/2022
Supervised By :Ankita Jodhani 07/07/2022

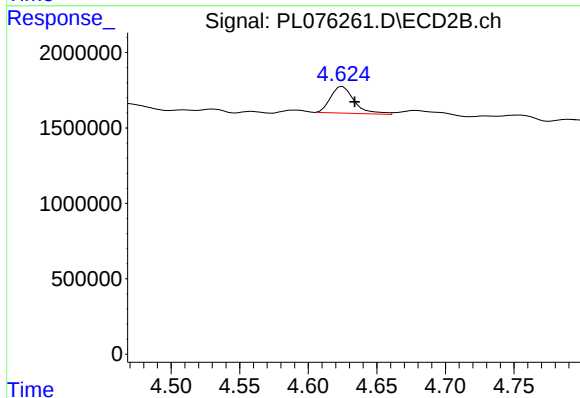


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.009 min
Response: 2110162
Conc: 1.11 ng/ml

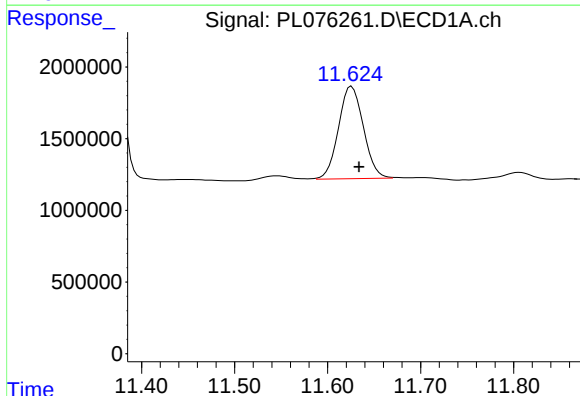

#28 Decachlorobiphenyl

R.T.: 11.624 min
Delta R.T.: -0.009 min
Response: 11988138
Conc: 19.05 ng/ml m

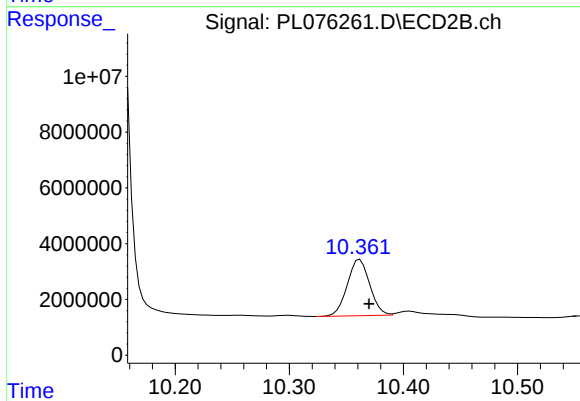

#28 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: -0.008 min
Response: 27519930
Conc: 17.92 ng/ml