

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070720\
 Data File : PL059748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 13:43
 Operator : DD\AJ
 Sample : L3230-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-C4-D4-C4A-D4A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 18:37:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.516	4.070	44972641	66726365	25.040	25.091
28)	SA Decachlor...	8.285	9.180	36076241	48732532	23.499	22.420

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070720\
Data File : PL059748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 13:43
Operator : DD\AJ
Sample : L3230-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-C4-D4-C4A-D4A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 18:37:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

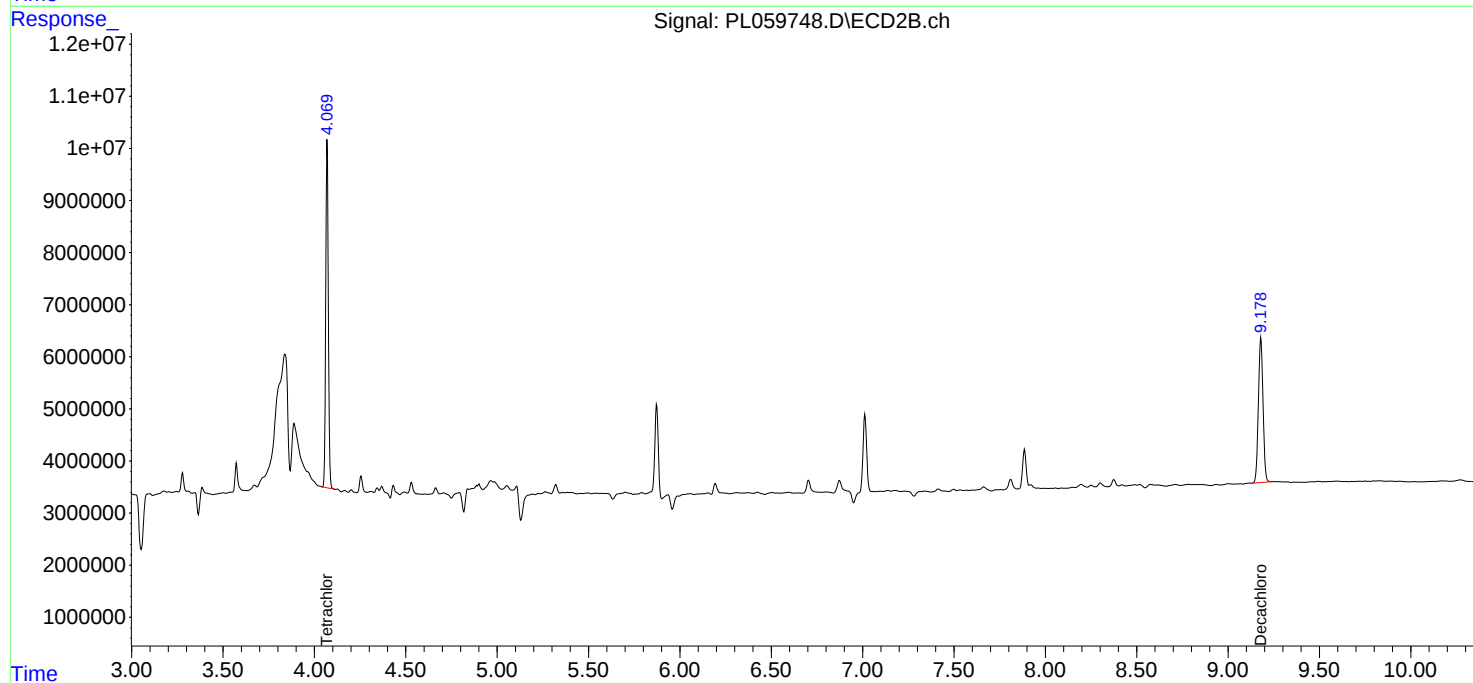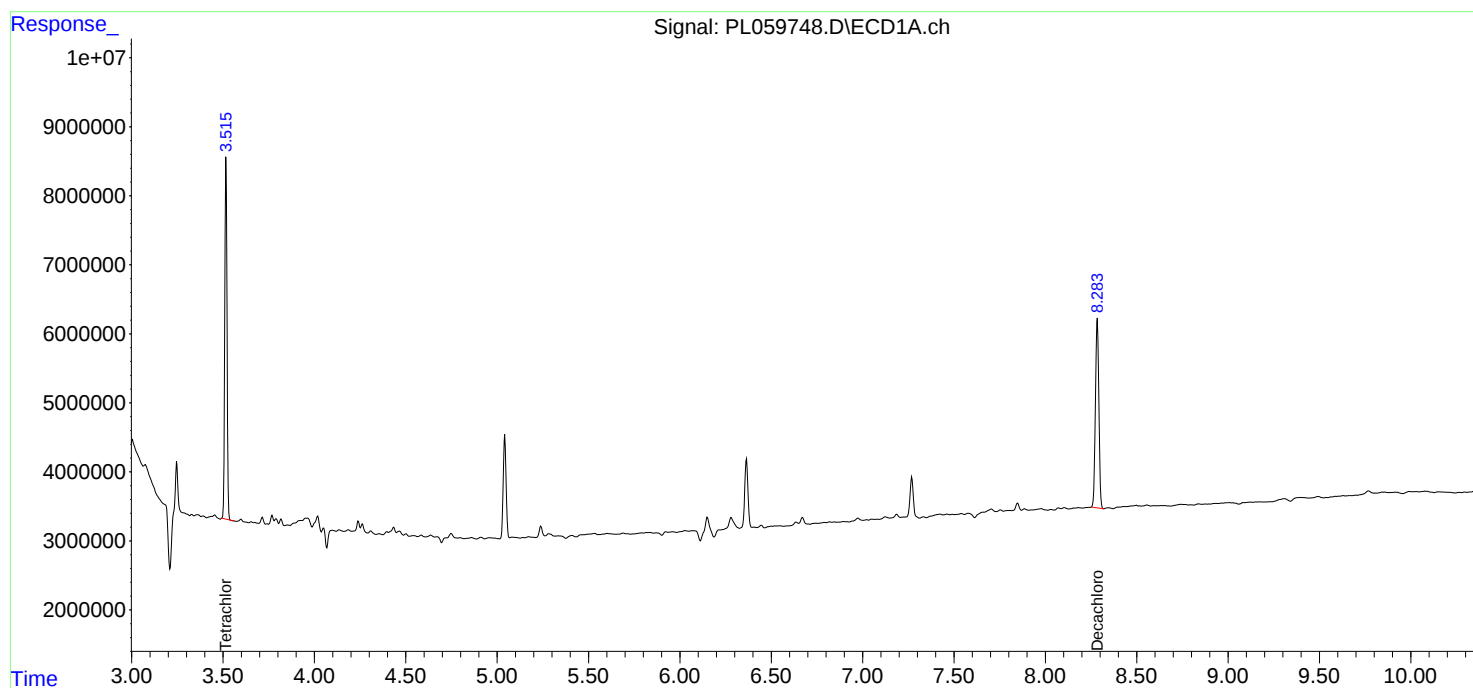


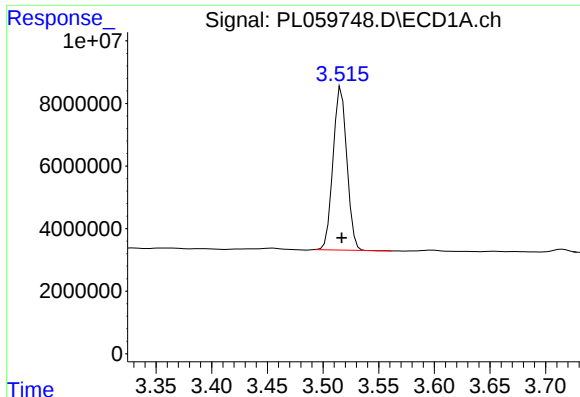

#1 Tetrachloro-m-xylene


R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 44972641
Conc: 25.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-C4-D4-C4A-D4A

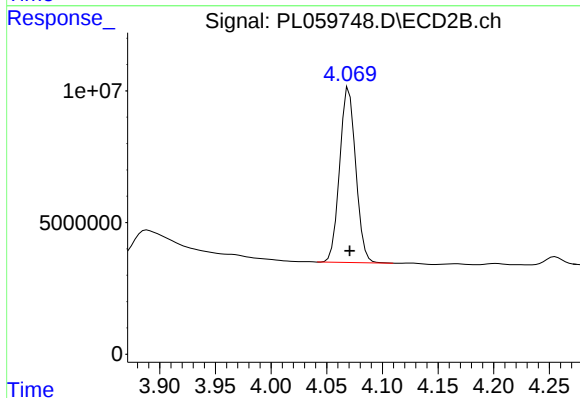


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 66726365
Conc: 25.09 ng/ml

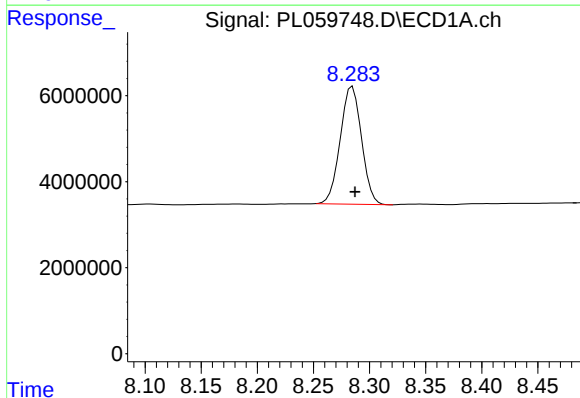

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 36076241
Conc: 23.50 ng/ml

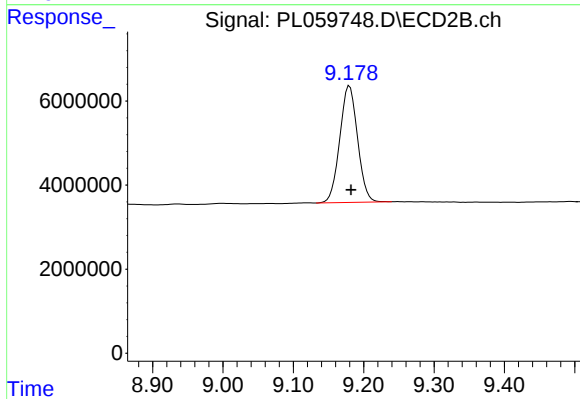

#28 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.002 min
Response: 48732532
Conc: 22.42 ng/ml