

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
 Data File : PL076308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 16:32
 Operator : AR\AJ
 Sample : N3584-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 23:59:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.637	4.625	4657444	12703754	6.158	6.698
28)	SA Decachlor...	11.624	10.360	2388890	7026933	3.796	4.575
Target Compounds							
2)	A alpha-BHC	0.000	5.338	0	9020511	N.D.	3.691 #
3)	MA gamma-BHC...	0.000	5.757	0	58800	N.D.	0.025 #
4)	MA Heptachlor	7.305f	0.000	951941	0	1.038	N.D. #
9)	A Endosulfan I	0.000	7.477	0	289510	N.D.	0.165 #
14)	MA Endrin	0.000	8.045	0	271692	N.D.	0.179 #
15)	B Endosulfa...	9.297	0.000	280188	0	0.442	N.D. #
17)	MA 4,4'-DDT	9.513	8.447f	248748	631071	0.407	0.427
21)	B Endrin ke...	10.177	0.000	771940	0	1.071	N.D. #
23)	Chlordane-1	7.042	0.000	562458	0	22.224	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
Data File : PL076308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 16:32
Operator : AR\AJ
Sample : N3584-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 23:59:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

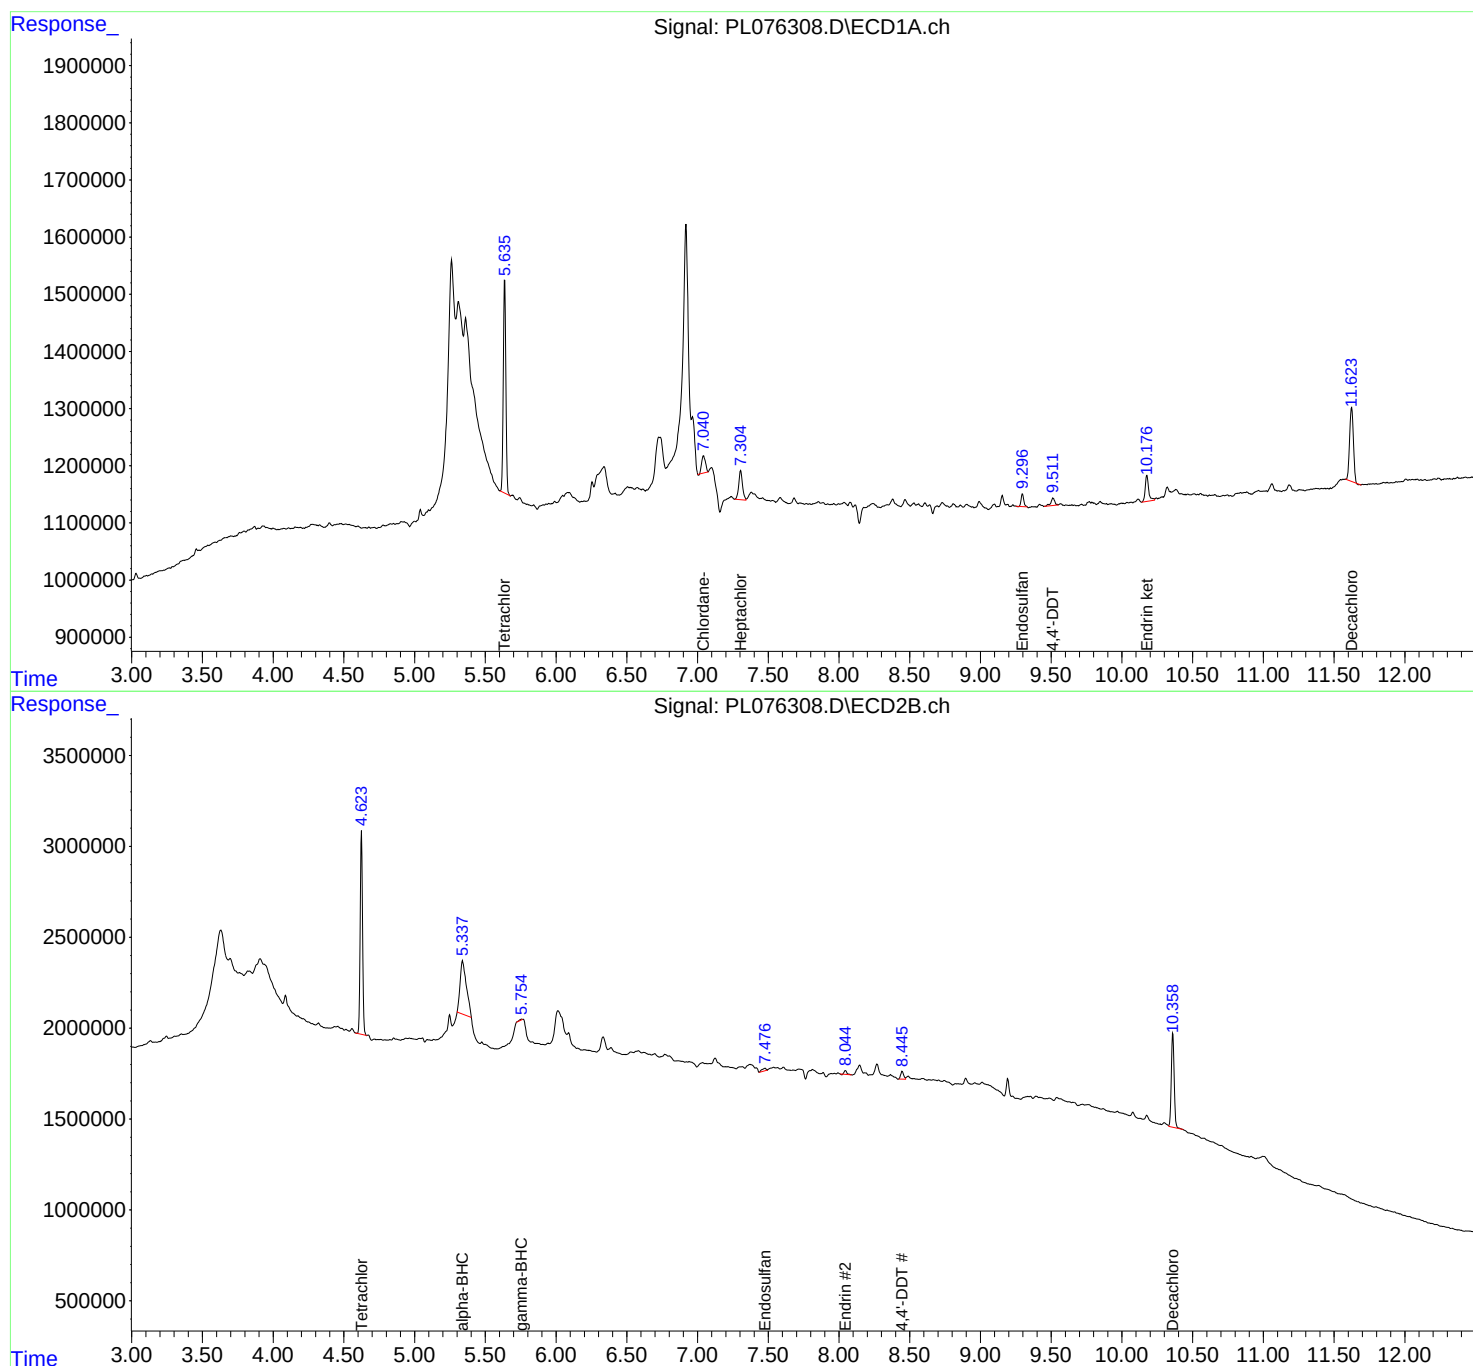


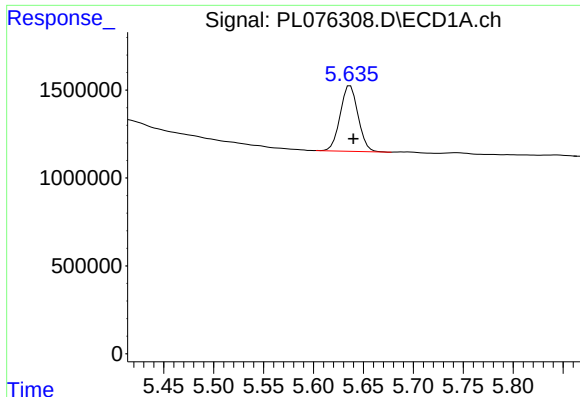

#1 Tetrachloro-m-xylene


R.T.: 5.637 min
Delta R.T.: -0.003 min
Response: 4657444
Conc: 6.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

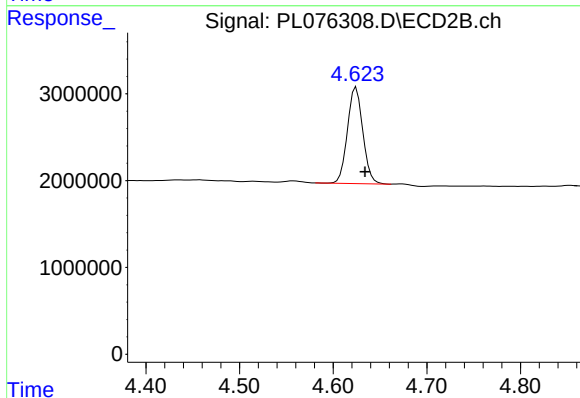


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.009 min
Response: 12703754
Conc: 6.70 ng/ml

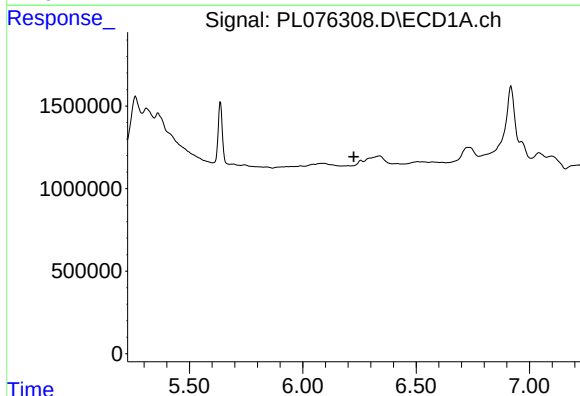


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

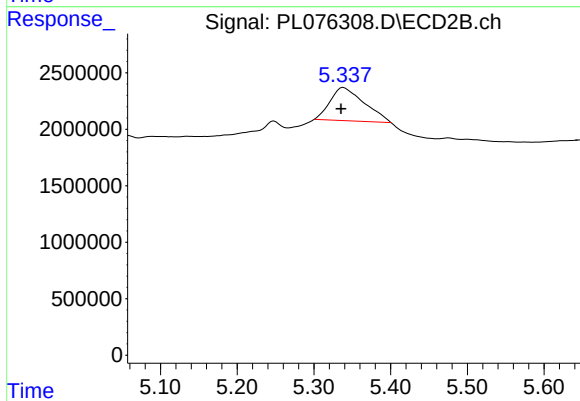

#2 alpha-BHC


R.T.: 5.338 min
Delta R.T.: 0.003 min
Response: 9020511
Conc: 3.69 ng/ml

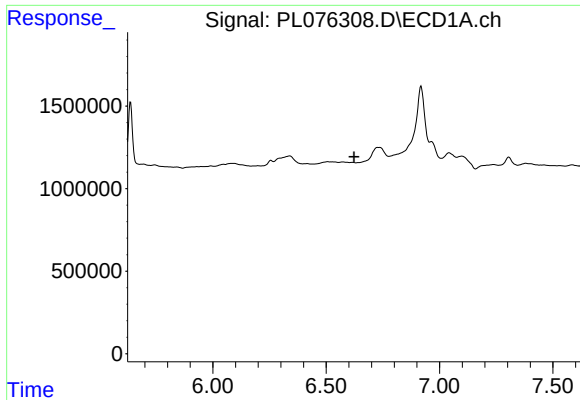

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

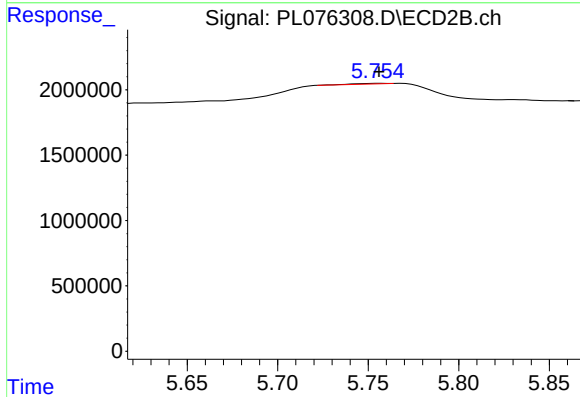


#3 gamma-BHC (Lindane)

R.T.: 5.757 min
Delta R.T.: 0.000 min
Response: 58800
Conc: 0.03 ng/ml

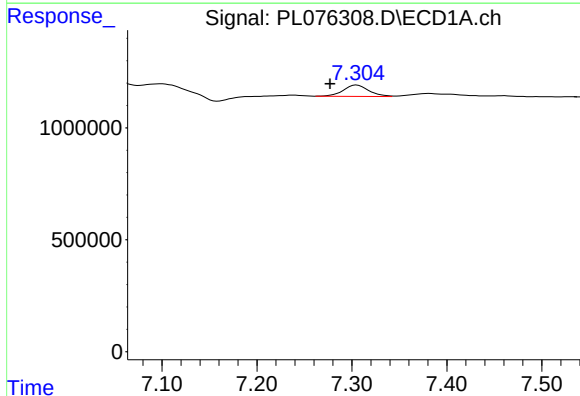


#4 Heptachlor

R.T.: 7.305 min
Delta R.T.: 0.028 min
Response: 951941
Conc: 1.04 ng/ml

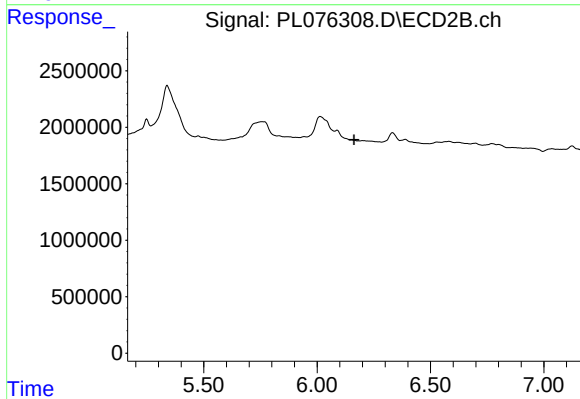

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

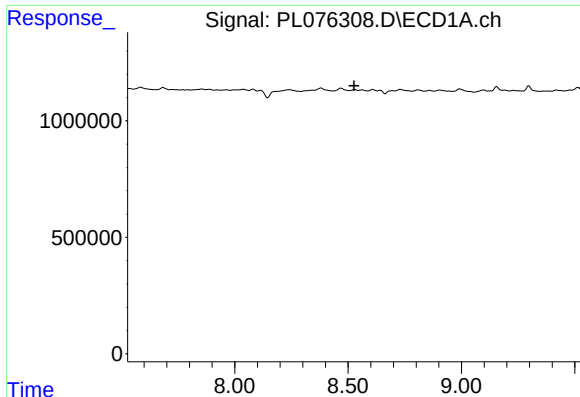

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

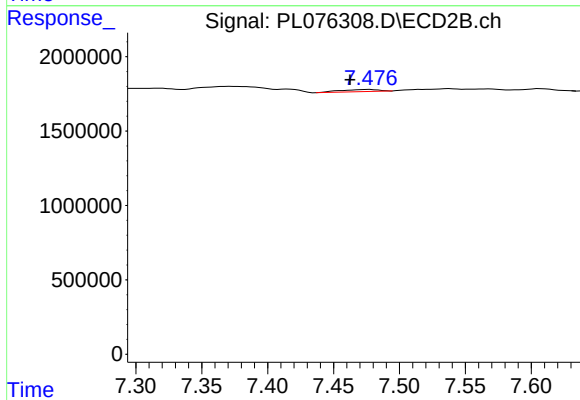


#9 Endosulfan I

R.T.: 7.477 min
Delta R.T.: 0.015 min
Response: 289510
Conc: 0.16 ng/ml

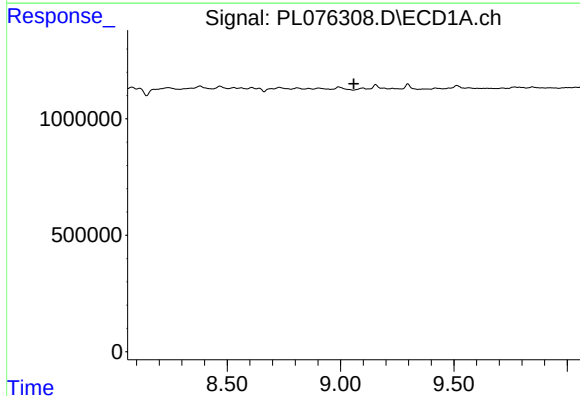


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

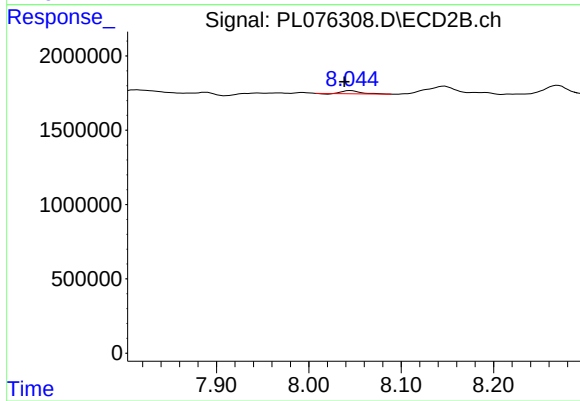

#14 Endrin


R.T.: 8.045 min
Delta R.T.: 0.007 min
Response: 271692
Conc: 0.18 ng/ml

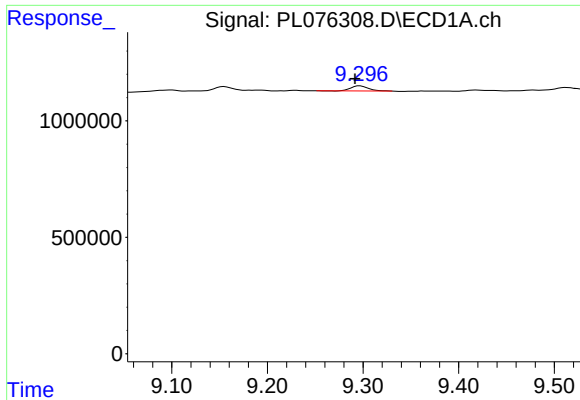

#15 Endosulfan II


R.T.: 9.297 min
Delta R.T.: 0.005 min
Response: 280188
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

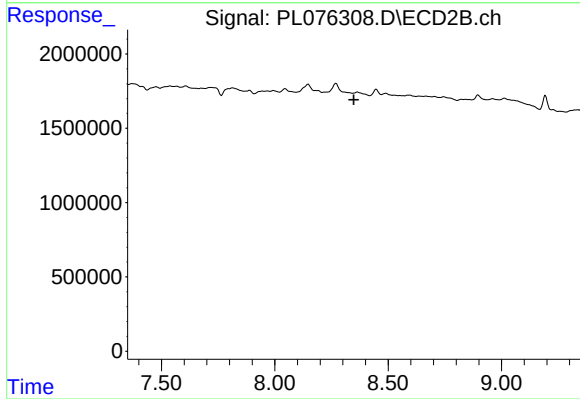


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

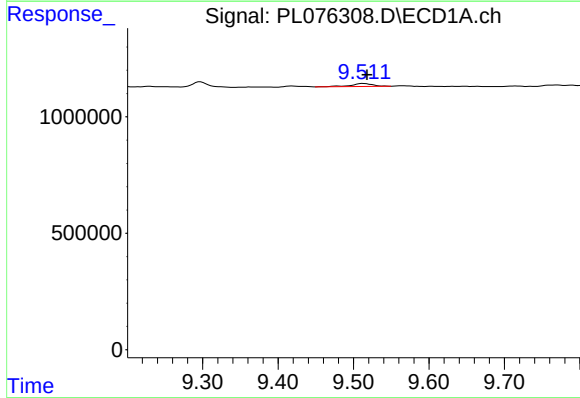


#17 4,4'-DDT

R.T.: 9.513 min
Delta R.T.: -0.005 min
Response: 248748
Conc: 0.41 ng/ml

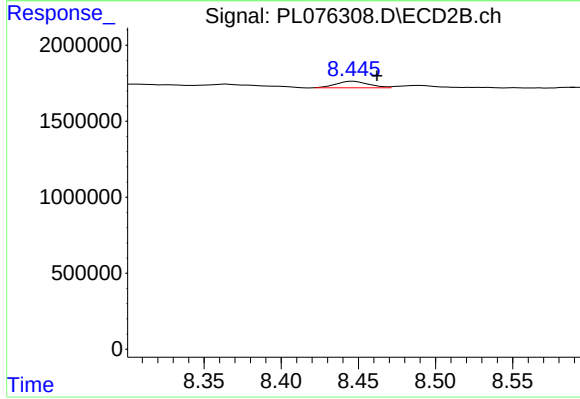

#17 4,4'-DDT


R.T.: 8.447 min
Delta R.T.: -0.015 min
Response: 631071
Conc: 0.43 ng/ml

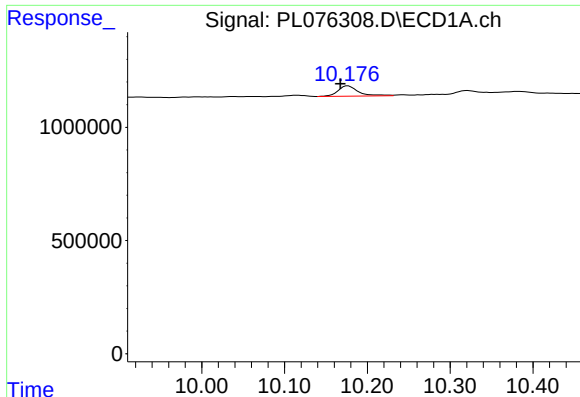

#21 Endrin ketone


R.T.: 10.177 min
Delta R.T.: 0.009 min
Response: 771940
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

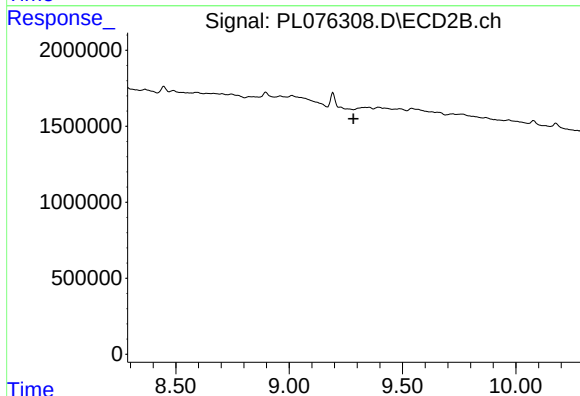


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

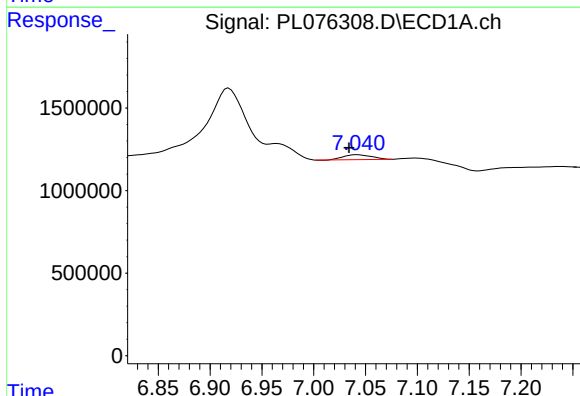


#23 Chlordane-1

R.T.: 7.042 min
Delta R.T.: 0.008 min
Response: 562458
Conc: 22.22 ng/ml

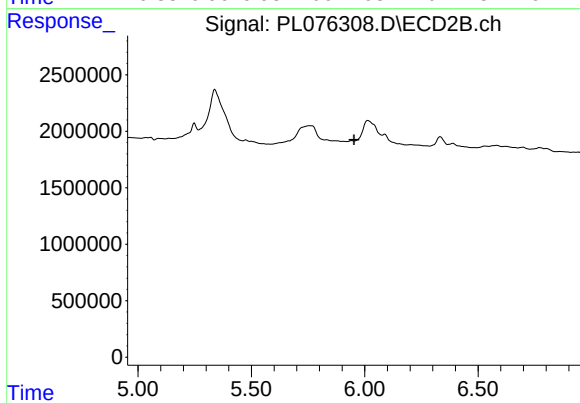

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

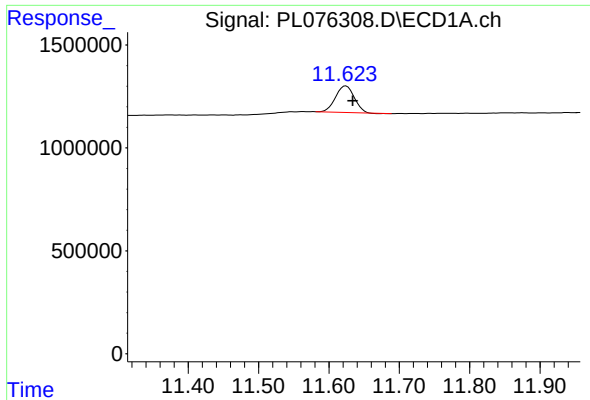

#28 Decachlorobiphenyl

R.T.: 11.624 min
Delta R.T.: -0.010 min
Response: 2388890
Conc: 3.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

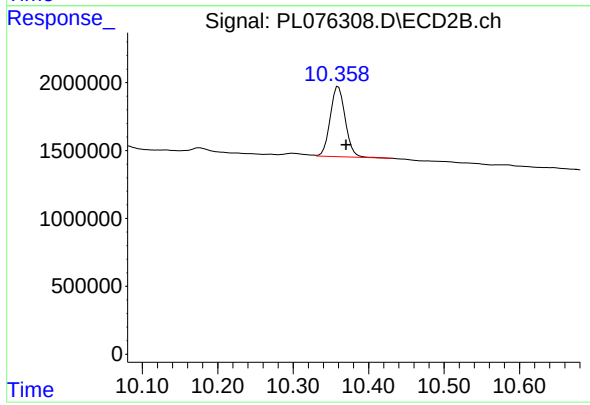

#28 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.010 min
Response: 7026933
Conc: 4.58 ng/ml