

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
 Data File : PL076313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 17:56
 Operator : AR\AJ
 Sample : N3597-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 00:02:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.638	4.625	5656773	16629261	7.479	8.768
28)	SA Decachlor...	11.623	10.360	3136481	9878950	4.984	6.432 #
Target Compounds							
4)	MA Heptachlor	7.304f	6.184f	286955	260201	0.313	0.115 #
7)	B delta-BHC	0.000	6.392	0	281654	N.D.	0.125 #
15)	B Endosulfa...	9.297	0.000	279505	0	0.441	N.D. #
16)	A 4,4'-DDD	9.222f	0.000	203892	0	0.360	N.D. #
17)	MA 4,4'-DDT	9.533f	8.490f	72765	1154578	0.119	0.781 #
19)	B Endosulfa...	0.000	8.773	0	384178	N.D.	0.250 #
21)	B Endrin ke...	10.177	0.000	1381324	0	1.916	N.D. #
23)	Chlordane-1	7.038	0.000	280728	0	11.092	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
Data File : PL076313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 17:56
Operator : AR\AJ
Sample : N3597-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 00:02:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

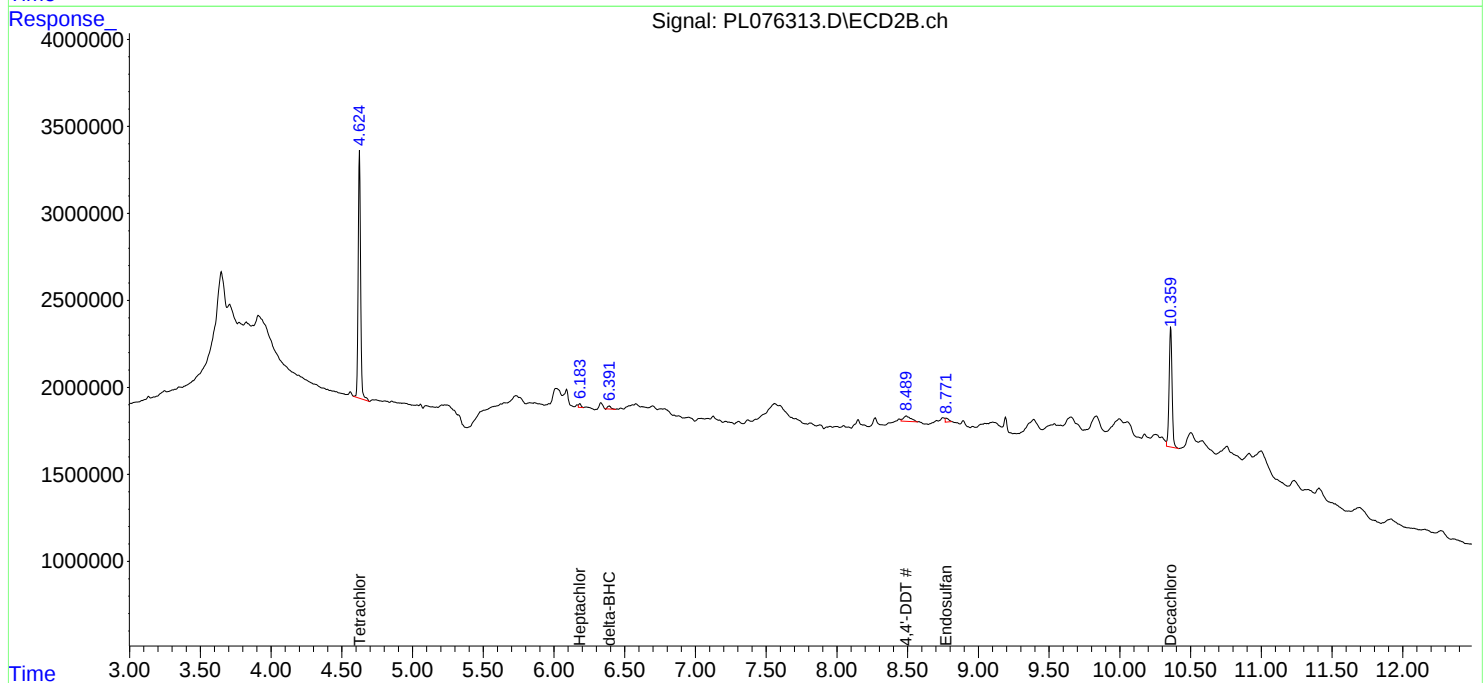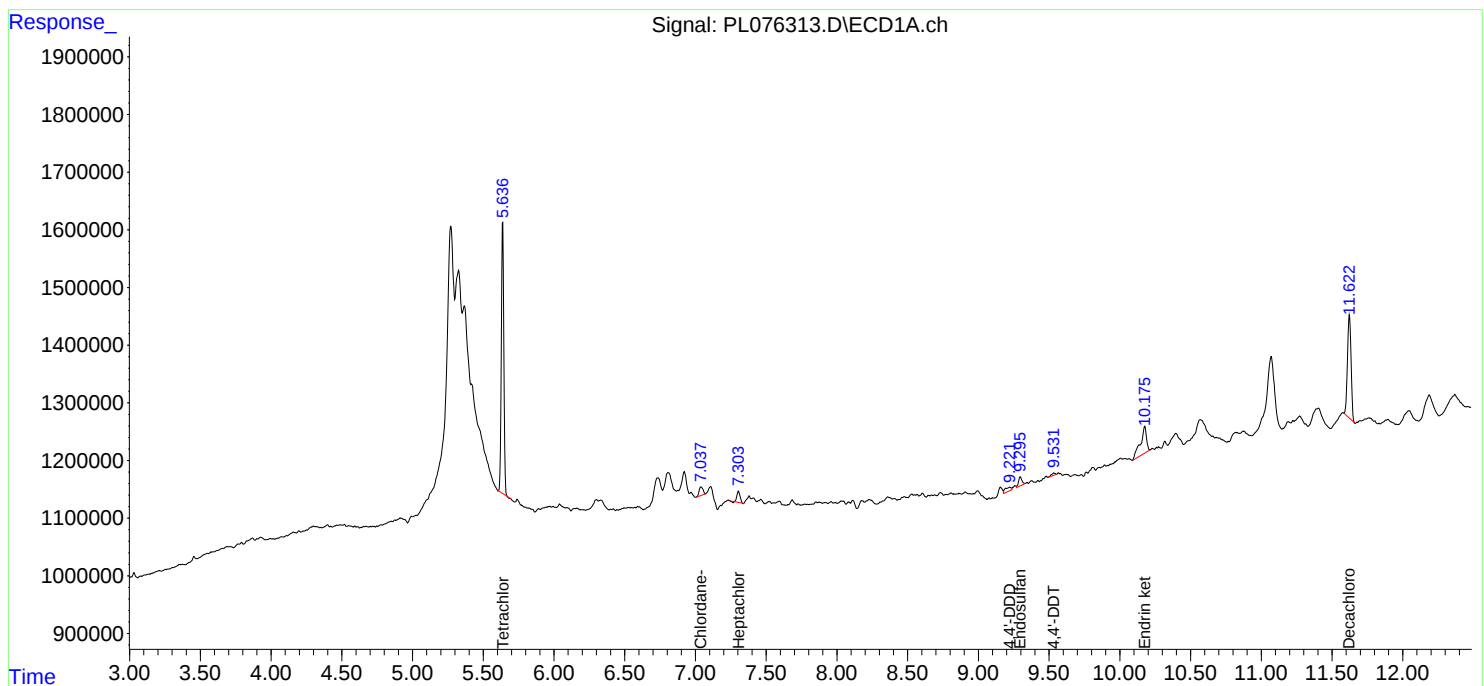


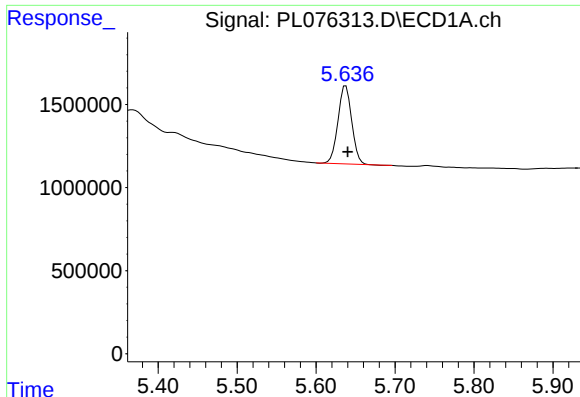

#1 Tetrachloro-m-xylene


R.T.: 5.638 min
Delta R.T.: -0.002 min
Response: 5656773
Conc: 7.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

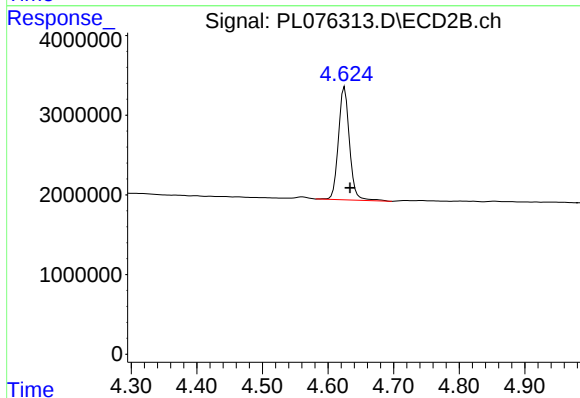


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.008 min
Response: 16629261
Conc: 8.77 ng/ml

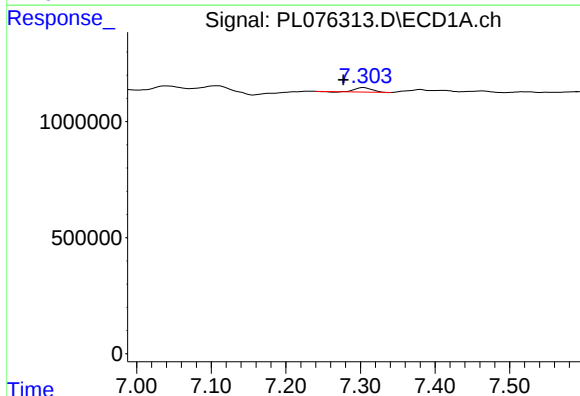


#4 Heptachlor

R.T.: 7.304 min
Delta R.T.: 0.027 min
Response: 286955
Conc: 0.31 ng/ml

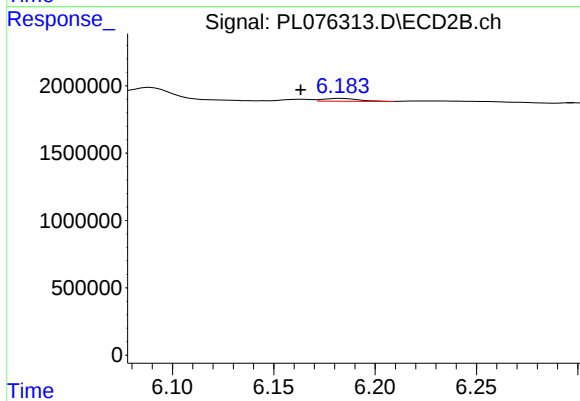

#4 Heptachlor


R.T.: 6.184 min
Delta R.T.: 0.021 min
Response: 260201
Conc: 0.11 ng/ml

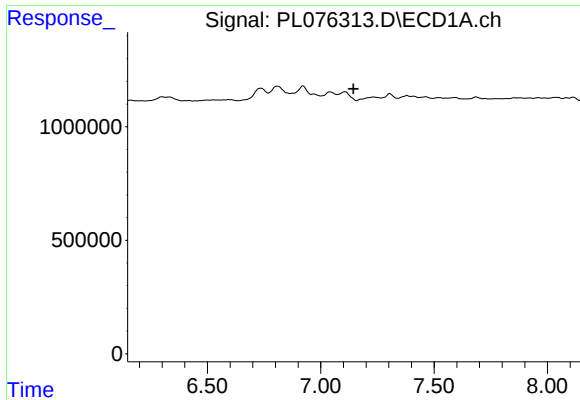

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

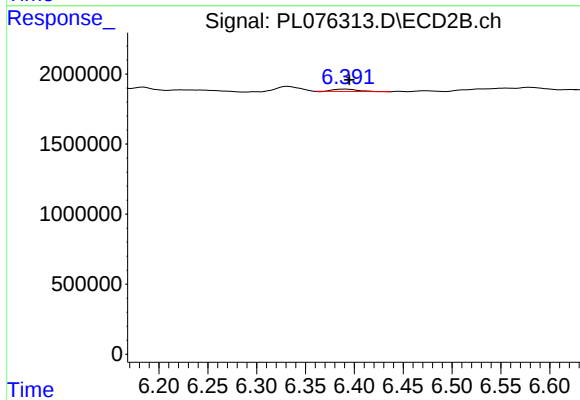


#7 delta-BHC

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 281654
Conc: 0.12 ng/ml

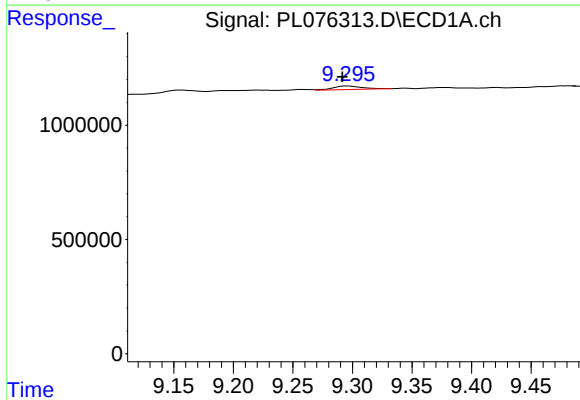


#15 Endosulfan II

R.T.: 9.297 min
Delta R.T.: 0.005 min
Response: 279505
Conc: 0.44 ng/ml

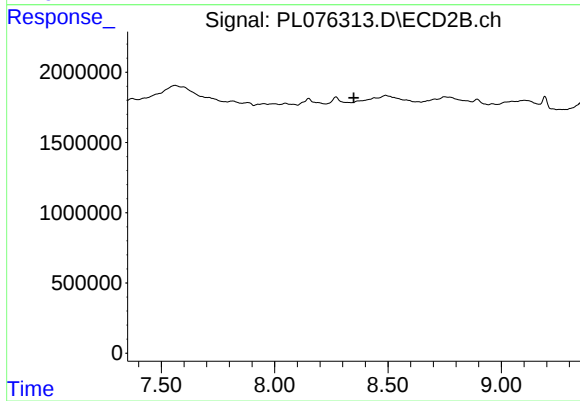

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

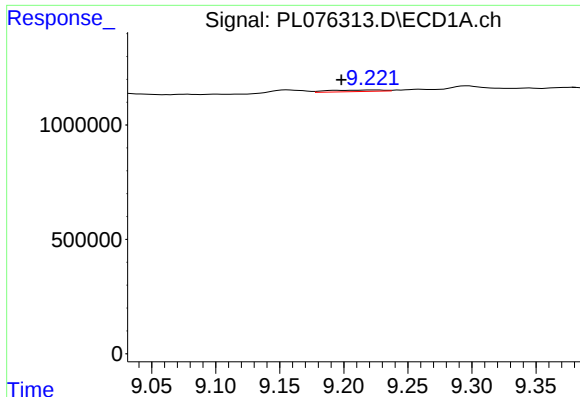

#16 4,4'-DDD


R.T.: 9.222 min
Delta R.T.: 0.024 min
Response: 203892
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

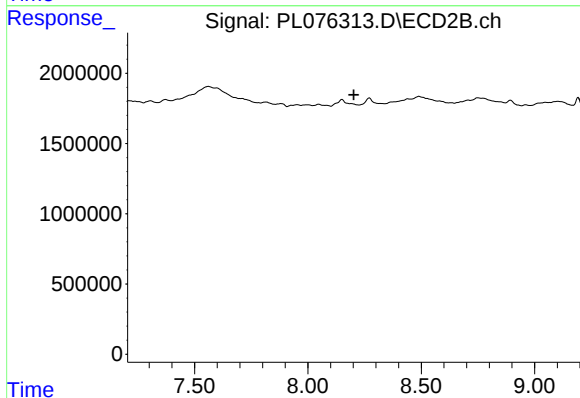


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.202 min
Response: 0
Conc: N.D.

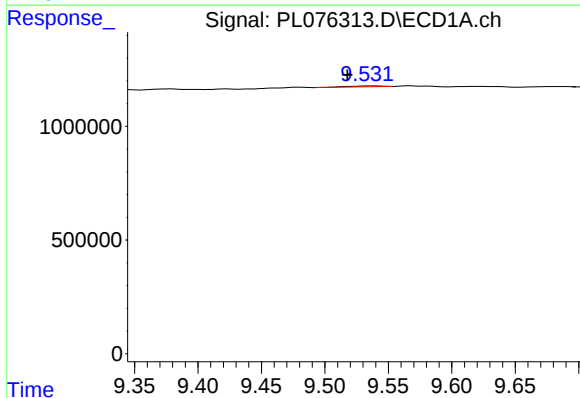


#17 4,4'-DDT

R.T.: 9.533 min
Delta R.T.: 0.015 min
Response: 72765
Conc: 0.12 ng/ml

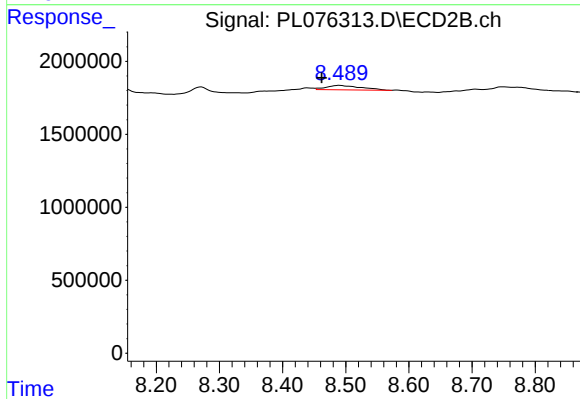

#17 4,4'-DDT


R.T.: 8.490 min
Delta R.T.: 0.028 min
Response: 1154578
Conc: 0.78 ng/ml

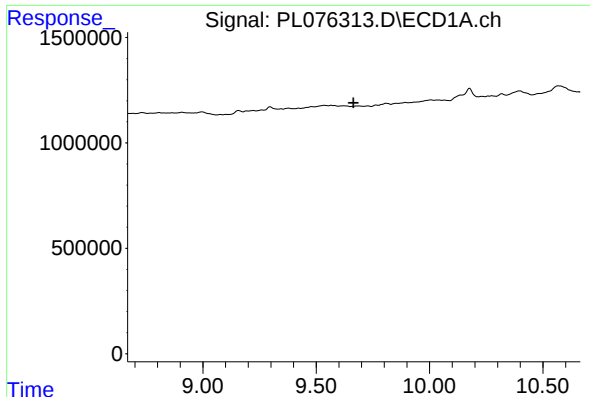

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

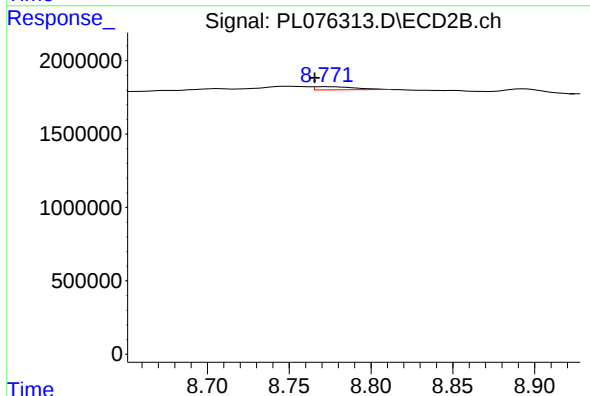


#19 Endosulfan Sulfate

R.T.: 8.773 min
Delta R.T.: 0.007 min
Response: 384178
Conc: 0.25 ng/ml

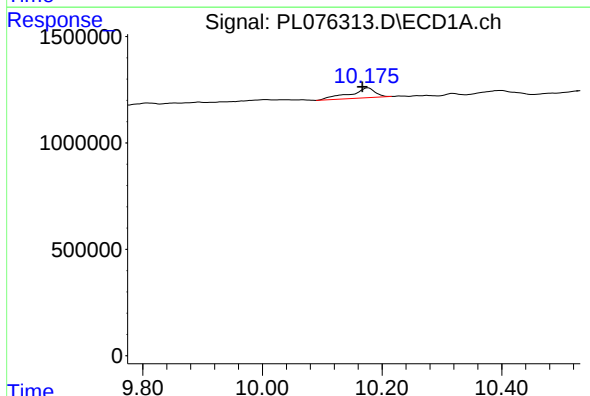


#21 Endrin ketone

R.T.: 10.177 min
Delta R.T.: 0.009 min
Response: 1381324
Conc: 1.92 ng/ml

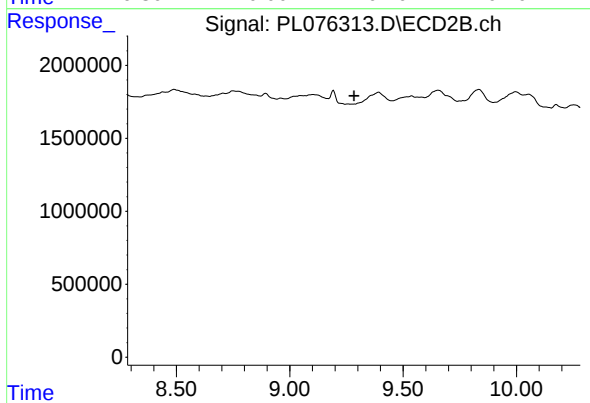

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.284 min
Response: 0
Conc: N.D.

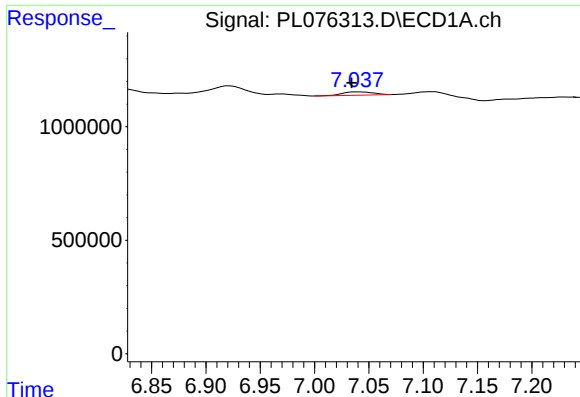

#23 Chlordane-1


R.T.: 7.038 min
Delta R.T.: 0.004 min
Response: 280728
Conc: 11.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

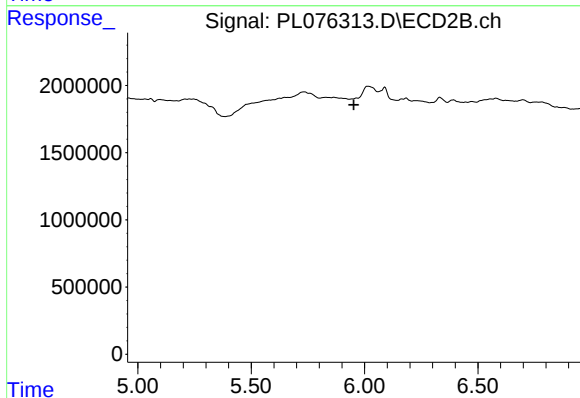


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

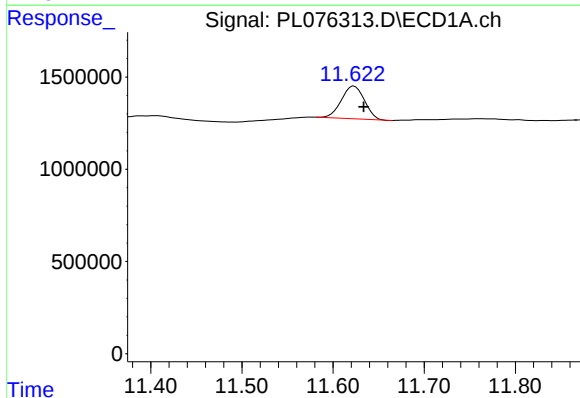

#28 Decachlorobiphenyl

R.T.: 11.623 min
Delta R.T.: -0.011 min
Response: 3136481
Conc: 4.98 ng/ml

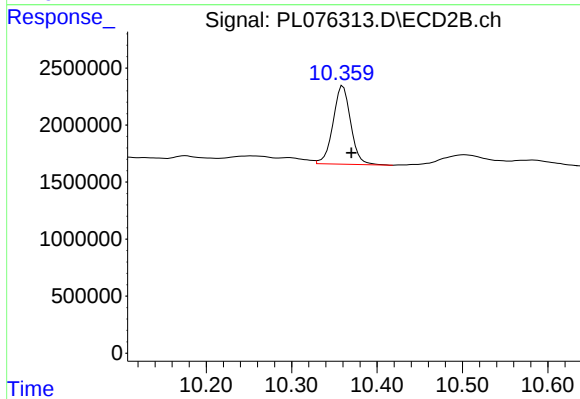

#28 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.010 min
Response: 9878950
Conc: 6.43 ng/ml