

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
 Data File : PL076315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 18:30
 Operator : AR\AJ
 Sample : N3597-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 00:03:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.637	4.624	6969118	19527441	9.215	10.296
28)	SA Decachlor...	11.624	10.359	4654489	13262695	7.397	8.635
Target Compounds							
2)	A alpha-BHC	0.000	5.344	0	1585862	N.D.	0.649 #
4)	MA Heptachlor	7.305f	6.164	213904	189346	0.233	0.083 #
6)	B beta-BHC	0.000	6.164f	0	189346	N.D.	0.182 #
7)	B delta-BHC	0.000	6.390	0	421149	N.D.	0.186 #
14)	MA Endrin	0.000	8.047	0	162618	N.D.	0.107 #
15)	B Endosulfa...	9.296	0.000	258840	0	0.408	N.D. #
18)	B Endrin al...	0.000	8.547	0	140286	N.D.	0.118 #
21)	B Endrin ke...	10.177	0.000	558776	0	0.775	N.D. #
23)	Chlordane-1	7.038	0.000	314989	0	12.446	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
Data File : PL076315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 18:30
Operator : AR\AJ
Sample : N3597-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 00:03:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

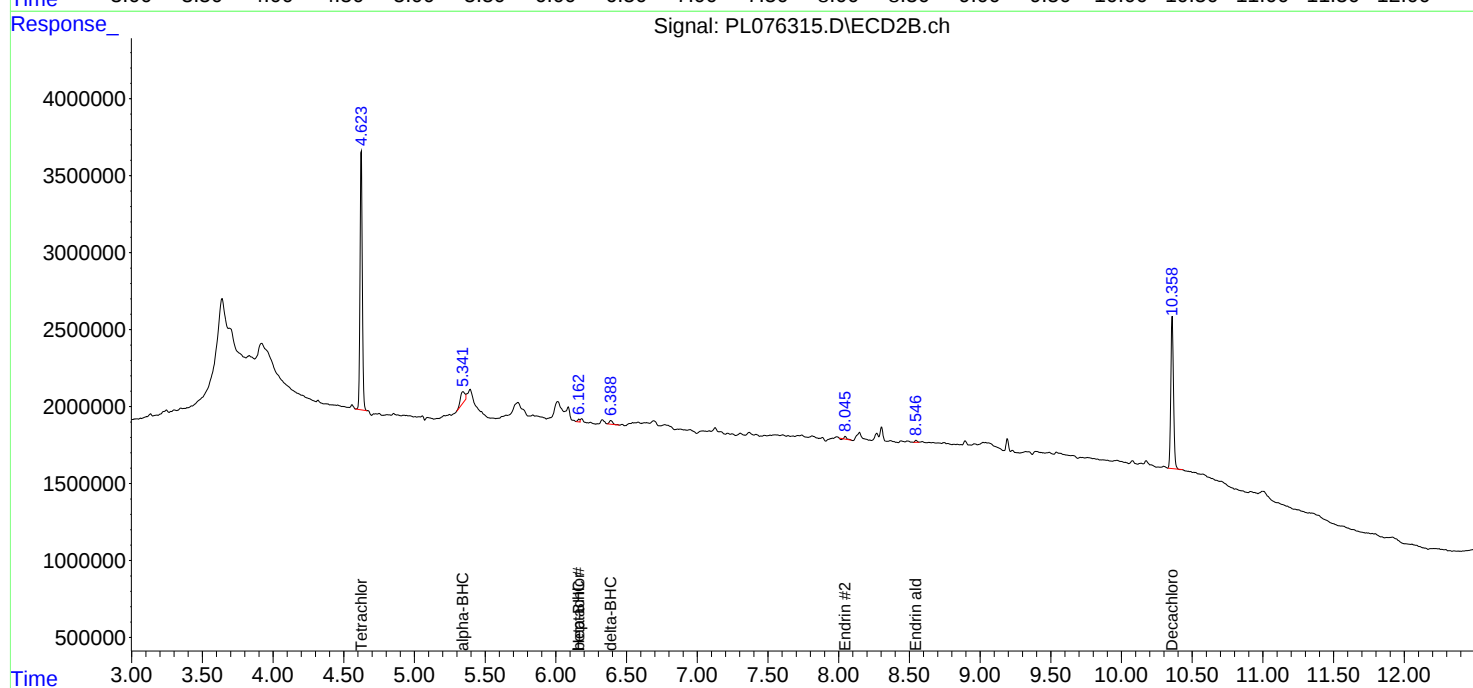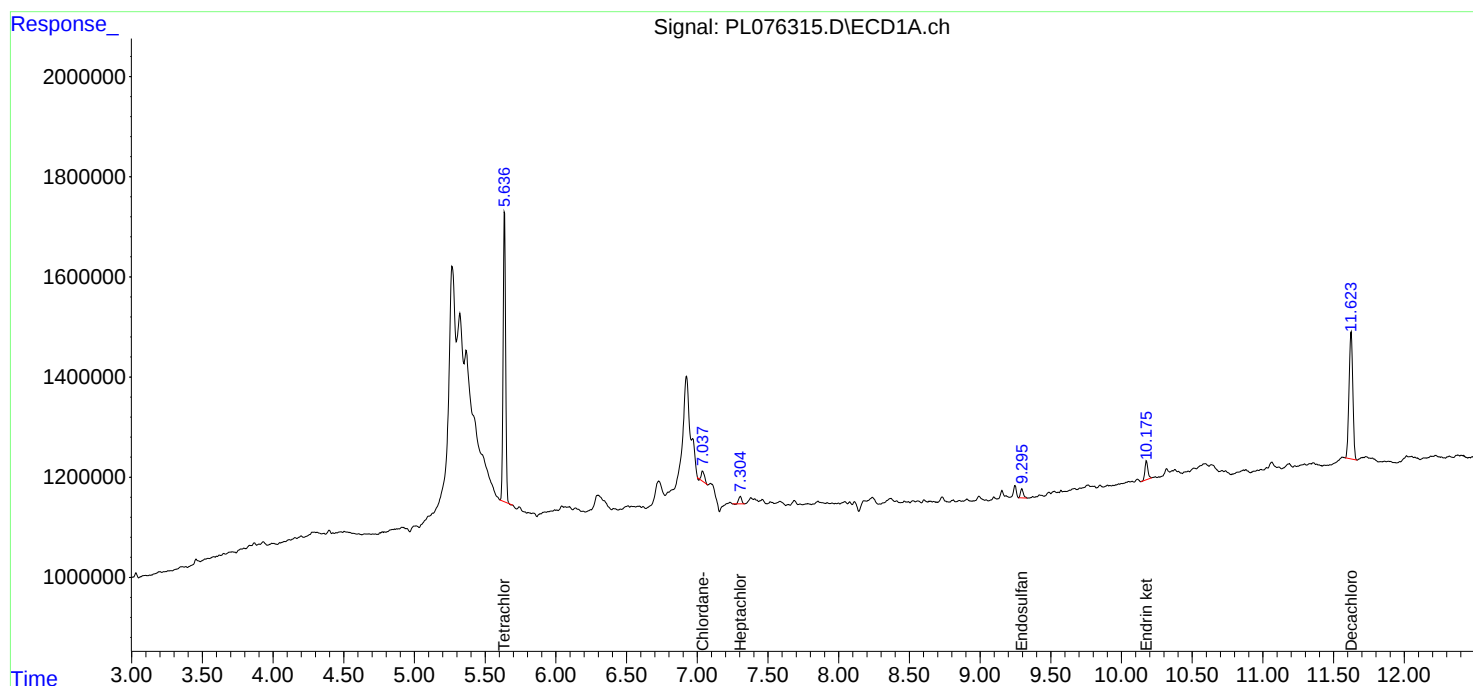


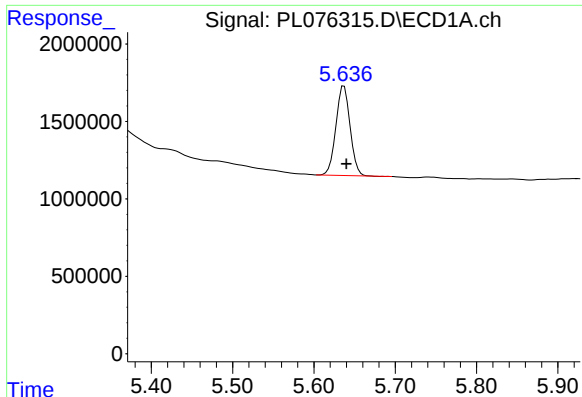

#1 Tetrachloro-m-xylene


R.T.: 5.637 min
Delta R.T.: -0.003 min
Response: 6969118
Conc: 9.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

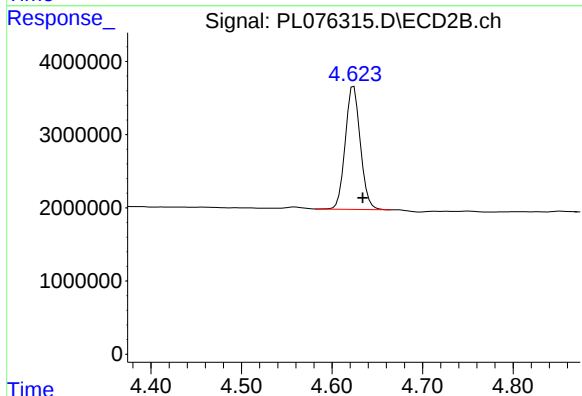


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: -0.010 min
Response: 19527441
Conc: 10.30 ng/ml

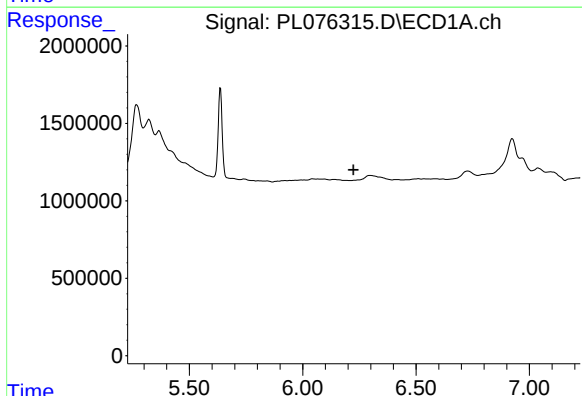


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

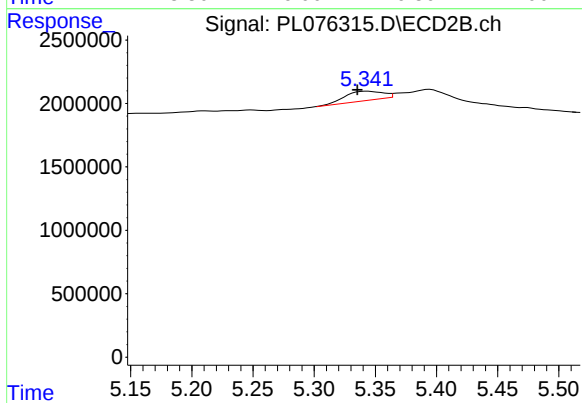

#2 alpha-BHC


R.T.: 5.344 min
Delta R.T.: 0.008 min
Response: 1585862
Conc: 0.65 ng/ml

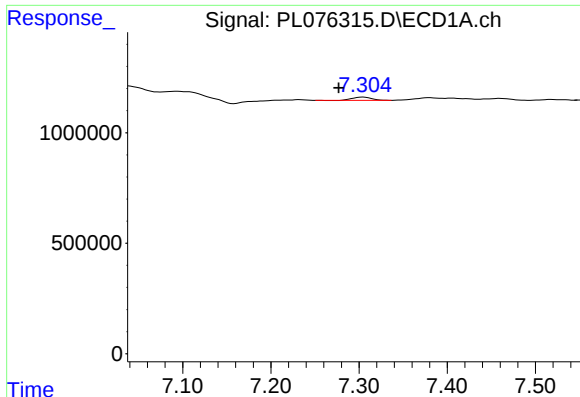

#4 Heptachlor


R.T.: 7.305 min
Delta R.T.: 0.028 min
Response: 213904
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

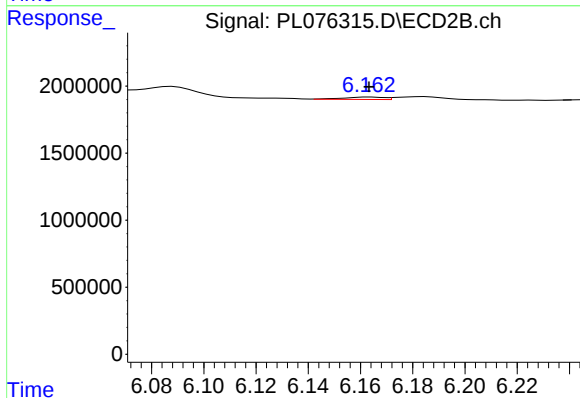


#4 Heptachlor

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 189346
Conc: 0.08 ng/ml

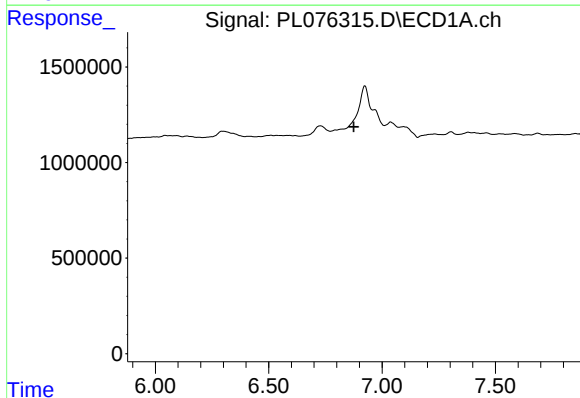


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.875 min
Response: 0
Conc: N.D.

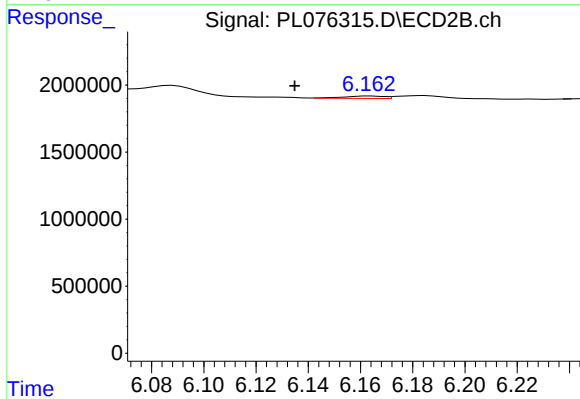

#6 beta-BHC


R.T.: 6.164 min
Delta R.T.: 0.029 min
Response: 189346
Conc: 0.18 ng/ml

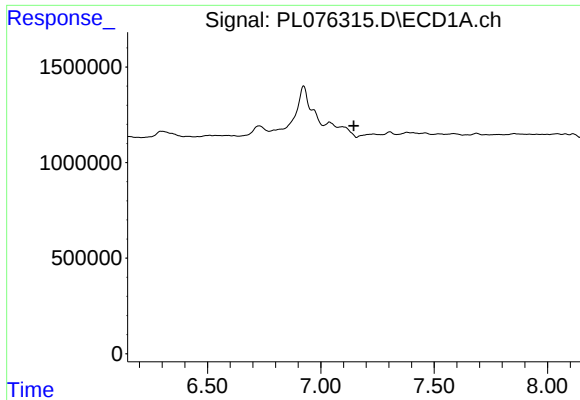

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

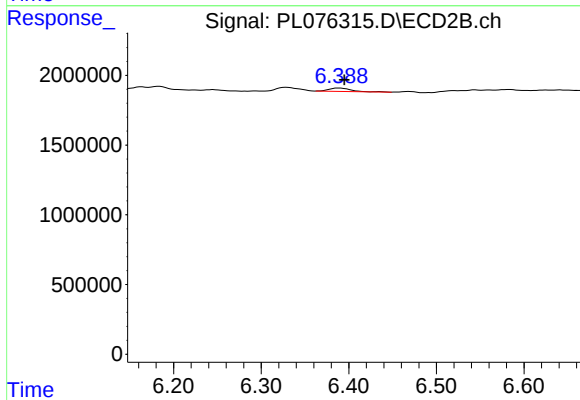


#7 delta-BHC

R.T.: 6.390 min
Delta R.T.: -0.006 min
Response: 421149
Conc: 0.19 ng/ml

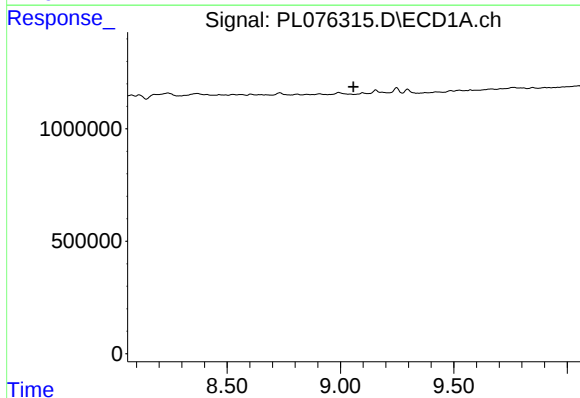


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

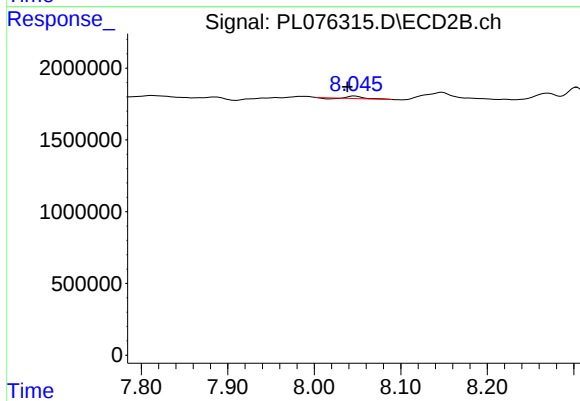

#14 Endrin


R.T.: 8.047 min
Delta R.T.: 0.009 min
Response: 162618
Conc: 0.11 ng/ml

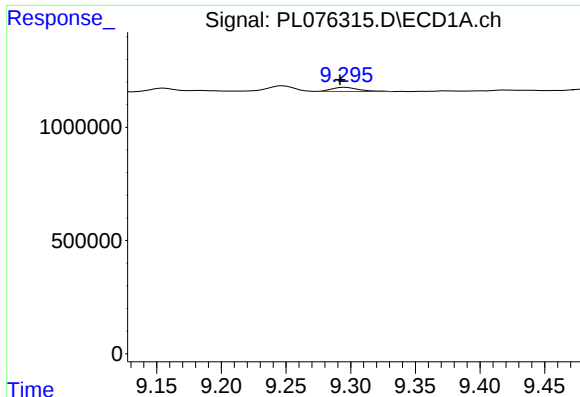

#15 Endosulfan II


R.T.: 9.296 min
Delta R.T.: 0.004 min
Response: 258840
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

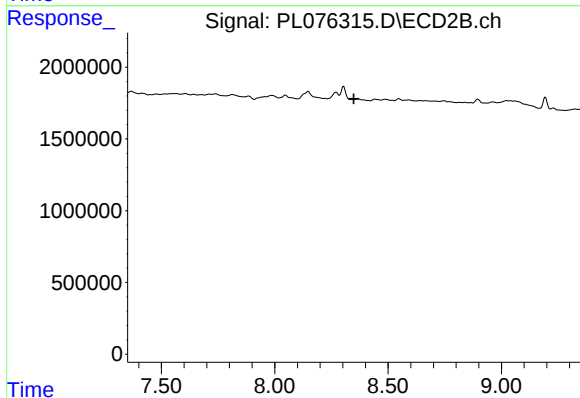


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

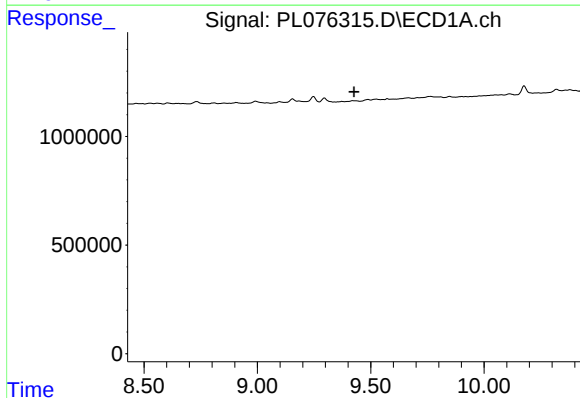


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.426 min
Response: 0
Conc: N.D.

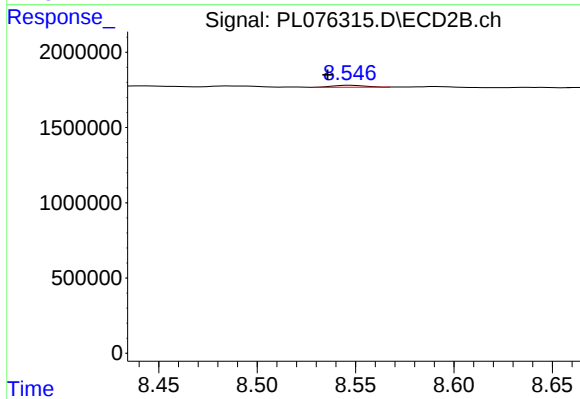

#18 Endrin aldehyde


R.T.: 8.547 min
Delta R.T.: 0.011 min
Response: 140286
Conc: 0.12 ng/ml

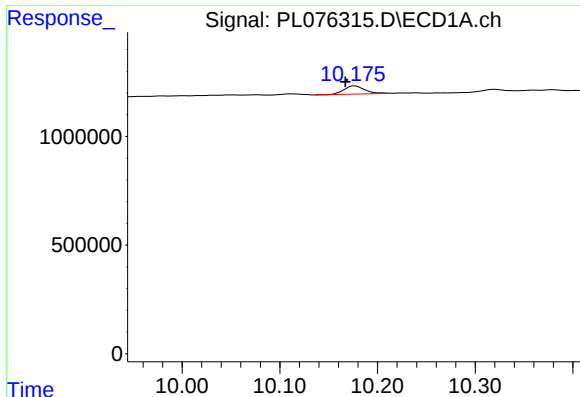

#21 Endrin ketone


R.T.: 10.177 min
Delta R.T.: 0.009 min
Response: 558776
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

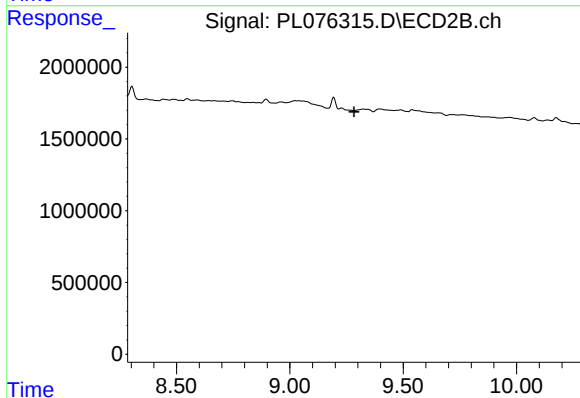


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

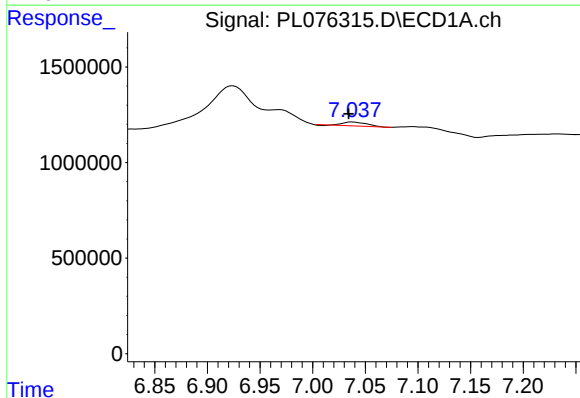


#23 Chlordane-1

R.T.: 7.038 min
Delta R.T.: 0.004 min
Response: 314989
Conc: 12.45 ng/ml

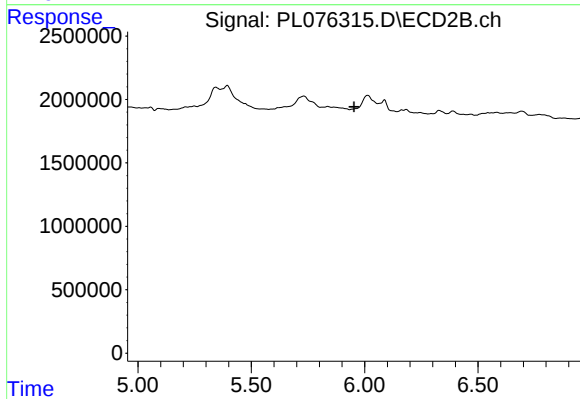

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.953 min
Response: 0
Conc: N.D.

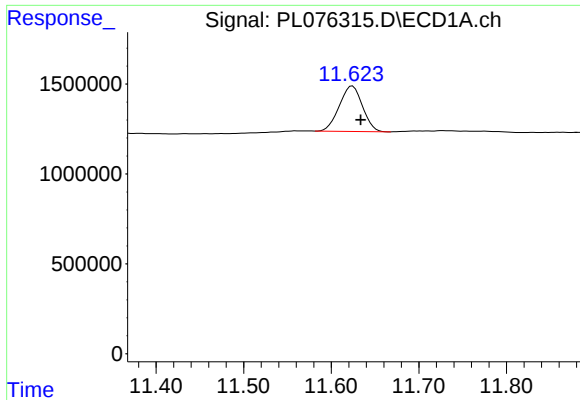

#28 Decachlorobiphenyl

R.T.: 11.624 min
Delta R.T.: -0.009 min
Response: 4654489
Conc: 7.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

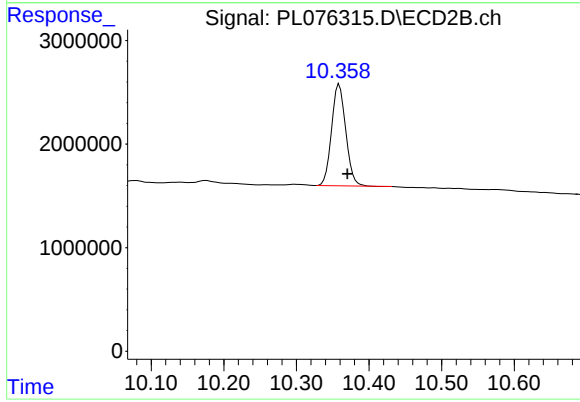

#28 Decachlorobiphenyl

R.T.: 10.359 min
Delta R.T.: -0.011 min
Response: 13262695
Conc: 8.64 ng/ml