

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
 Data File : PL076319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 20:44
 Operator : AR\AJ
 Sample : N3597-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 00:04:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.637	4.624	6757028	19489853	8.934	10.276
28)	SA Decachlor...	11.622	10.359	5312022	15057372	8.442	9.804
Target Compounds							
2)	A alpha-BHC	0.000	5.344	0	673966	N.D.	0.276 #
4)	MA Heptachlor	7.305f	6.182f	278309	186293	0.303	0.082 #
7)	B delta-BHC	0.000	6.390	0	395720	N.D.	0.175 #
10)	B gamma-Chl...	0.000	7.307f	0	228812	N.D.	0.119 #
14)	MA Endrin	0.000	8.046	0	55364	N.D.	0.036 #
15)	B Endosulfa...	9.296	0.000	236092	0	0.372	N.D. #
21)	B Endrin ke...	10.176	0.000	691400	0	0.959	N.D. #
25)	Chlordane-3	0.000	7.307f	0	228812	N.D.	1.297 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
Data File : PL076319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 20:44
Operator : AR\AJ
Sample : N3597-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 00:04:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

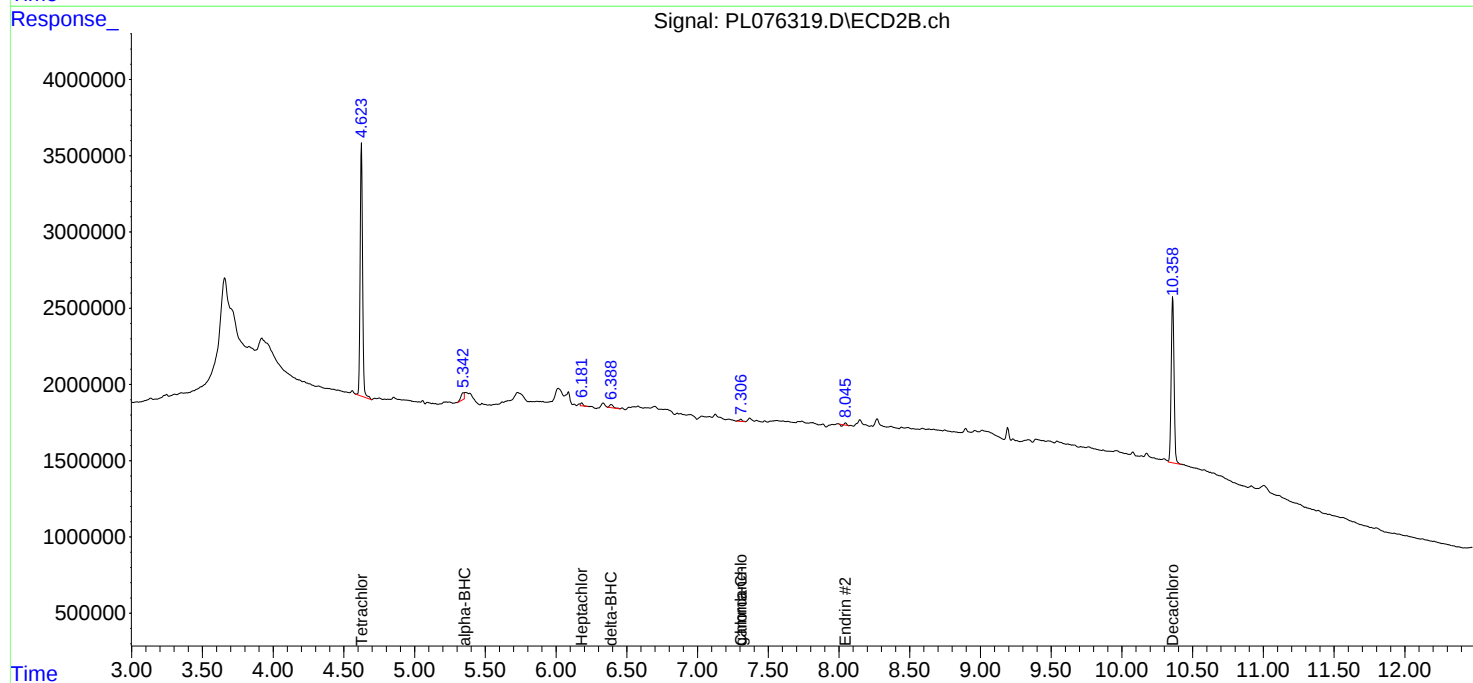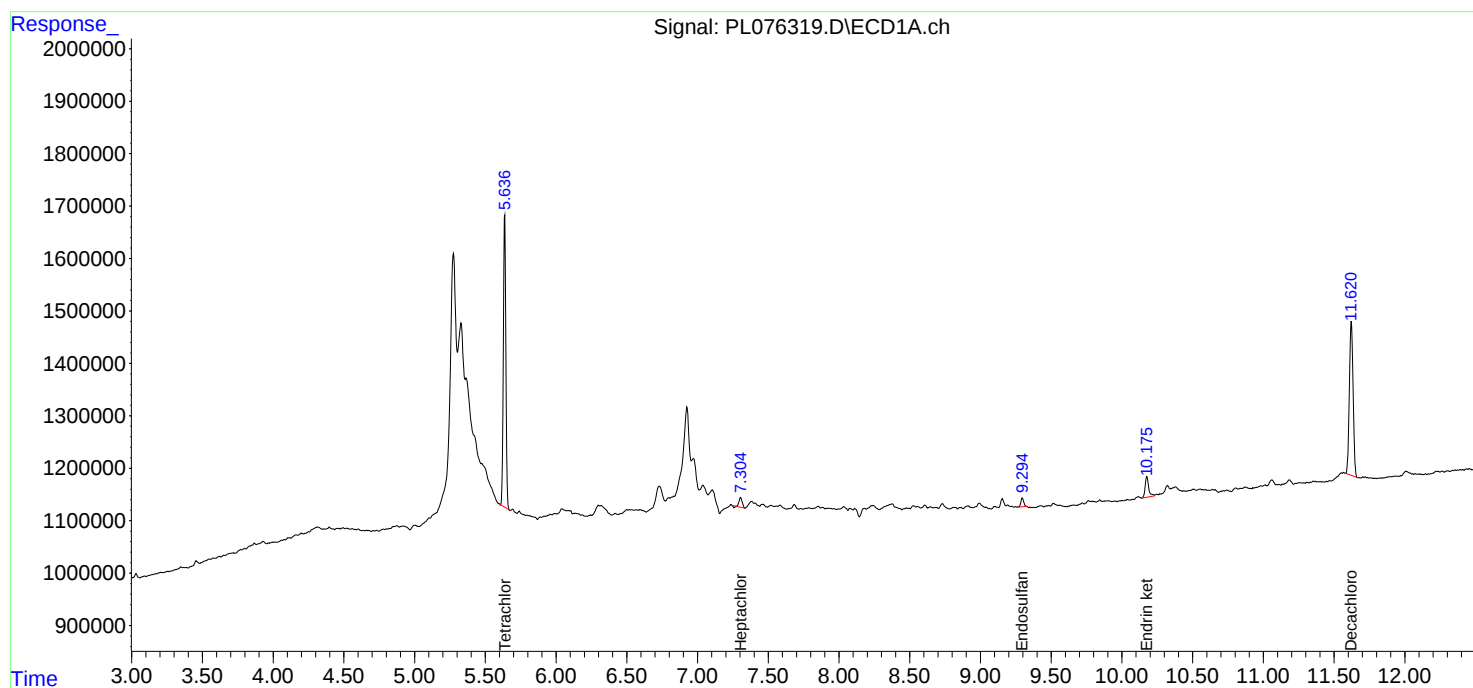


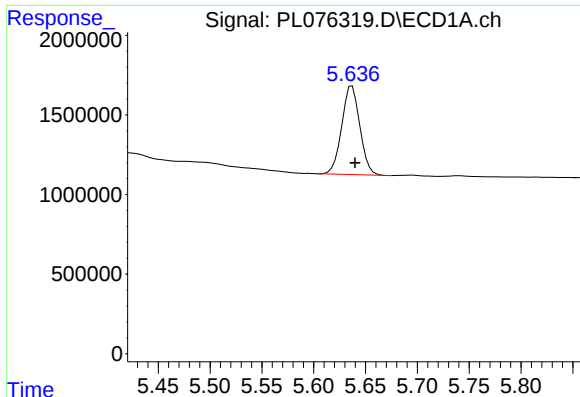

#1 Tetrachloro-m-xylene


R.T.: 5.637 min
Delta R.T.: -0.003 min
Response: 6757028
Conc: 8.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

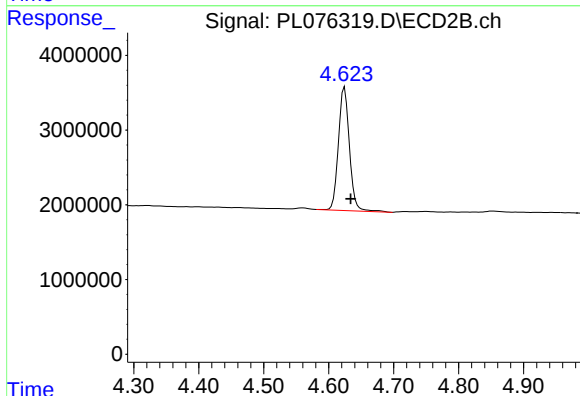


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: -0.009 min
Response: 19489853
Conc: 10.28 ng/ml

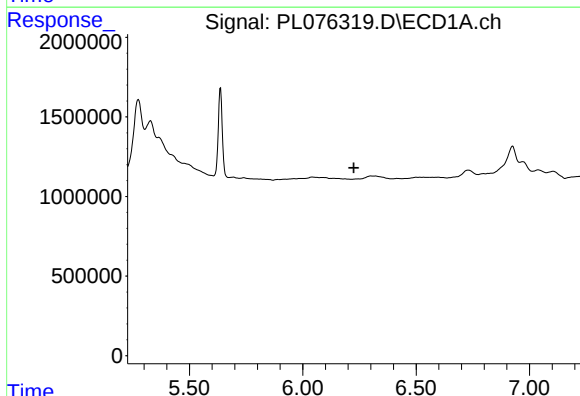


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

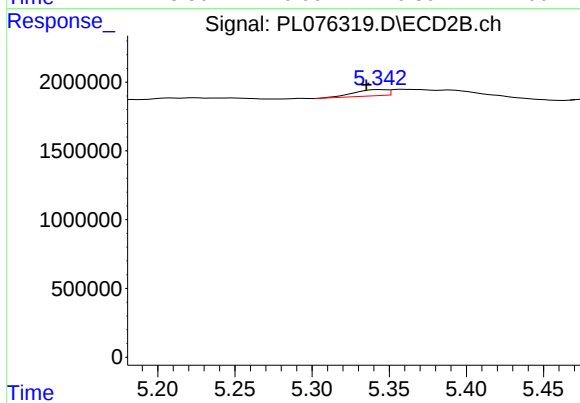

#2 alpha-BHC


R.T.: 5.344 min
Delta R.T.: 0.009 min
Response: 673966
Conc: 0.28 ng/ml

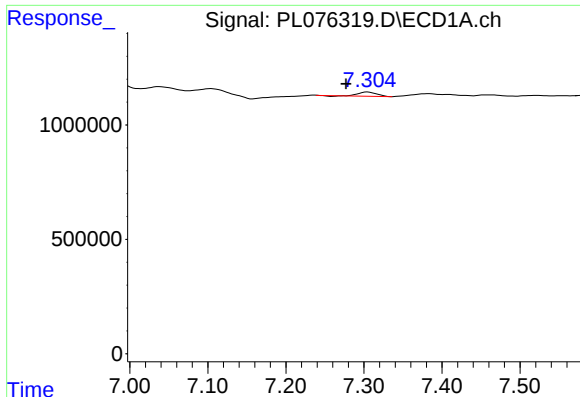

#4 Heptachlor


R.T.: 7.305 min
Delta R.T.: 0.028 min
Response: 278309
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

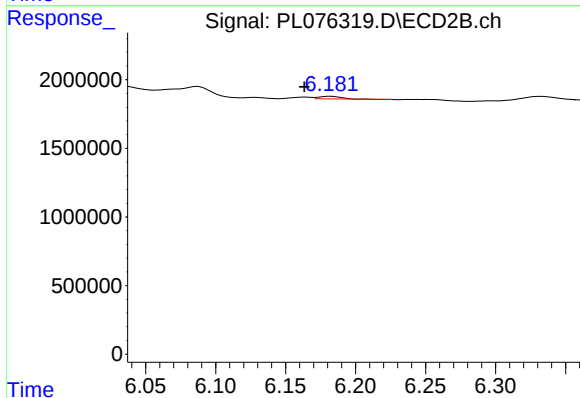


#4 Heptachlor

R.T.: 6.182 min
Delta R.T.: 0.019 min
Response: 186293
Conc: 0.08 ng/ml

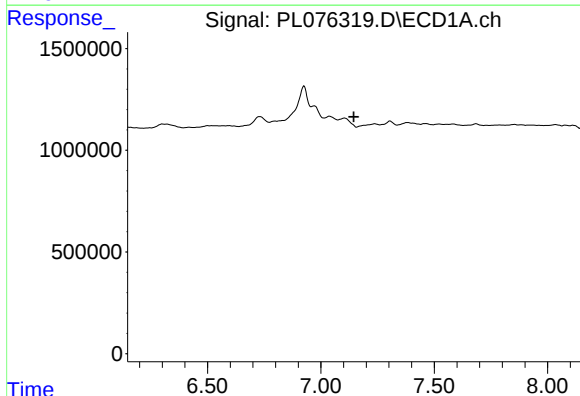


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

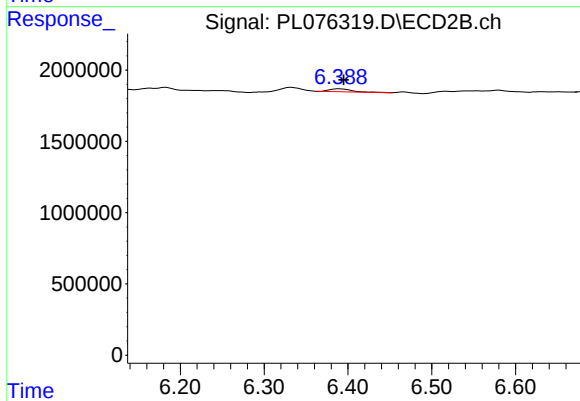

#7 delta-BHC


R.T.: 6.390 min
Delta R.T.: -0.005 min
Response: 395720
Conc: 0.18 ng/ml

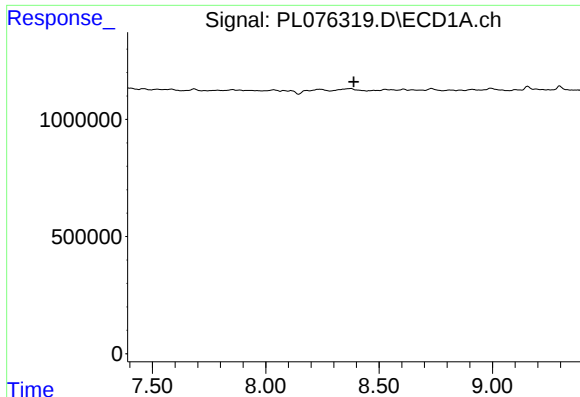

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

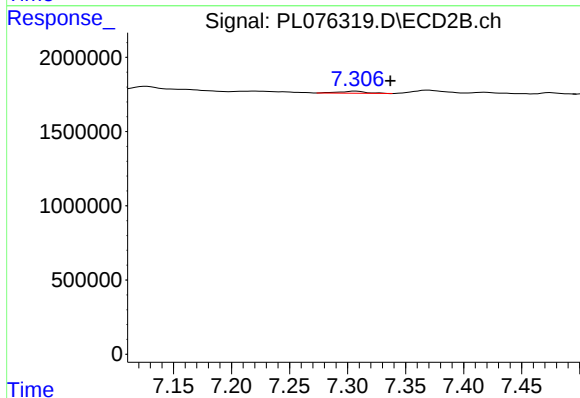


#10 gamma-Chlordane

R.T.: 7.307 min
Delta R.T.: -0.029 min
Response: 228812
Conc: 0.12 ng/ml

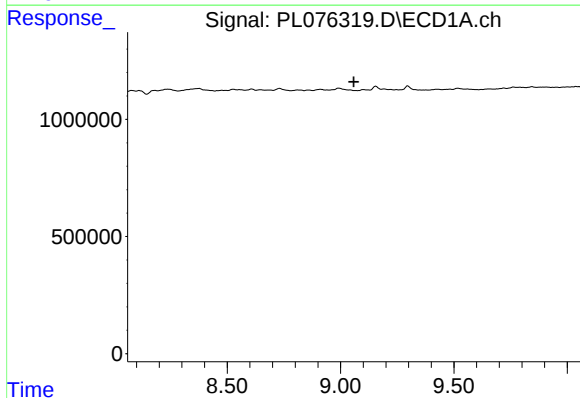


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

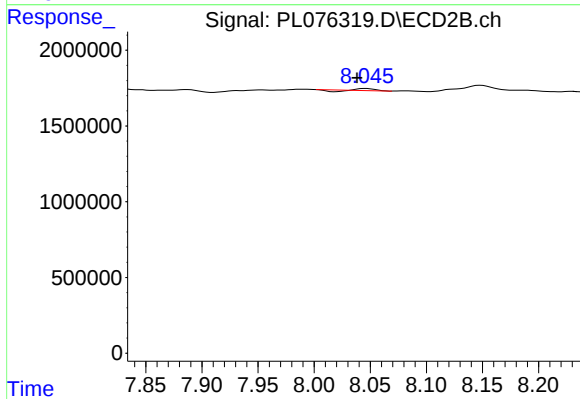

#14 Endrin


R.T.: 8.046 min
Delta R.T.: 0.008 min
Response: 55364
Conc: 0.04 ng/ml

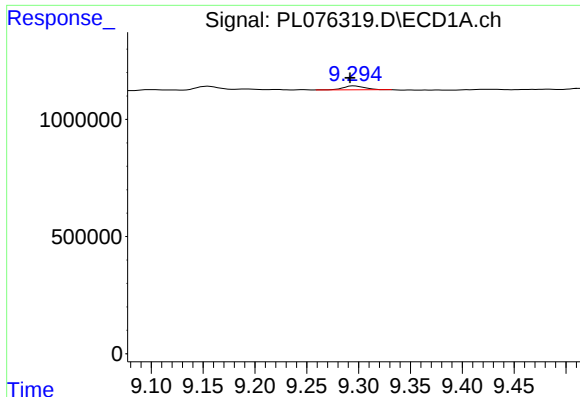

#15 Endosulfan II


R.T.: 9.296 min
Delta R.T.: 0.004 min
Response: 236092
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

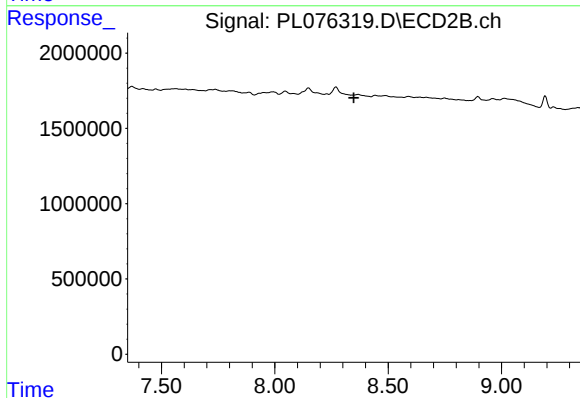


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

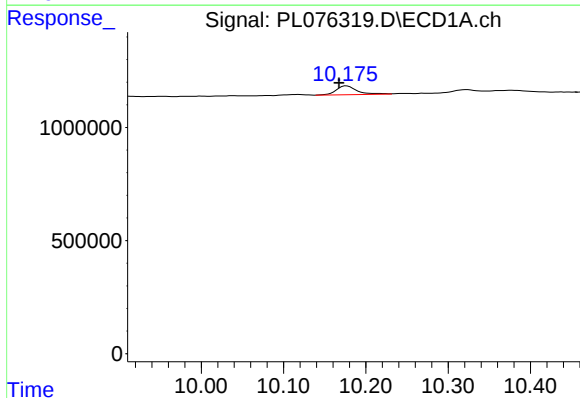


#21 Endrin ketone

R.T.: 10.176 min
Delta R.T.: 0.009 min
Response: 691400
Conc: 0.96 ng/ml

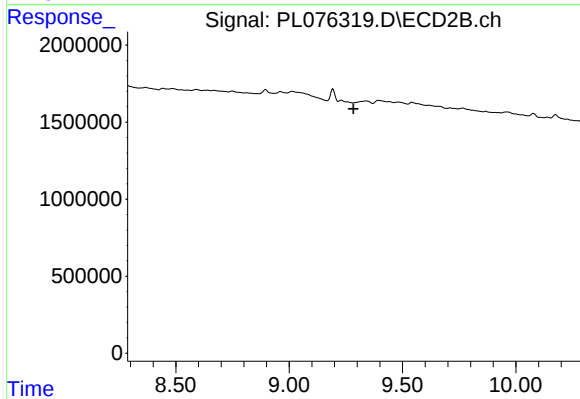

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

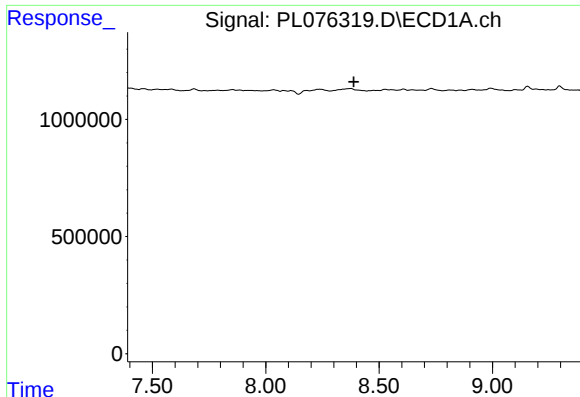

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

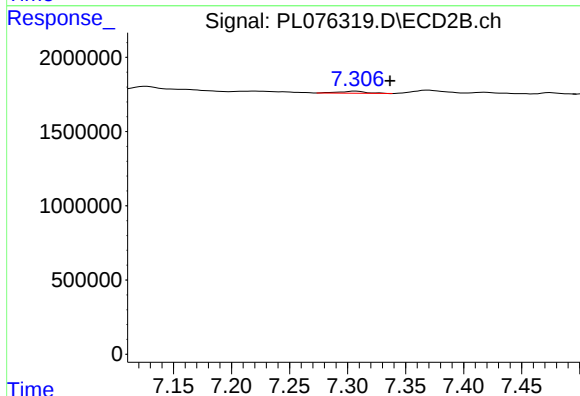


#25 Chlordane-3

R.T.: 7.307 min
Delta R.T.: -0.029 min
Response: 228812
Conc: 1.30 ng/ml

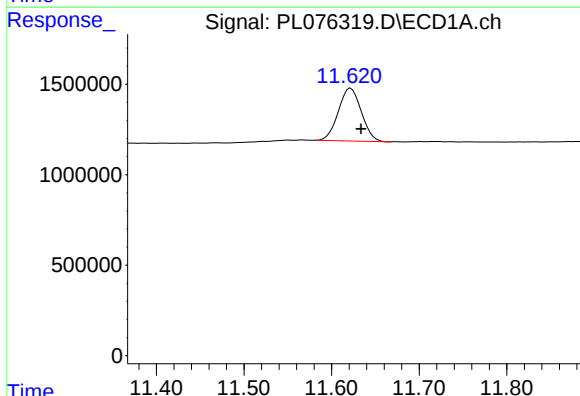

#28 Decachlorobiphenyl

R.T.: 11.622 min
Delta R.T.: -0.012 min
Response: 5312022
Conc: 8.44 ng/ml

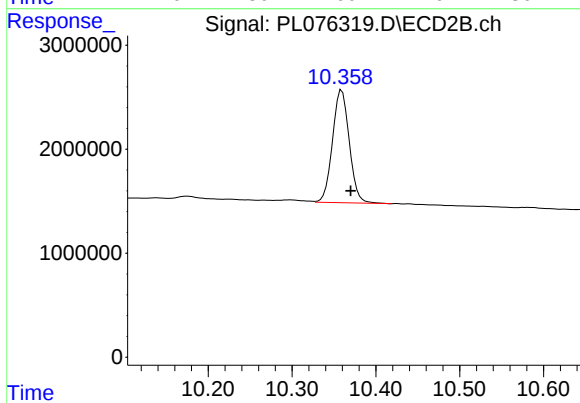

#28 Decachlorobiphenyl

R.T.: 10.359 min
Delta R.T.: -0.011 min
Response: 15057372
Conc: 9.80 ng/ml