

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
 Data File : PL076308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 16:32
 Operator : AR\AJ
 Sample : N3584-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26572

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/08/2022
 Supervised By : Ankita Jodhani 07/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 23:59:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.637	4.625	4657444	12703754	6.158	6.698
2) SA Decachlor...	11.623	10.360	2416918	7026933	3.841m	4.575

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070722\
Data File : PL076308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 16:32
Operator : AR\AJ
Sample : N3584-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/08/2022
Supervised By : Ankita Jodhani 07/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 23:59:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

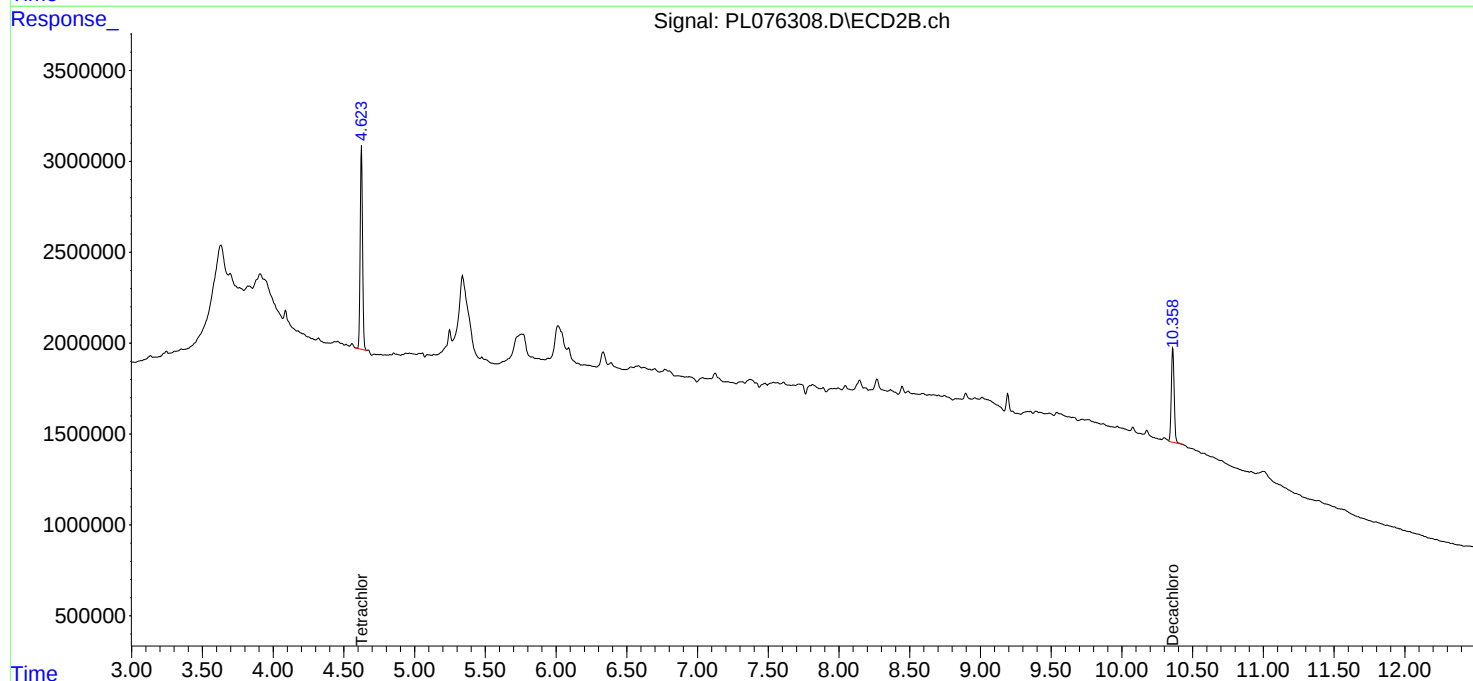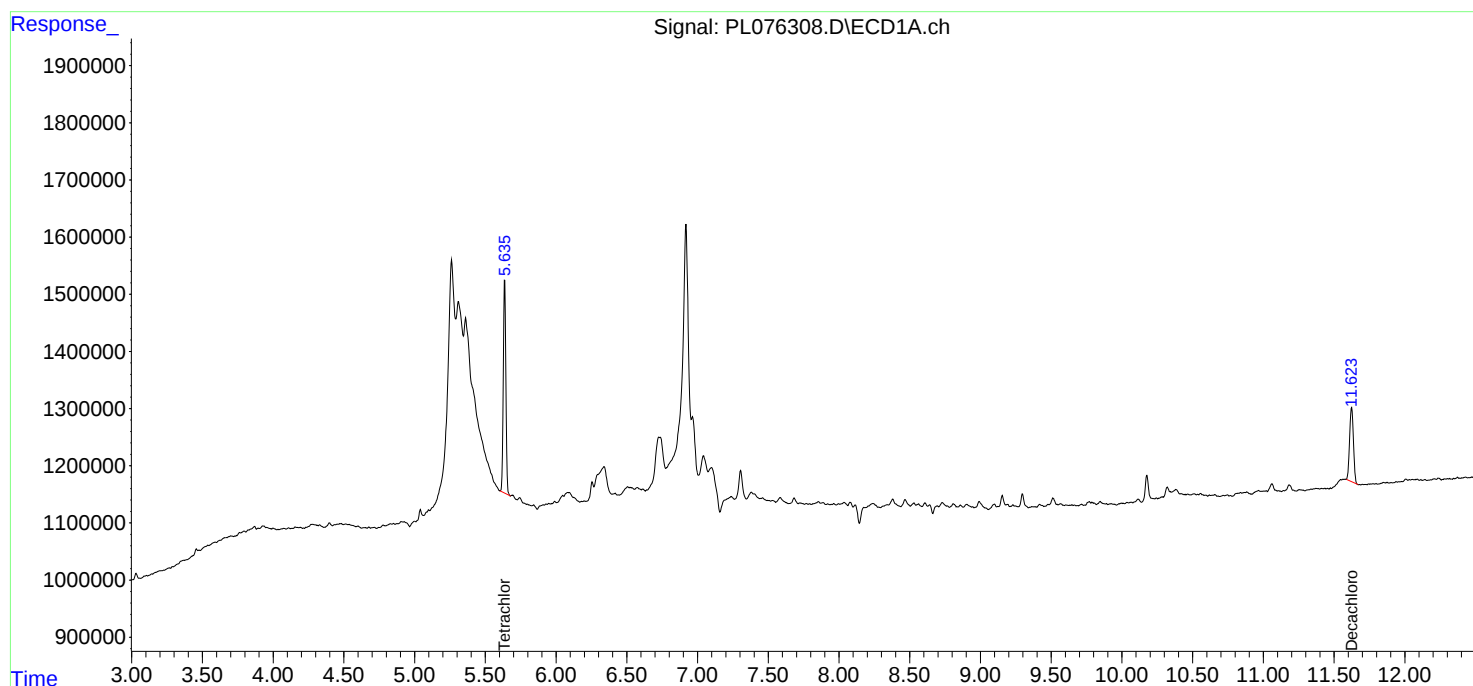

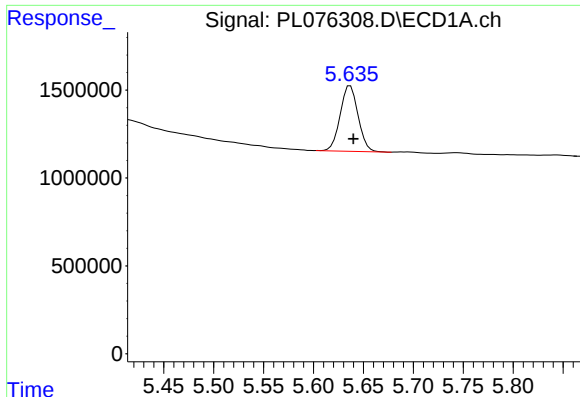


#1 Tetrachloro-m-xylene

R.T.: 5.637 min
Delta R.T.: -0.003 min
Response: 4657444
Conc: 6.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022

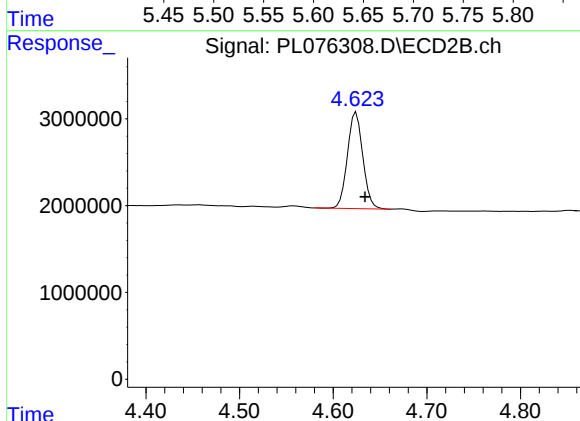


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.009 min
Response: 12703754
Conc: 6.70 ng/ml

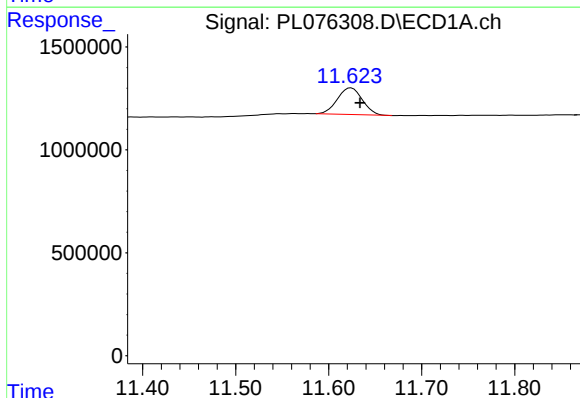

#28 Decachlorobiphenyl

R.T.: 11.623 min
Delta R.T.: -0.011 min
Response: 2416918
Conc: 3.84 ng/ml m

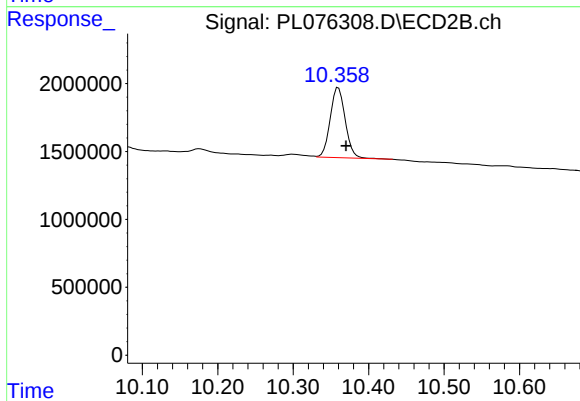

#28 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: -0.010 min
Response: 7026933
Conc: 4.58 ng/ml