

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
 Data File : PL096245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 12:03
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 14:10:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 14:08:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.828	350.7E6	720.1E6	101.066	100.693
28)	SA Decachlor...	9.020	7.996	265.0E6	476.0E6	99.900	99.760
Target Compounds							
23)	Chlordane-1	4.693	3.841	182.9E6	243.0E6	1015.139	1015.728
24)	Chlordane-2	5.217	4.421	188.7E6	267.6E6	995.055	991.522
25)	Chlordane-3	5.920	5.054	770.9E6	827.9E6	1021.517	1018.824
26)	Chlordane-4	6.005	5.118	924.6E6	742.3E6	1015.727	1011.252
27)	Chlordane-5	6.841	6.012	147.1E6	289.8E6	1011.167	1011.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
Data File : PL096245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 12:03
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 14:10:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 14:08:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

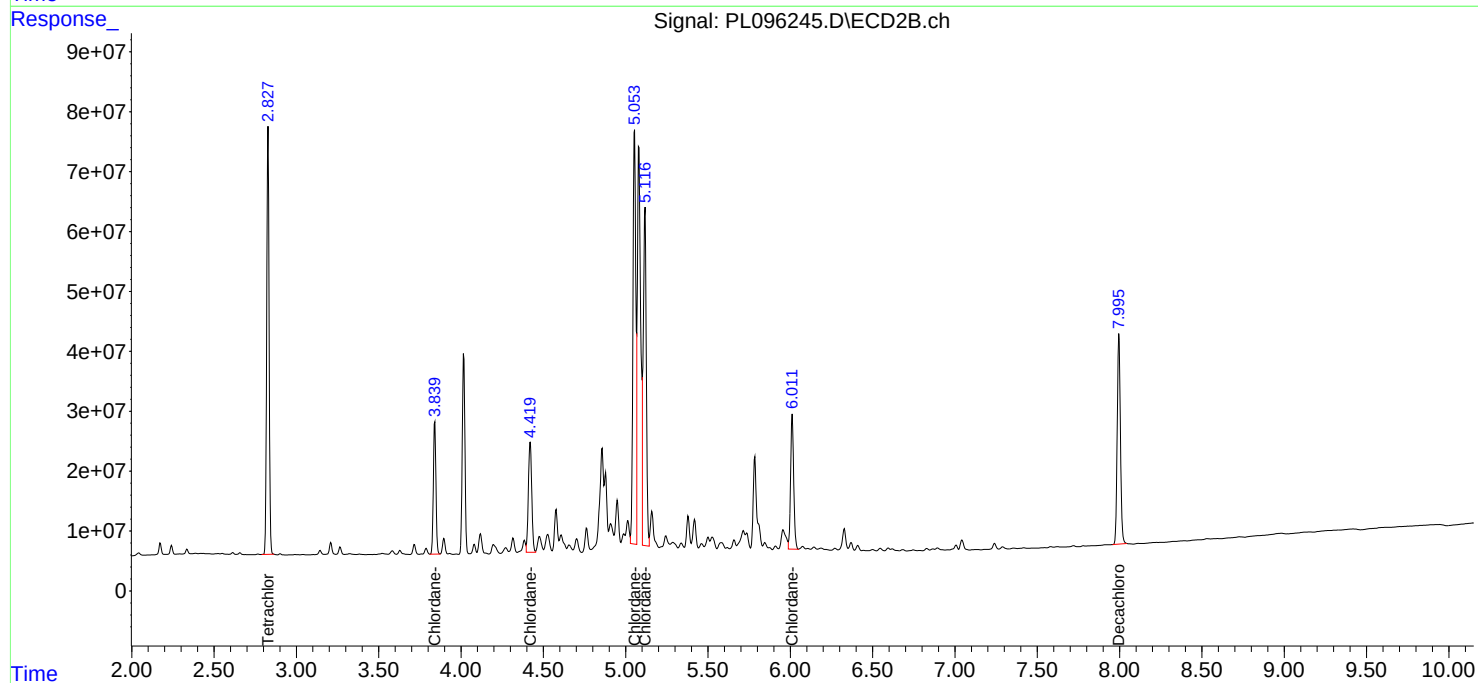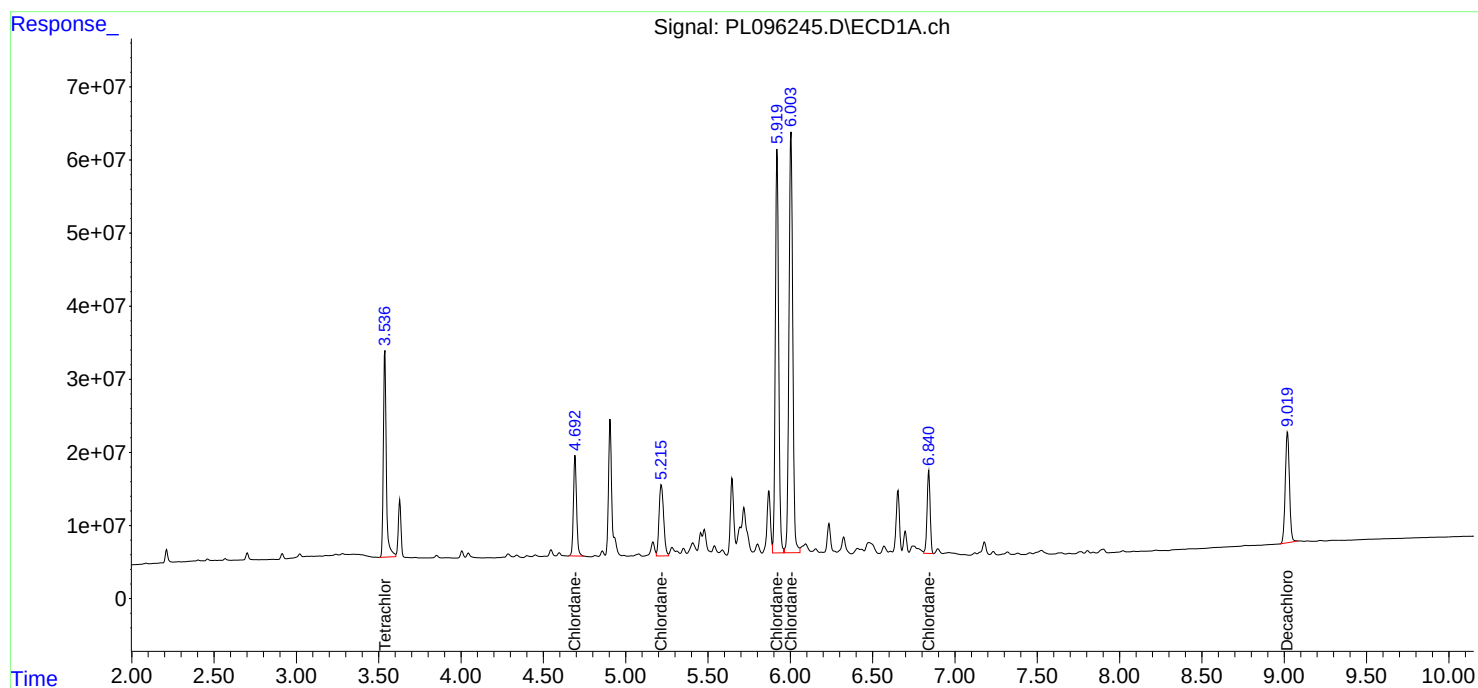


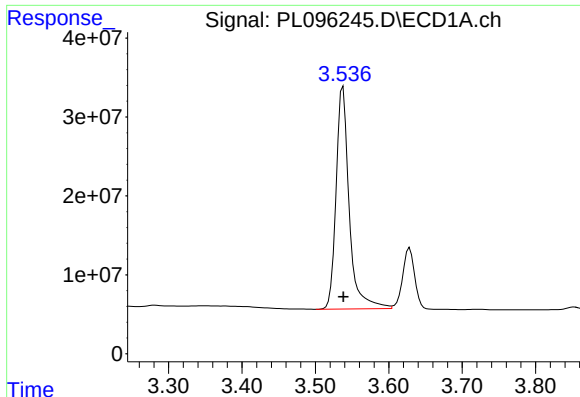

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 350684429
Conc: 101.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

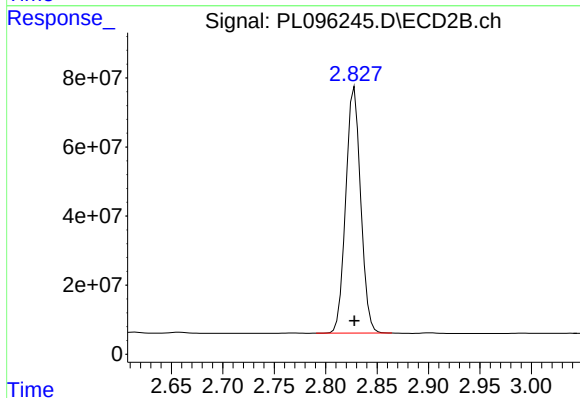


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 720056644
Conc: 100.69 ng/ml

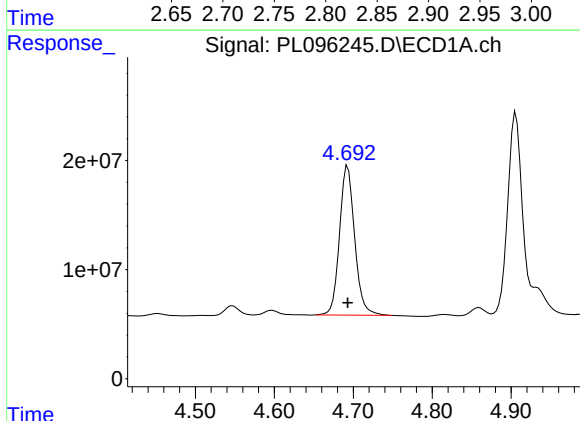


#23 Chlordane-1

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 182864148
Conc: 1015.14 ng/ml

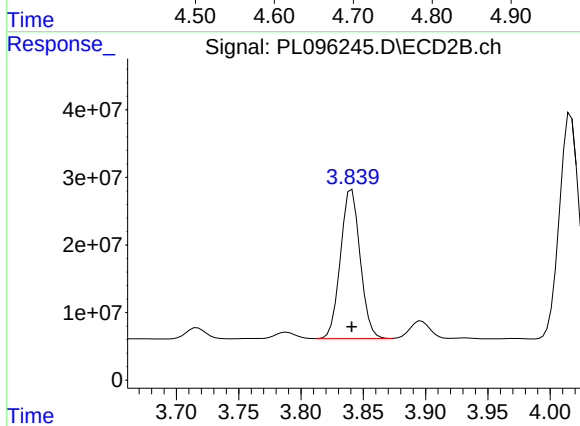

#23 Chlordane-1


R.T.: 3.841 min
Delta R.T.: 0.000 min
Response: 243002582
Conc: 1015.73 ng/ml

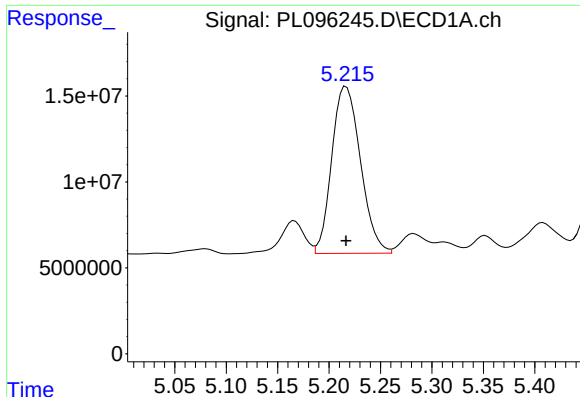

#24 Chlordane-2


R.T.: 5.217 min
Delta R.T.: 0.000 min
Response: 188693294
Conc: 995.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

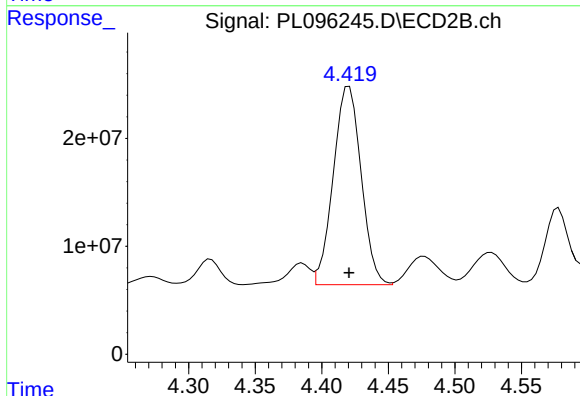


#24 Chlordane-2

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 267595570
Conc: 991.52 ng/ml

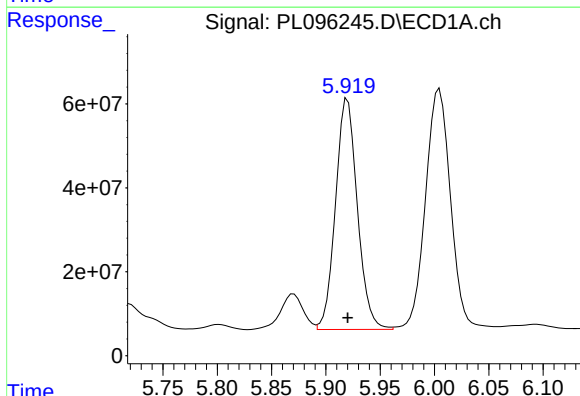


#25 Chlordane-3

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 770918176
Conc: 1021.52 ng/ml

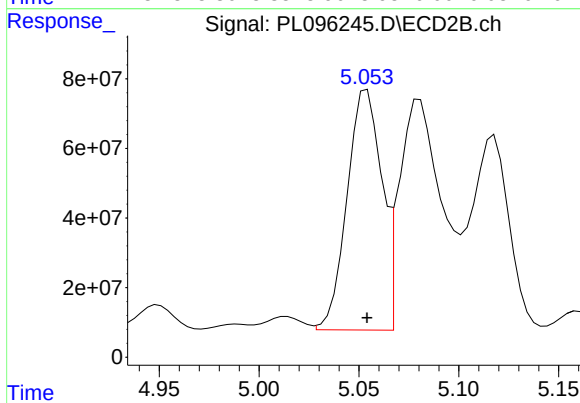

#25 Chlordane-3


R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 827866582
Conc: 1018.82 ng/ml

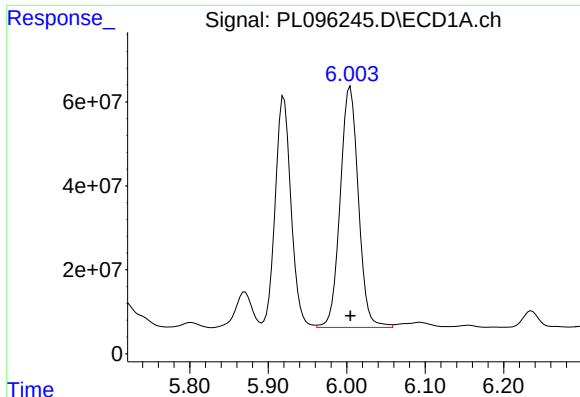

#26 Chlordane-4


R.T.: 6.005 min
Delta R.T.: 0.000 min
Response: 924619051
Conc: 1015.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

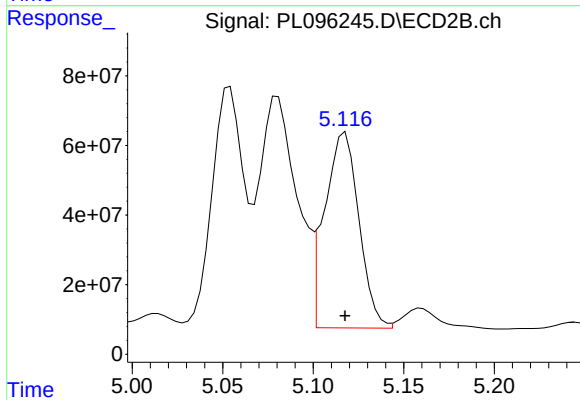


#26 Chlordane-4

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 742292745
Conc: 1011.25 ng/ml

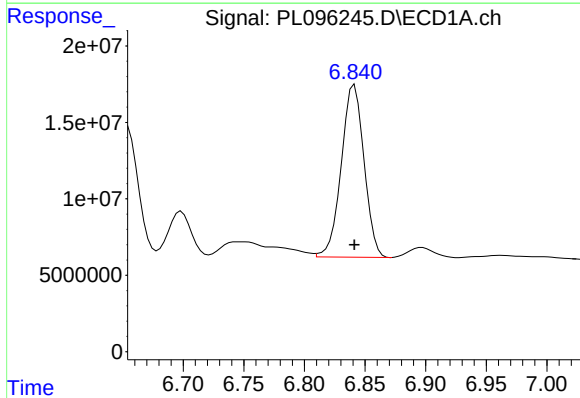


#27 Chlordane-5

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 147097505
Conc: 1011.17 ng/ml

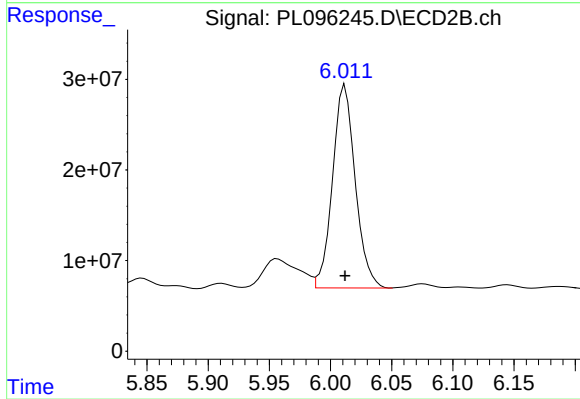

#27 Chlordane-5


R.T.: 6.012 min
Delta R.T.: 0.000 min
Response: 289804509
Conc: 1011.95 ng/ml

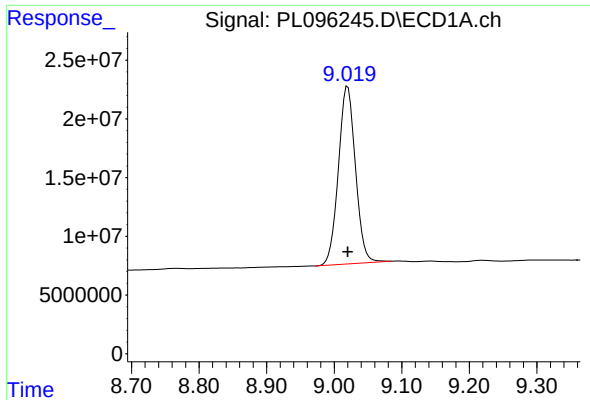

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 264963036
Conc: 99.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

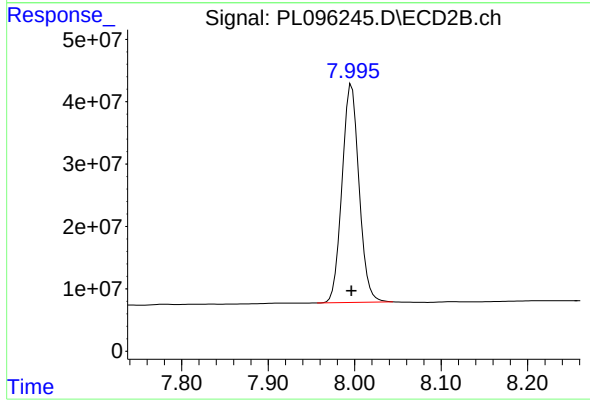

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 475990626
Conc: 99.76 ng/ml