

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
 Data File : PL096246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 12:17
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 14:12:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 14:08:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.828	260.9E6	540.7E6	75.135	75.402
28)	SA Decachlor...	9.021	7.996	197.7E6	348.8E6	74.704	73.725
Target Compounds							
23)	Chlordane-1	4.693	3.840	136.0E6	180.1E6	753.144	751.765
24)	Chlordane-2	5.218	4.421	142.6E6	203.0E6	751.365	751.500
25)	Chlordane-3	5.920	5.054	572.3E6	615.7E6	755.497	755.162
26)	Chlordane-4	6.004	5.118	686.9E6	549.1E6	753.060	748.732
27)	Chlordane-5	6.841	6.012	108.0E6	216.0E6	745.106	752.860



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
Data File : PL096246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 12:17
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 14:12:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 14:08:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

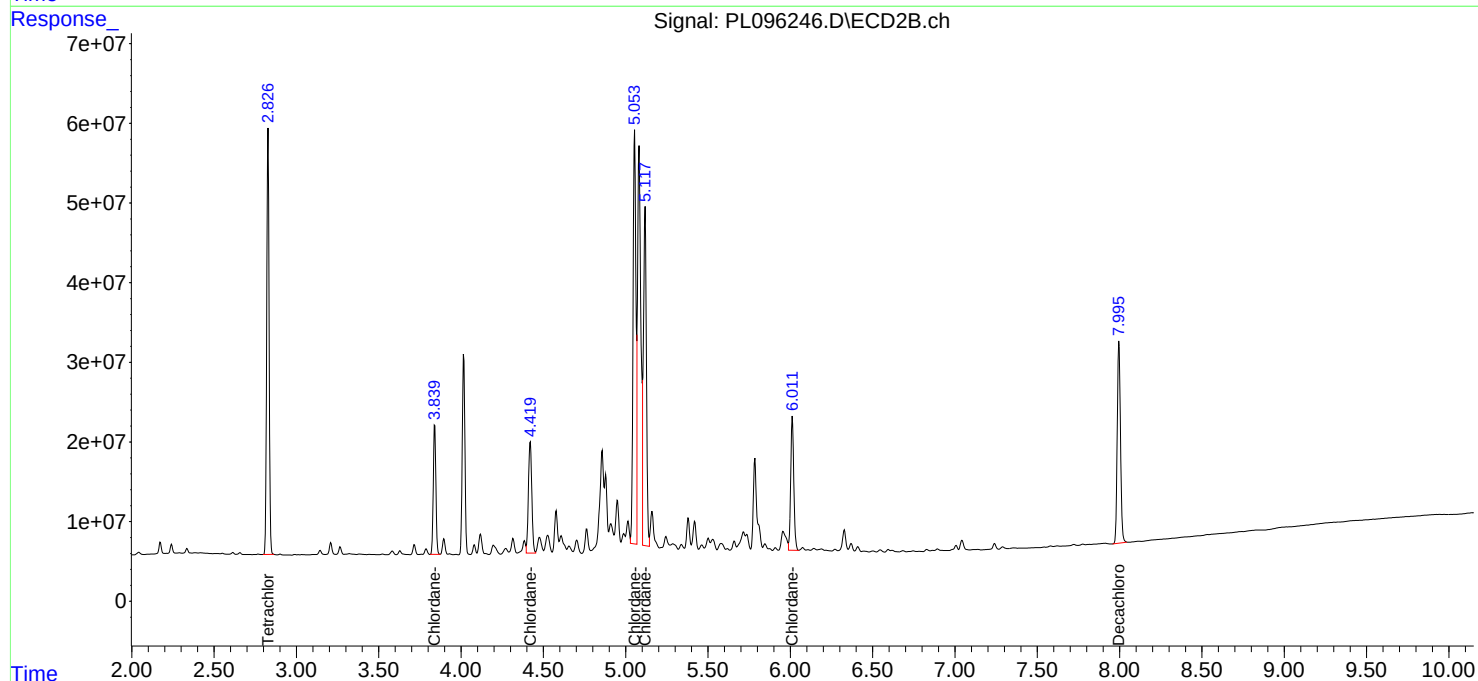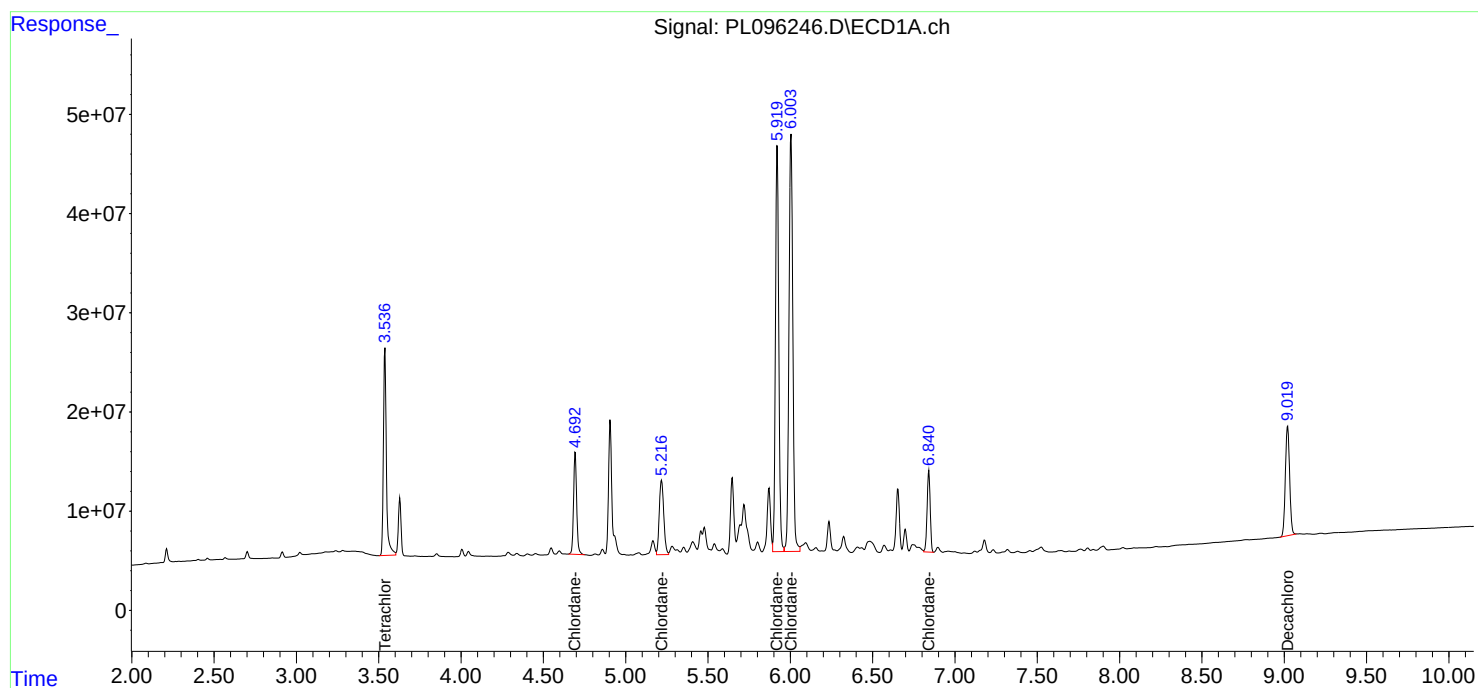


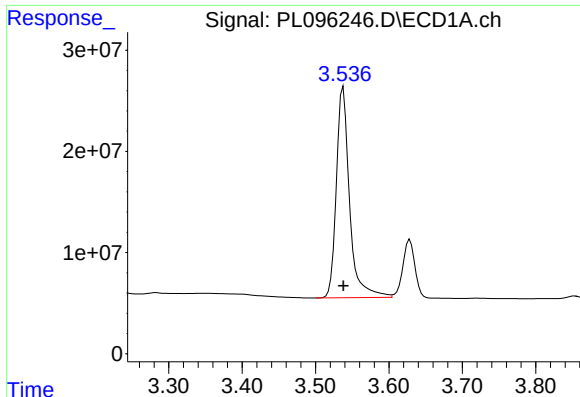

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 260940898
Conc: 75.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

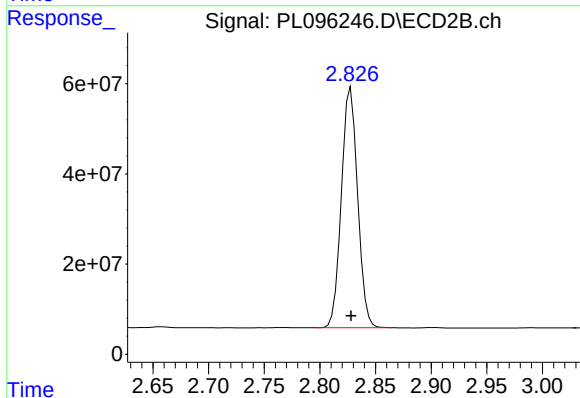


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 540656232
Conc: 75.40 ng/ml

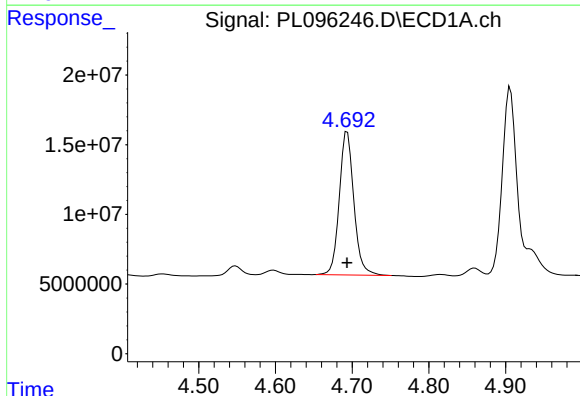


#23 Chlordane-1

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 135954184
Conc: 753.14 ng/ml

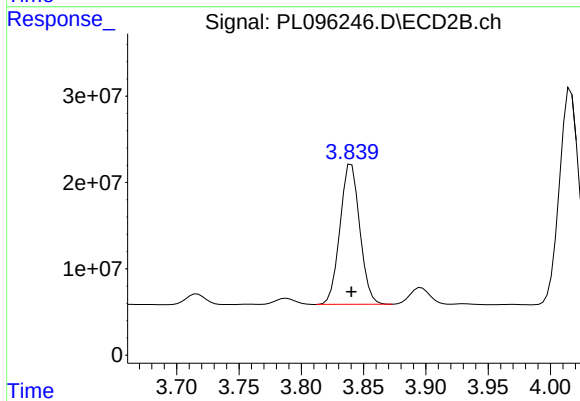

#23 Chlordane-1


R.T.: 3.840 min
Delta R.T.: 0.000 min
Response: 180063945
Conc: 751.76 ng/ml

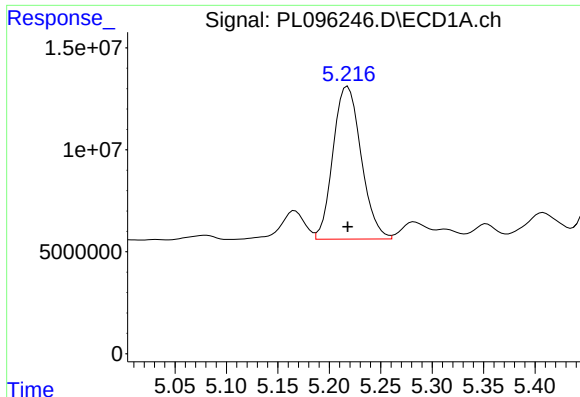

#24 Chlordane-2


R.T.: 5.218 min
Delta R.T.: 0.000 min
Response: 142611870
Conc: 751.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

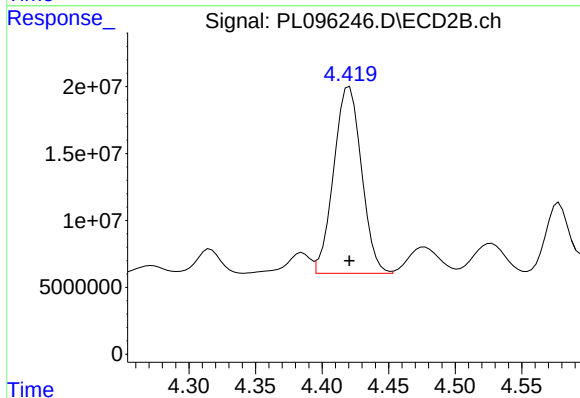


#24 Chlordane-2

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 203020459
Conc: 751.50 ng/ml

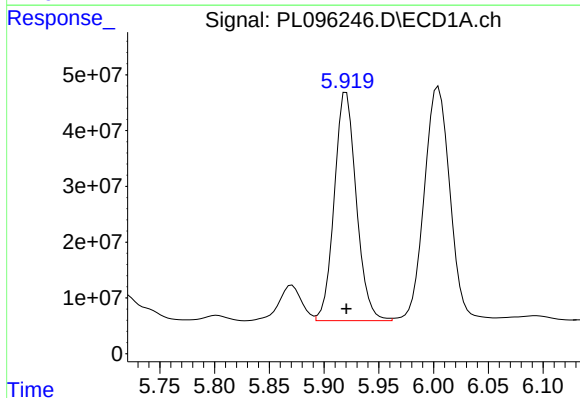


#25 Chlordane-3

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 572255748
Conc: 755.50 ng/ml

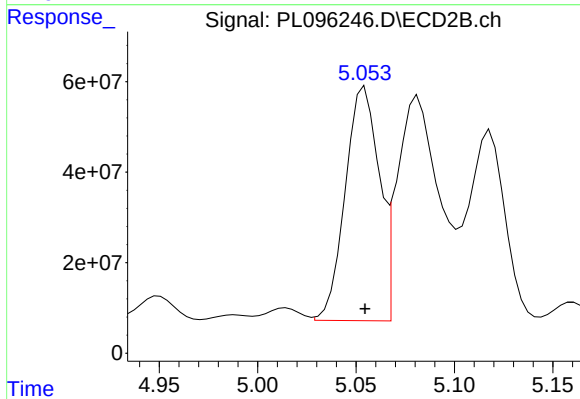

#25 Chlordane-3


R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 615741512
Conc: 755.16 ng/ml

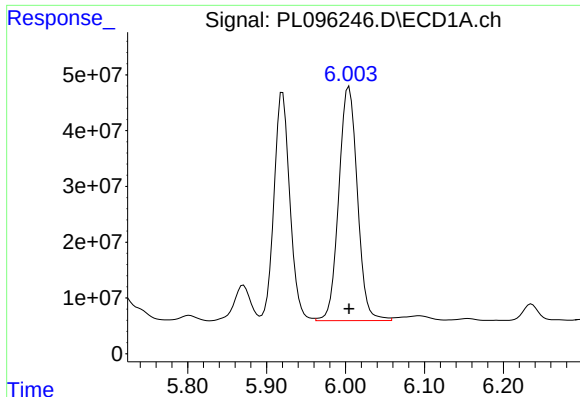

#26 Chlordane-4


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 686914256
Conc: 753.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

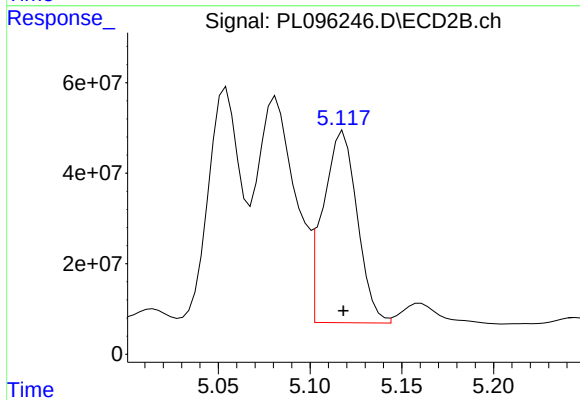


#26 Chlordane-4

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 549129910
Conc: 748.73 ng/ml

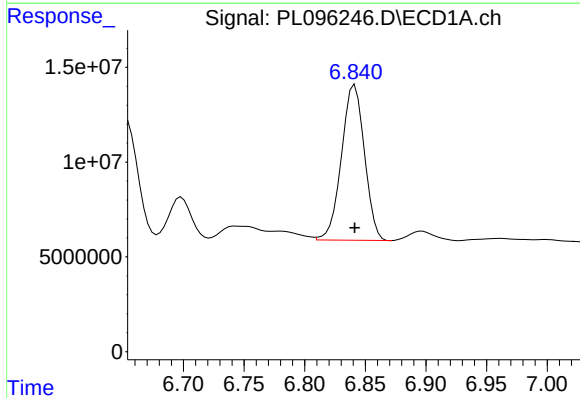


#27 Chlordane-5

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 108040365
Conc: 745.11 ng/ml

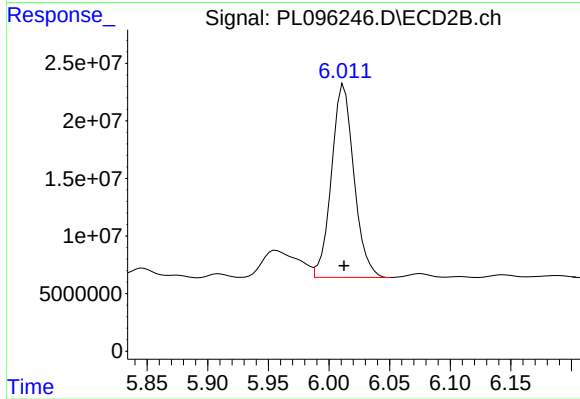

#27 Chlordane-5


R.T.: 6.012 min
Delta R.T.: 0.000 min
Response: 216016946
Conc: 752.86 ng/ml

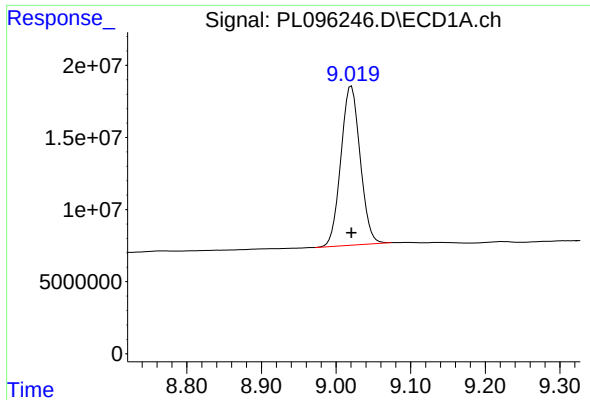

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 197745337
Conc: 74.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

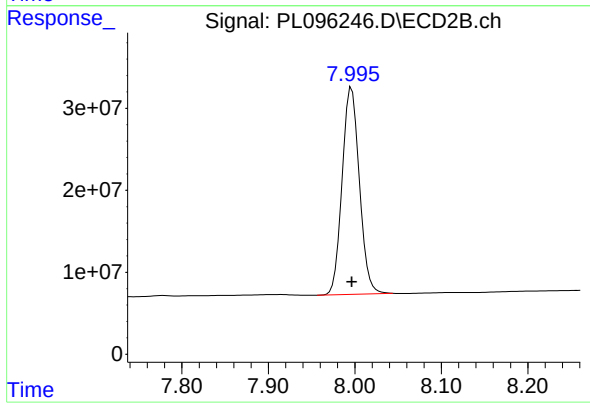

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 348807733
Conc: 73.73 ng/ml