

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
 Data File : PL096248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 12:44
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 14:15:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 14:08:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.828	88266232	176.5E6	25.310	24.708
28)	SA Decachlor...	9.021	7.997	86381759	140.6E6	30.319	28.382
Target Compounds							
23)	Chlordane-1	4.693	3.841	45003342	58967292	249.478	247.130
24)	Chlordane-2	5.217	4.421	50942770	70587790	263.549	258.371
25)	Chlordane-3	5.920	5.055	183.5E6	196.2E6	244.160	242.911
26)	Chlordane-4	6.004	5.118	225.1E6	183.7E6	247.578	250.384
27)	Chlordane-5	6.841	6.013	37021320	70785739	253.969	247.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070725\
Data File : PL096248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 12:44
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 14:15:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 14:08:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

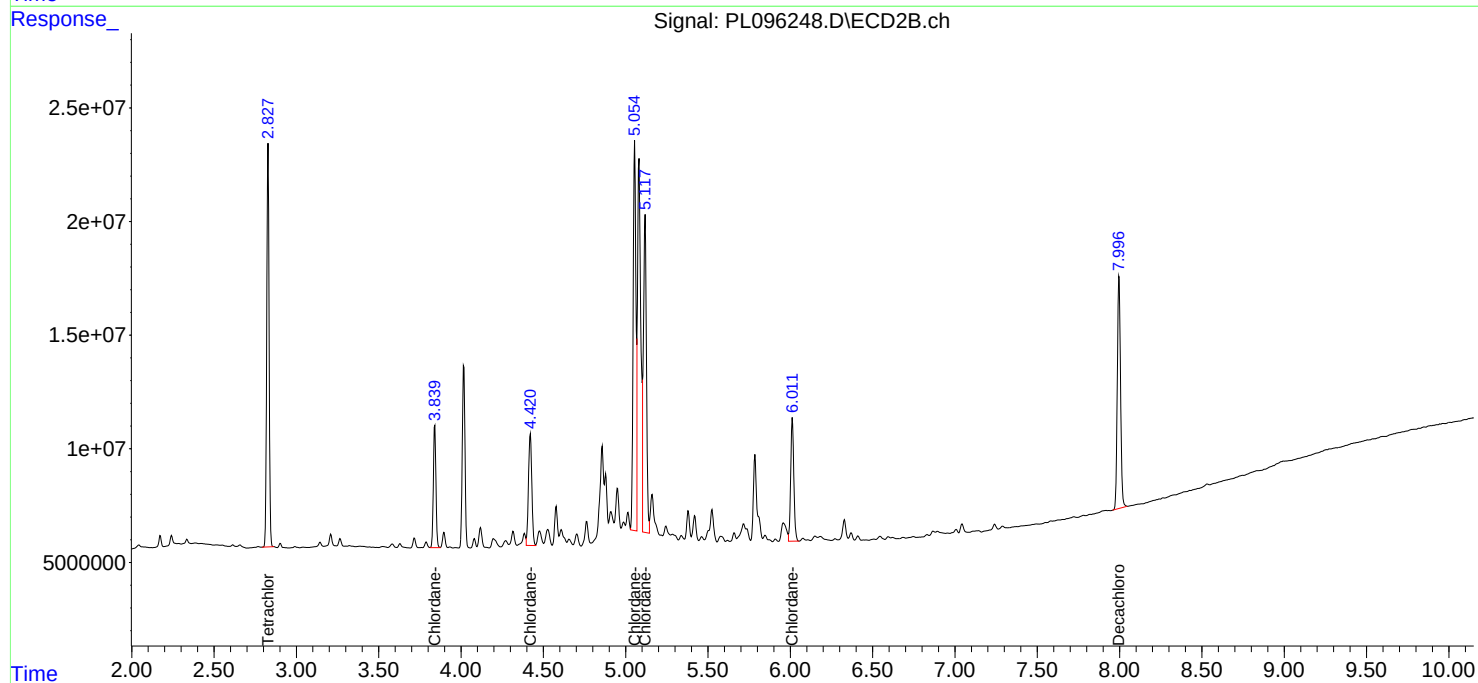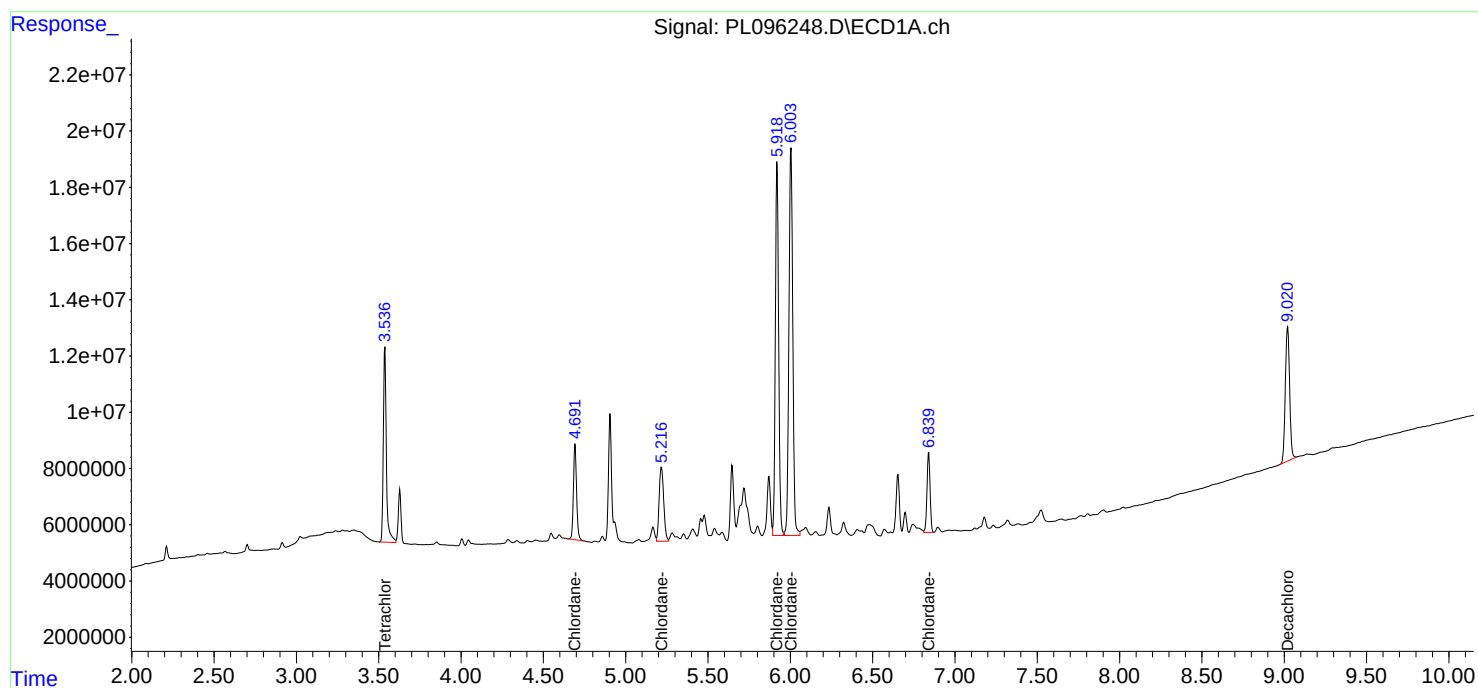


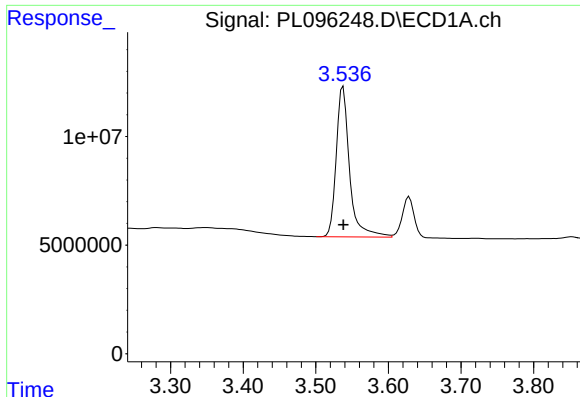

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 88266232
Conc: 25.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

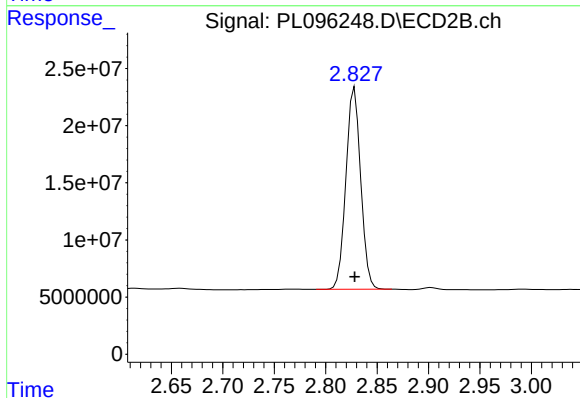


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 176476920
Conc: 24.71 ng/ml

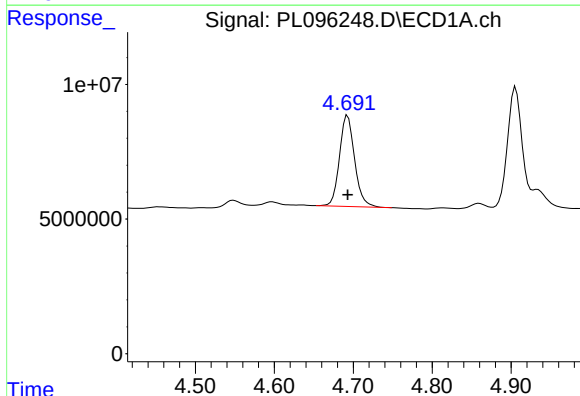


#23 Chlordane-1

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 45003342
Conc: 249.48 ng/ml

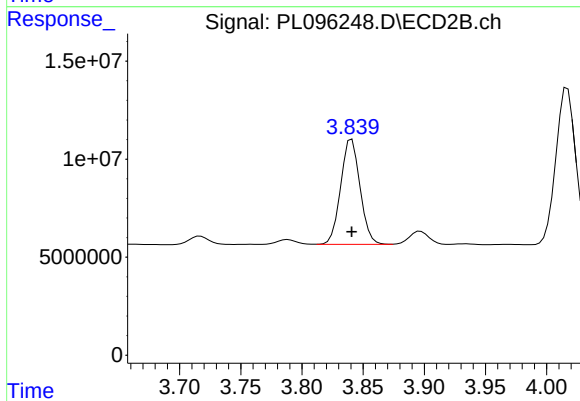

#23 Chlordane-1


R.T.: 3.841 min
Delta R.T.: 0.000 min
Response: 58967292
Conc: 247.13 ng/ml

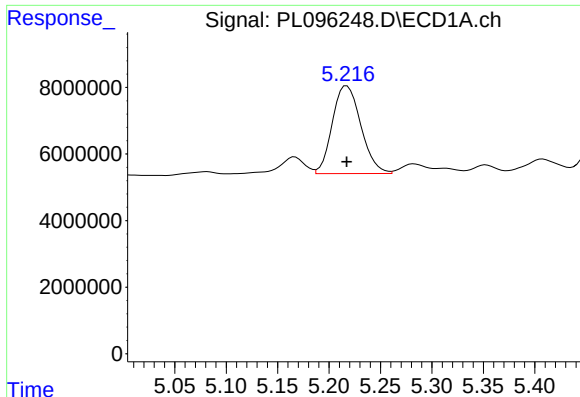

#24 Chlordane-2


R.T.: 5.217 min
Delta R.T.: 0.000 min
Response: 50942770
Conc: 263.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

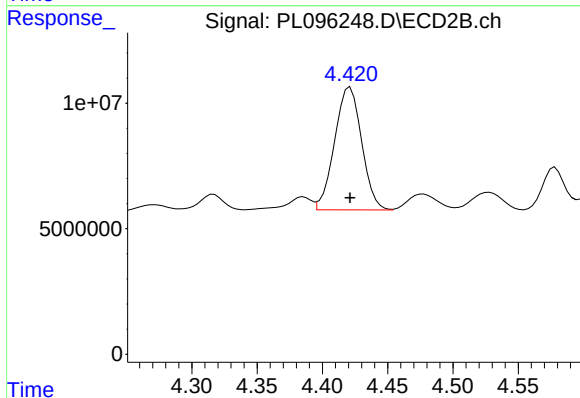


#24 Chlordane-2

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 70587790
Conc: 258.37 ng/ml

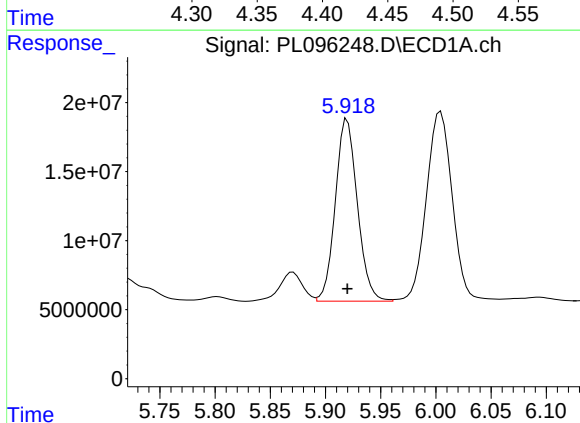


#25 Chlordane-3

R.T.: 5.920 min
Delta R.T.: 0.000 min
Response: 183511473
Conc: 244.16 ng/ml

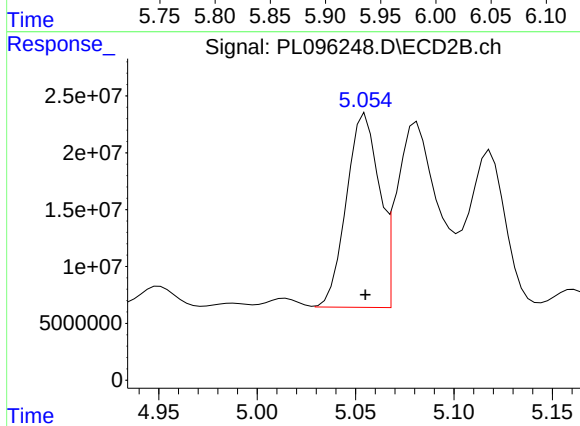

#25 Chlordane-3


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 196209590
Conc: 242.91 ng/ml

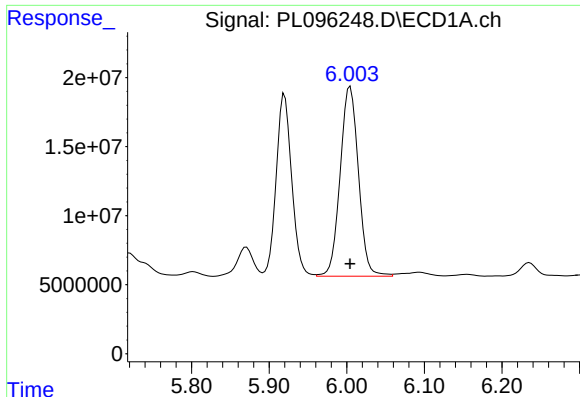

#26 Chlordane-4


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 225104873
Conc: 247.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

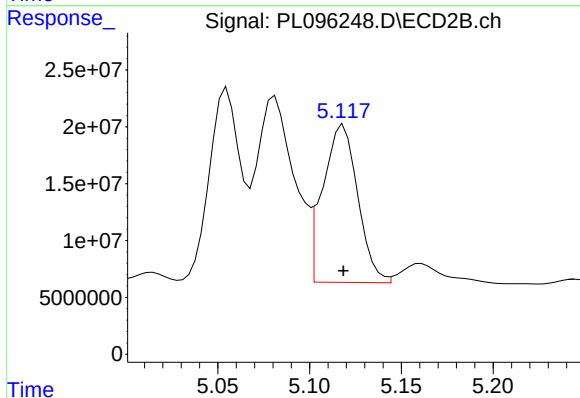


#26 Chlordane-4

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 183729315
Conc: 250.38 ng/ml

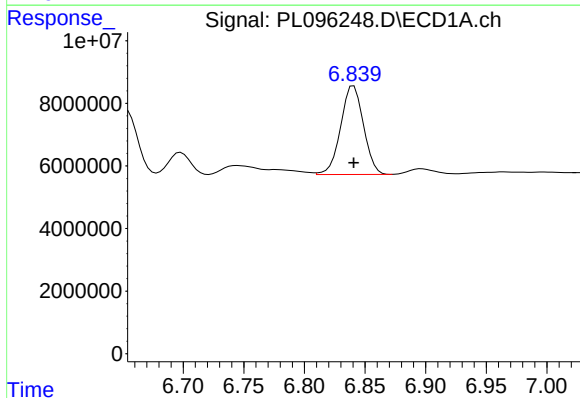


#27 Chlordane-5

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 37021320
Conc: 253.97 ng/ml

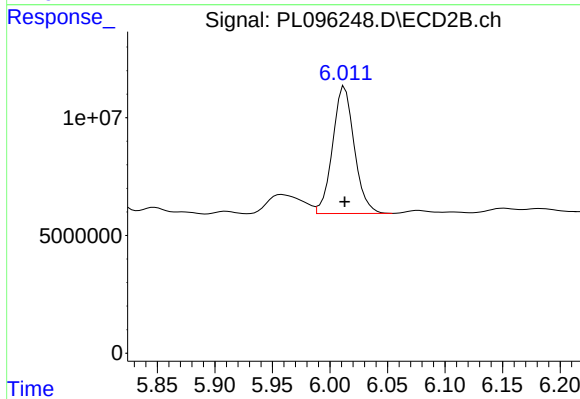

#27 Chlordane-5


R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 70785739
Conc: 247.52 ng/ml

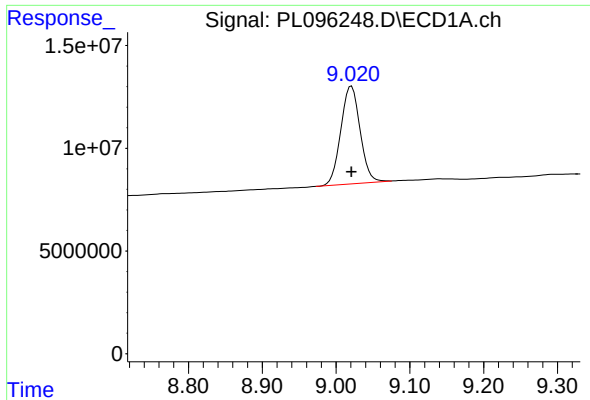

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 86381759
Conc: 30.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

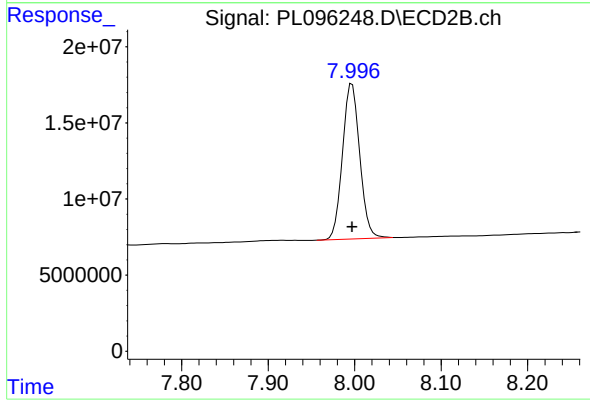

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 140619520
Conc: 28.38 ng/ml