

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070820\
 Data File : PL059777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2020 15:15
 Operator : DD\AJ
 Sample : L3203-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-06

Manual Integrations
 APPROVED

Ankita
 7/9/2020 10:19:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 17:24:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	33632378	50735556	18.726	19.078
28)	SA Decachlor...	8.285	9.180	28098638	38814857	18.303m	17.857m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070820\
Data File : PL059777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2020 15:15
Operator : DD\AJ
Sample : L3203-13
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
7/9/2020 10:19:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 17:24:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

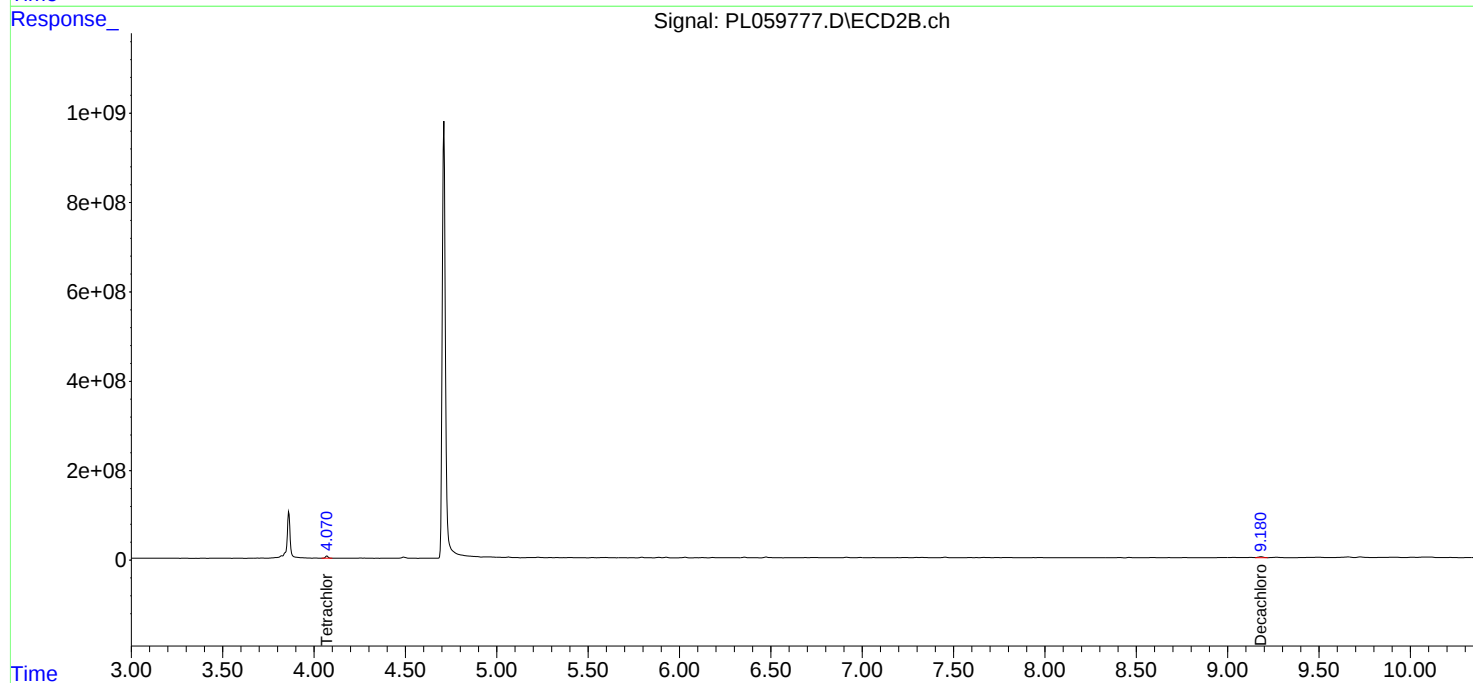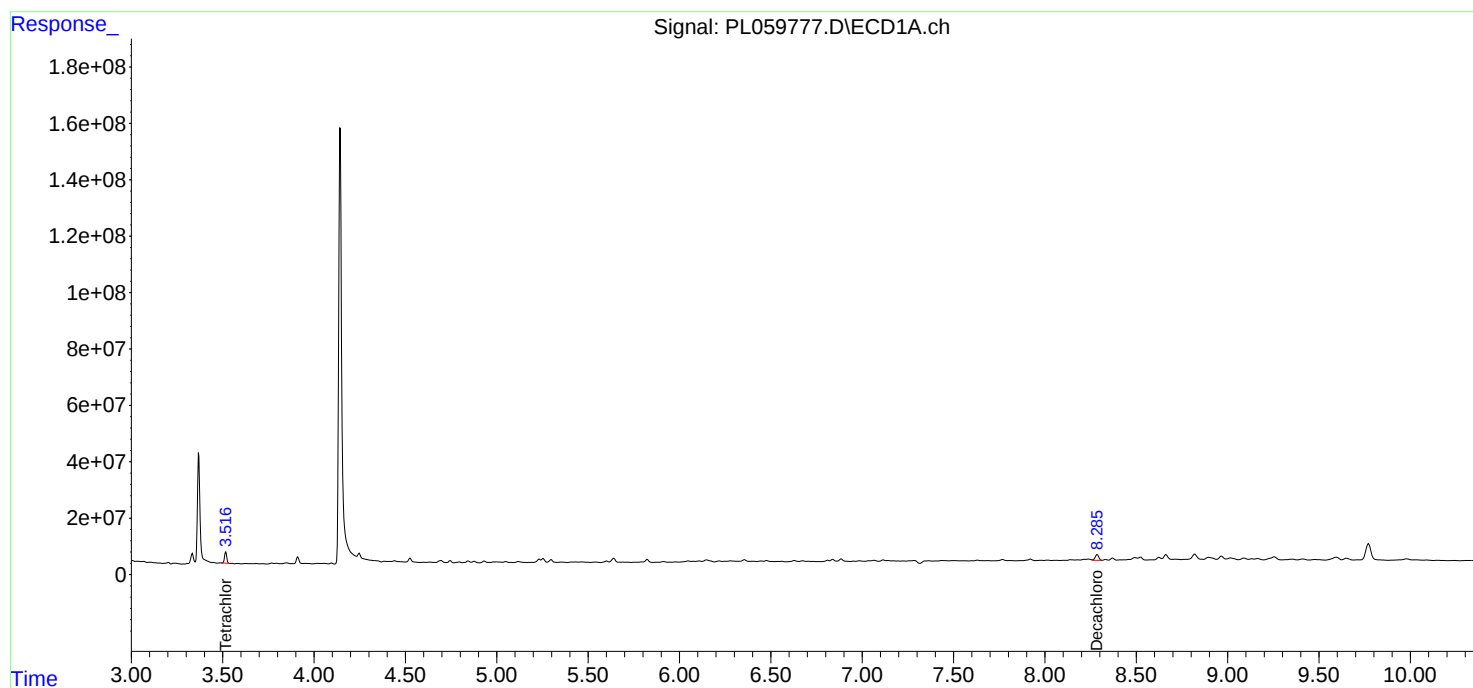

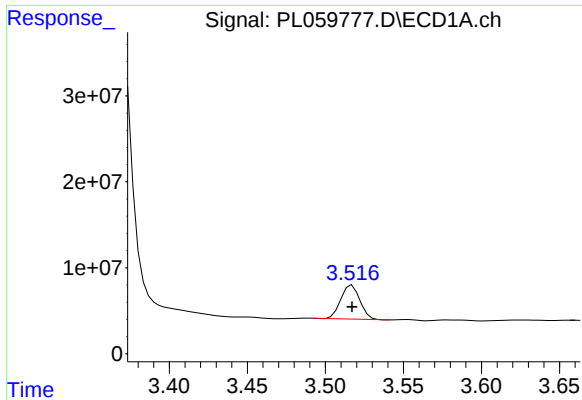


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 33632378
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
7/9/2020 10:19:33 AM

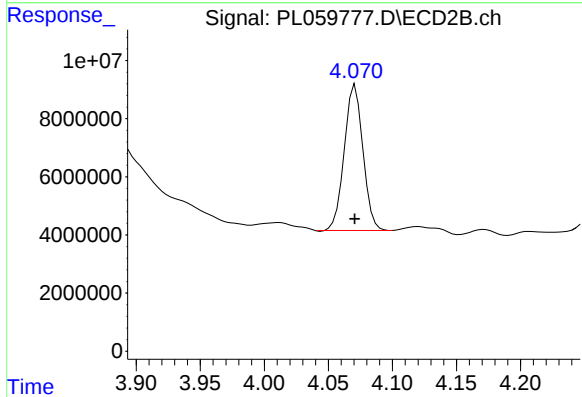


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 50735556
Conc: 19.08 ng/ml

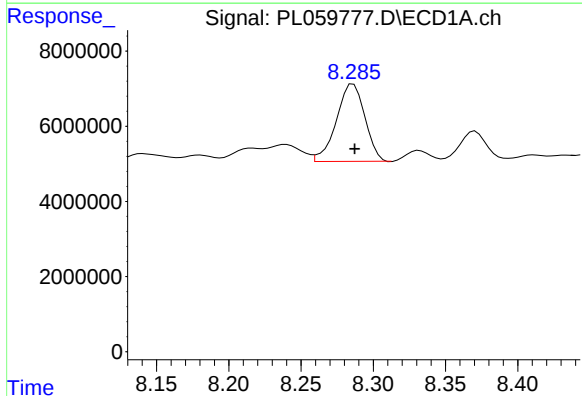

#28 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 28098638
Conc: 18.30 ng/ml m

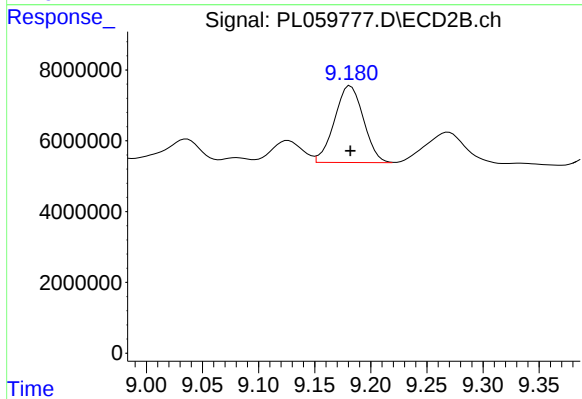

#28 Decachlorobiphenyl

R.T.: 9.180 min
Delta R.T.: -0.002 min
Response: 38814857
Conc: 17.86 ng/ml m