

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070825\
 Data File : PL096258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2025 08:59
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:55:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.659	0.000	292.6E6	0	70.509	N.D.	#
9) A	Endosulfan I	6.035	0.000	43047350	0	10.663	N.D.	#
11) B	alpha-Chl...	0.000	5.111	0	47028538	N.D.	6.254	#
13) MA	Dieldrin	0.000	5.429	0	4585623	N.D.	0.672	#
14) MA	Endrin	0.000	5.720	0	37862567	N.D.	6.211	#
15) B	Endosulfa...	6.752	0.000	4462164	0	1.286	N.D.	#
26)	Chlordane-4	0.000	5.111	0	47028538	N.D.	62.586	#
27)	Chlordane-5	6.839	0.000	2991549	0	19.820	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070825\
Data File : PL096258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2025 08:59
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:55:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

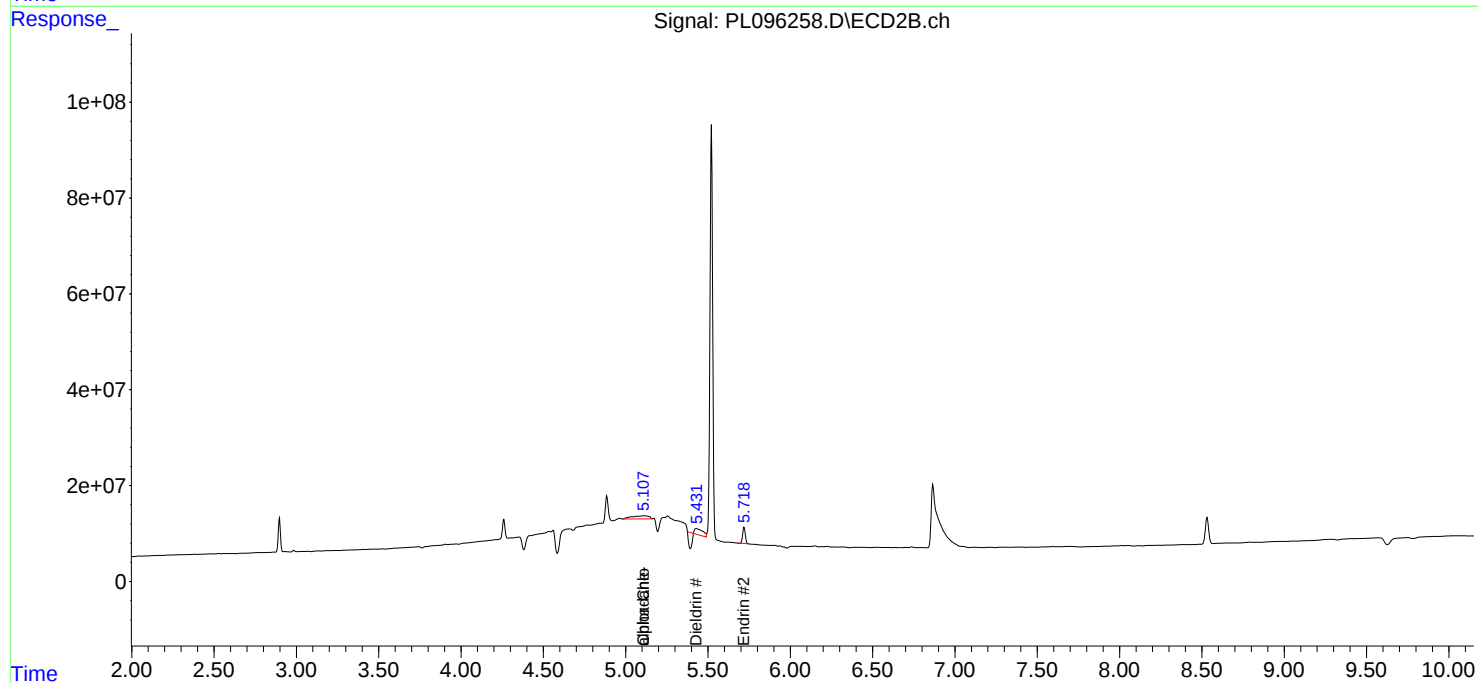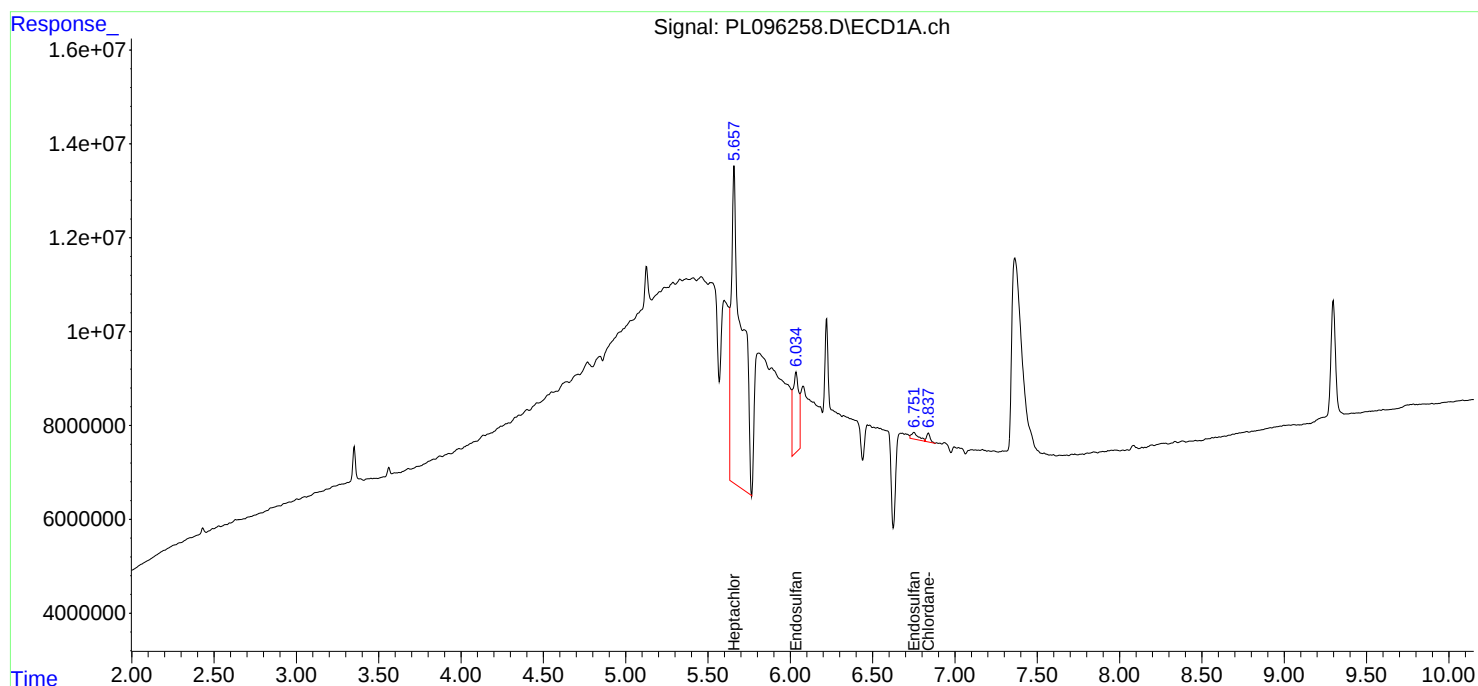


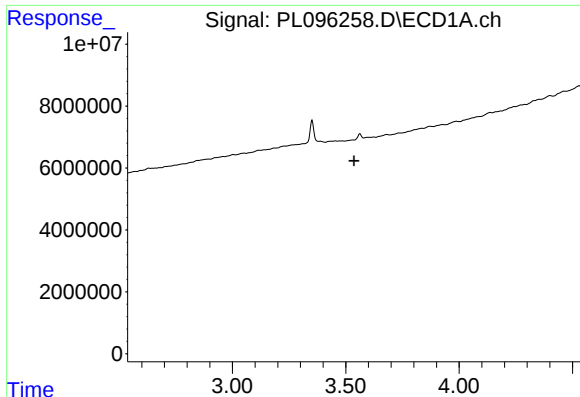

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

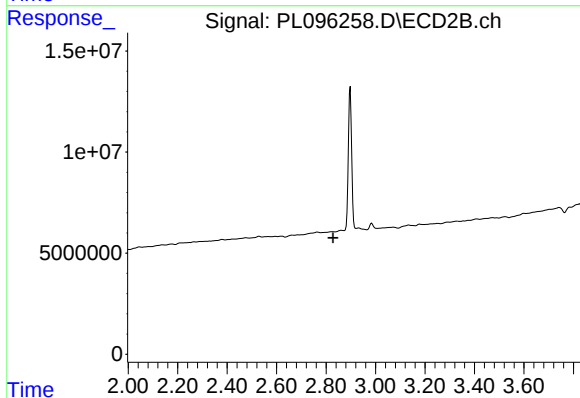


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.828 min
Response: 0
Conc: N.D.

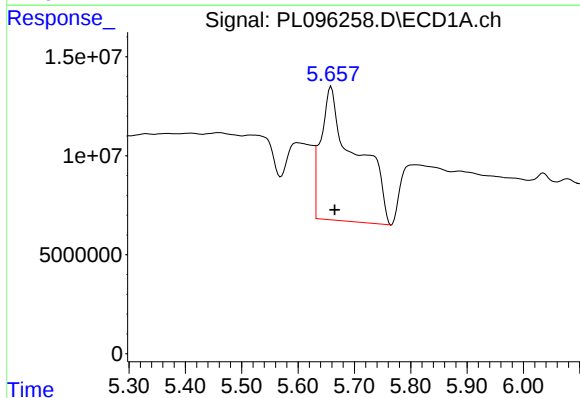


#8 Heptachlor epoxide

R.T.: 5.659 min
Delta R.T.: -0.006 min
Response: 292552134
Conc: 70.51 ng/ml

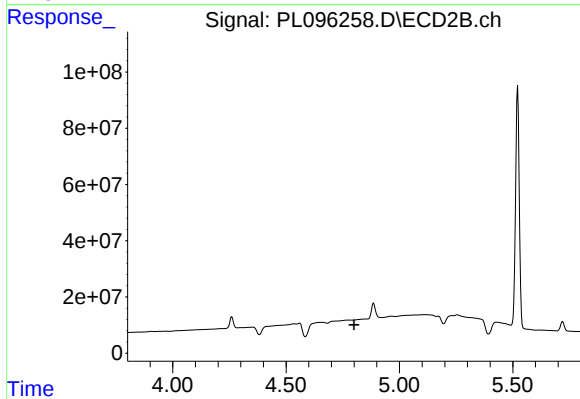

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

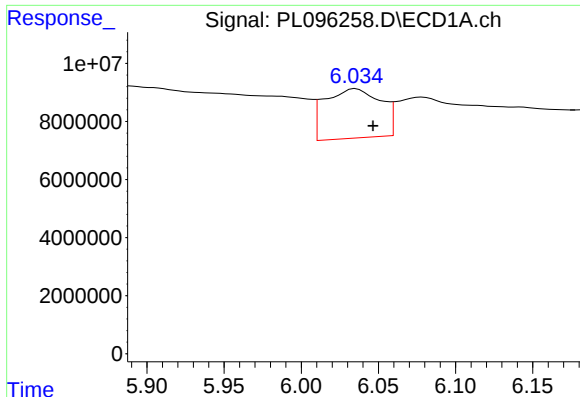

#9 Endosulfan I


R.T.: 6.035 min
Delta R.T.: -0.011 min
Response: 43047350
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

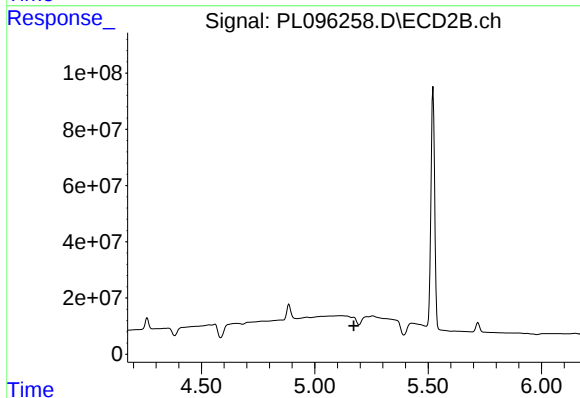


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.172 min
Response: 0
Conc: N.D.

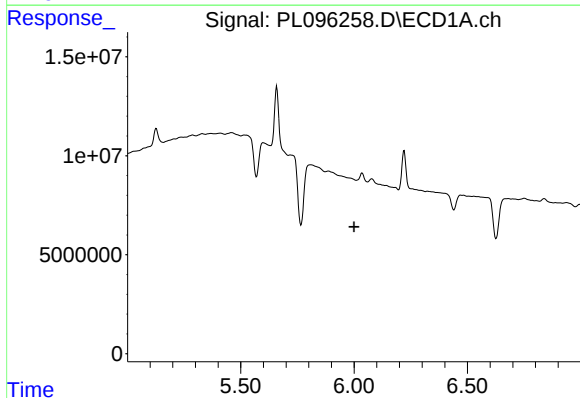


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.000 min
Response: 0
Conc: N.D.

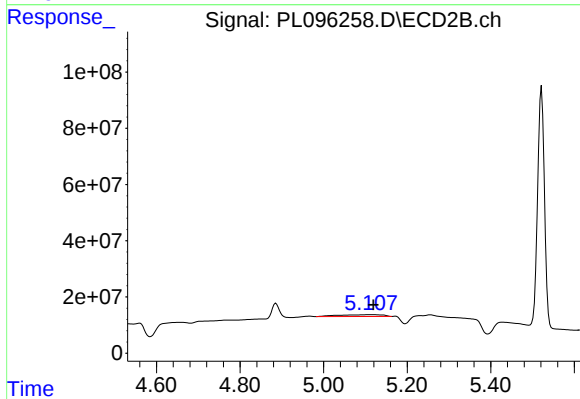

#11 alpha-Chlordane


R.T.: 5.111 min
Delta R.T.: -0.008 min
Response: 47028538
Conc: 6.25 ng/ml

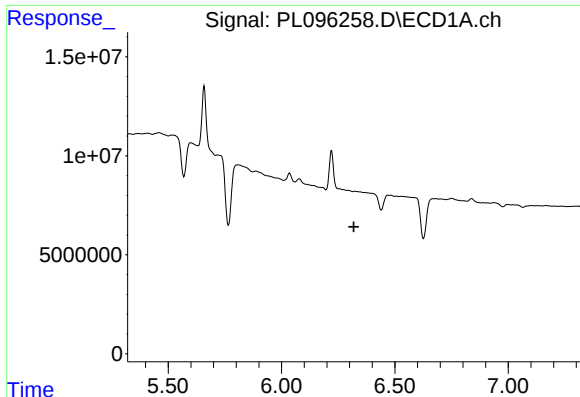

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

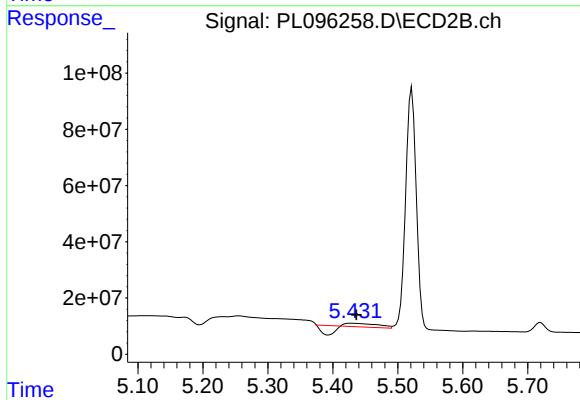


#13 Dieldrin

R.T.: 5.429 min
Delta R.T.: -0.007 min
Response: 4585623
Conc: 0.67 ng/ml

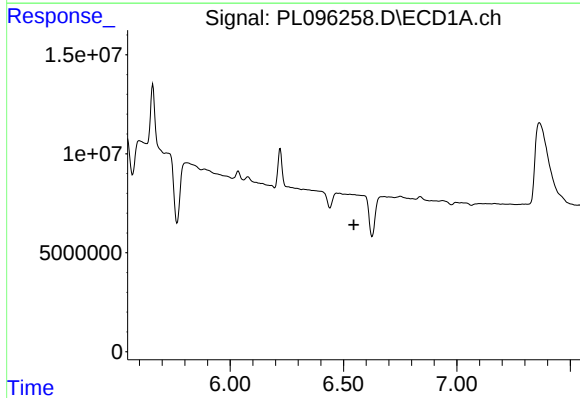


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

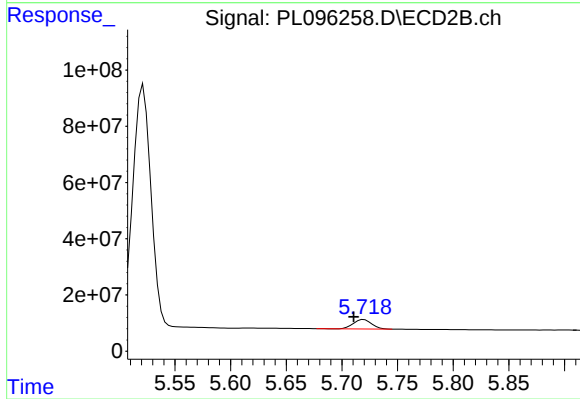

#14 Endrin


R.T.: 5.720 min
Delta R.T.: 0.009 min
Response: 37862567
Conc: 6.21 ng/ml

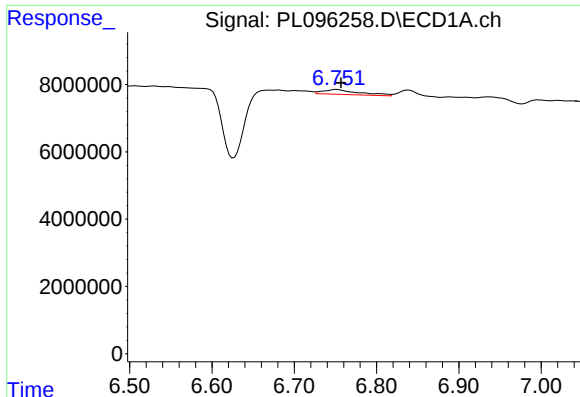

#15 Endosulfan II


R.T.: 6.752 min
Delta R.T.: -0.005 min
Response: 4462164
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

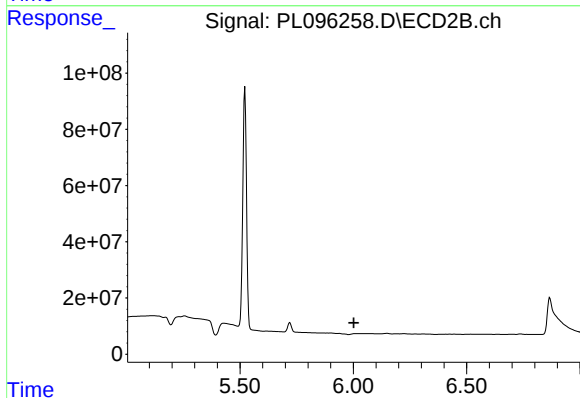


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

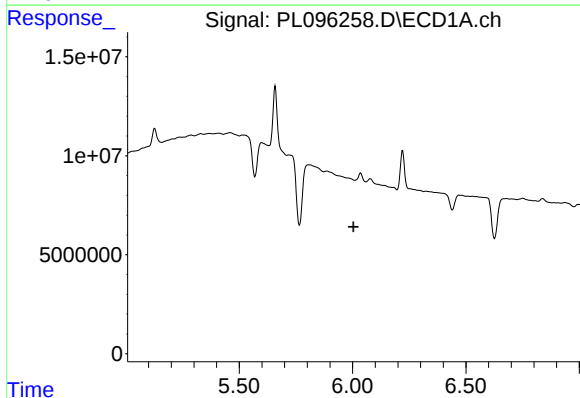


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.

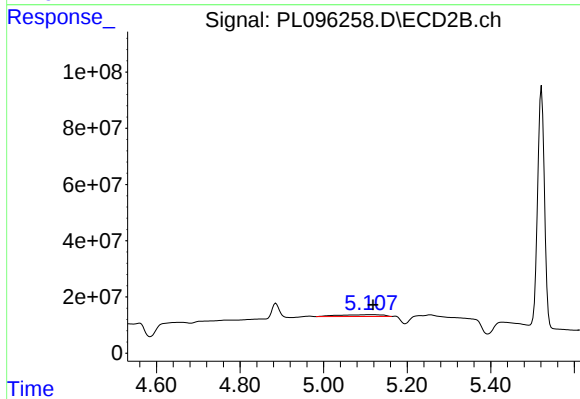

#26 Chlordane-4


R.T.: 5.111 min
Delta R.T.: -0.008 min
Response: 47028538
Conc: 62.59 ng/ml

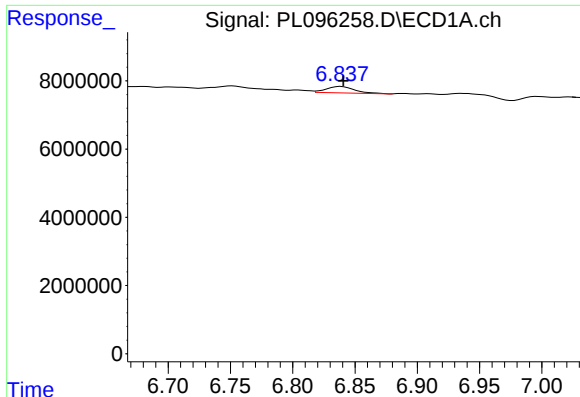

#27 Chlordane-5


R.T.: 6.839 min
Delta R.T.: -0.002 min
Response: 2991549
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

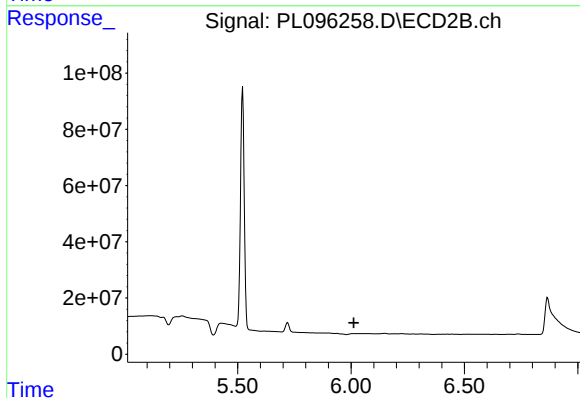


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.013 min
Response: 0
Conc: N.D.

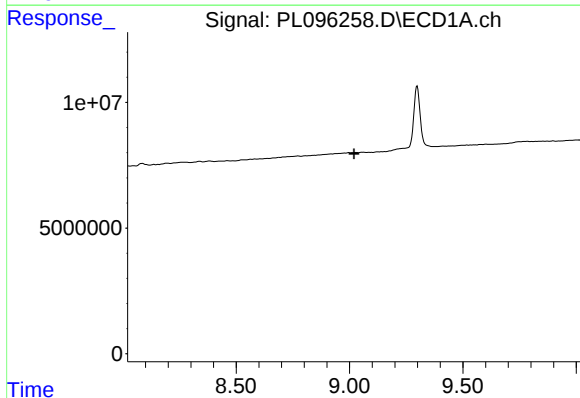

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.020 min
Response: 0
Conc: N.D.

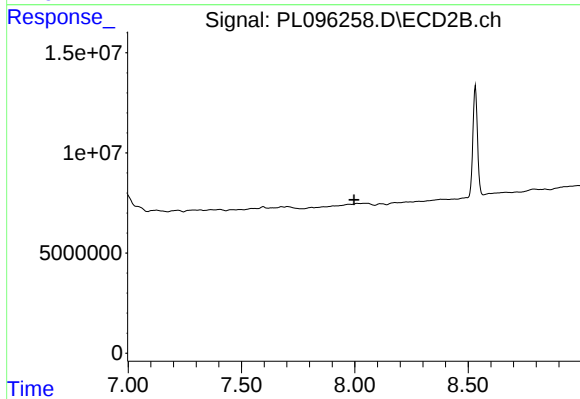

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.997 min
Response: 0
Conc: N.D.