

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
 Data File : PL050240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2019 09:37
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 00:53:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
16) A	4,4'-DDD	5.947	0.000	363.6E6	0	28.800	N.D. #
17) MA	4,4'-DDT	6.176	0.000	313.3E6	0	23.598	N.D. #
18) B	Endrin al...	6.266	0.000	141.7E6	0	12.000	N.D. #
24)	Chlordane-2	4.660	0.000	289.5E6	0	495.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
Data File : PL050240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2019 09:37
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 00:53:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

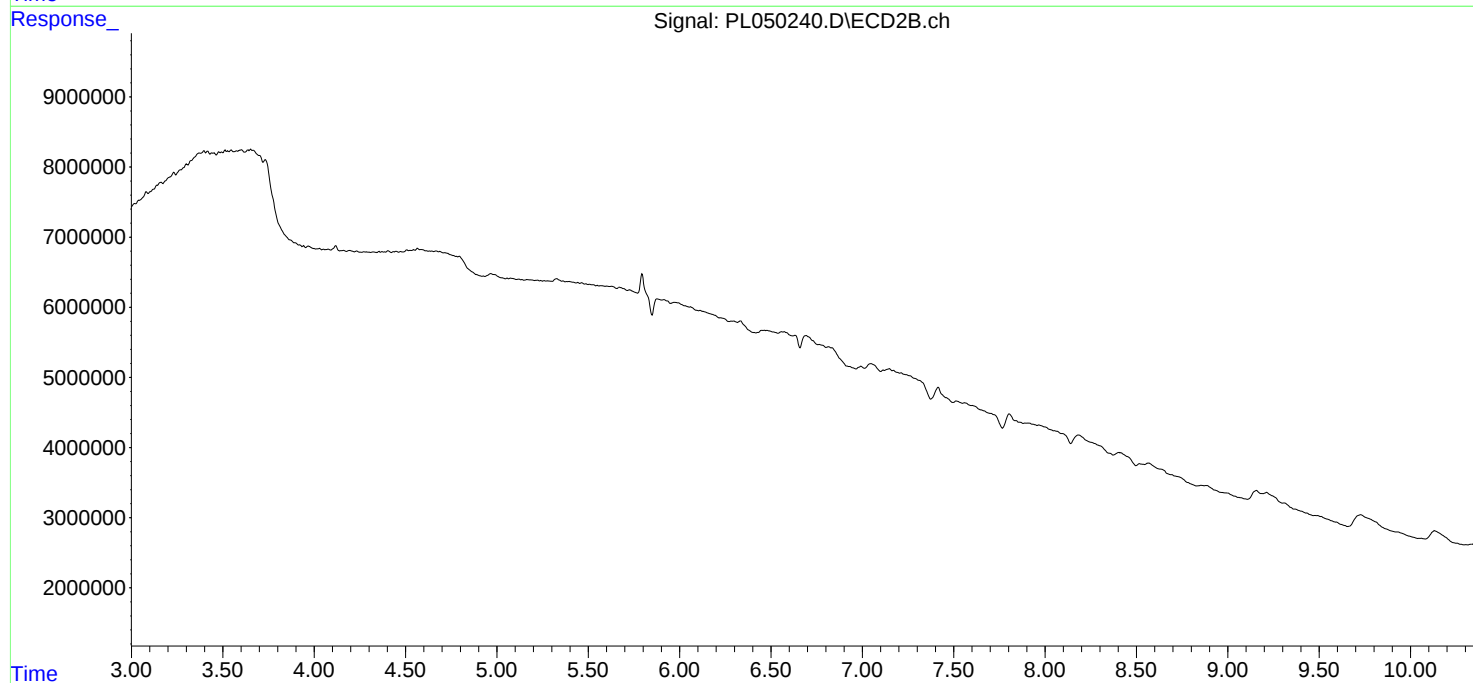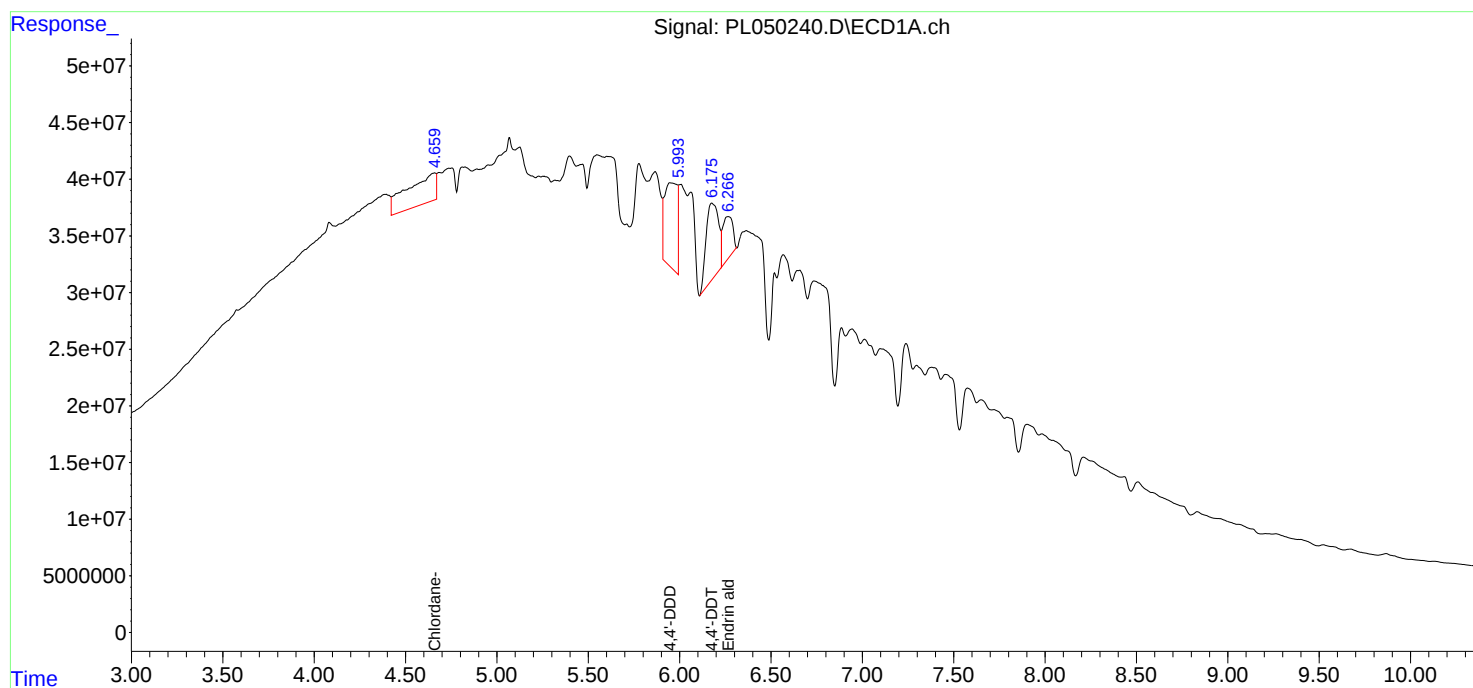


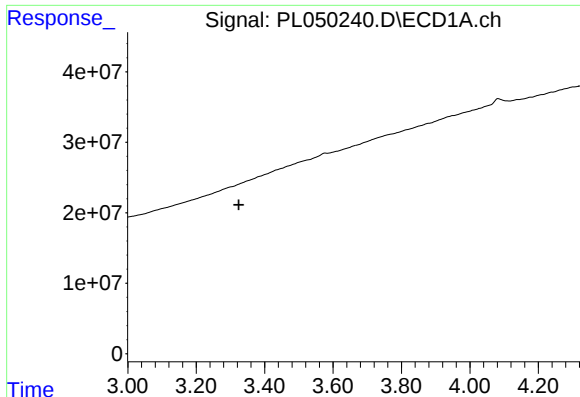

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

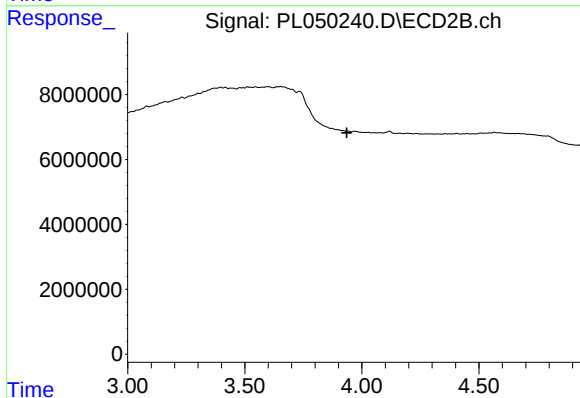


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.935 min
Response: 0
Conc: N.D.

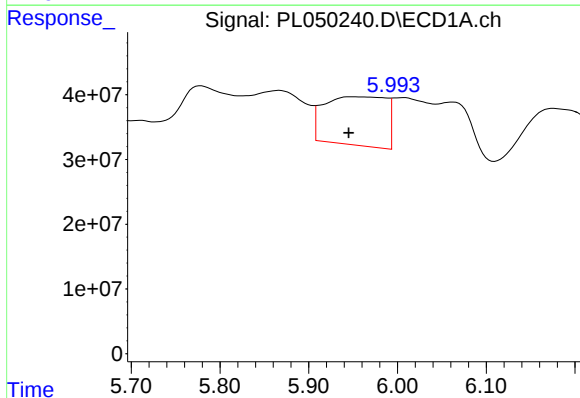


#16 4,4'-DDD

R.T.: 5.947 min
Delta R.T.: 0.002 min
Response: 363565287
Conc: 28.80 ng/ml

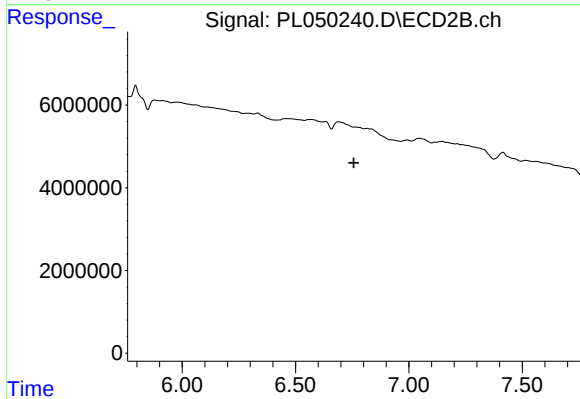

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

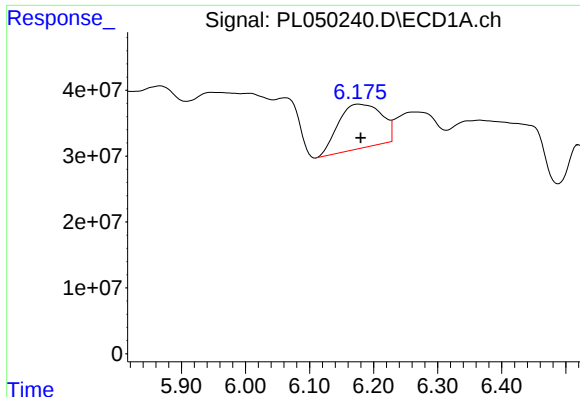

#17 4,4'-DDT


R.T.: 6.176 min
Delta R.T.: -0.003 min
Response: 313277036
Conc: 23.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

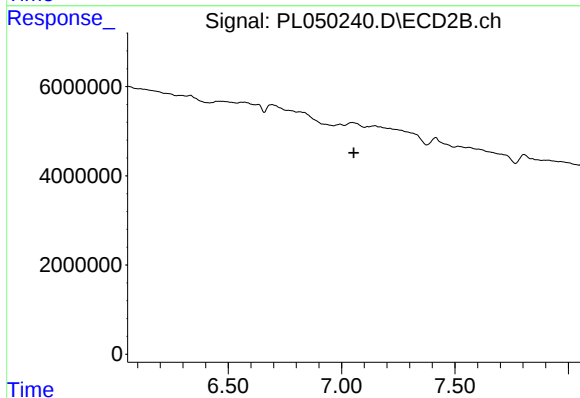


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

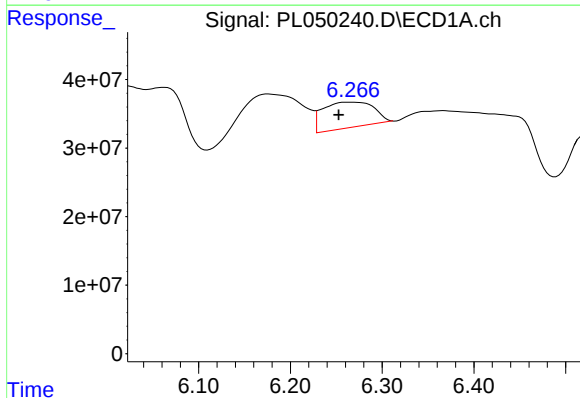


#18 Endrin aldehyde

R.T.: 6.266 min
Delta R.T.: 0.013 min
Response: 141740850
Conc: 12.00 ng/ml

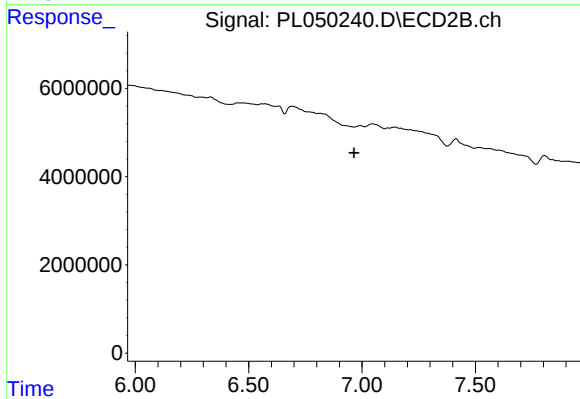

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.965 min
Response: 0
Conc: N.D.

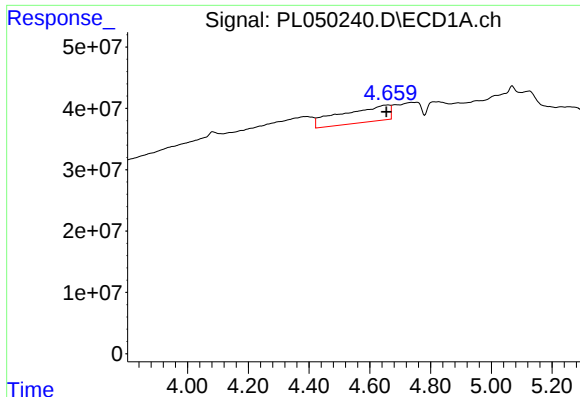

#24 Chlordane-2


R.T.: 4.660 min
Delta R.T.: 0.006 min
Response: 289472538
Conc: 495.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

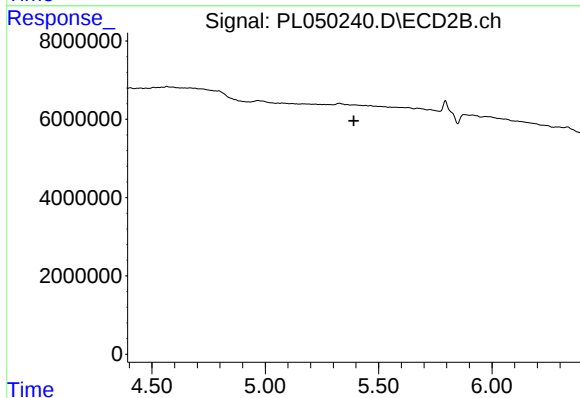


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

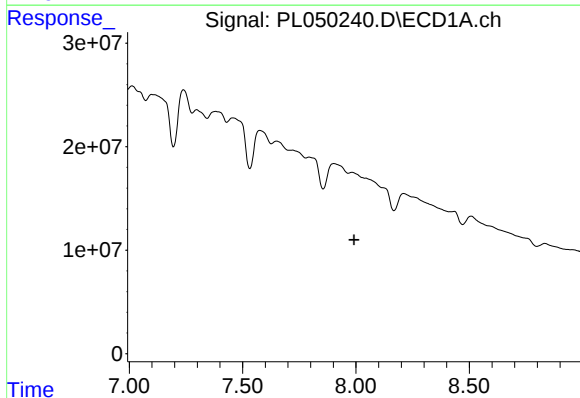

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

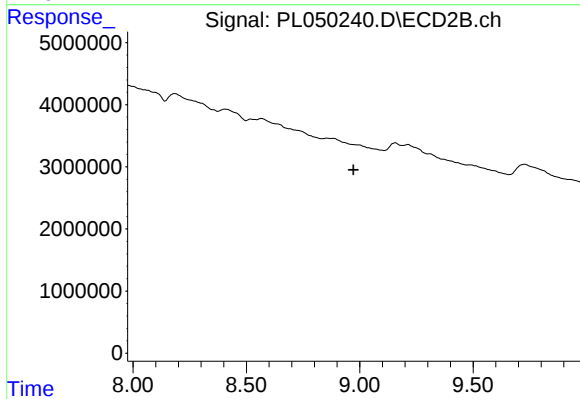

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.973 min
Response: 0
Conc: N.D.