

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
 Data File : PL050249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2019 13:52
 Operator : SM\AJ
 Sample : K3627-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-070819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 00:55:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.932	116.7E6	31687048	10.352	10.349
28)	SA Decachlor...	7.983	8.964	106.5E6	32312658	8.385	9.625
Target Compounds							
10)	B gamma-Chl...	5.224	0.000	21861630	0	1.279	N.D. #
11)	B alpha-Chl...	0.000	6.101	0	12740928	N.D.	3.445 #
25)	Chlordane-3	5.224	0.000	21861630	0	11.640	N.D. #
26)	Chlordane-4	0.000	6.101	0	12740928	N.D.	21.437 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
Data File : PL050249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2019 13:52
Operator : SM\AJ
Sample : K3627-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-070819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 00:55:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

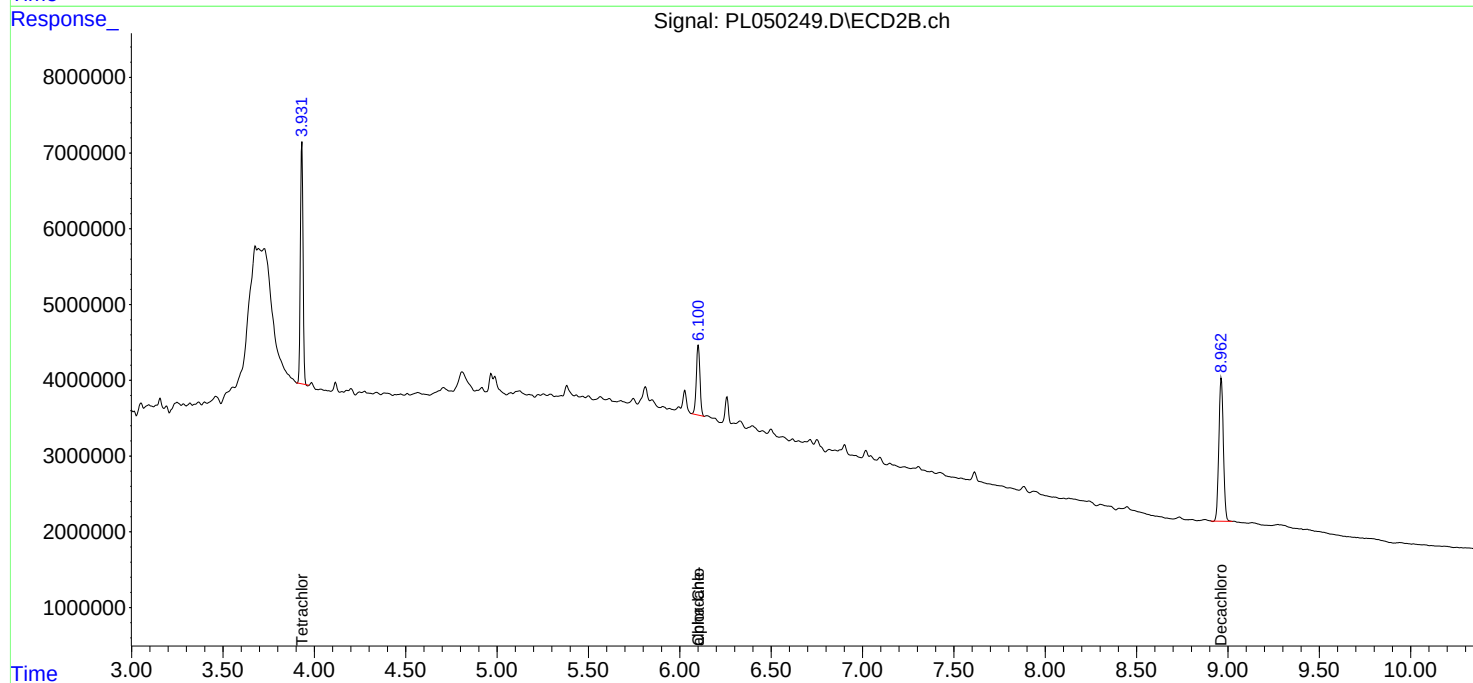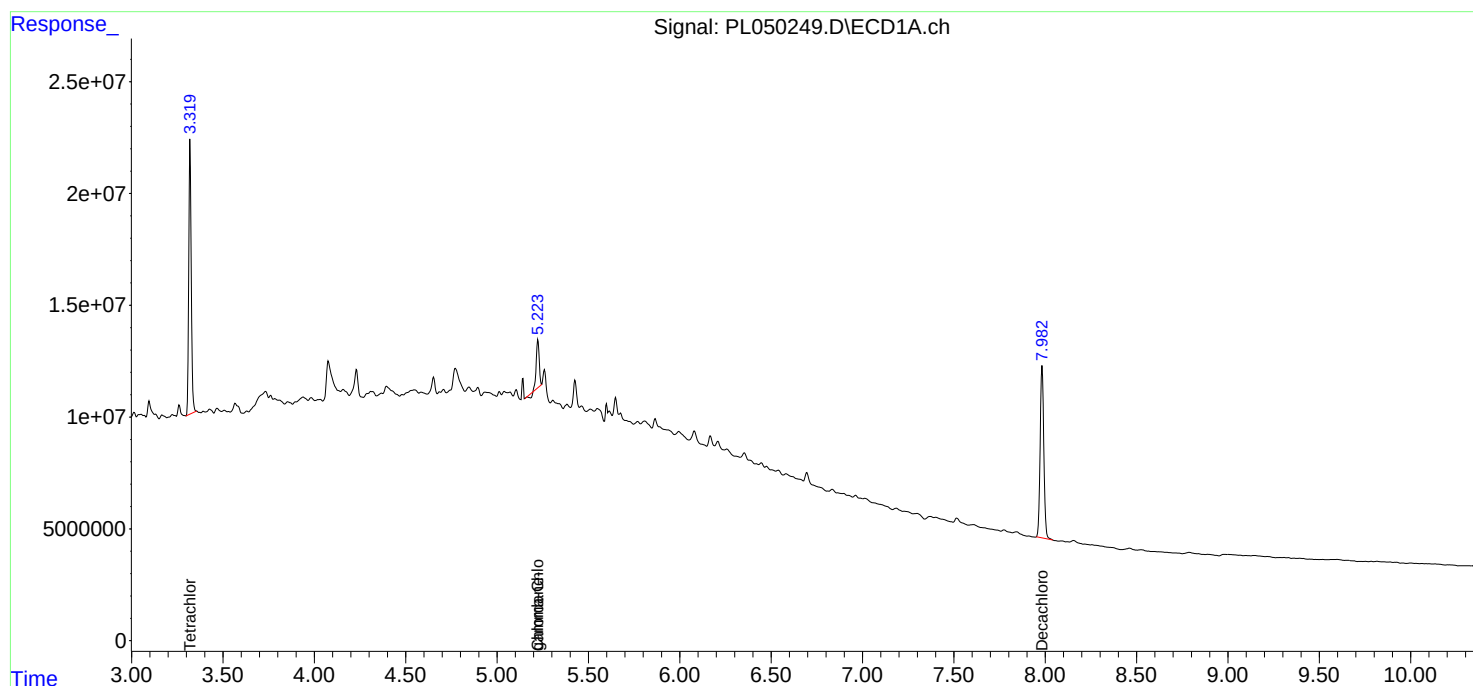


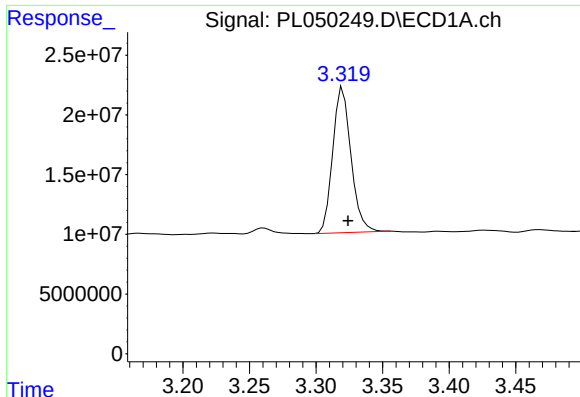

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 116747368
Conc: 10.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-070819

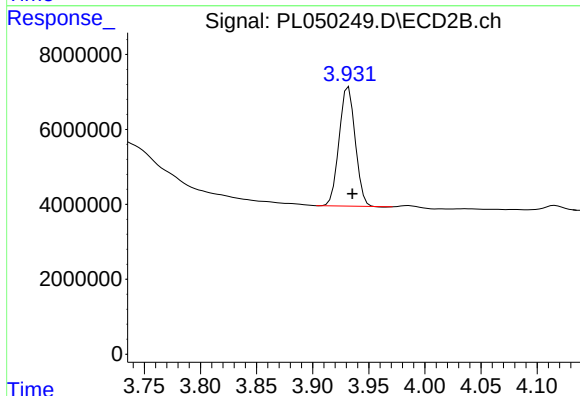


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 31687048
Conc: 10.35 ng/ml

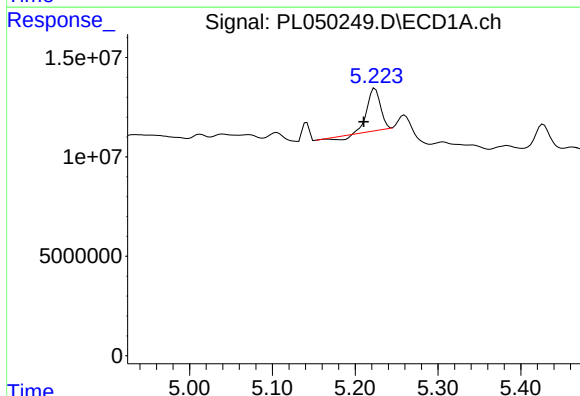


#10 gamma-Chlordane

R.T.: 5.224 min
Delta R.T.: 0.014 min
Response: 21861630
Conc: 1.28 ng/ml

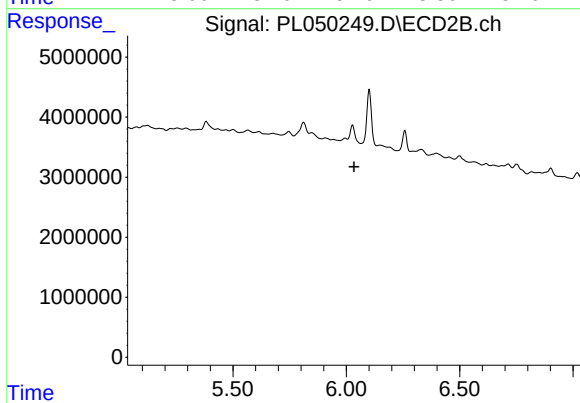

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.034 min
Response: 0
Conc: N.D.

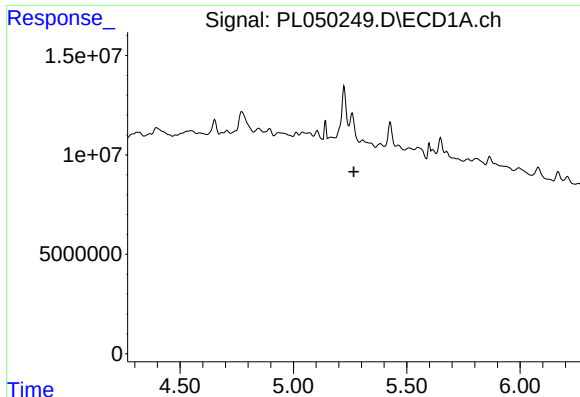

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-070819

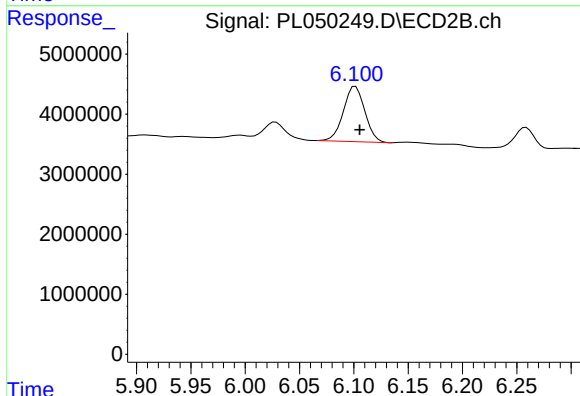


#11 alpha-Chlordane

R.T.: 6.101 min
Delta R.T.: -0.004 min
Response: 12740928
Conc: 3.44 ng/ml

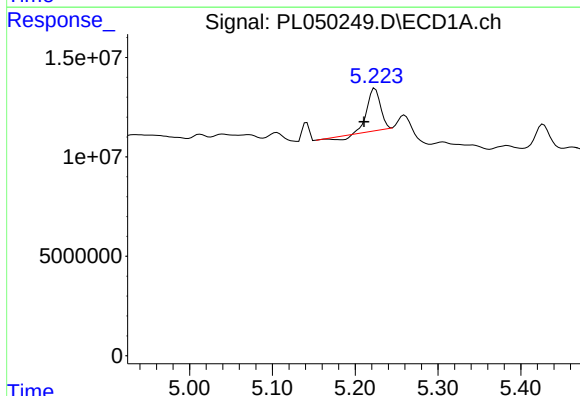


#25 Chlordane-3

R.T.: 5.224 min
Delta R.T.: 0.013 min
Response: 21861630
Conc: 11.64 ng/ml

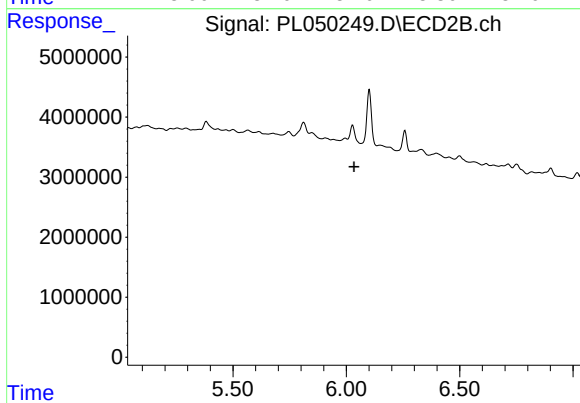

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.035 min
Response: 0
Conc: N.D.

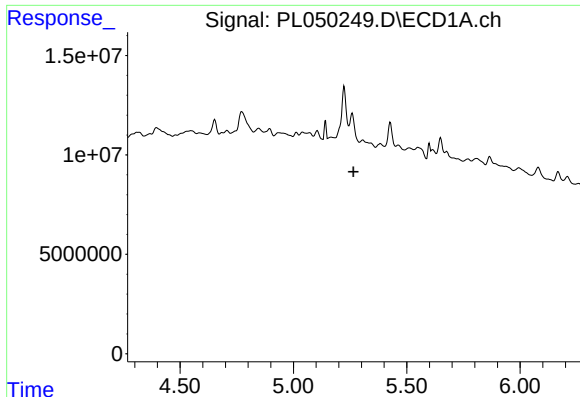

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-070819

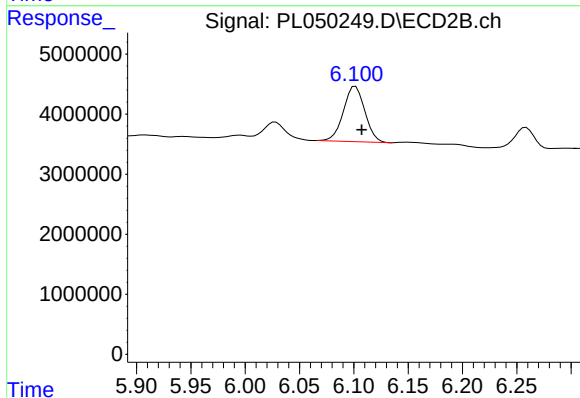


#26 Chlorodane-4

R.T.: 6.101 min
Delta R.T.: -0.006 min
Response: 12740928
Conc: 21.44 ng/ml

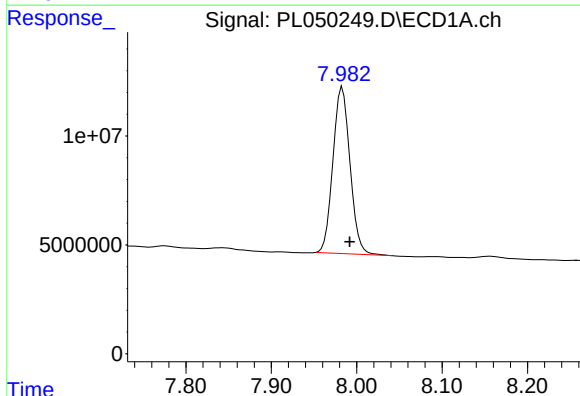

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.009 min
Response: 106538139
Conc: 8.38 ng/ml

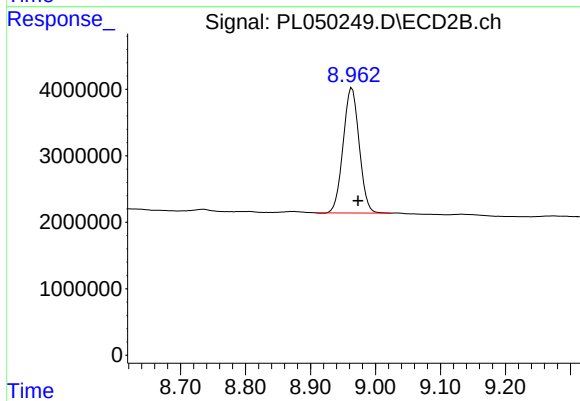

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.009 min
Response: 32312658
Conc: 9.63 ng/ml