

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
 Data File : PL050258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2019 16:03
 Operator : SM\AJ
 Sample : K3700-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-052

Manual Integrations
 APPROVED

Ankita
 7/10/2019 9:52:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 00:58:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.932	85352362	22977161	7.568	7.505
28)	SA Decachlor...	7.985	8.964	76133876	20831776	5.992	6.205
Target Compounds							
11)	B alpha-Chl...	5.259	6.102	6522659	5334195	0.393m	1.442m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070919\
Data File : PL050258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2019 16:03
Operator : SM\AJ
Sample : K3700-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-052


Manual Integrations
APPROVED

Ankita
7/10/2019 9:52:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 00:58:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

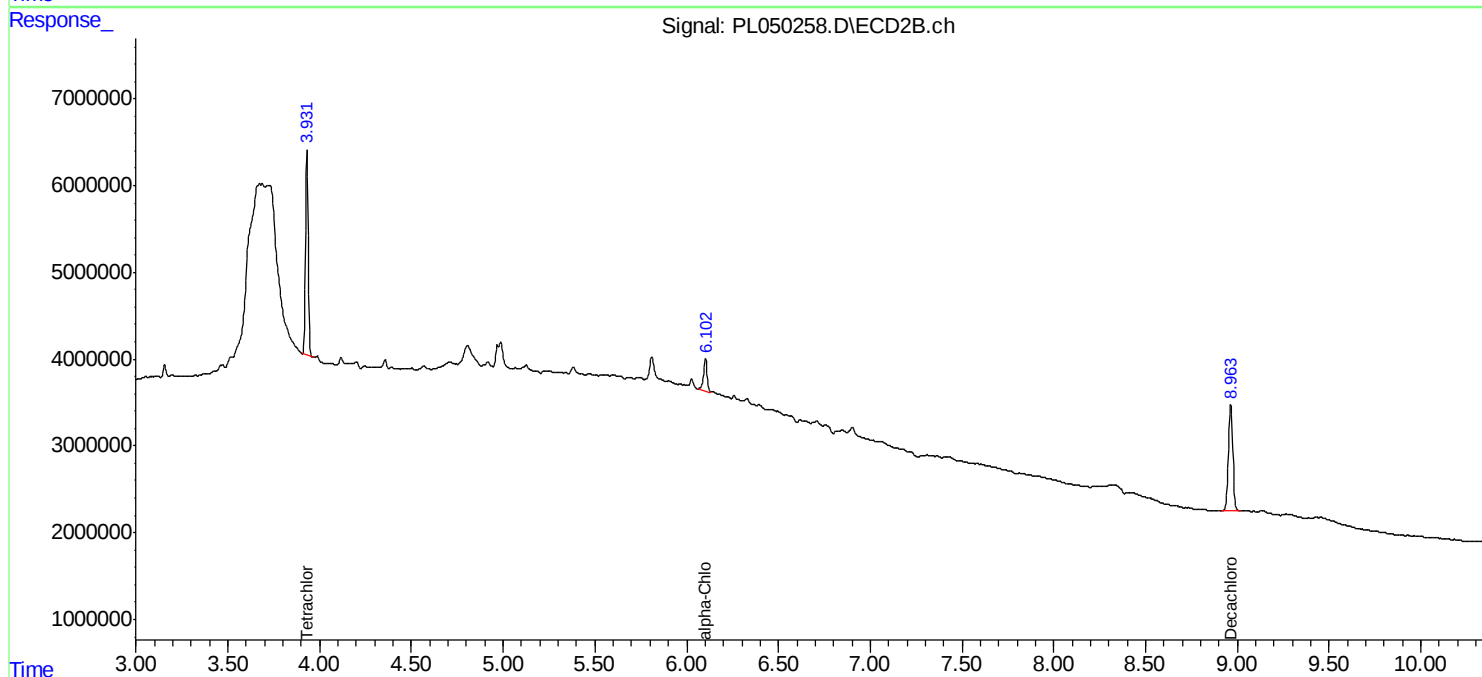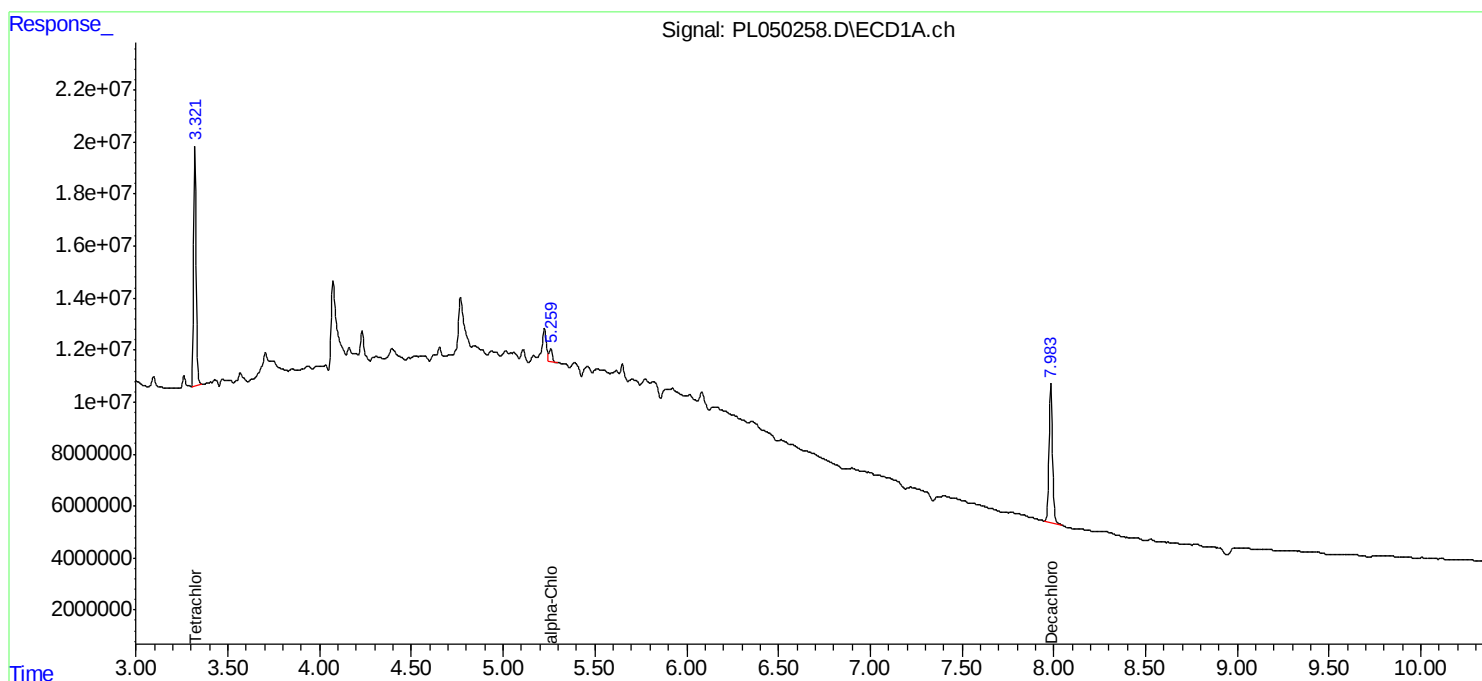

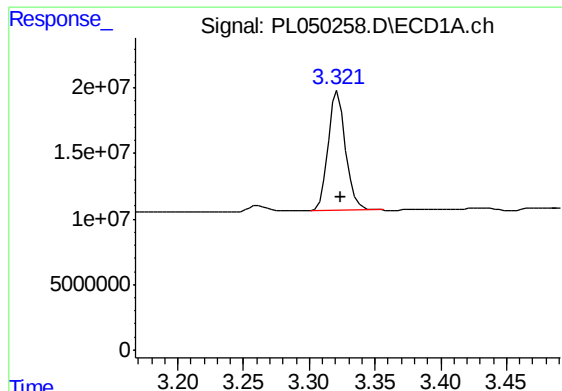


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 85352362
Conc: 7.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-052


Manual Integrations
APPROVED

Ankita
7/10/2019 9:52:12 AM

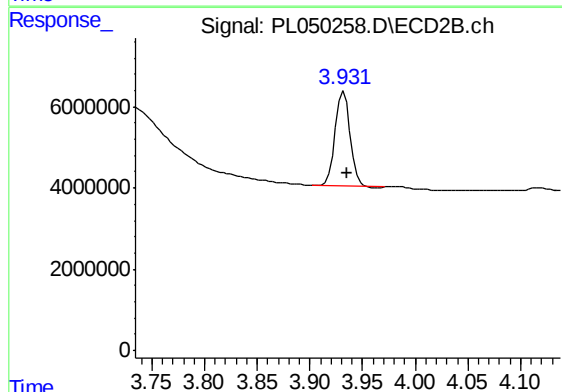


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 22977161
Conc: 7.50 ng/ml

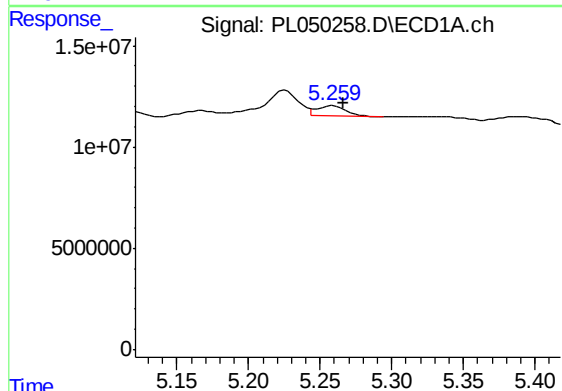


#11 alpha-Chlordane

R.T.: 5.259 min
Delta R.T.: -0.008 min
Response: 6522659
Conc: 0.39 ng/ml m

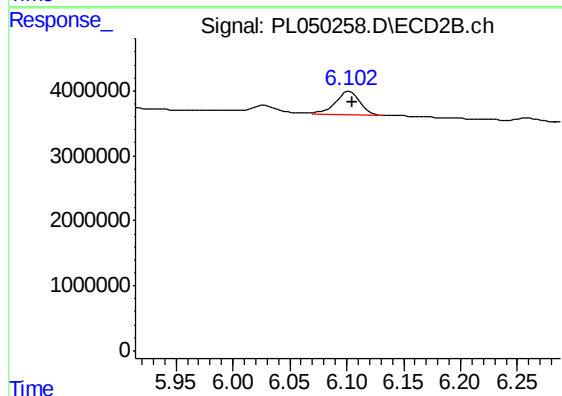

#11 alpha-Chlordane

R.T.: 6.102 min
Delta R.T.: -0.004 min
Response: 5334195
Conc: 1.44 ng/ml m

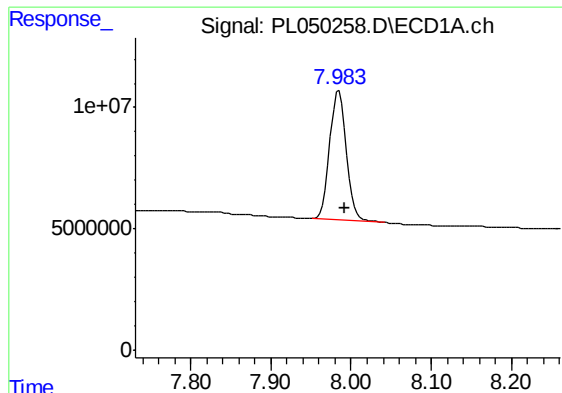


#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.008 min
Response: 76133876
Conc: 5.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-052

Manual Integrations
APPROVED

Ankita
7/10/2019 9:52:12 AM

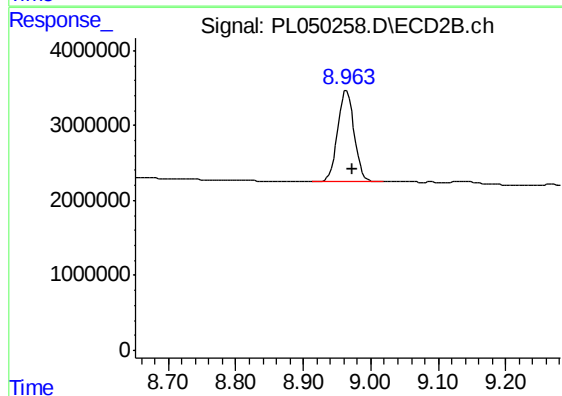

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.009 min
Response: 20831776
Conc: 6.21 ng/ml