

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070925\
 Data File : PL096282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 11:13
 Operator : AR\AJ
 Sample : PB168534BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 06:39:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.826	69319165	110.4E6	18.997	19.122
28)	SA Decachlor...	9.024	7.997	58315923	98849168	20.730	19.823
Target Compounds							
20)	A Methoxychlor	7.492f	0.000	12081999	0	7.669	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070925\
Data File : PL096282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2025 11:13
Operator : AR\AJ
Sample : PB168534BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 06:39:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

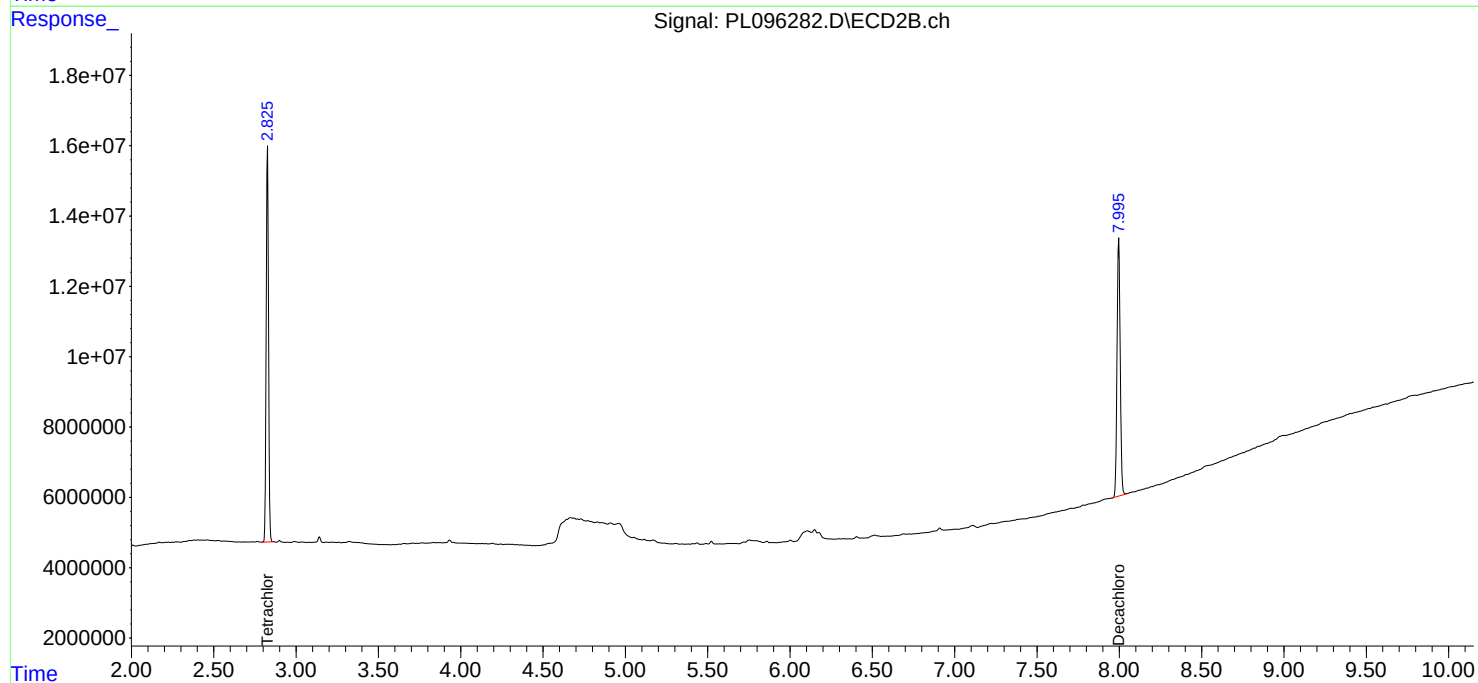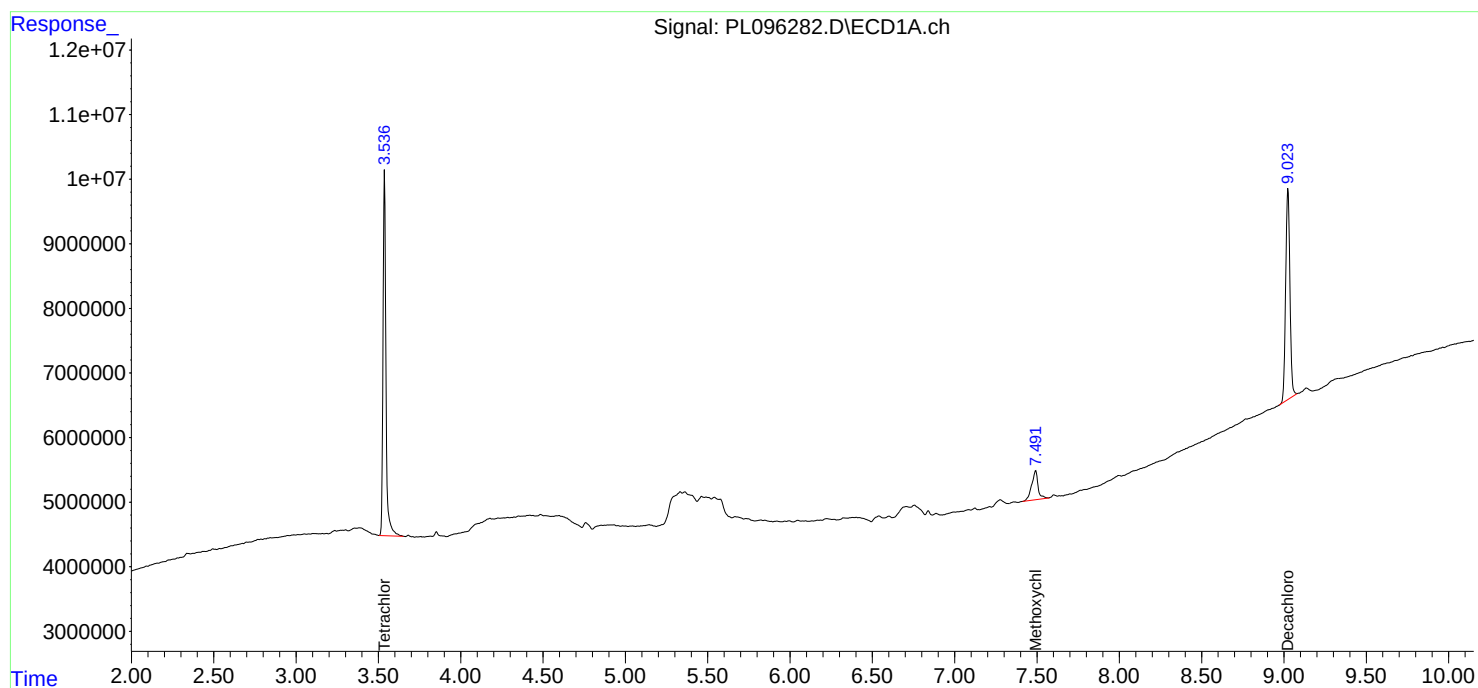


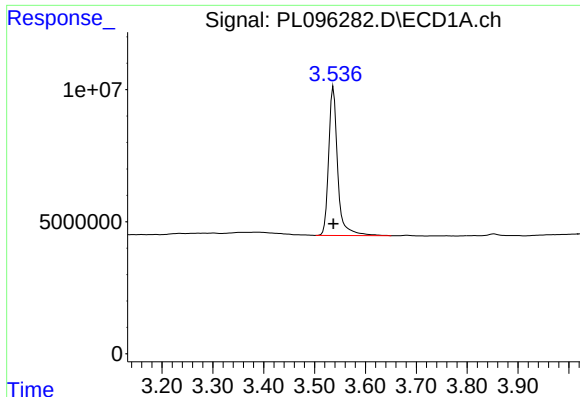

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 69319165
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

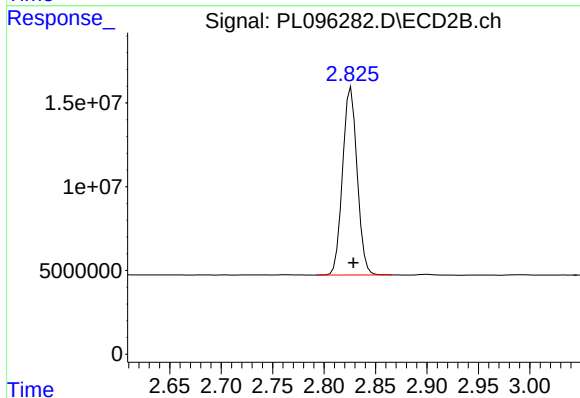


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 110355759
Conc: 19.12 ng/ml

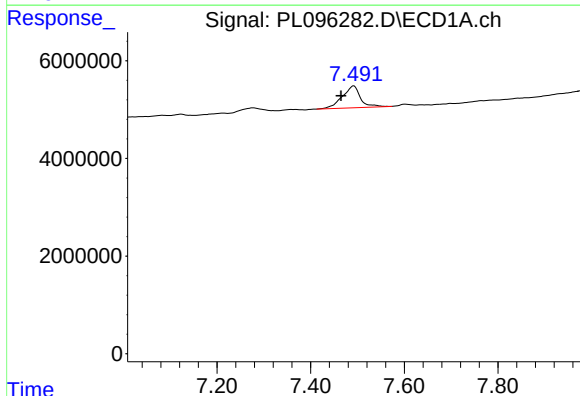


#20 Methoxychlor

R.T.: 7.492 min
Delta R.T.: 0.028 min
Response: 12081999
Conc: 7.67 ng/ml

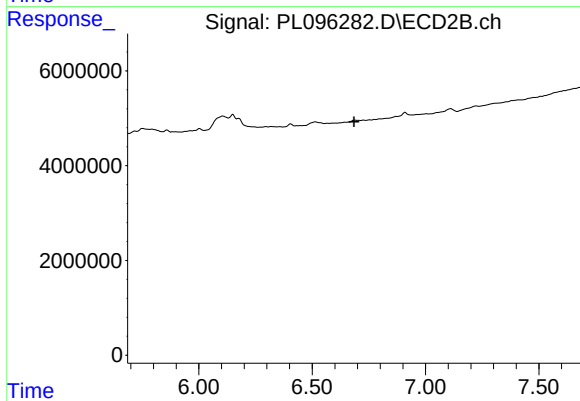

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.685 min
Response: 0
Conc: N.D.

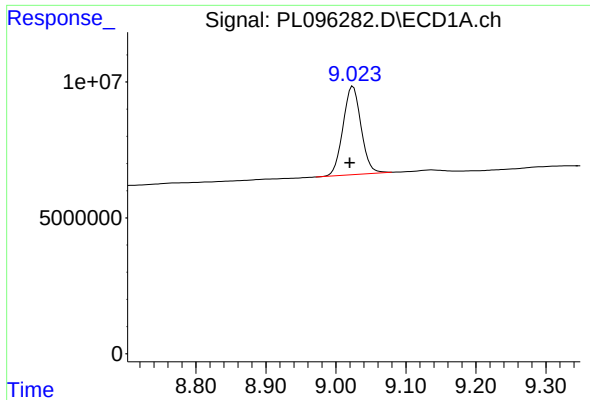

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.004 min
Response: 58315923
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

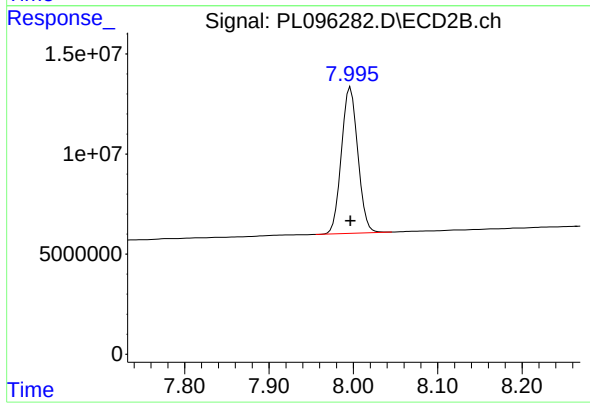

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 98849168
Conc: 19.82 ng/ml