

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070925\
 Data File : PL096286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2025 12:41
 Operator : AR\AJ
 Sample : Q2126-03
 Misc : MDL CHLOR 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 06:39:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.827	60083551	100.4E6	16.466	17.394
28)	SA Decachlor...	9.022	7.995	51663520	89338656	18.366	17.916
Target Compounds							
4)	MA Heptachlor	4.905	4.014	10503890	8308697	2.293	1.092 #
10)	B gamma-Chl...	5.918	5.053	17562198	17896263	3.969	2.549 #
11)	B alpha-Chl...	6.004	5.116	21961514	16231102	5.015	2.158 #
15)	B Endosulfa...	0.000	6.010	0	6628219	N.D.	1.130 #
23)	Chlordane-1	0.000	3.838	0	5724288	N.D.	24.218 #
24)	Chlordane-2	0.000	4.419	0	6954674	N.D.	25.303 #
25)	Chlordane-3	5.918	5.053	17562198	17896263	23.837	22.244
26)	Chlordane-4	6.004	5.116	21961514	16231102	24.477	21.600
27)	Chlordane-5	6.840	6.010	4507404	6628219	29.863	23.384



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070925\
Data File : PL096286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2025 12:41
Operator : AR\AJ
Sample : Q2126-03
Misc : MDL CHLOR 25PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 06:39:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

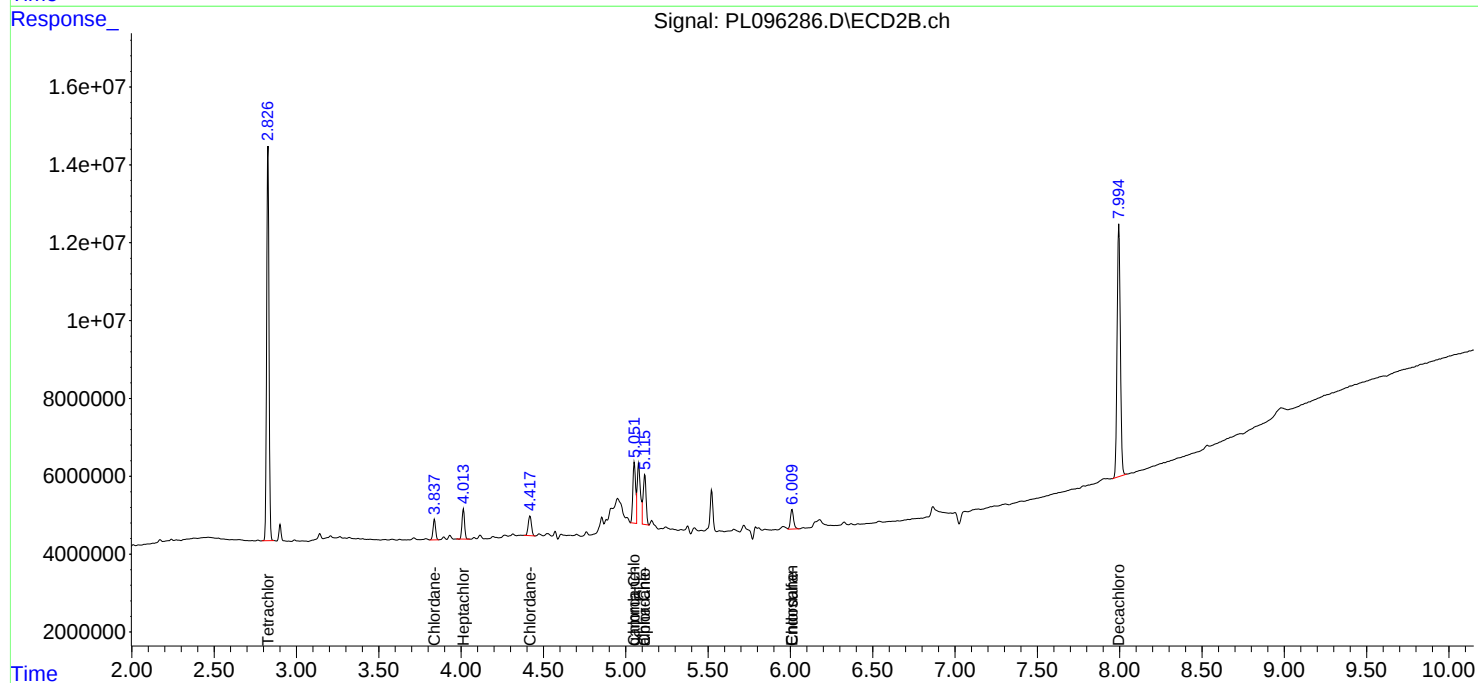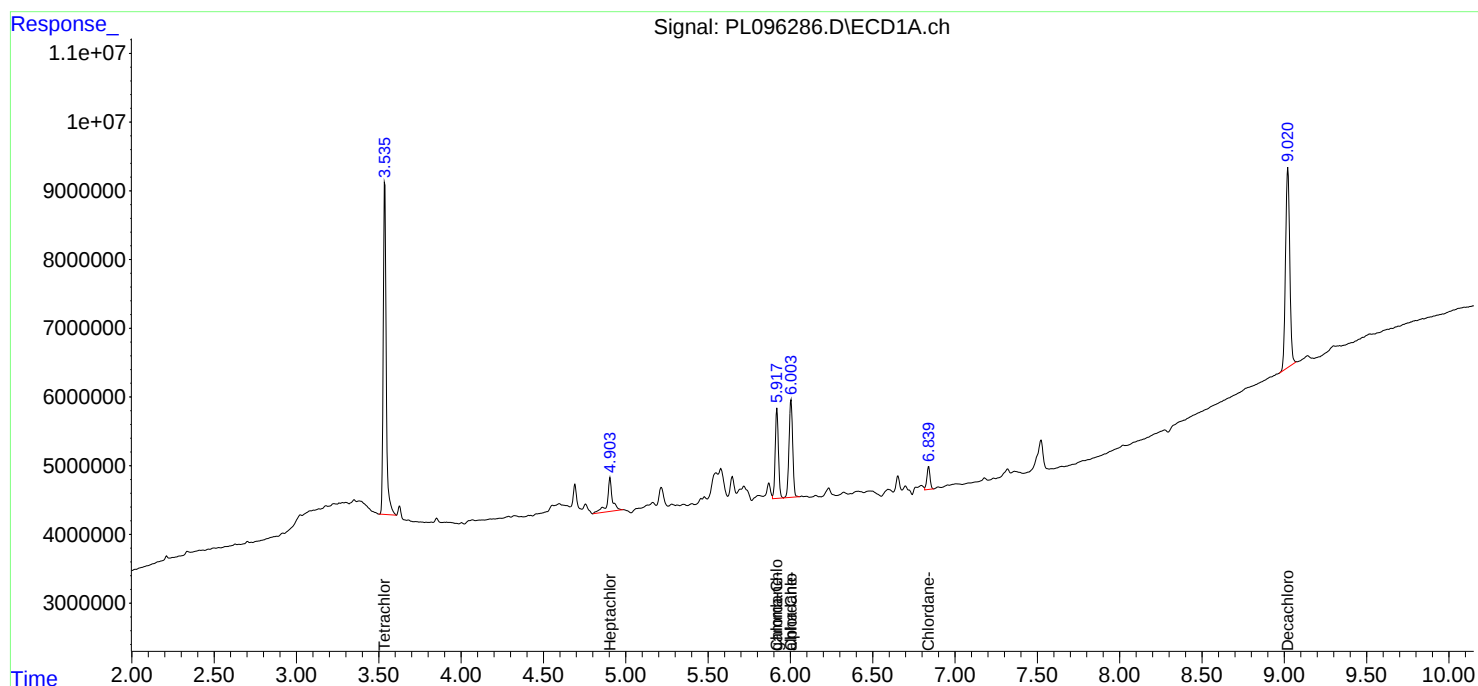


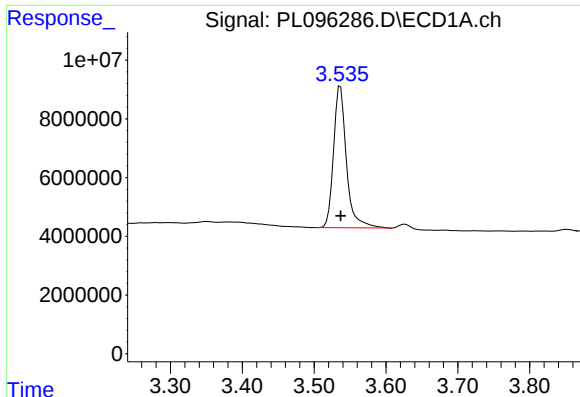

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 60083551
Conc: 16.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

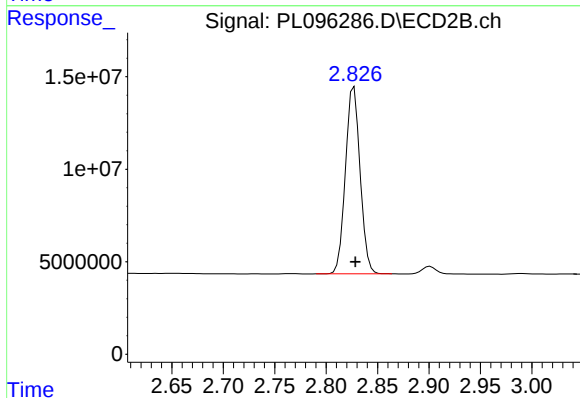


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: -0.001 min
Response: 100385747
Conc: 17.39 ng/ml

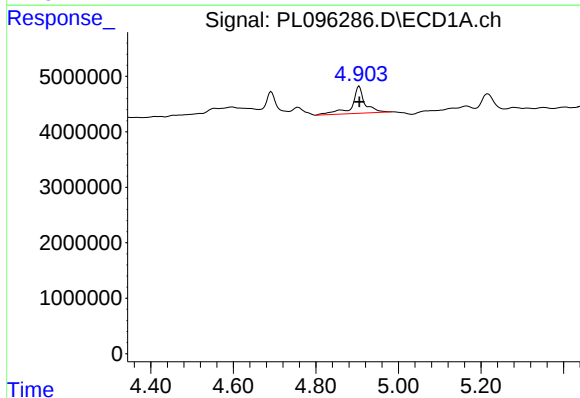


#4 Heptachlor

R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 10503890
Conc: 2.29 ng/ml

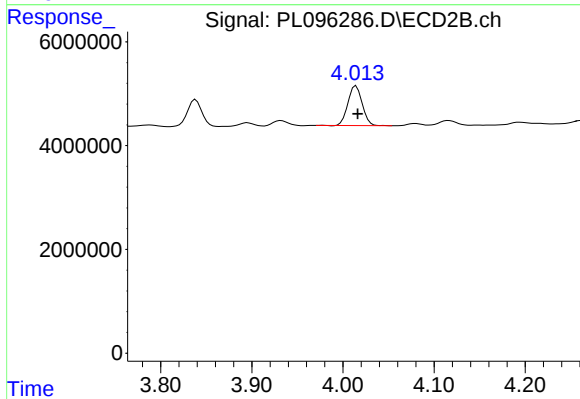

#4 Heptachlor


R.T.: 4.014 min
Delta R.T.: -0.002 min
Response: 8308697
Conc: 1.09 ng/ml

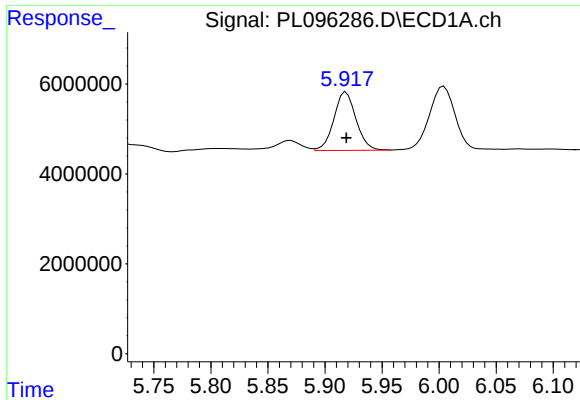

#10 gamma-Chlordane


R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 17562198
Conc: 3.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

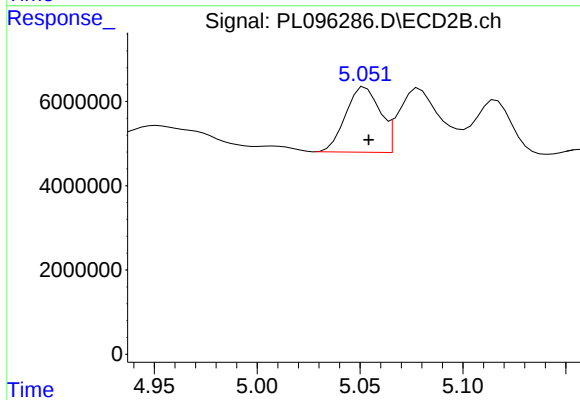


#10 gamma-Chlordane

R.T.: 5.053 min
Delta R.T.: -0.002 min
Response: 17896263
Conc: 2.55 ng/ml

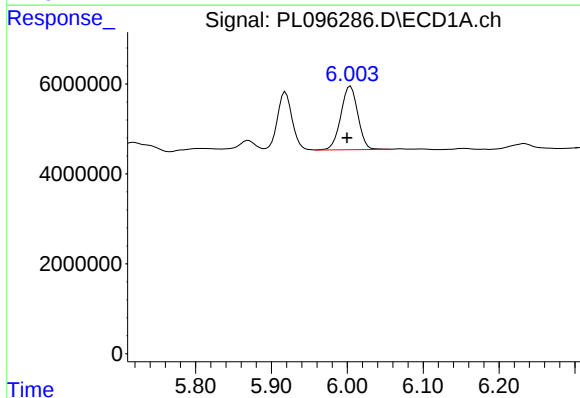


#11 alpha-Chlordane

R.T.: 6.004 min
Delta R.T.: 0.005 min
Response: 21961514
Conc: 5.02 ng/ml

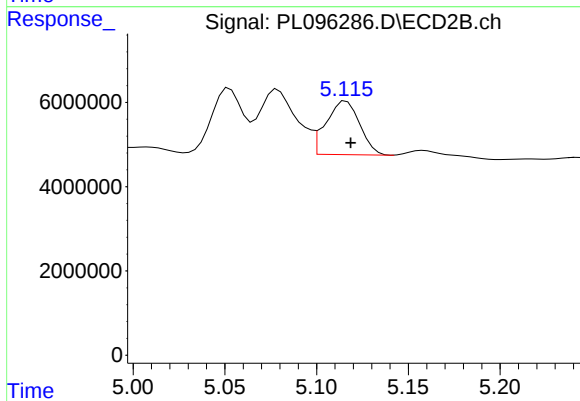

#11 alpha-Chlordane


R.T.: 5.116 min
Delta R.T.: -0.002 min
Response: 16231102
Conc: 2.16 ng/ml

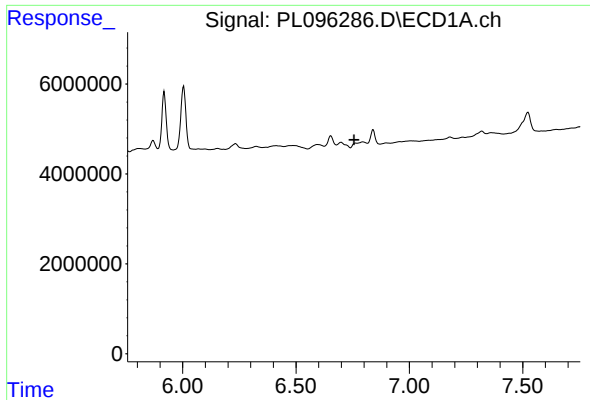

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

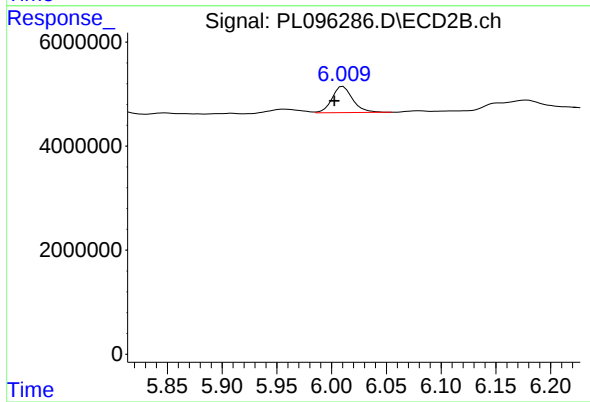


#15 Endosulfan II

R.T.: 6.010 min
Delta R.T.: 0.008 min
Response: 6628219
Conc: 1.13 ng/ml

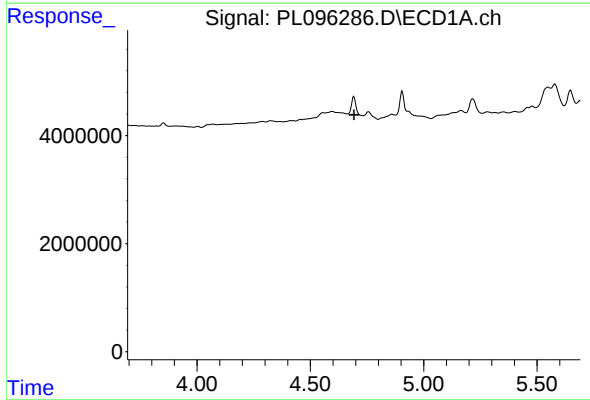


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.693 min
Response: 0
Conc: N.D.

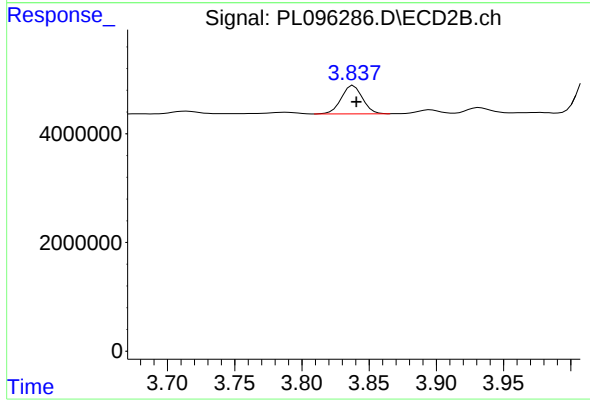

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: -0.002 min
Response: 5724288
Conc: 24.22 ng/ml

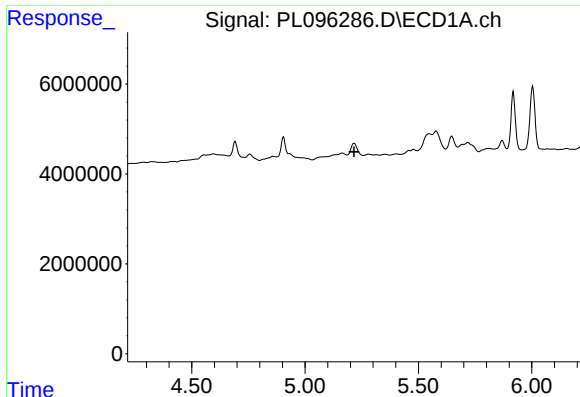

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

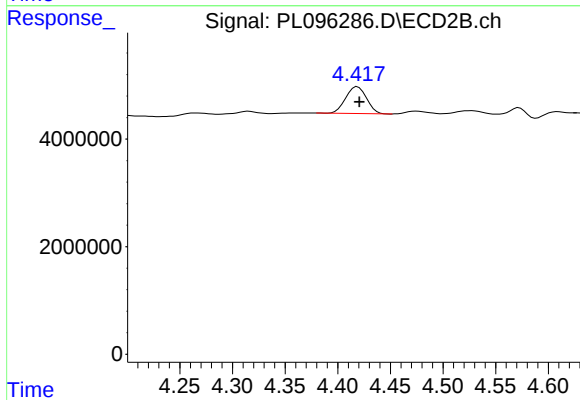


#24 Chlordane-2

R.T.: 4.419 min
Delta R.T.: -0.002 min
Response: 6954674
Conc: 25.30 ng/ml

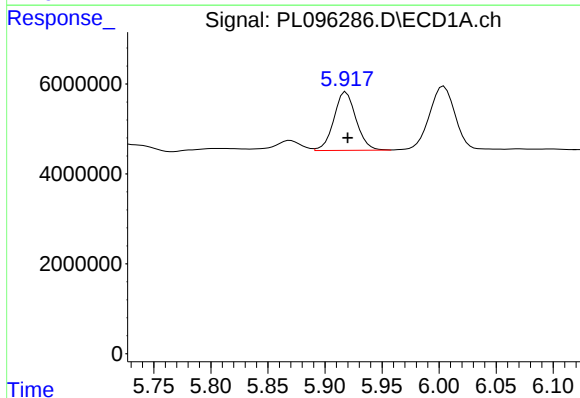


#25 Chlordane-3

R.T.: 5.918 min
Delta R.T.: -0.001 min
Response: 17562198
Conc: 23.84 ng/ml

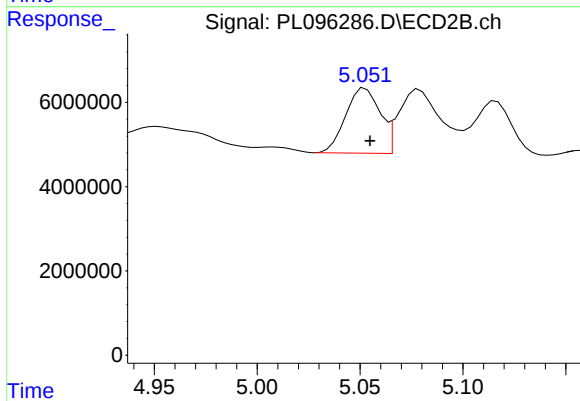

#25 Chlordane-3


R.T.: 5.053 min
Delta R.T.: -0.002 min
Response: 17896263
Conc: 22.24 ng/ml

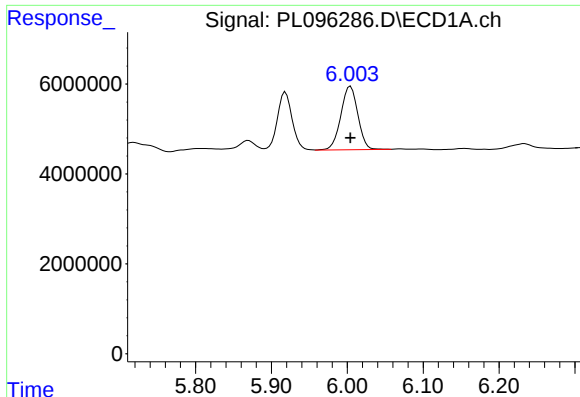

#26 Chlordane-4


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 21961514
Conc: 24.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

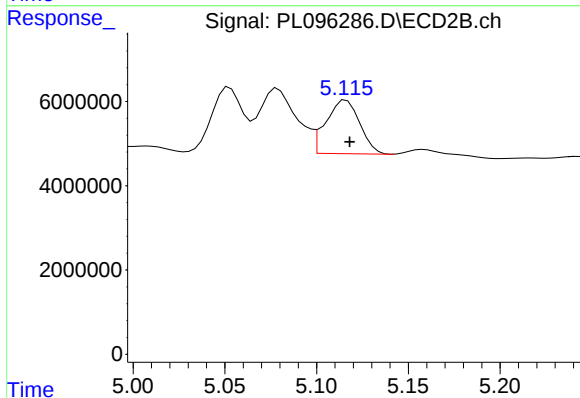


#26 Chlordane-4

R.T.: 5.116 min
Delta R.T.: -0.002 min
Response: 16231102
Conc: 21.60 ng/ml

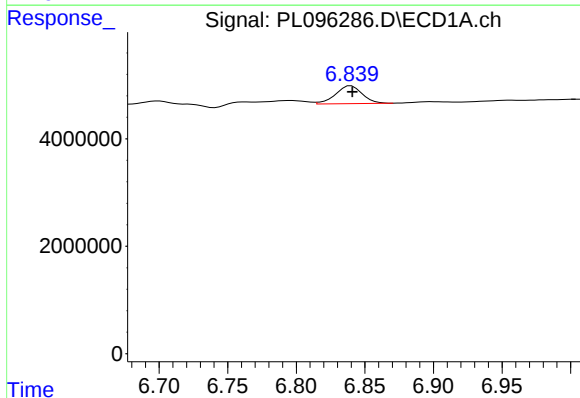


#27 Chlordane-5

R.T.: 6.840 min
Delta R.T.: 0.000 min
Response: 4507404
Conc: 29.86 ng/ml

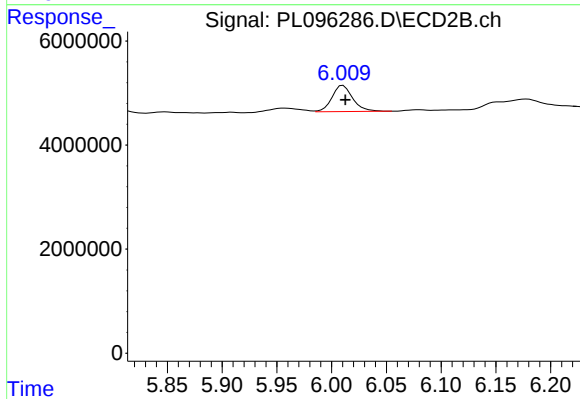

#27 Chlordane-5


R.T.: 6.010 min
Delta R.T.: -0.002 min
Response: 6628219
Conc: 23.38 ng/ml

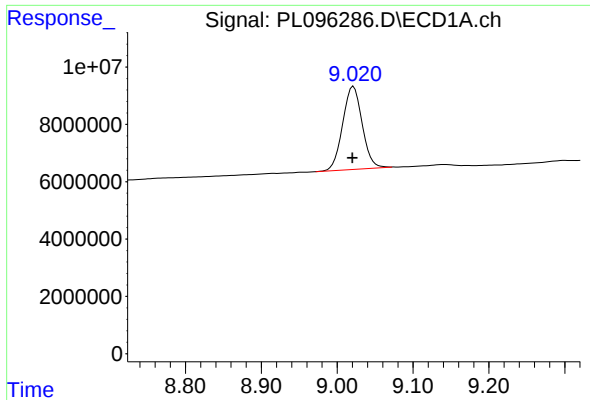

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.002 min
Response: 51663520
Conc: 18.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

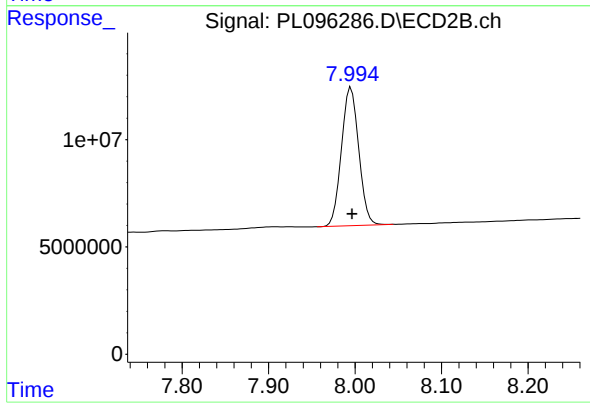

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.001 min
Response: 89338656
Conc: 17.92 ng/ml