

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071118\
 Data File : PL037868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 12:55
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 05:16:36 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	3.935	127.4E6	50223392	16.105	18.153
28)	SA Decachlor...	8.009	8.946	129.0E6	48300624	21.380	24.346
Target Compounds							
6)	B beta-BHC	4.250f	0.000	5293784	0	1.161	N.D. #
23)	Chlordane-1	4.250	0.000	5293784	0	17.241	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071118\
Data File : PL037868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 12:55
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:16:36 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

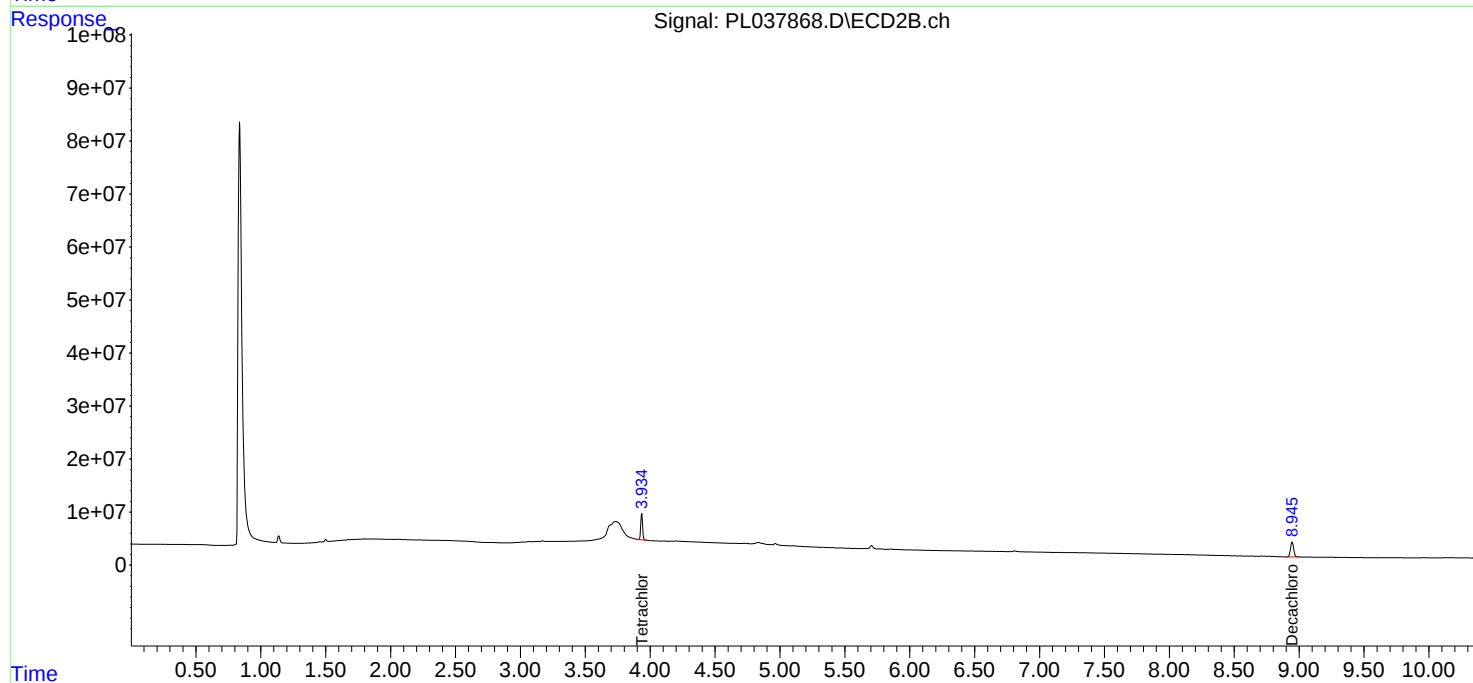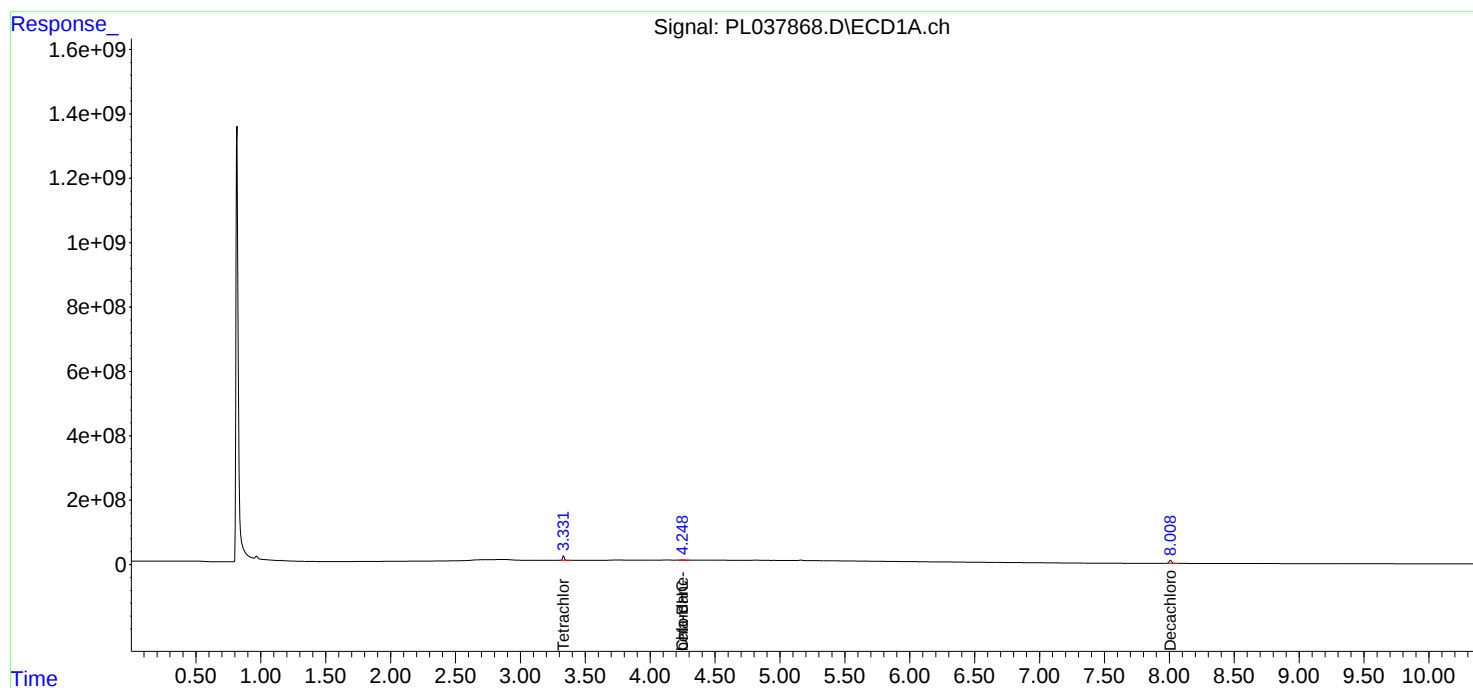


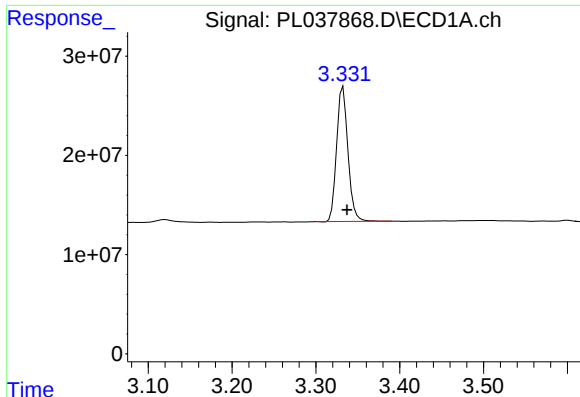

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.005 min
Response: 127399103
Conc: 16.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

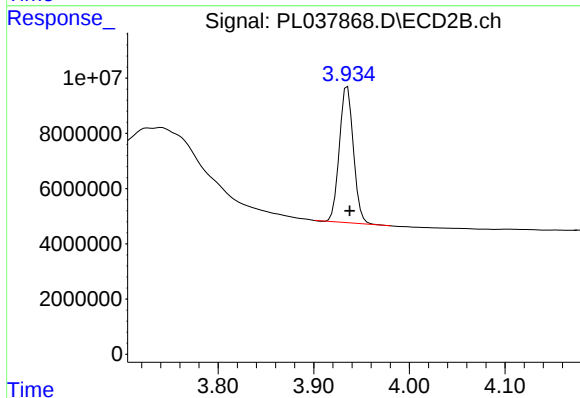


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 50223392
Conc: 18.15 ng/ml

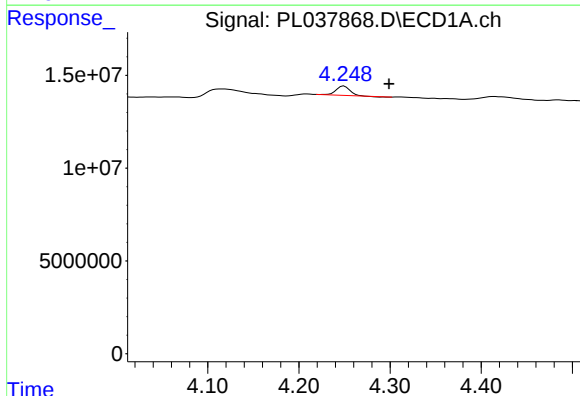


#6 beta-BHC

R.T.: 4.250 min
Delta R.T.: -0.049 min
Response: 5293784
Conc: 1.16 ng/ml

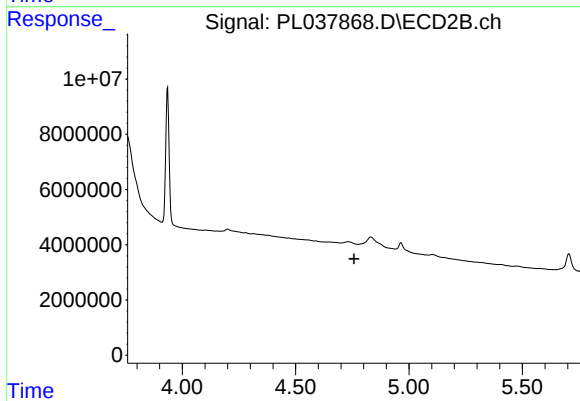

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

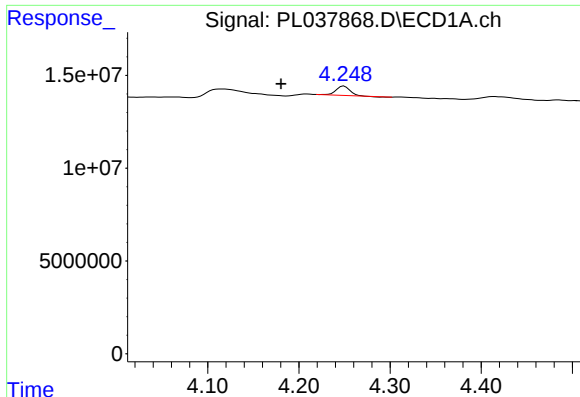

#23 Chlordane-1


R.T.: 4.250 min
Delta R.T.: 0.069 min
Response: 5293784
Conc: 17.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

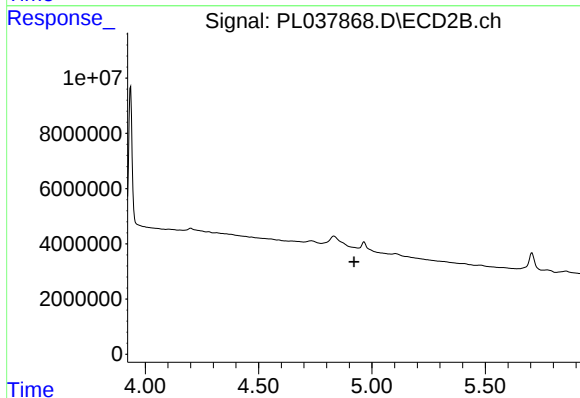


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.921 min
Response: 0
Conc: N.D.

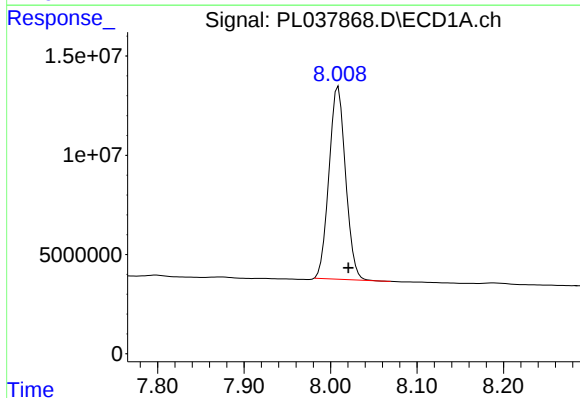

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: -0.012 min
Response: 129010160
Conc: 21.38 ng/ml

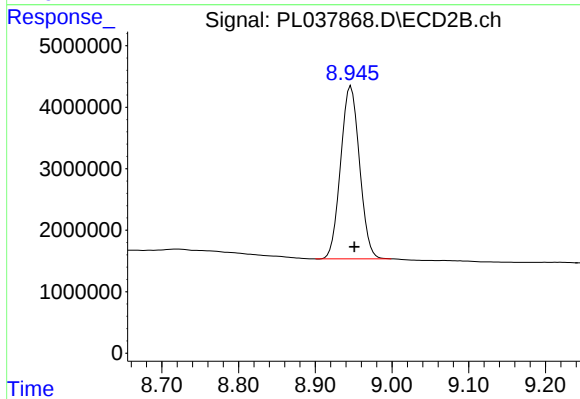

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.004 min
Response: 48300624
Conc: 24.35 ng/ml