

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071118\
 Data File : PL037876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2018 14:48
 Operator : AJ\SJ
 Sample : J3918-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-204-255-ETS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 05:18:04 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	3.935	62378877	25669478	7.886	9.278
28)	SA Decachlor...	8.009	8.947	80651399	31107491	13.366	15.680
Target Compounds							
2)	A alpha-BHC	3.718f	0.000	7493306	0	0.612	N.D. #
8)	B Heptachlo...	5.058f	0.000	9599616	0	1.025	N.D. #
10)	B gamma-Chl...	5.202	0.000	8022537	0	0.857	N.D. #
12)	B 4,4'-DDE	5.449	0.000	7032978	0	0.796	N.D. #
13)	MA Dieldrin	5.571	0.000	10962781	0	1.238	N.D. #
14)	MA Endrin	5.887f	0.000	4936543	0	0.627	N.D. #
17)	MA 4,4'-DDT	6.190	0.000	10325554	0	1.599	N.D. #
23)	Chlordane-1	4.249	0.000	8812989	0	28.702	N.D. #
25)	Chlordane-3	5.202	0.000	8022537	0	7.548	N.D. #
27)	Chlordane-5	5.887	0.000	4936543	0	37.721	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071118\
Data File : PL037876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2018 14:48
Operator : AJ\SJ
Sample : J3918-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:18:04 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

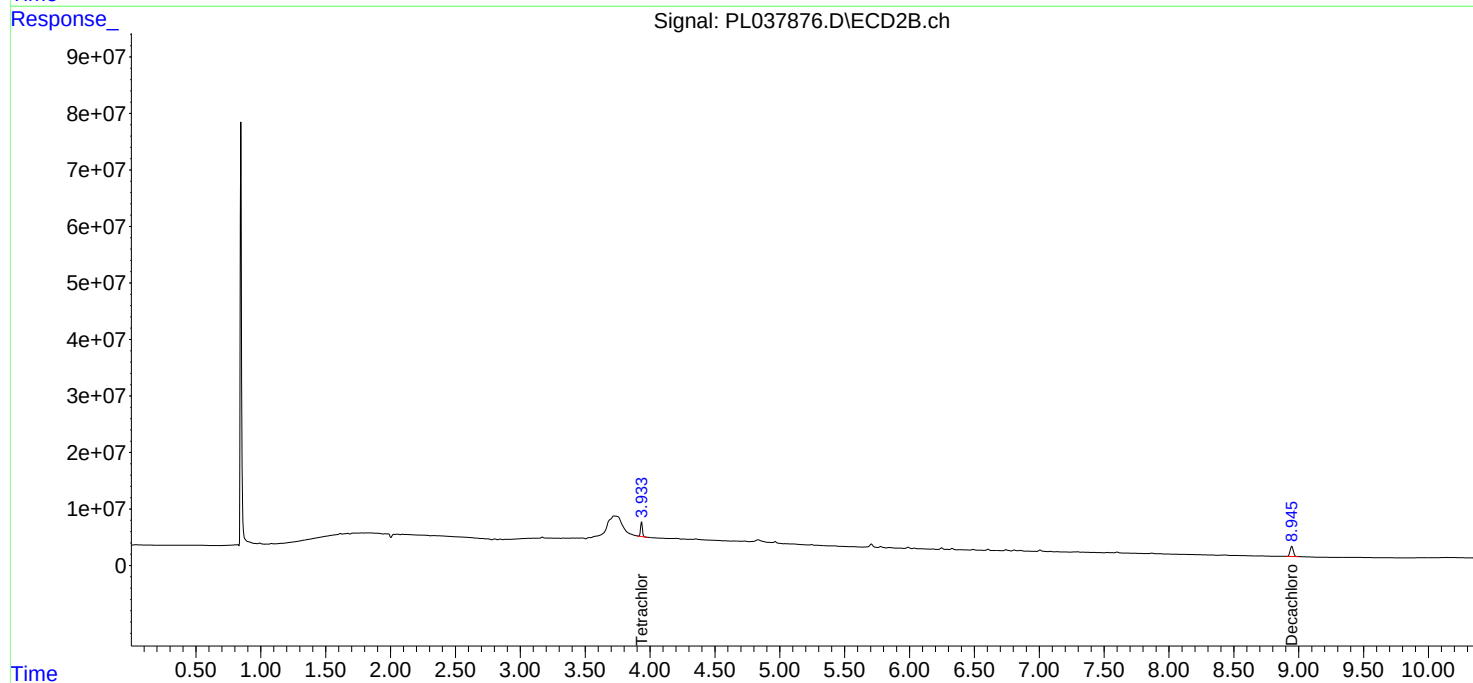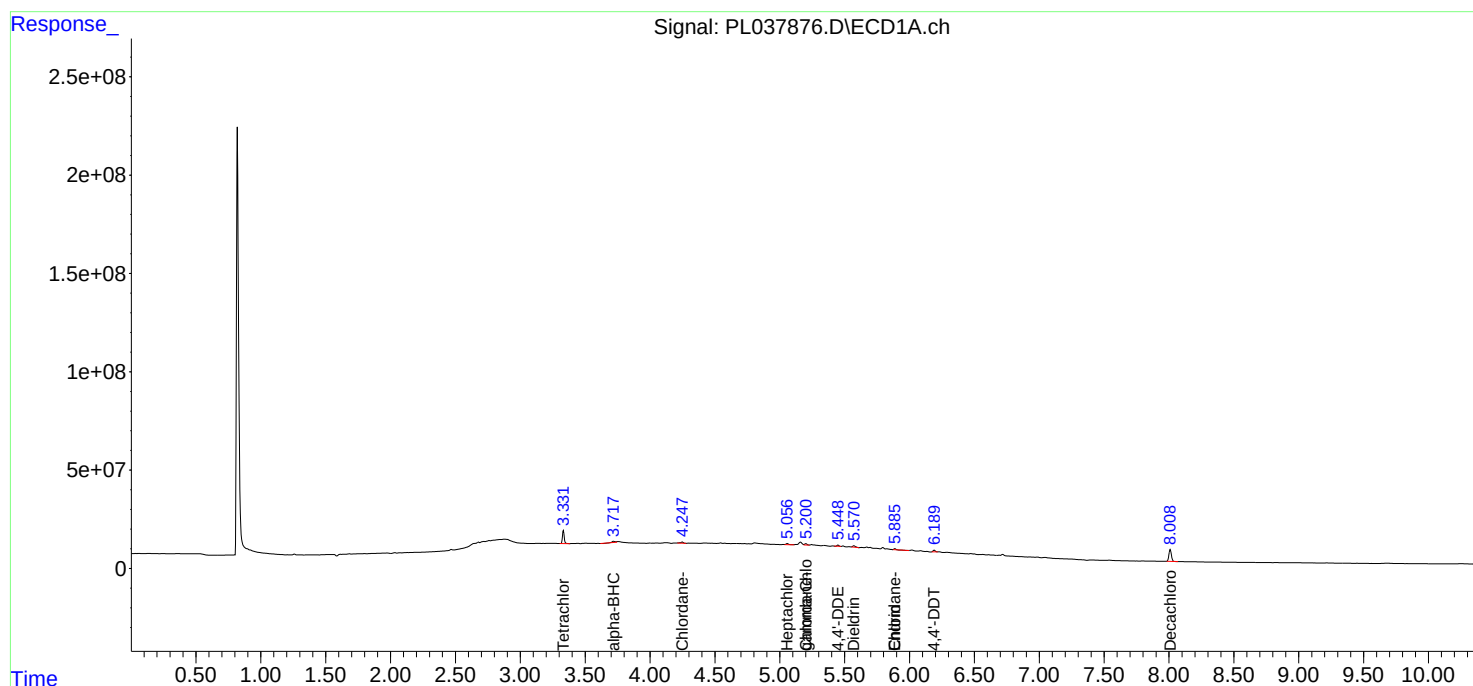


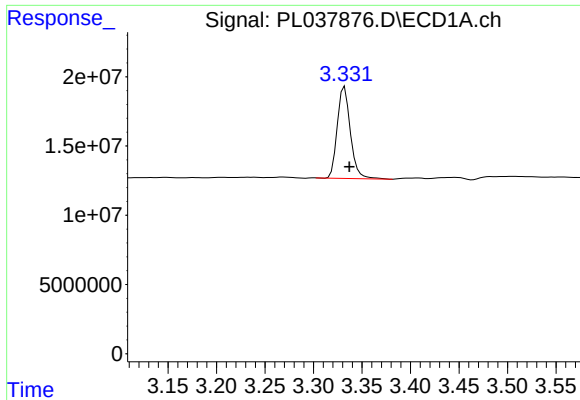

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.005 min
Response: 62378877
Conc: 7.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

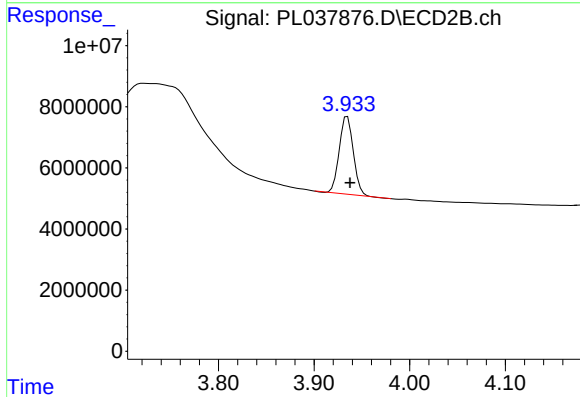


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 25669478
Conc: 9.28 ng/ml

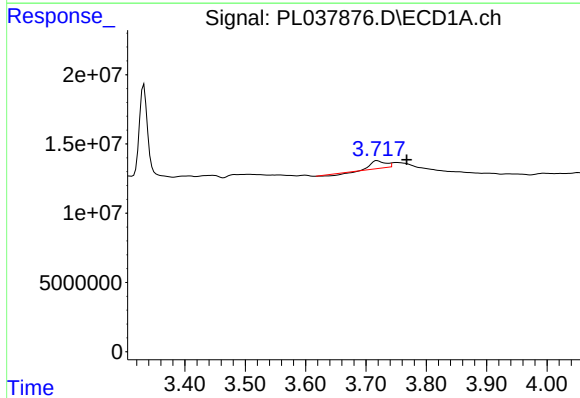


#2 alpha-BHC

R.T.: 3.718 min
Delta R.T.: -0.049 min
Response: 7493306
Conc: 0.61 ng/ml

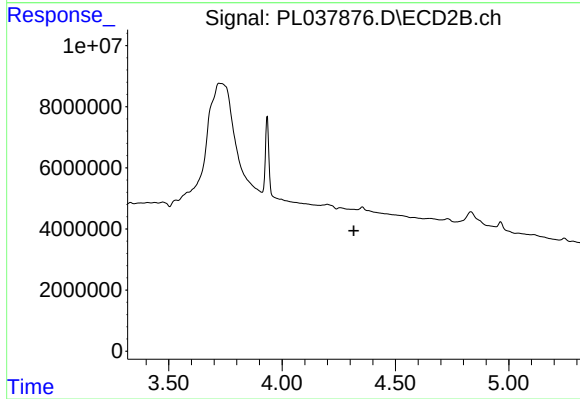

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.317 min
Response: 0
Conc: N.D.

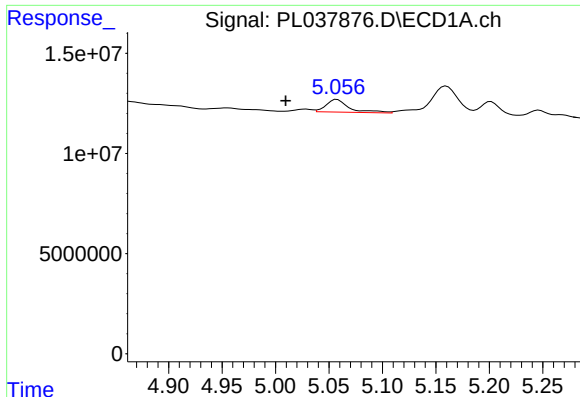

#8 Heptachlor epoxide


R.T.: 5.058 min
Delta R.T.: 0.048 min
Response: 9599616
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

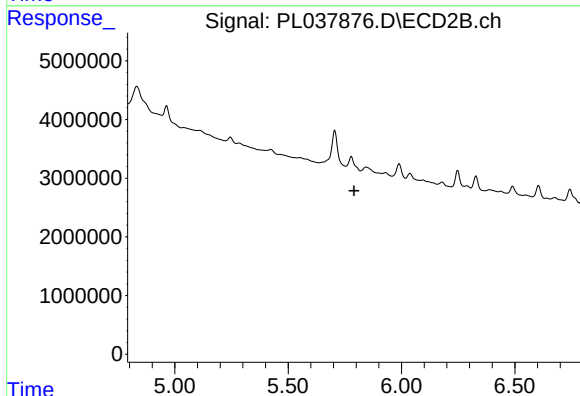


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.790 min
Response: 0
Conc: N.D.

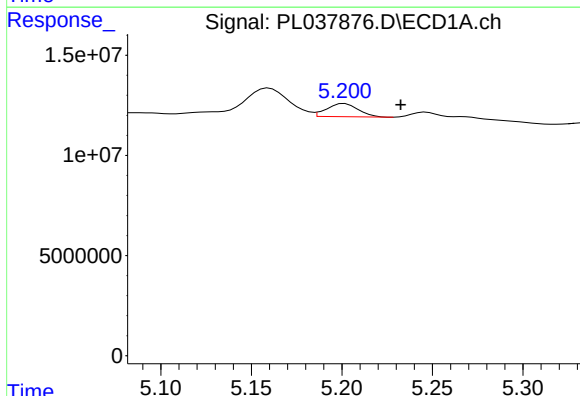


#10 gamma-Chlordane

R.T.: 5.202 min
Delta R.T.: -0.031 min
Response: 8022537
Conc: 0.86 ng/ml

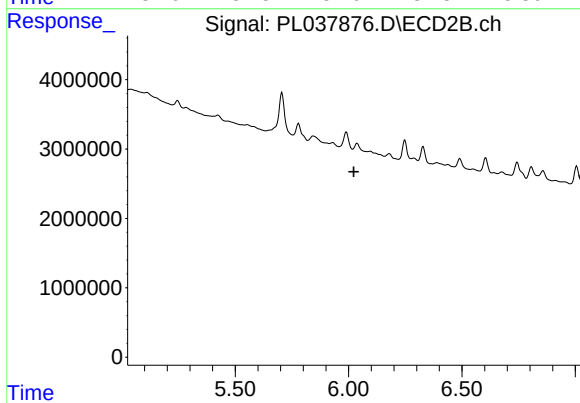

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

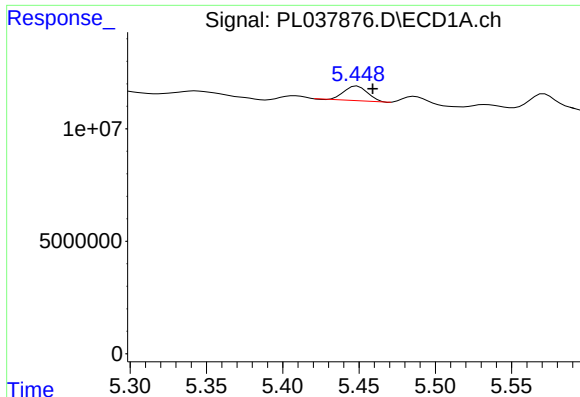

#12 4,4'-DDE


R.T.: 5.449 min
Delta R.T.: -0.010 min
Response: 7032978
Conc: 0.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

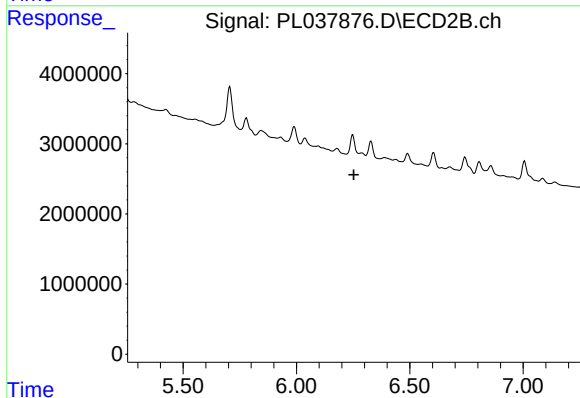


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

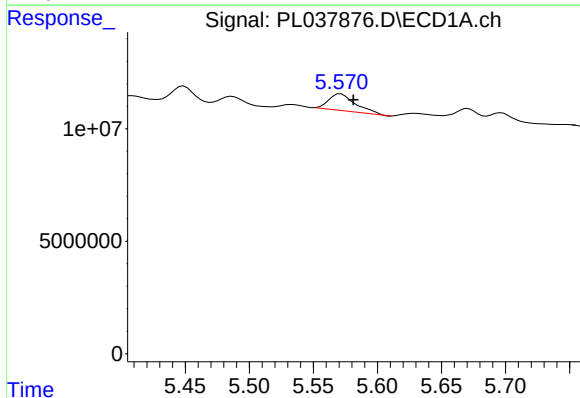


#13 Dieldrin

R.T.: 5.571 min
Delta R.T.: -0.010 min
Response: 10962781
Conc: 1.24 ng/ml

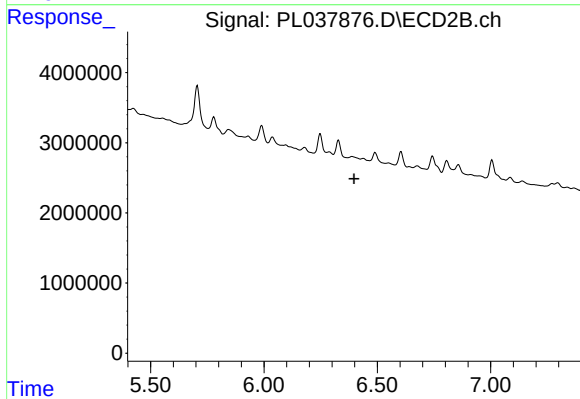

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

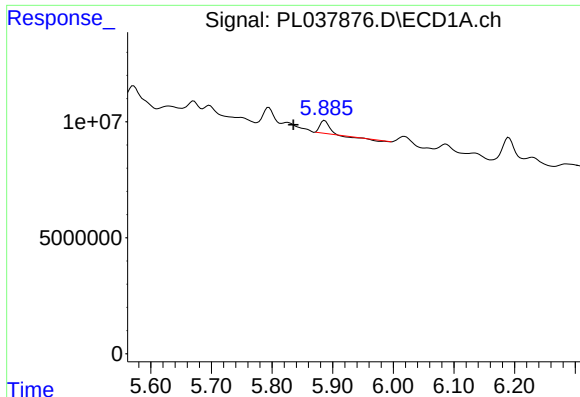

#14 Endrin


R.T.: 5.887 min
Delta R.T.: 0.052 min
Response: 4936543
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

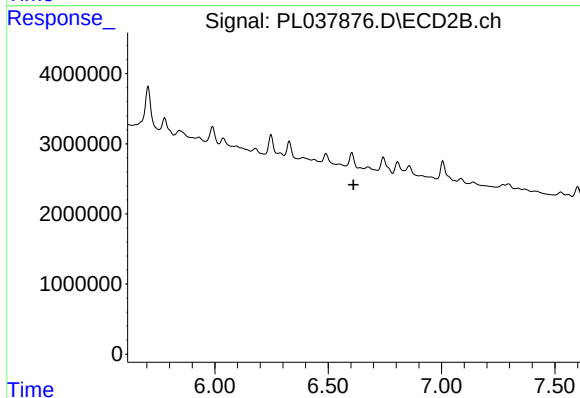


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

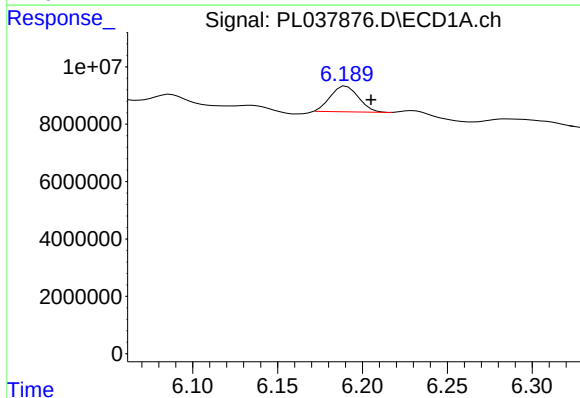


#17 4,4'-DDT

R.T.: 6.190 min
Delta R.T.: -0.015 min
Response: 10325554
Conc: 1.60 ng/ml

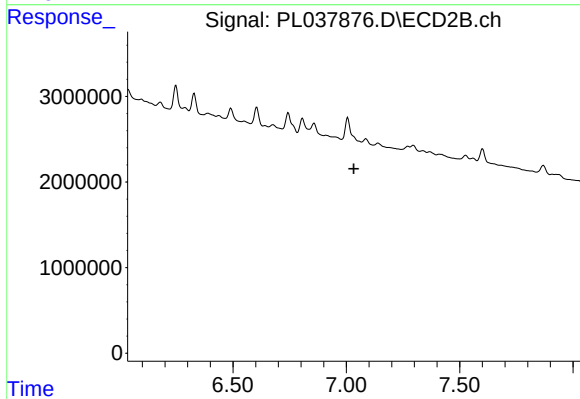

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

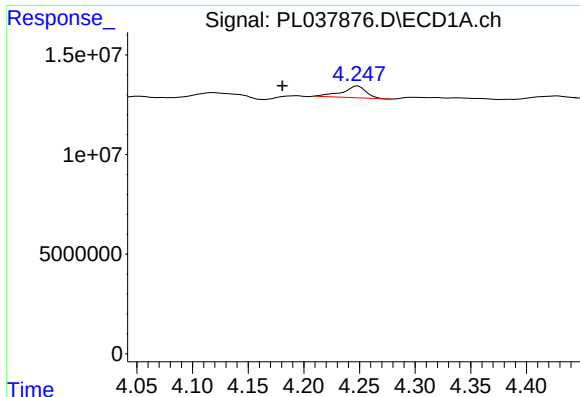

#23 Chlordane-1


R.T.: 4.249 min
Delta R.T.: 0.068 min
Response: 8812989
Conc: 28.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

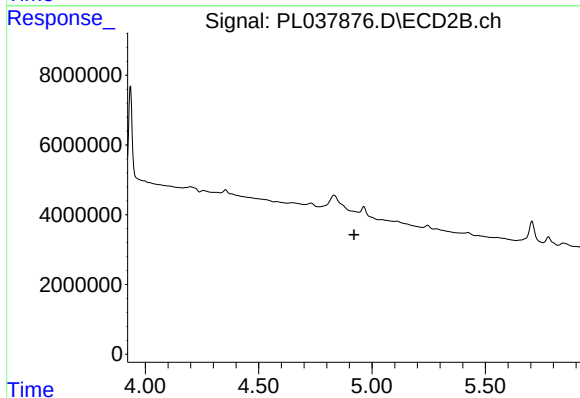


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

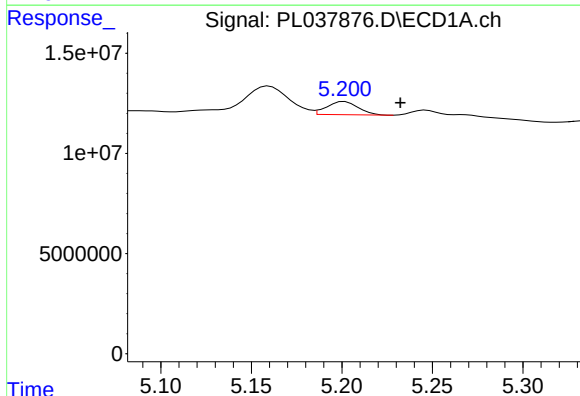


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: -0.031 min
Response: 8022537
Conc: 7.55 ng/ml

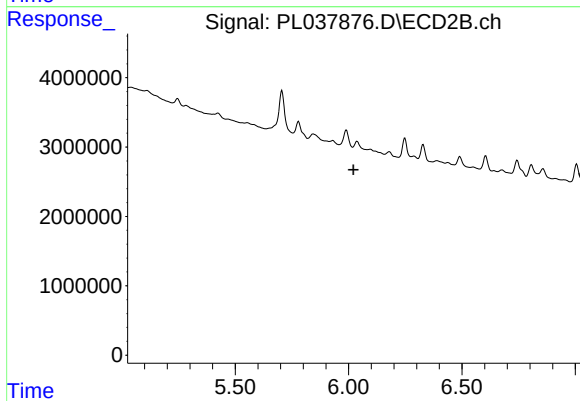

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

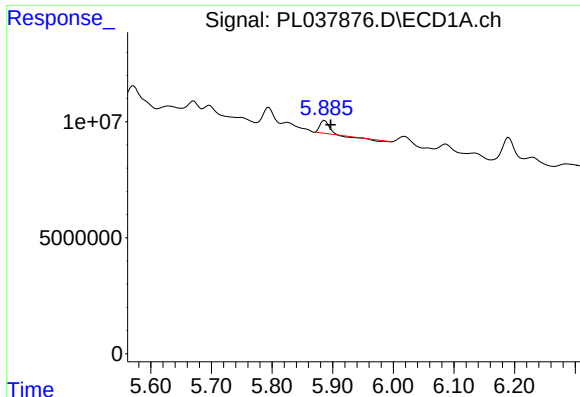

#27 Chlordane-5


R.T.: 5.887 min
Delta R.T.: -0.010 min
Response: 4936543
Conc: 37.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-204-255-ETS

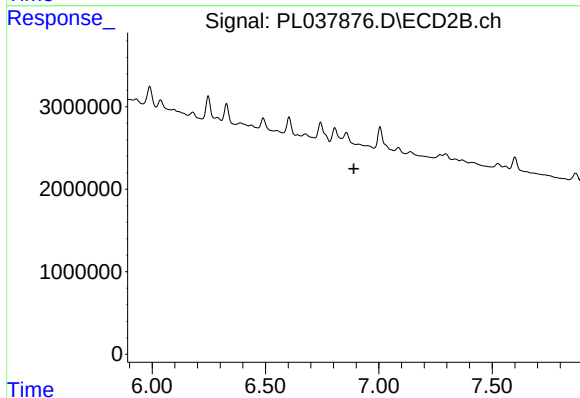


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

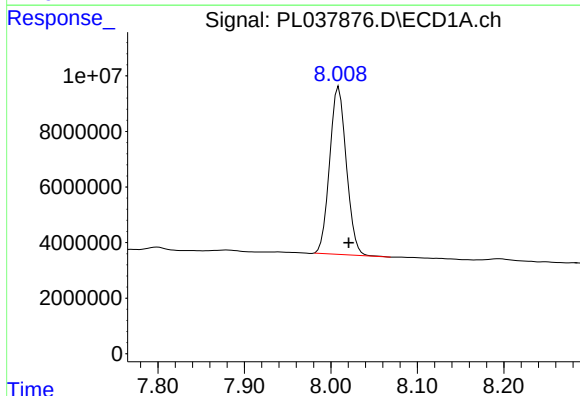

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: -0.011 min
Response: 80651399
Conc: 13.37 ng/ml

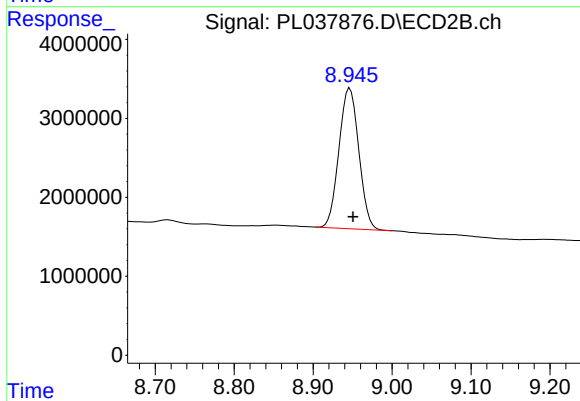

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 31107491
Conc: 15.68 ng/ml