

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071119\
 Data File : PL050298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2019 15:33
 Operator : SM\AJ
 Sample : K3733-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:23:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.932	86455781	25055032	7.666	8.183
28)	SA Decachlor...	7.984	8.964	54489120	21463688	4.288	6.394 #
Target Compounds							
8)	B Heptachlo...	0.000	5.789	0	8786177	N.D.	2.417 #
10)	B gamma-Chl...	5.182f	0.000	31150844	0	1.823	N.D. #
12)	B 4,4'-DDE	5.427	6.260	40878023	20068154	2.454	5.783 #
13)	MA Dieldrin	5.568	6.400	47848337	16782814	2.872	4.731 #
14)	MA Endrin	0.000	6.619	0	6352817	N.D.	2.012 #
16)	A 4,4'-DDD	0.000	6.754	0	31882458	N.D.	12.196 #
17)	MA 4,4'-DDT	6.169	0.000	107.4E6	0	8.092	N.D. #
19)	B Endosulfa...	6.449	0.000	19431639	0	1.499	N.D. #
20)	A Methoxychlor	6.696f	0.000	2006771	0	0.308	N.D. #
25)	Chlordane-3	5.182f	0.000	31150844	0	16.585	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071119\
Data File : PL050298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2019 15:33
Operator : SM\AJ
Sample : K3733-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:23:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

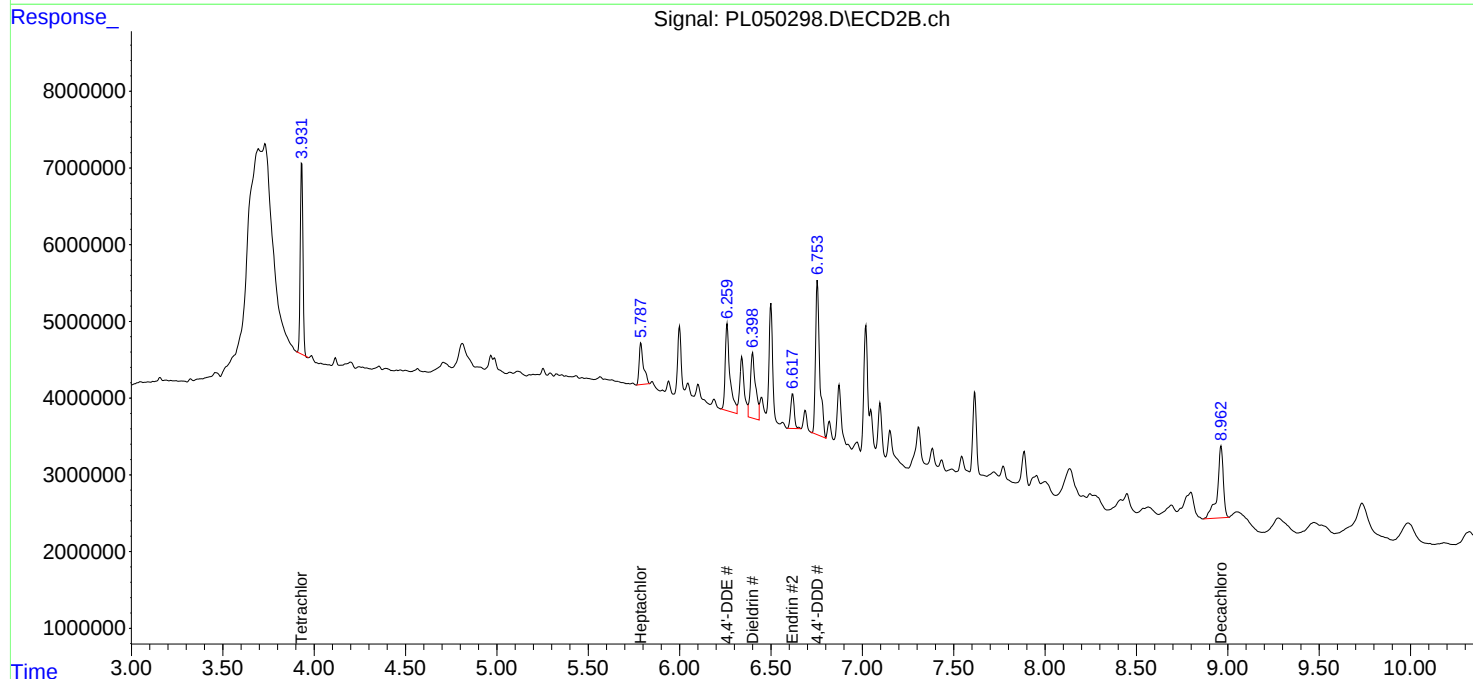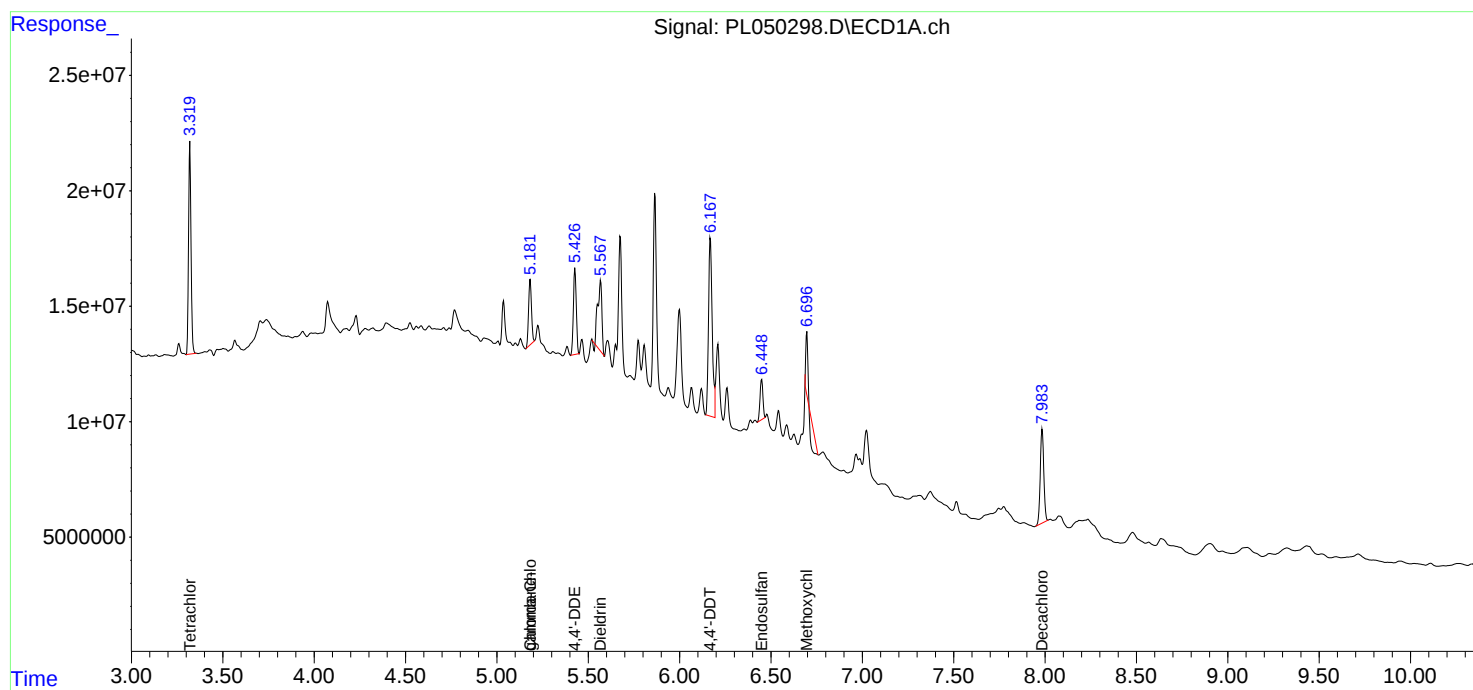


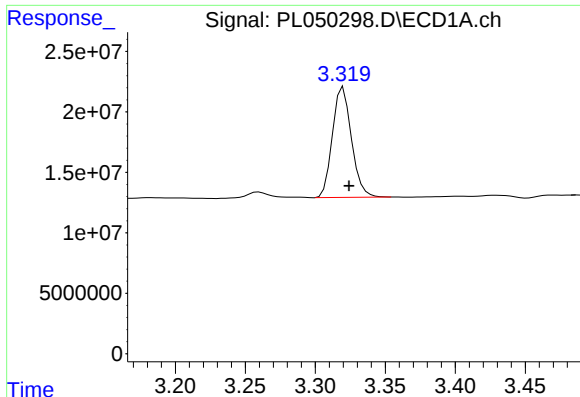

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 86455781
Conc: 7.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

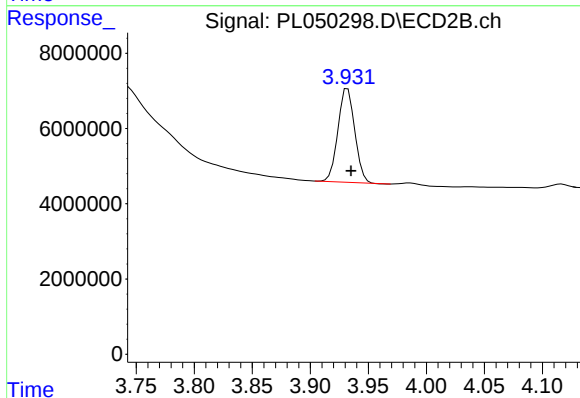


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 25055032
Conc: 8.18 ng/ml

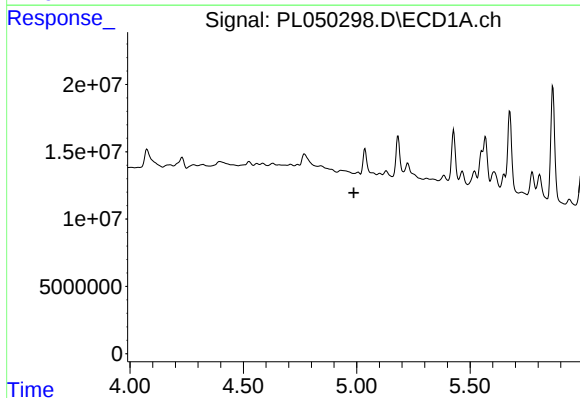


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

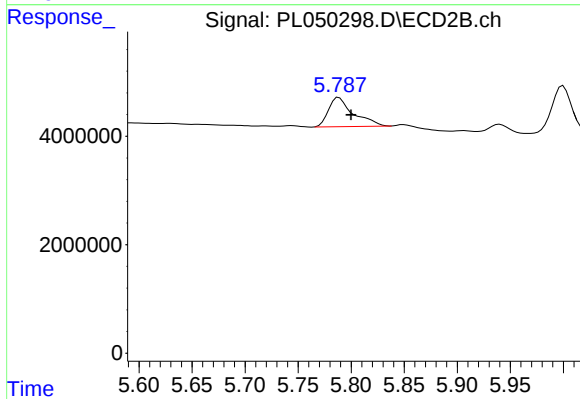

#8 Heptachlor epoxide


R.T.: 5.789 min
Delta R.T.: -0.012 min
Response: 8786177
Conc: 2.42 ng/ml

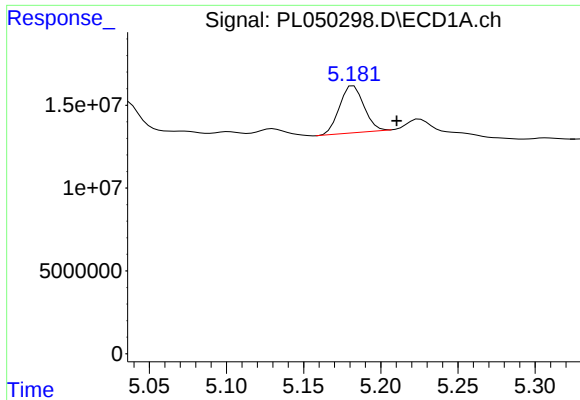

#10 gamma-Chlordane


R.T.: 5.182 min
Delta R.T.: -0.028 min
Response: 31150844
Conc: 1.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

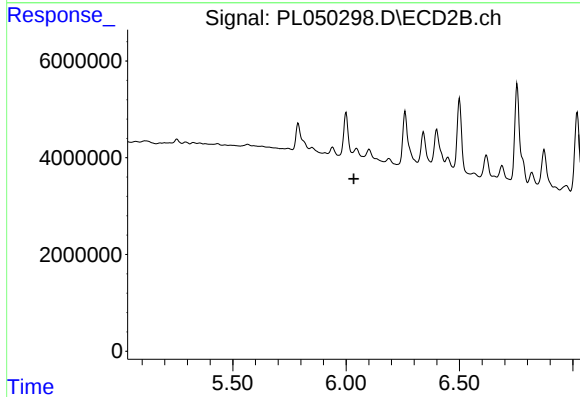


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.034 min
Response: 0
Conc: N.D.

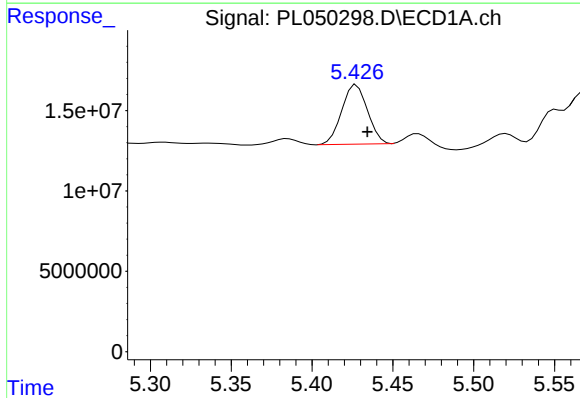


#12 4,4'-DDE

R.T.: 5.427 min
Delta R.T.: -0.007 min
Response: 40878023
Conc: 2.45 ng/ml

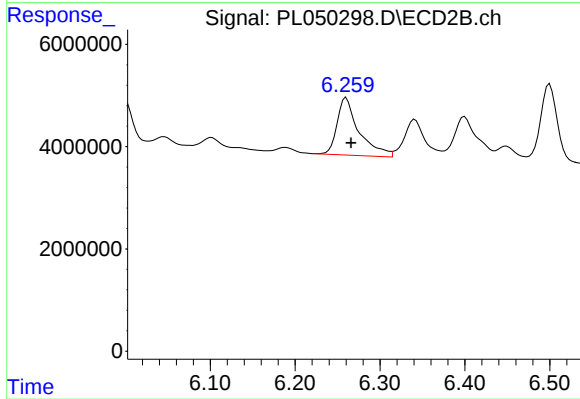

#12 4,4'-DDE


R.T.: 6.260 min
Delta R.T.: -0.006 min
Response: 20068154
Conc: 5.78 ng/ml

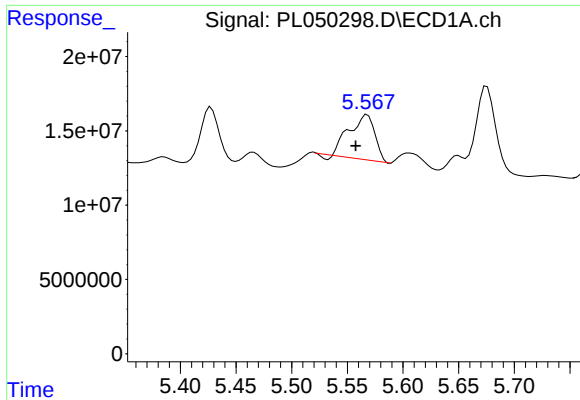

#13 Dieldrin


R.T.: 5.568 min
Delta R.T.: 0.010 min
Response: 47848337
Conc: 2.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

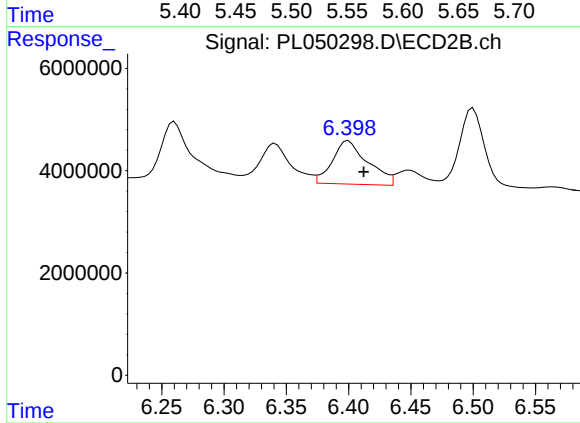


#13 Dieldrin

R.T.: 6.400 min
Delta R.T.: -0.012 min
Response: 16782814
Conc: 4.73 ng/ml

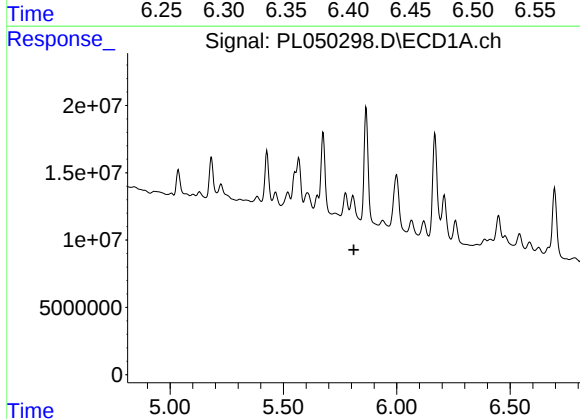


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

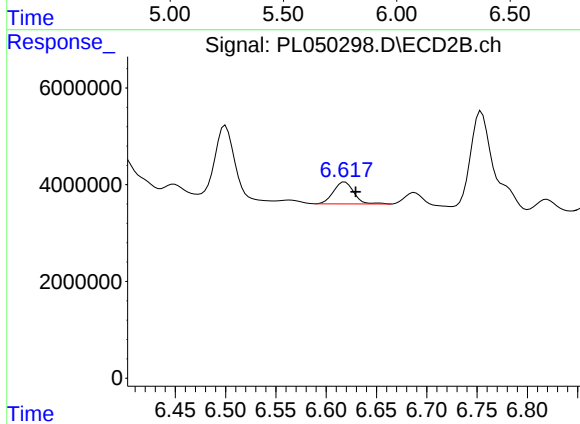

#14 Endrin


R.T.: 6.619 min
Delta R.T.: -0.011 min
Response: 6352817
Conc: 2.01 ng/ml

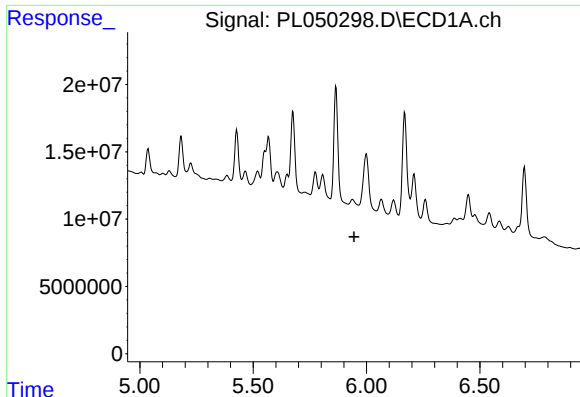

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

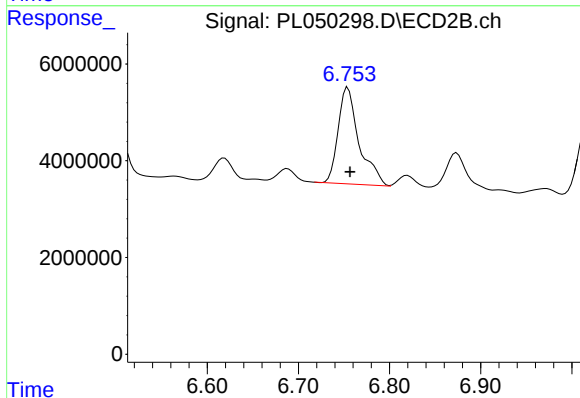


#16 4,4'-DDD

R.T.: 6.754 min
Delta R.T.: -0.003 min
Response: 31882458
Conc: 12.20 ng/ml

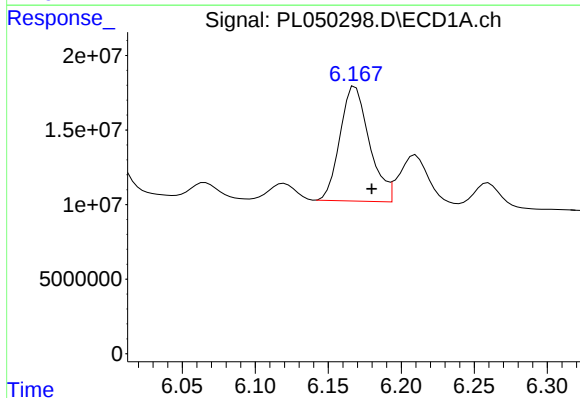


#17 4,4'-DDT

R.T.: 6.169 min
Delta R.T.: -0.011 min
Response: 107423389
Conc: 8.09 ng/ml

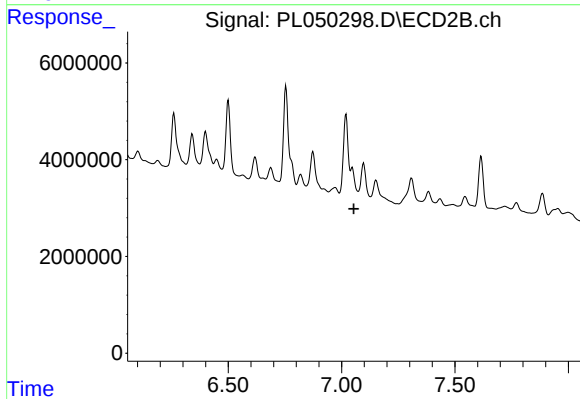

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.054 min
Response: 0
Conc: N.D.

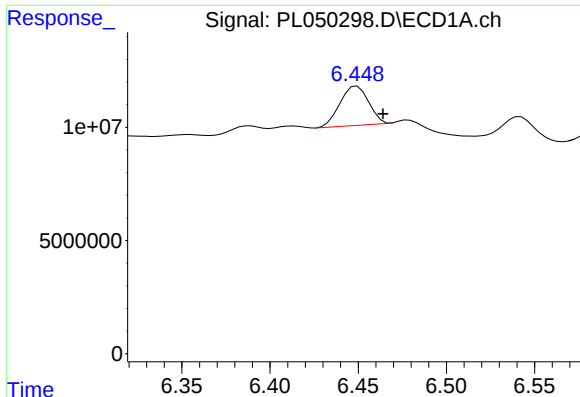

#19 Endosulfan Sulfate


R.T.: 6.449 min
Delta R.T.: -0.015 min
Response: 19431639
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

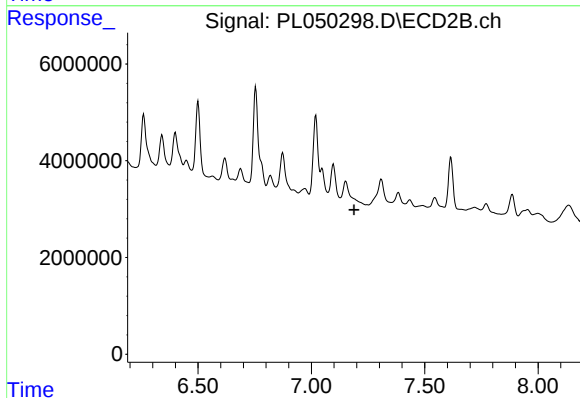


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

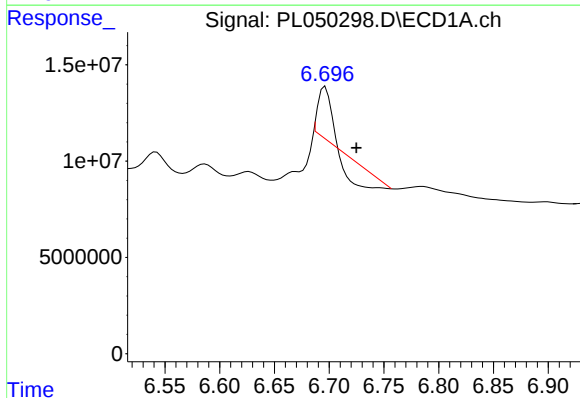


#20 Methoxychlor

R.T.: 6.696 min
Delta R.T.: -0.028 min
Response: 2006771
Conc: 0.31 ng/ml

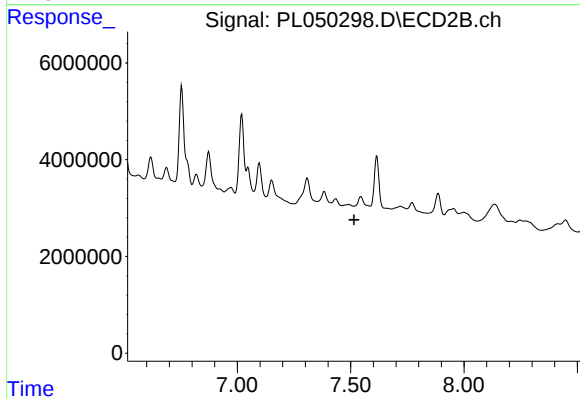

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.515 min
Response: 0
Conc: N.D.

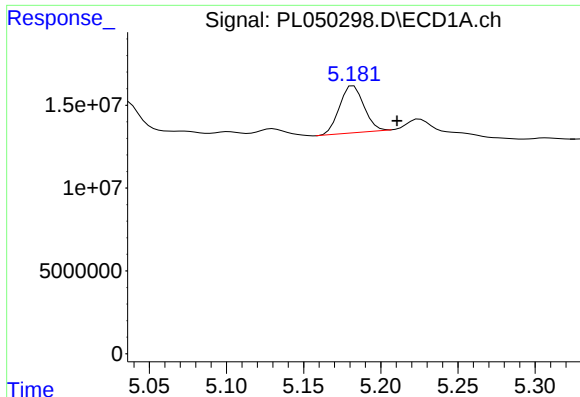

#25 Chlordane-3


R.T.: 5.182 min
Delta R.T.: -0.028 min
Response: 31150844
Conc: 16.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

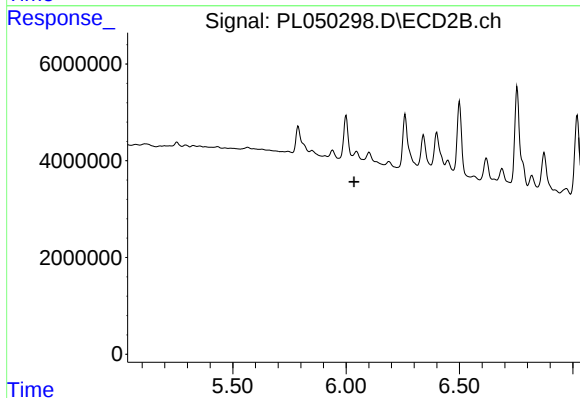


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

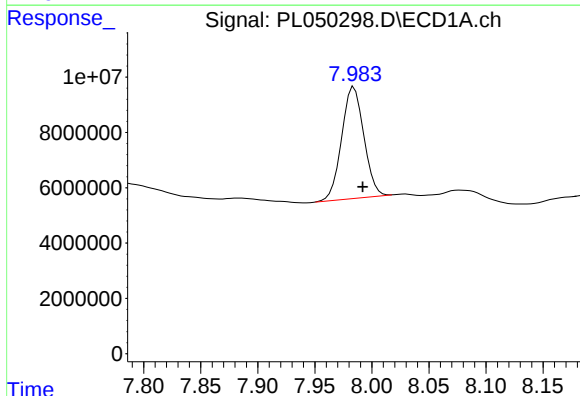

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: -0.008 min
Response: 54489120
Conc: 4.29 ng/ml

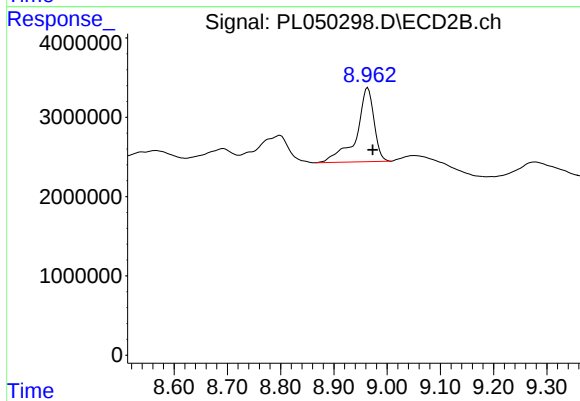

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.009 min
Response: 21463688
Conc: 6.39 ng/ml