

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071119\
 Data File : PL050315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2019 22:24
 Operator : SM\AJ
 Sample : K3621-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 04:28:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.932	133.6E6	39484401	11.850	12.896
28)	SA Decachlor...	7.985	8.966	112.5E6	39557747	8.857	11.784 #
Target Compounds							
4)	MA Heptachlor	4.307	5.106	32821790	11046408	1.806	2.552 #
6)	B beta-BHC	4.307f	0.000	32821790	0	4.487	N.D. #
10)	B gamma-Chl...	5.224	6.029	23992237	5688192	1.404	1.526
11)	B alpha-Chl...	0.000	6.103	0	13418252	N.D.	3.628 #
25)	Chlordane-3	5.224	6.029	23992237	5688192	12.774	11.431
26)	Chlordane-4	0.000	6.103	0	13418252	N.D.	22.577 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071119\
Data File : PL050315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2019 22:24
Operator : SM\AJ
Sample : K3621-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:28:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

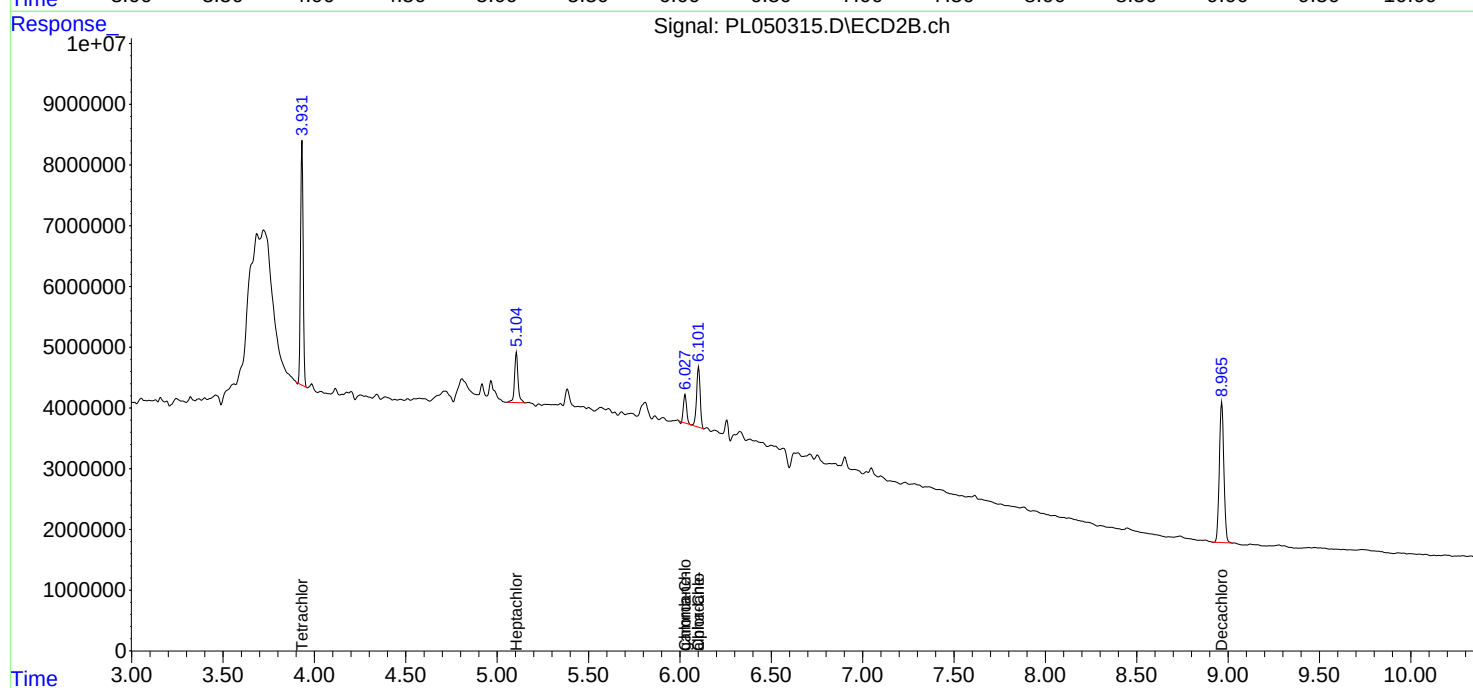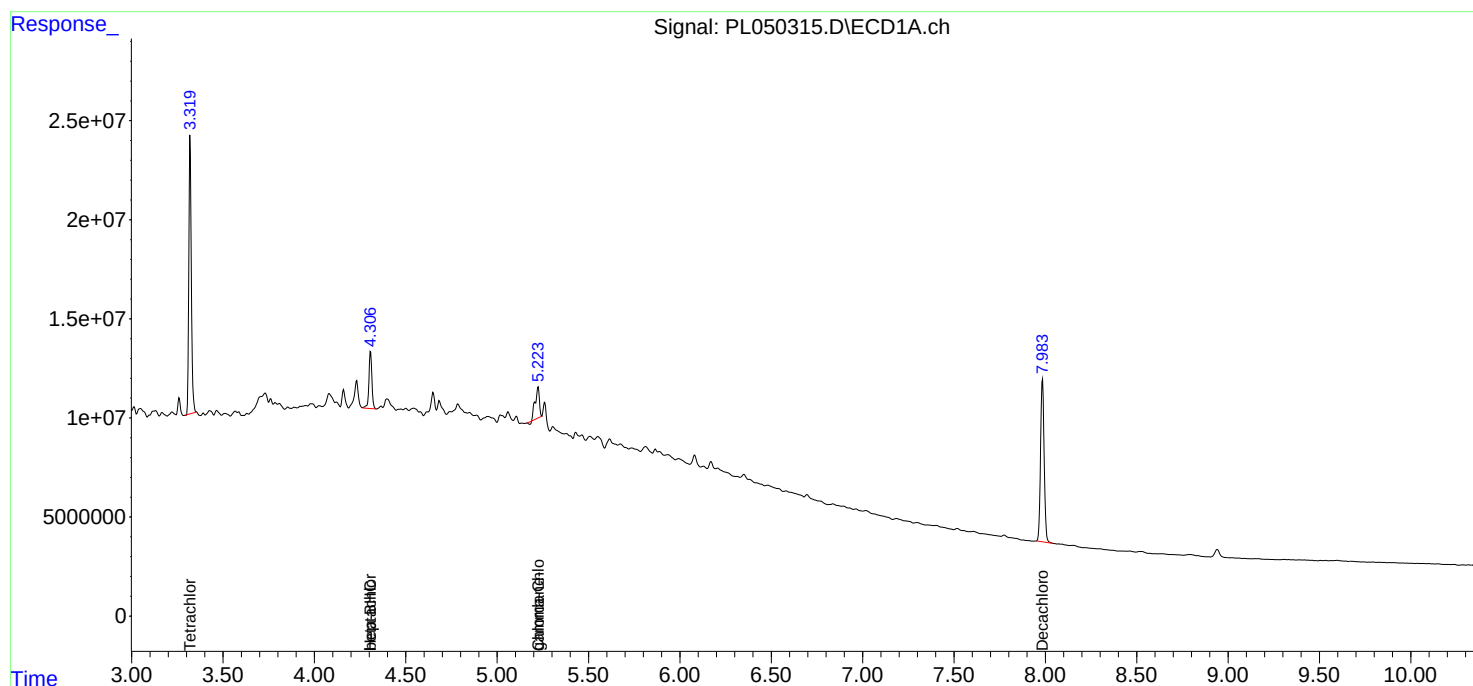


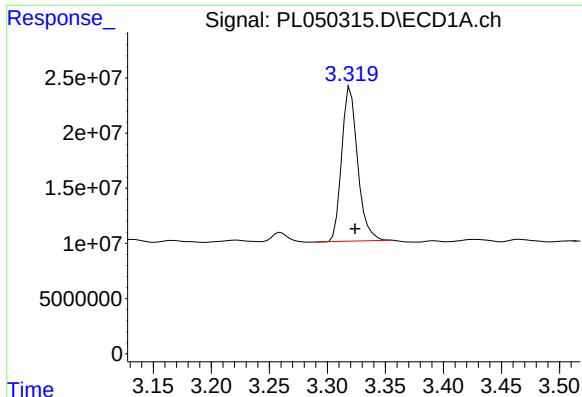

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 133637799
Conc: 11.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

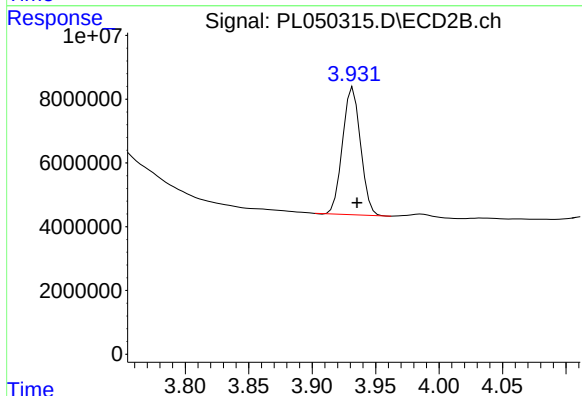


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 39484401
Conc: 12.90 ng/ml

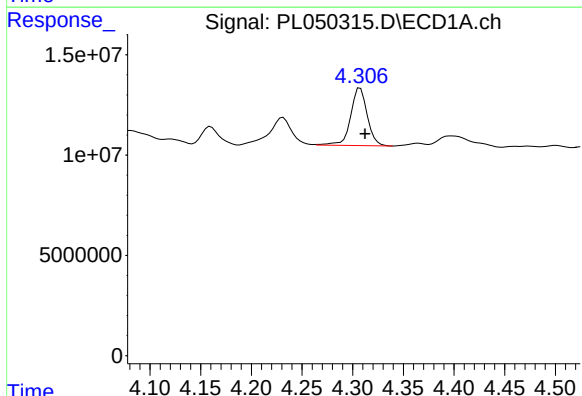


#4 Heptachlor

R.T.: 4.307 min
Delta R.T.: -0.005 min
Response: 32821790
Conc: 1.81 ng/ml

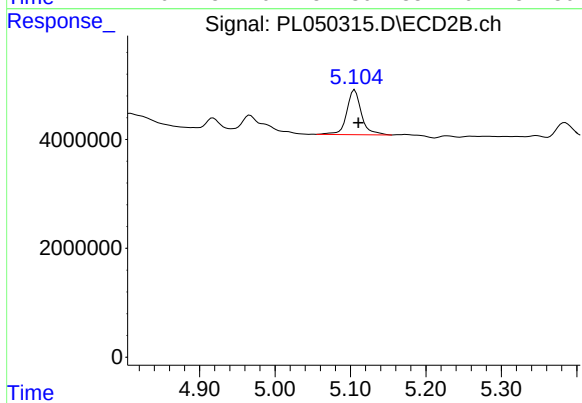

#4 Heptachlor


R.T.: 5.106 min
Delta R.T.: -0.005 min
Response: 11046408
Conc: 2.55 ng/ml

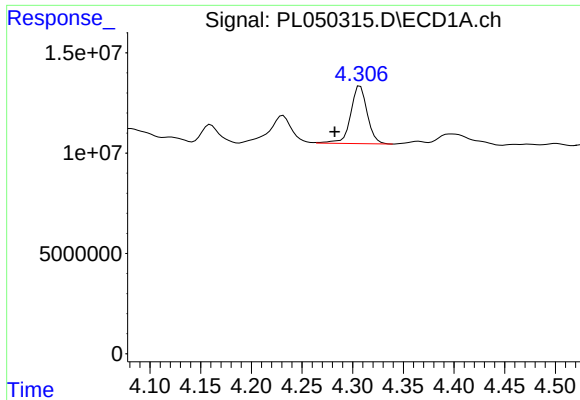

#6 beta-BHC


R.T.: 4.307 min
Delta R.T.: 0.025 min
Response: 32821790
Conc: 4.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

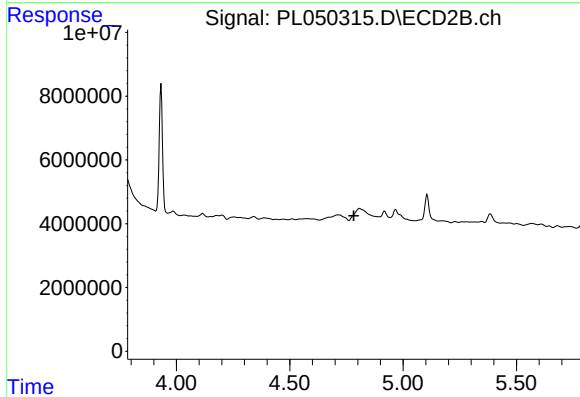


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

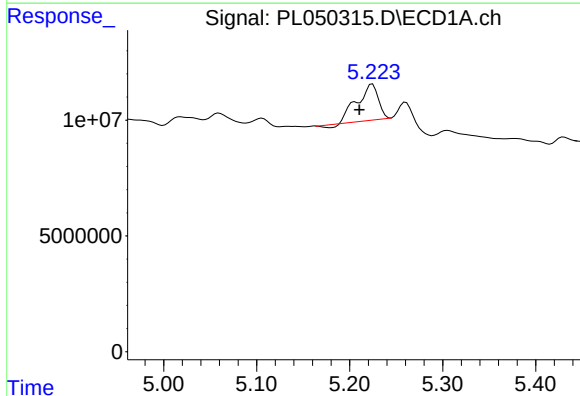


#10 gamma-Chlordane

R.T.: 5.224 min
Delta R.T.: 0.014 min
Response: 23992237
Conc: 1.40 ng/ml

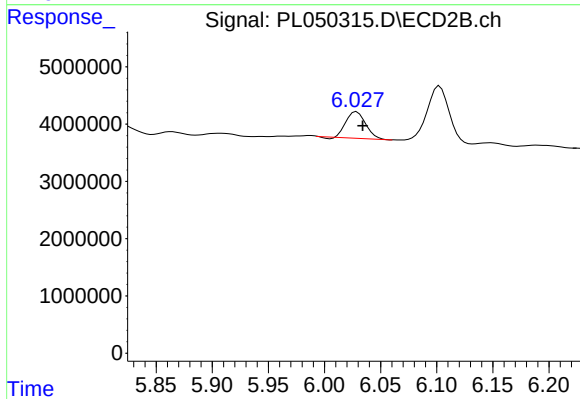

#10 gamma-Chlordane


R.T.: 6.029 min
Delta R.T.: -0.005 min
Response: 5688192
Conc: 1.53 ng/ml

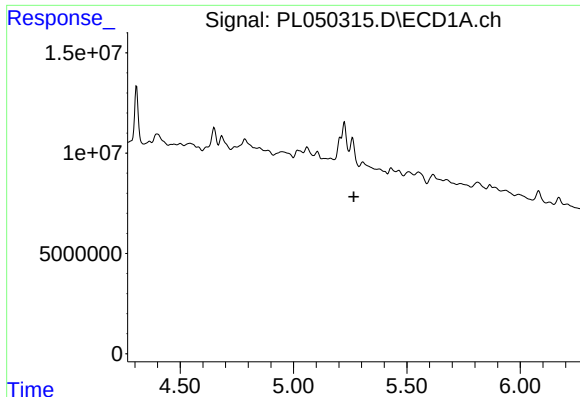

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

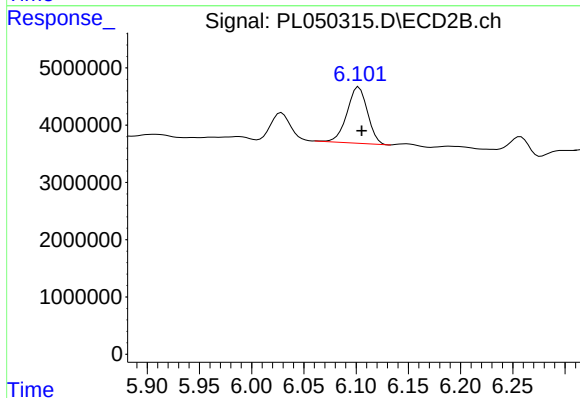


#11 alpha-Chlordane

R.T.: 6.103 min
Delta R.T.: -0.003 min
Response: 13418252
Conc: 3.63 ng/ml

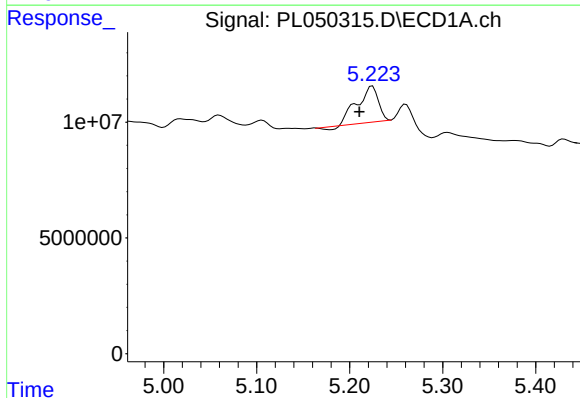


#25 Chlordane-3

R.T.: 5.224 min
Delta R.T.: 0.014 min
Response: 23992237
Conc: 12.77 ng/ml

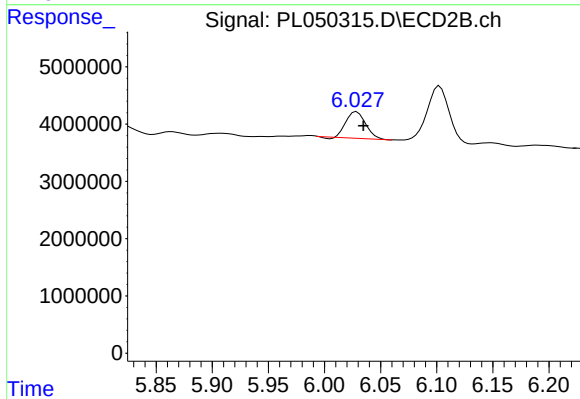

#25 Chlordane-3


R.T.: 6.029 min
Delta R.T.: -0.006 min
Response: 5688192
Conc: 11.43 ng/ml

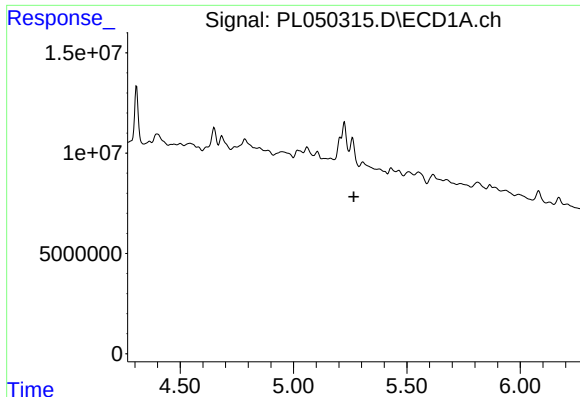

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

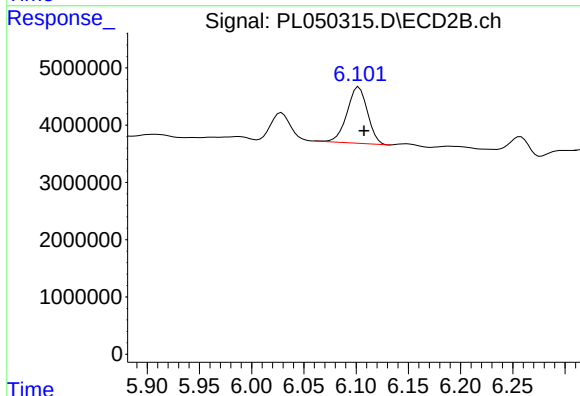


#26 Chlordane-4

R.T.: 6.103 min
Delta R.T.: -0.005 min
Response: 13418252
Conc: 22.58 ng/ml

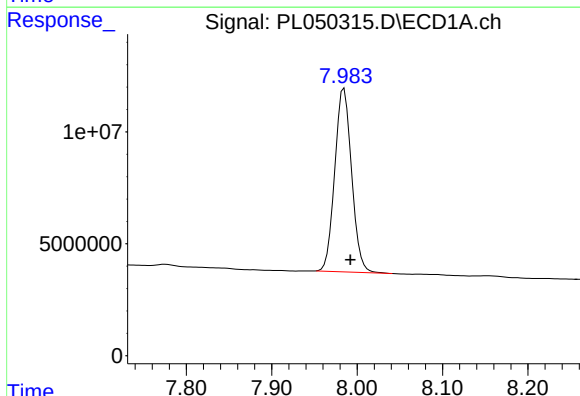

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 112535009
Conc: 8.86 ng/ml

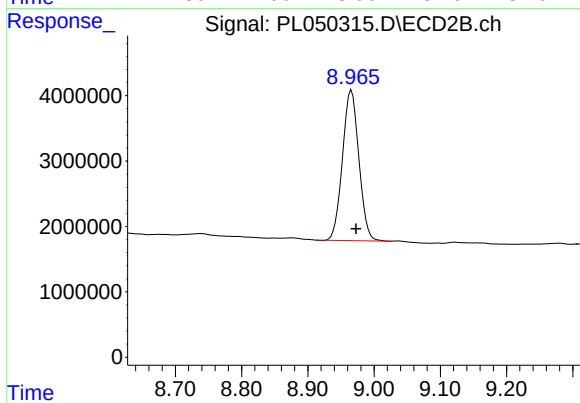

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 39557747
Conc: 11.78 ng/ml