

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
 Data File : PL076357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 09:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 23:54:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	10.375	0	1007063	N.D.	0.600 #
Target Compounds							
2)	A alpha-BHC	6.199f	0.000	241079	0	0.257	N.D. #
7)	B delta-BHC	0.000	6.397	0	276512	N.D.	0.116 #
8)	B Heptachlo...	8.125	0.000	1462024	0	1.878	N.D. #
11)	B alpha-Chl...	0.000	7.380f	0	211760	N.D.	0.105 #
14)	MA Endrin	0.000	8.055f	0	669423	N.D.	0.463 #
15)	B Endosulfa...	9.304	0.000	220928	0	0.370	N.D. #
20)	A Methoxychlor	0.000	9.065f	0	13286557	N.D.	15.575 #
21)	B Endrin ke...	10.185f	0.000	768646	0	1.137	N.D. #
22)	Mirex	10.636	0.000	1043364	0	2.040	N.D. #
24)	Chlordane-2	0.000	6.657f	0	5675598	N.D.	87.480 #
26)	Chlordane-4	0.000	7.380f	0	211760	N.D.	1.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
Data File : PL076357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 09:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 23:54:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

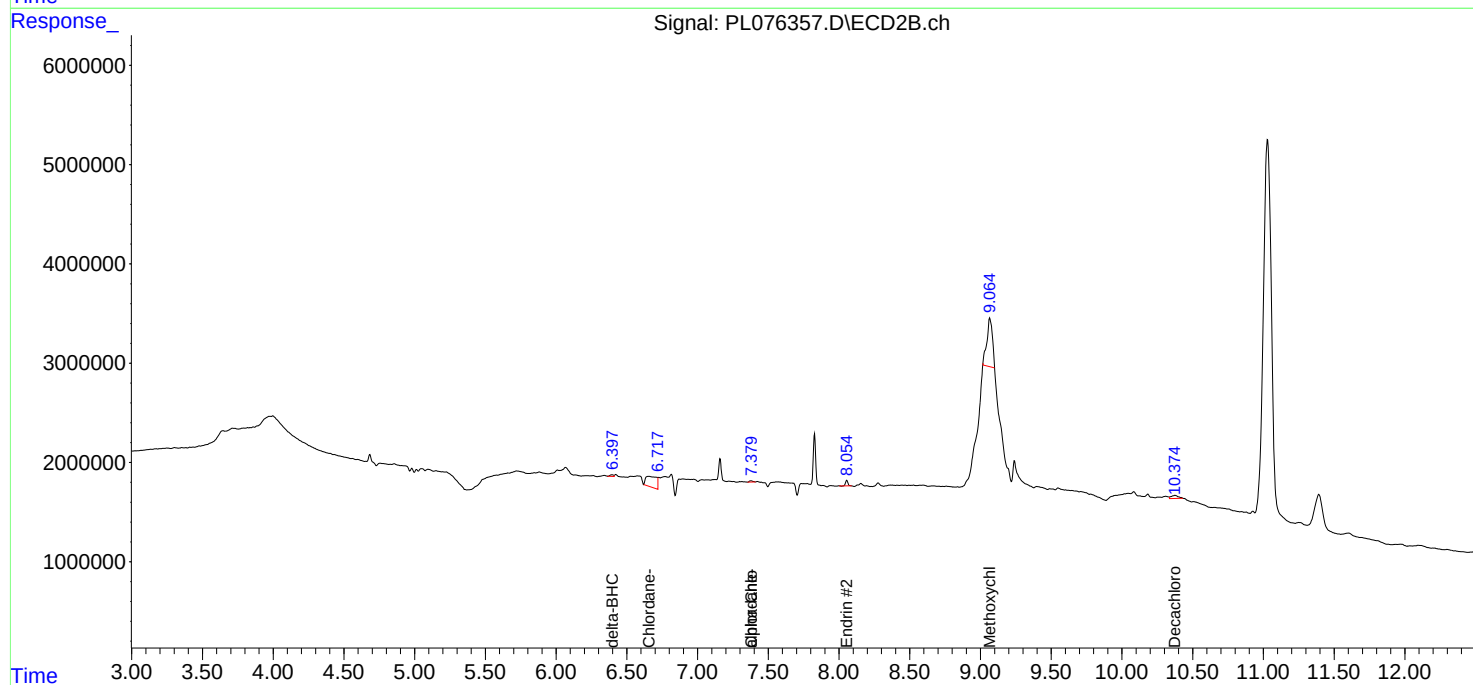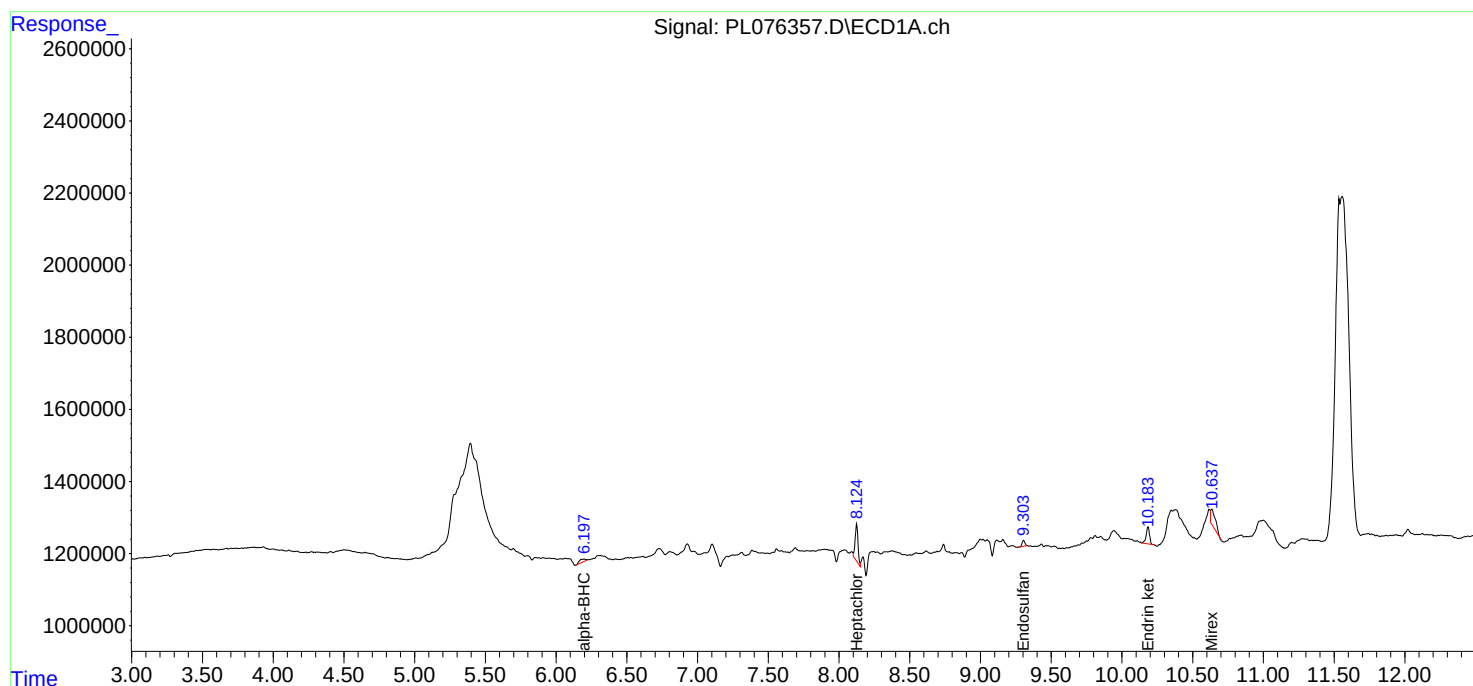


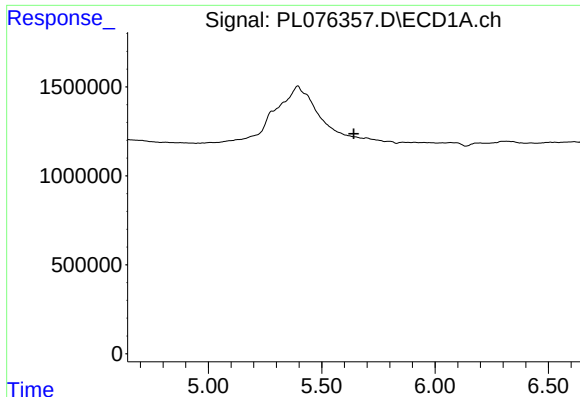

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.641 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

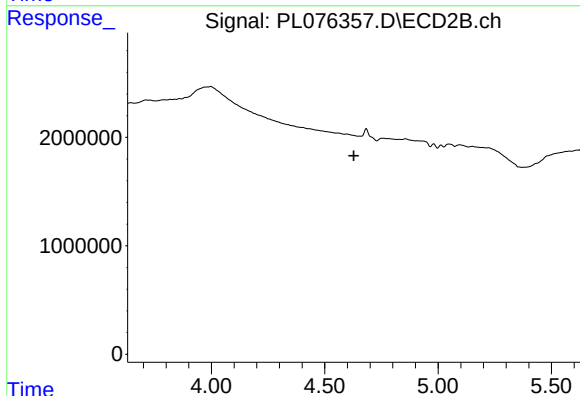


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

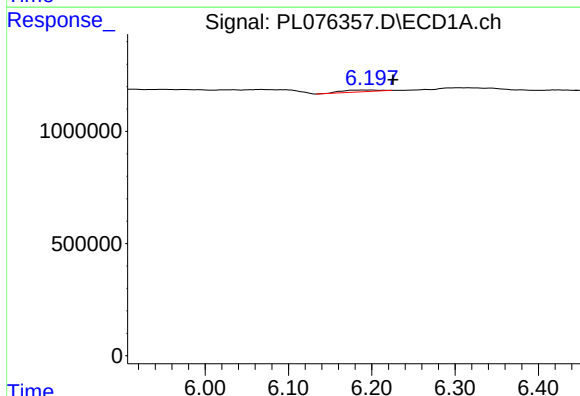


#2 alpha-BHC

R.T.: 6.199 min
Delta R.T.: -0.026 min
Response: 241079
Conc: 0.26 ng/ml

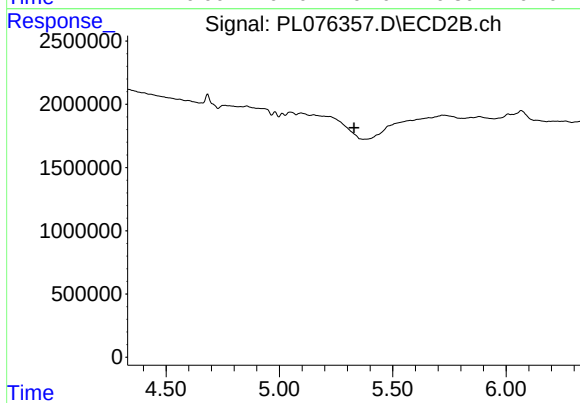

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 5.329 min
Response: 0
Conc: N.D.

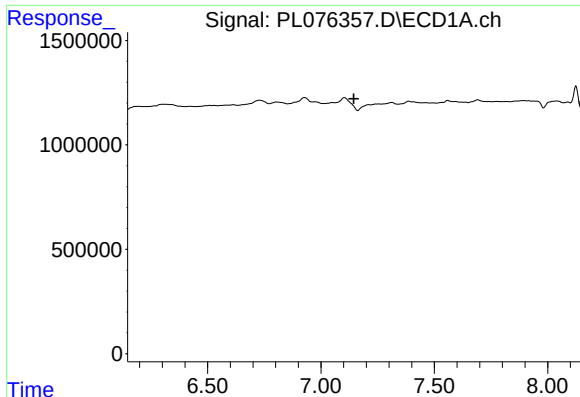

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

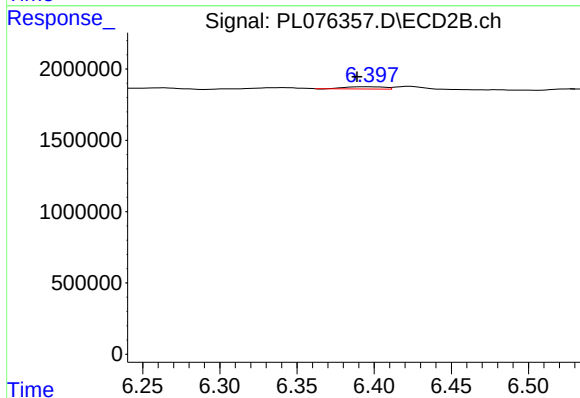


#7 delta-BHC

R.T.: 6.397 min
Delta R.T.: 0.009 min
Response: 276512
Conc: 0.12 ng/ml

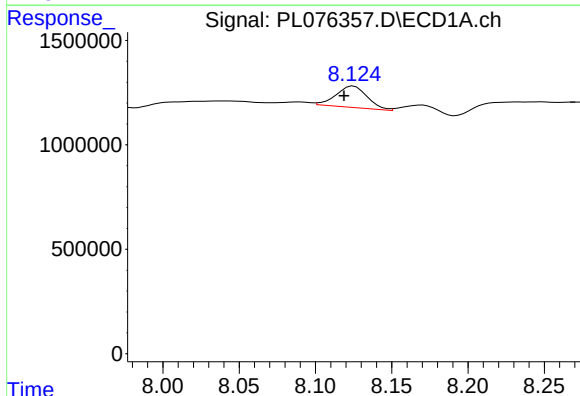


#8 Heptachlor epoxide

R.T.: 8.125 min
Delta R.T.: 0.006 min
Response: 1462024
Conc: 1.88 ng/ml

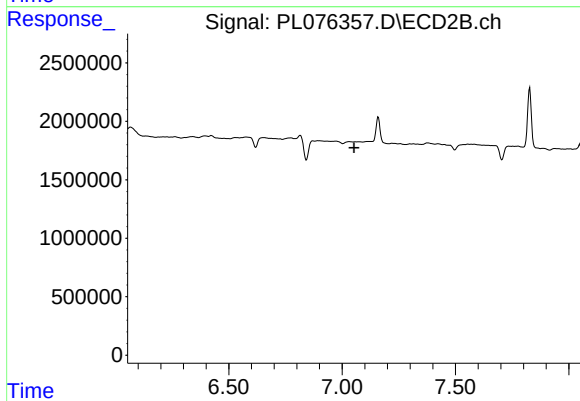

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.053 min
Response: 0
Conc: N.D.

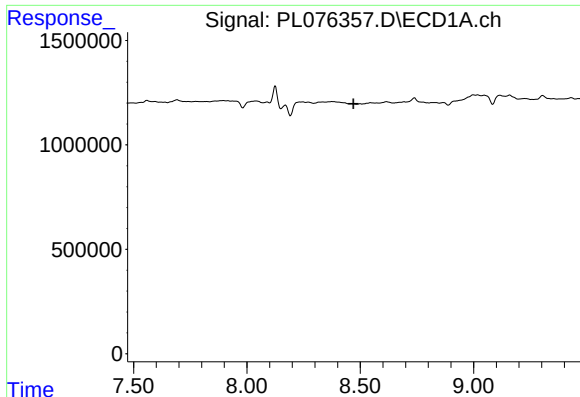

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

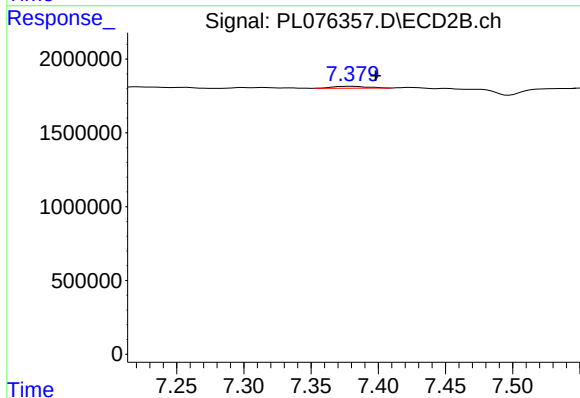


#11 alpha-Chlordane

R.T.: 7.380 min
Delta R.T.: -0.018 min
Response: 211760
Conc: 0.11 ng/ml

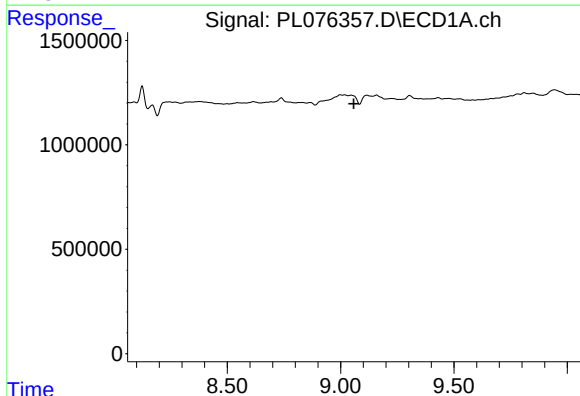


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

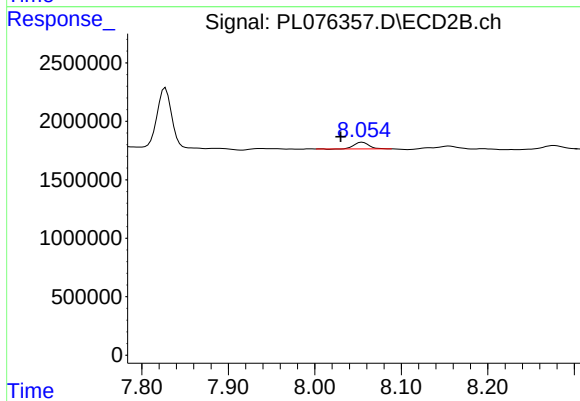

#14 Endrin


R.T.: 8.055 min
Delta R.T.: 0.025 min
Response: 669423
Conc: 0.46 ng/ml

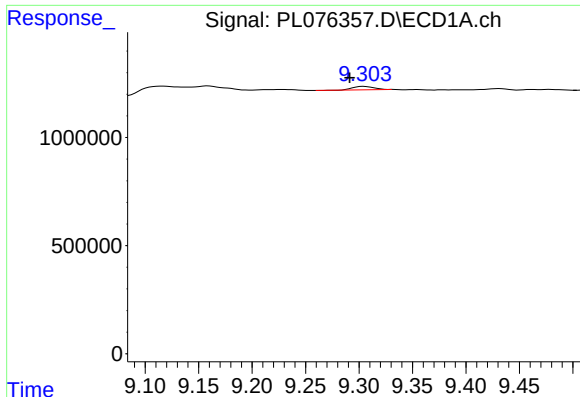

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.013 min
Response: 220928
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

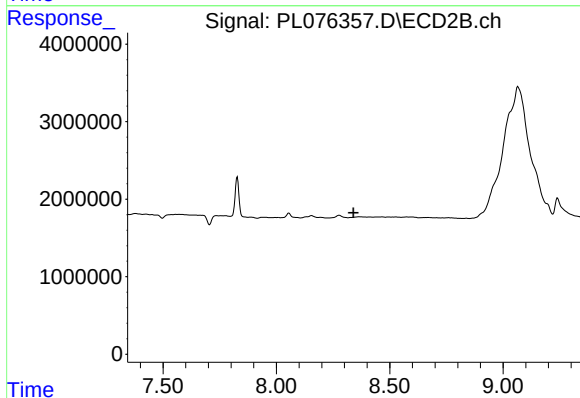


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.340 min
Response: 0
Conc: N.D.

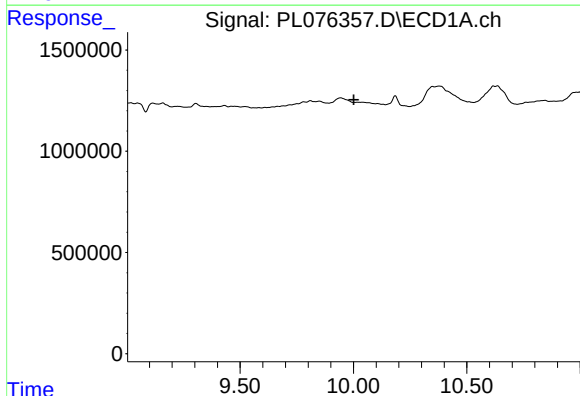


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 10.002 min
Response: 0
Conc: N.D.

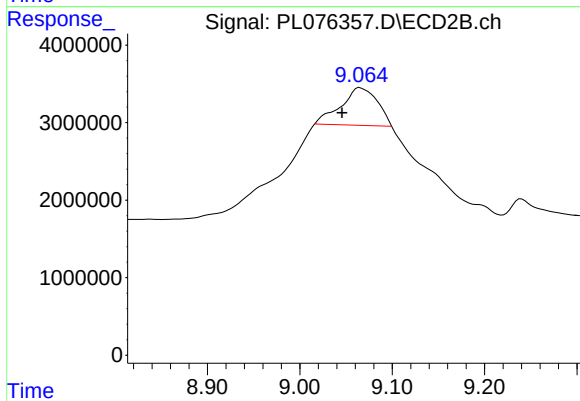

#20 Methoxychlor


R.T.: 9.065 min
Delta R.T.: 0.019 min
Response: 13286557
Conc: 15.58 ng/ml

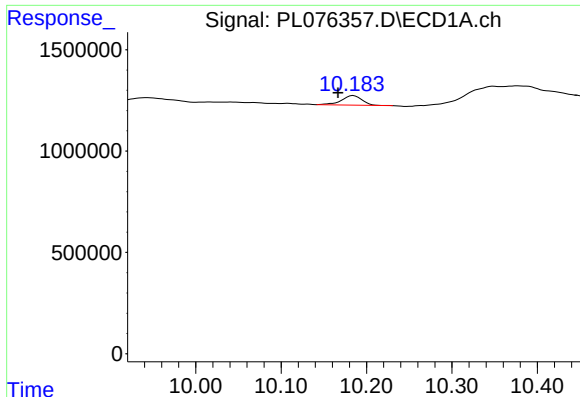

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.018 min
Response: 768646
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

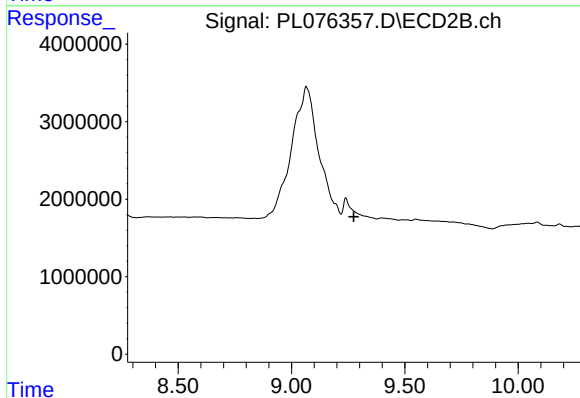


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

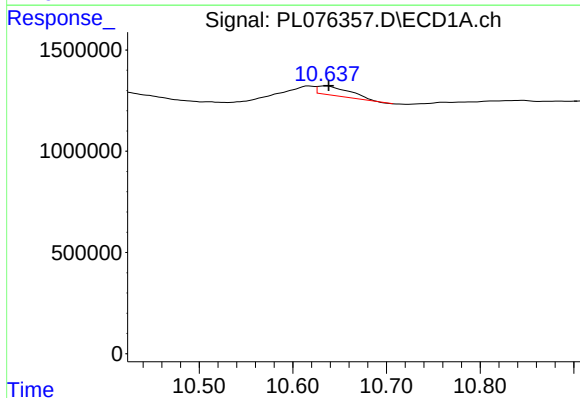


#22 Mirex

R.T.: 10.636 min
Delta R.T.: -0.002 min
Response: 1043364
Conc: 2.04 ng/ml

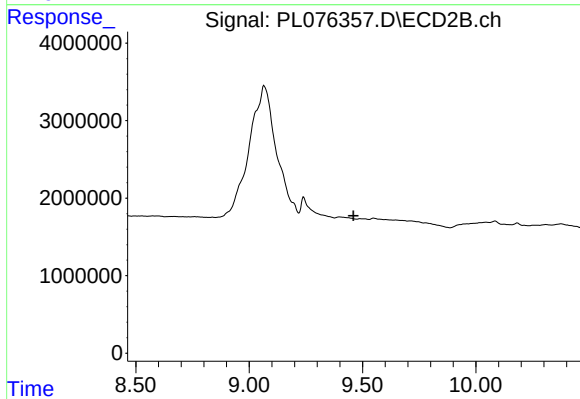

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.460 min
Response: 0
Conc: N.D.

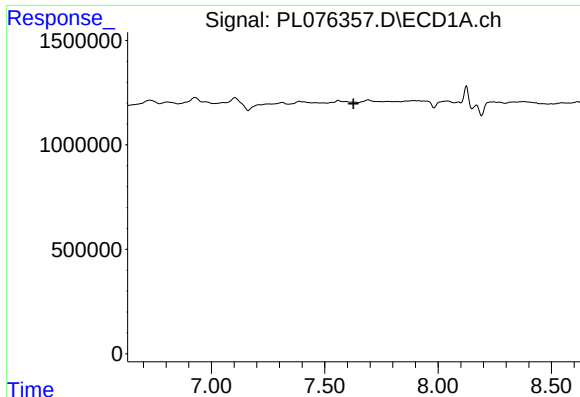

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.627 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

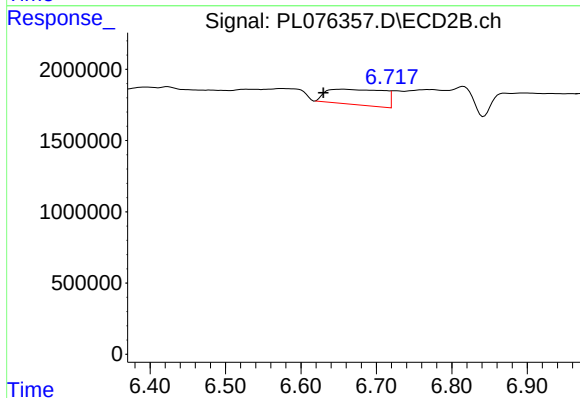


#24 Chlordane-2

R.T.: 6.657 min
Delta R.T.: 0.027 min
Response: 5675598
Conc: 87.48 ng/ml

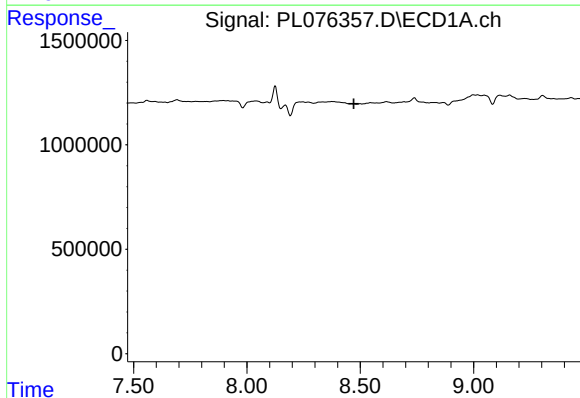


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

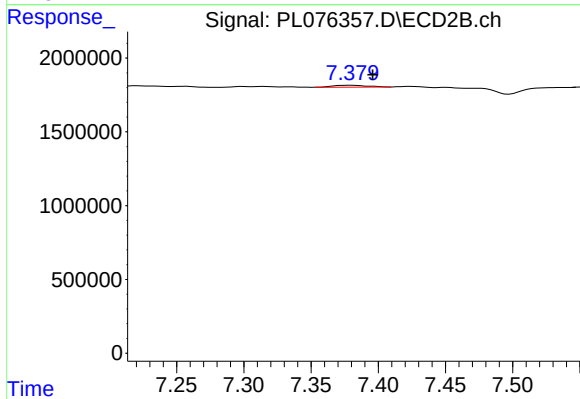

#26 Chlordane-4


R.T.: 7.380 min
Delta R.T.: -0.016 min
Response: 211760
Conc: 1.15 ng/ml

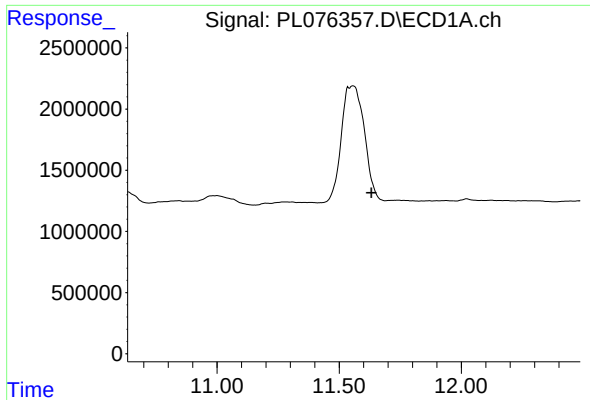

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

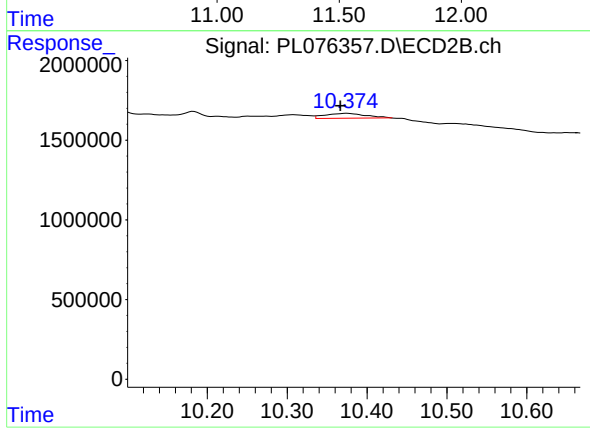

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.008 min
Response: 1007063
Conc: 0.60 ng/ml