

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
 Data File : PL076358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 10:09
 Operator : AR\AJ
 Sample : L.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 23:54:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.630	14624084	35267480	20.300	17.443
28)	SA Decachlor...	11.635	10.368	13003001	29908356	22.040	17.825
Target Compounds							
4)	MA Heptachlor	0.000	6.136f	0	340368	N.D.	0.140 #
6)	B beta-BHC	0.000	6.136	0	340368	N.D.	0.311 #
7)	B delta-BHC	7.122f	6.397	676410	546188	1.010	0.228 #
8)	B Heptachlo...	0.000	7.055	0	247646	N.D.	0.126 #
11)	B alpha-Chl...	0.000	7.377f	0	86931	N.D.	0.043 #
15)	B Endosulfa...	9.303	0.000	345365	0	0.578	N.D. #
17)	MA 4,4'-DDT	0.000	8.455	0	83189	N.D.	0.053 #
21)	B Endrin ke...	10.185f	0.000	962688	0	1.424	N.D. #
26)	Chlordane-4	0.000	7.377f	0	86931	N.D.	0.471 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
Data File : PL076358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 10:09
Operator : AR\AJ
Sample : L.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 23:54:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

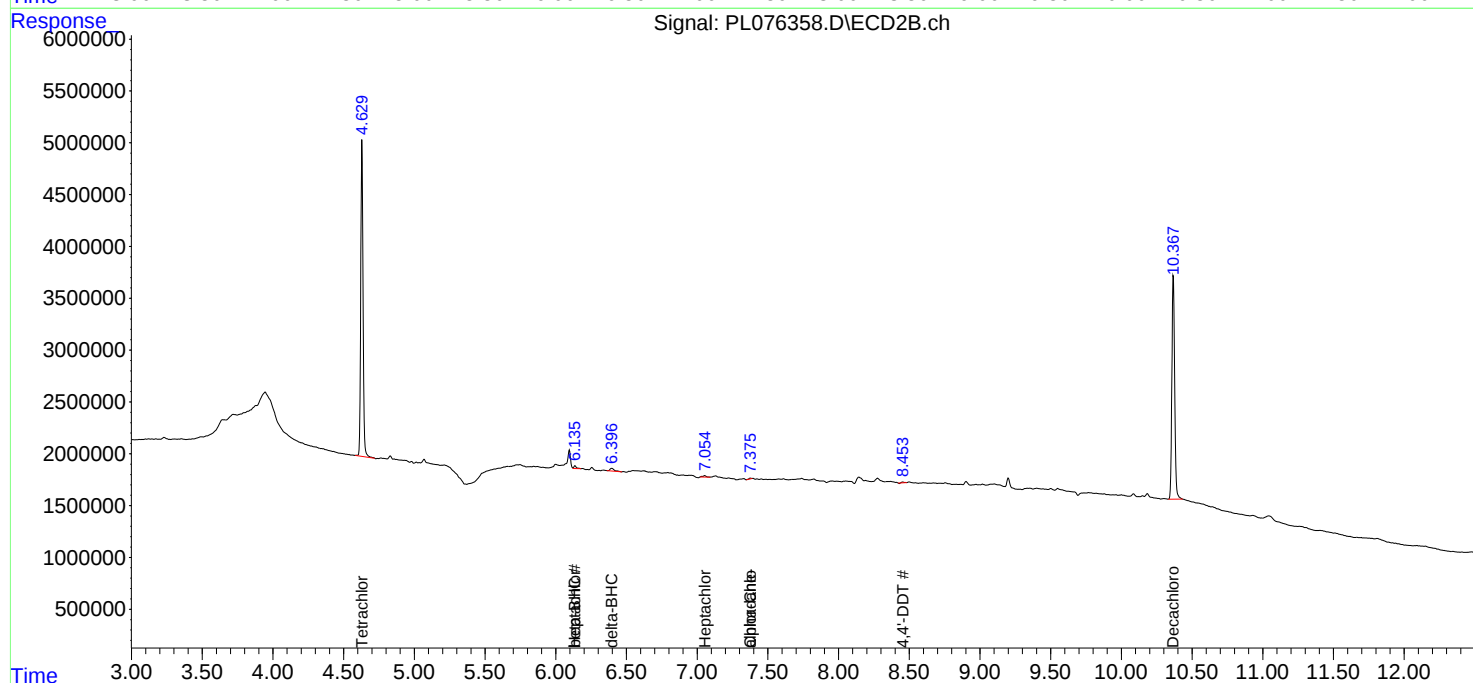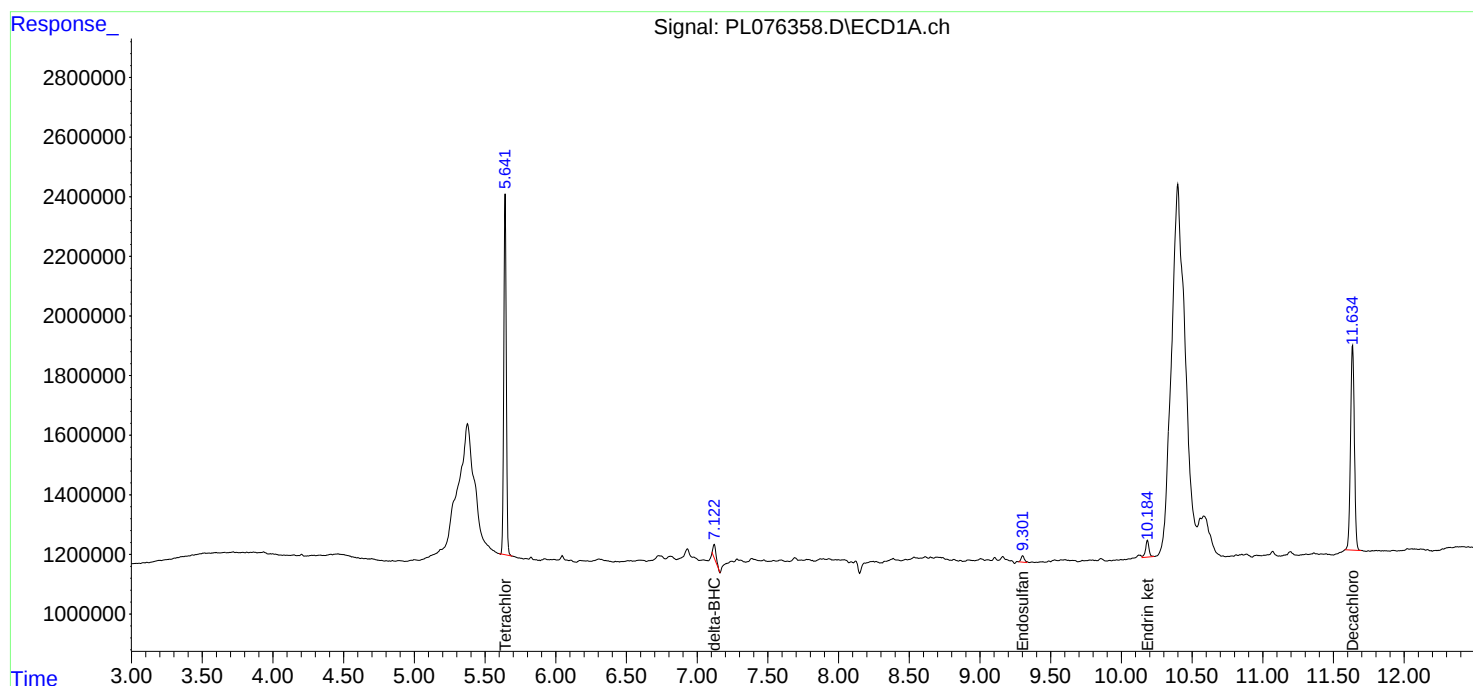


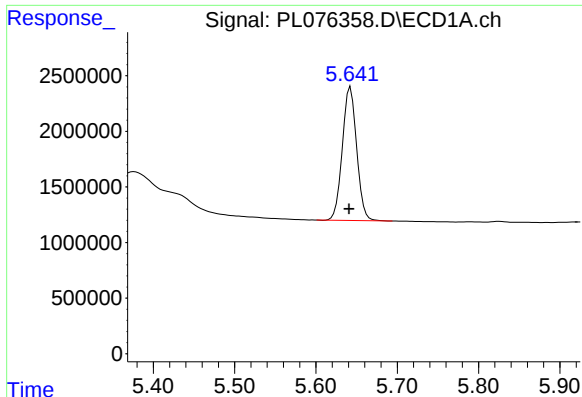

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 14624084
Conc: 20.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

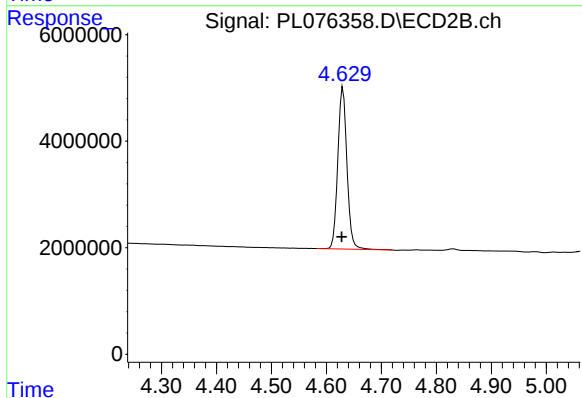


#1 Tetrachloro-m-xylene

R.T.: 4.630 min
Delta R.T.: 0.002 min
Response: 35267480
Conc: 17.44 ng/ml

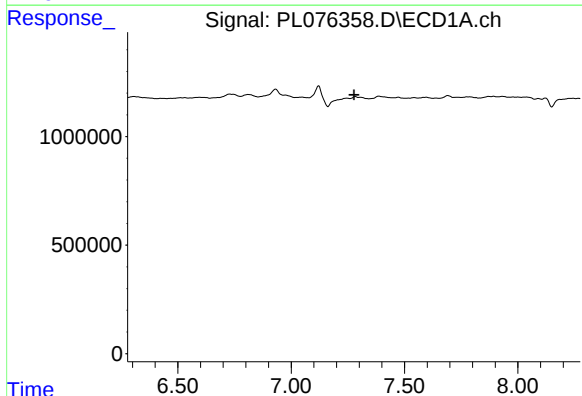


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.278 min
Response: 0
Conc: N.D.

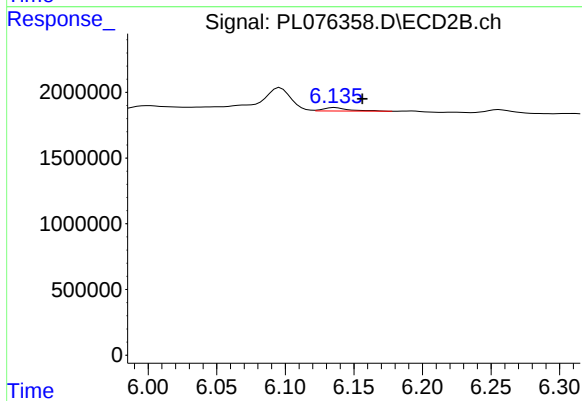

#4 Heptachlor


R.T.: 6.136 min
Delta R.T.: -0.020 min
Response: 340368
Conc: 0.14 ng/ml

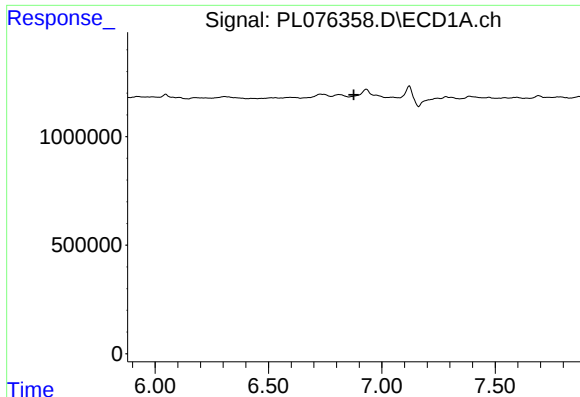

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

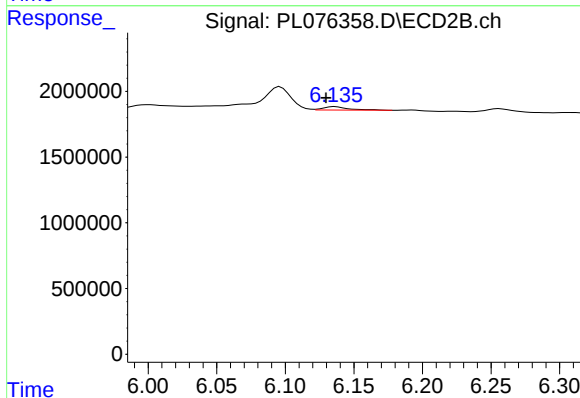


#6 beta-BHC

R.T.: 6.136 min
Delta R.T.: 0.007 min
Response: 340368
Conc: 0.31 ng/ml

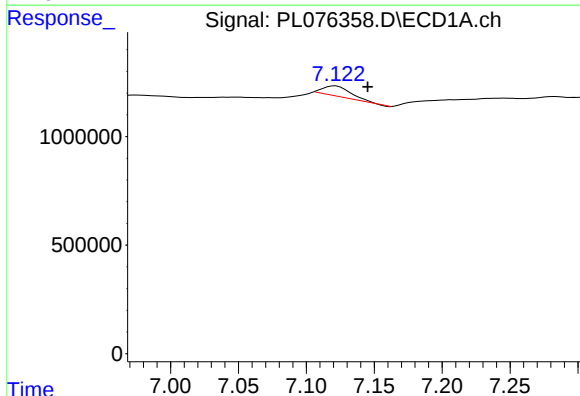


#7 delta-BHC

R.T.: 7.122 min
Delta R.T.: -0.024 min
Response: 676410
Conc: 1.01 ng/ml

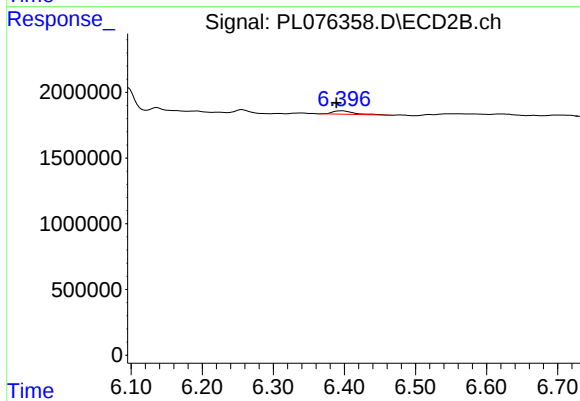

#7 delta-BHC


R.T.: 6.397 min
Delta R.T.: 0.008 min
Response: 546188
Conc: 0.23 ng/ml

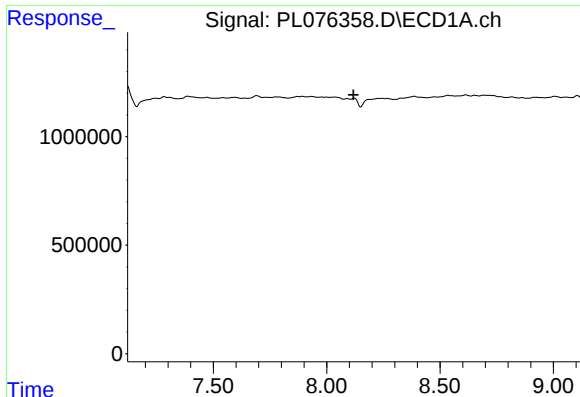

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 8.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

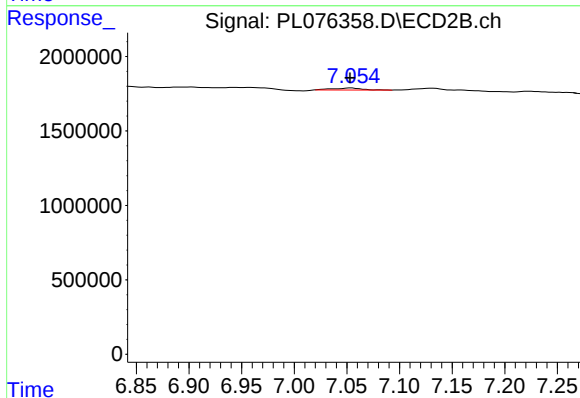


#8 Heptachlor epoxide

R.T.: 7.055 min
Delta R.T.: 0.002 min
Response: 247646
Conc: 0.13 ng/ml

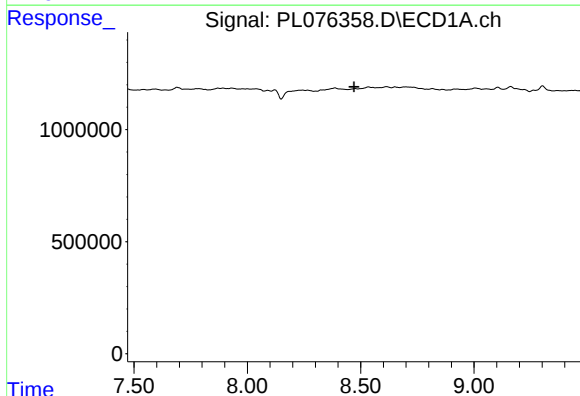


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.471 min
Response: 0
Conc: N.D.

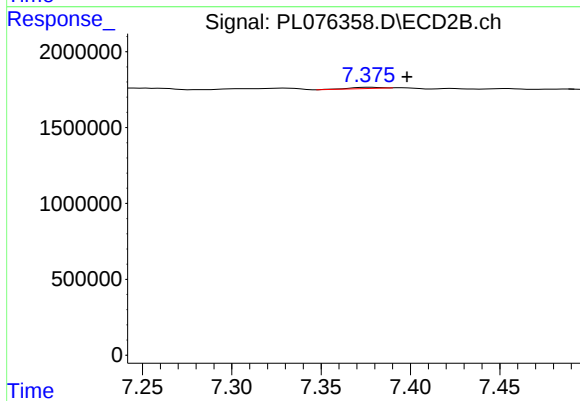

#11 alpha-Chlordane


R.T.: 7.377 min
Delta R.T.: -0.021 min
Response: 86931
Conc: 0.04 ng/ml

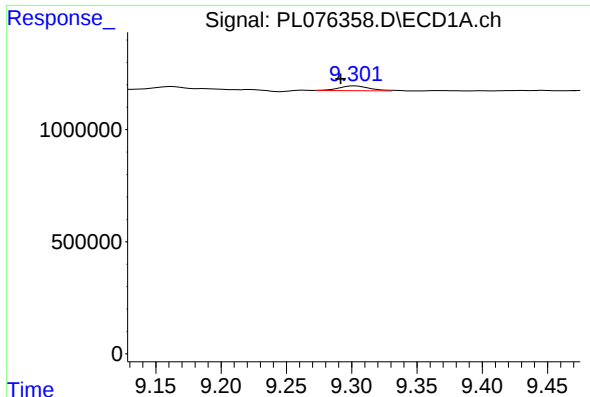

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.011 min
Response: 345365
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

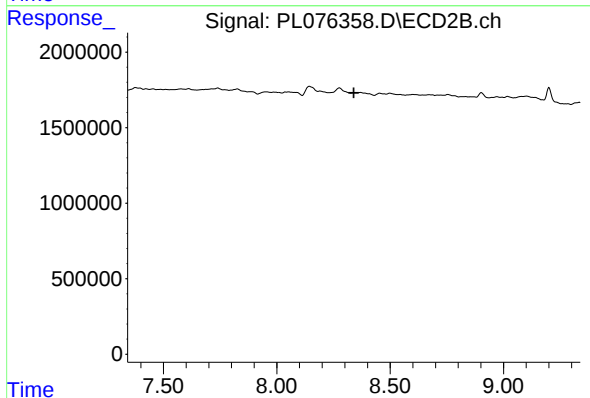


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.340 min
Response: 0
Conc: N.D.

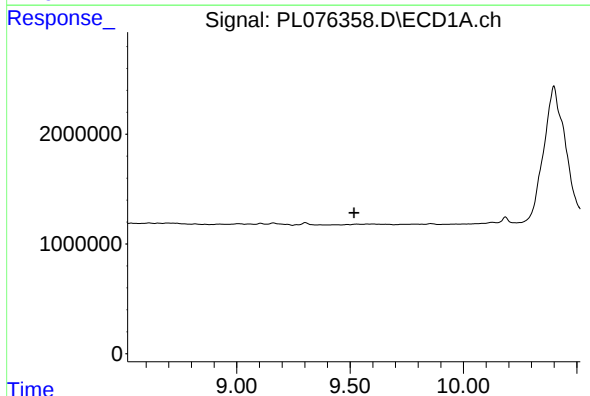


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.517 min
Response: 0
Conc: N.D.

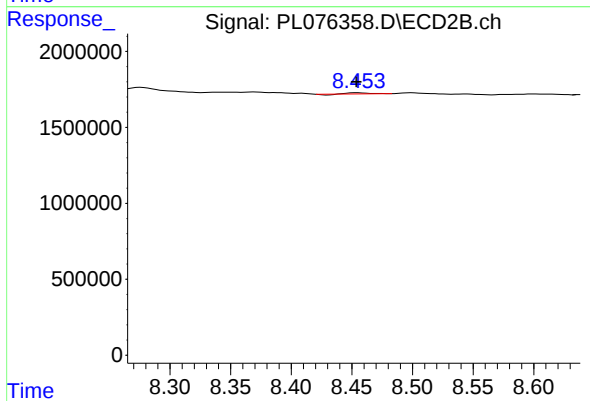

#17 4,4'-DDT


R.T.: 8.455 min
Delta R.T.: 0.001 min
Response: 83189
Conc: 0.05 ng/ml

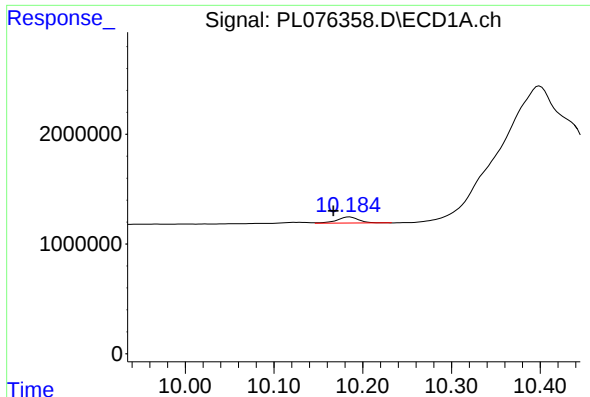

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.018 min
Response: 962688
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

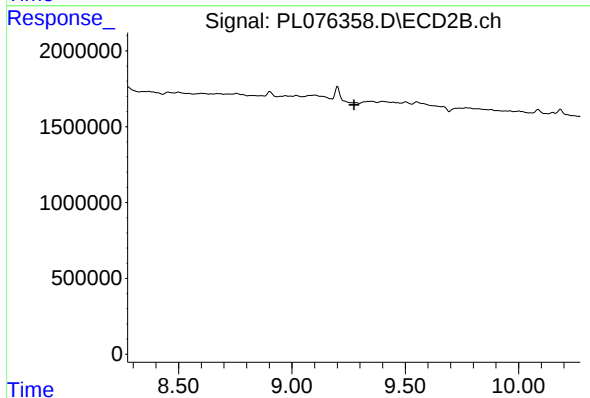


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

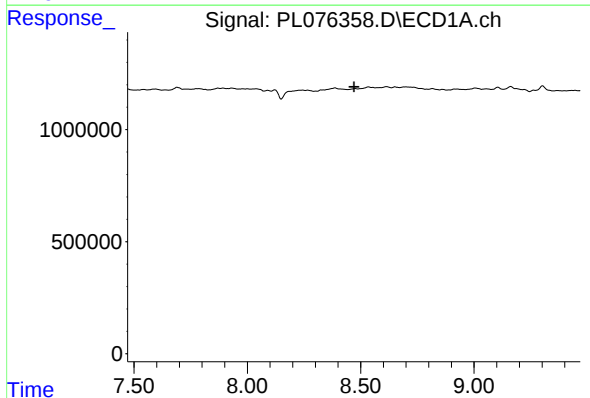


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

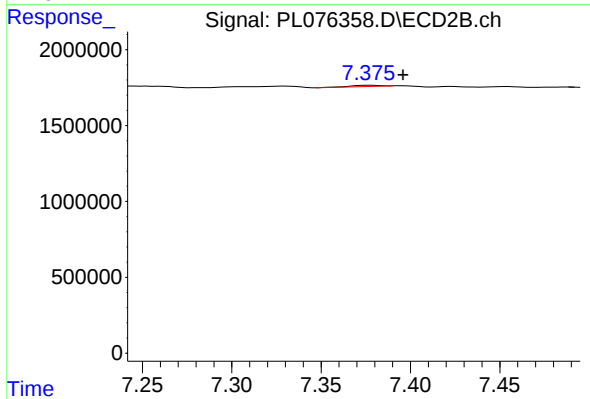

#26 Chlordane-4


R.T.: 7.377 min
Delta R.T.: -0.019 min
Response: 86931
Conc: 0.47 ng/ml

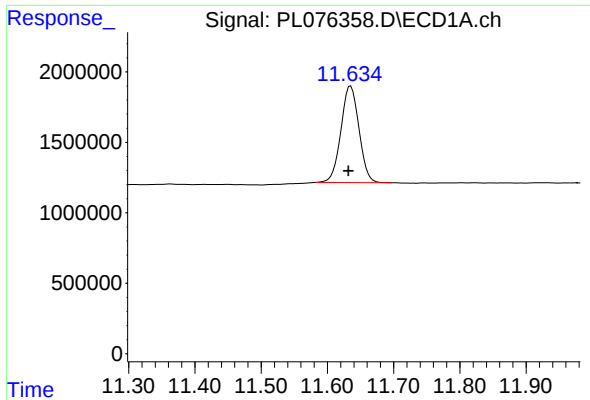

#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: 0.003 min
Response: 13003001
Conc: 22.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

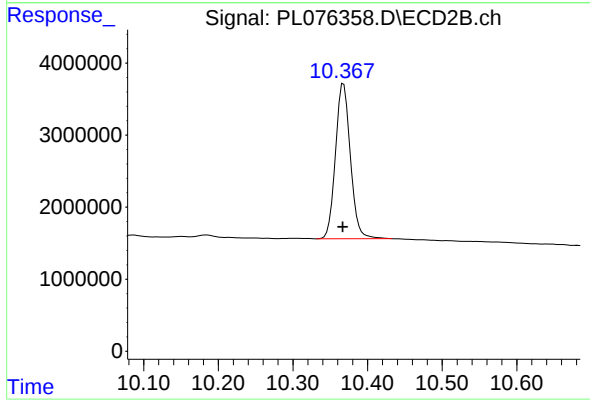

#28 Decachlorobiphenyl

R.T.: 10.368 min
Delta R.T.: 0.001 min
Response: 29908356
Conc: 17.82 ng/ml